

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080322\
 Data File : PL076864.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2022 14:13
 Operator : AR\AJ
 Sample : N4016-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MH-DS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 00:13:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:34:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.641	20100613	51825213	21.114	22.453
28)	SA Decachlor...	8.914	7.749	15869310	39001248	19.970	20.286
Target Compounds							
10)	B gamma-Chl...	5.825	4.815	919728	2665946	0.900m	1.089
11)	B alpha-Chl...	5.904	4.878	1145566	2930749	1.093	1.222



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080322\
Data File : PL076864.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2022 14:13
Operator : AR\AJ
Sample : N4016-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MH-DS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 00:13:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:34:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

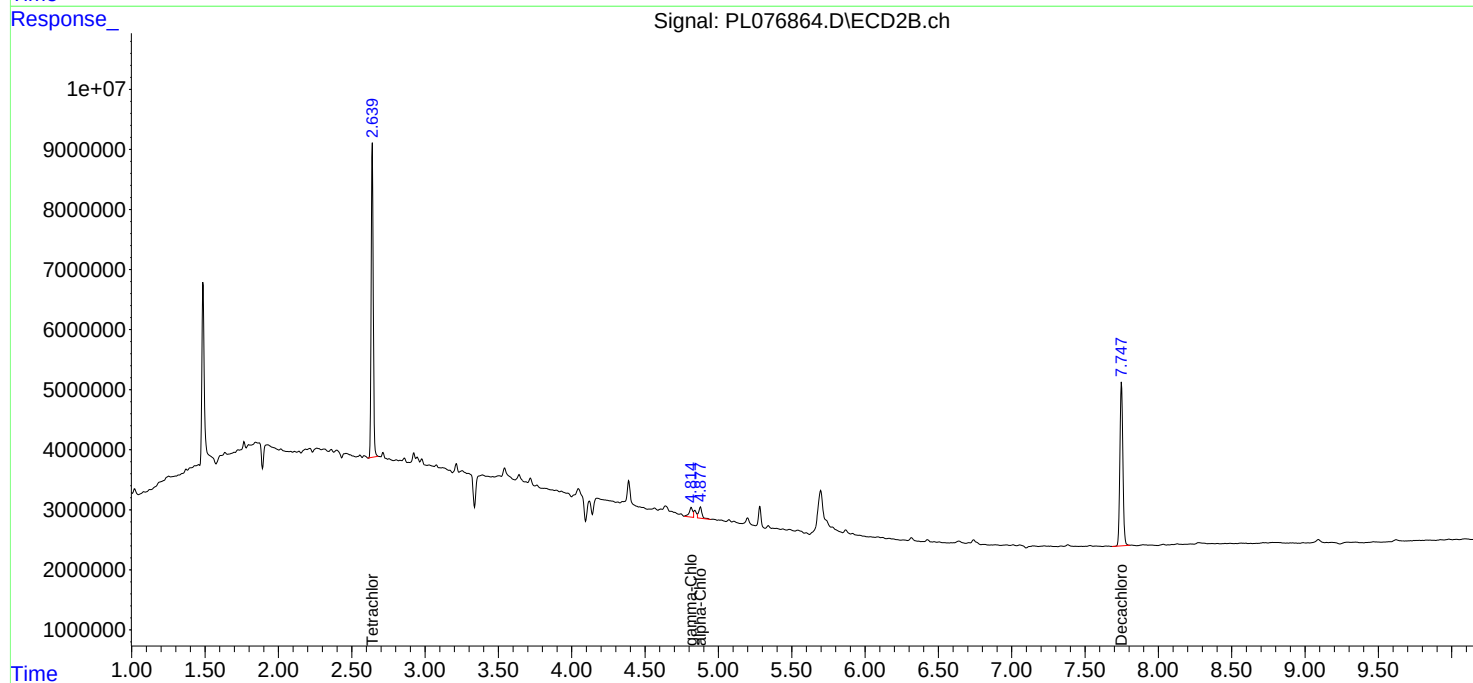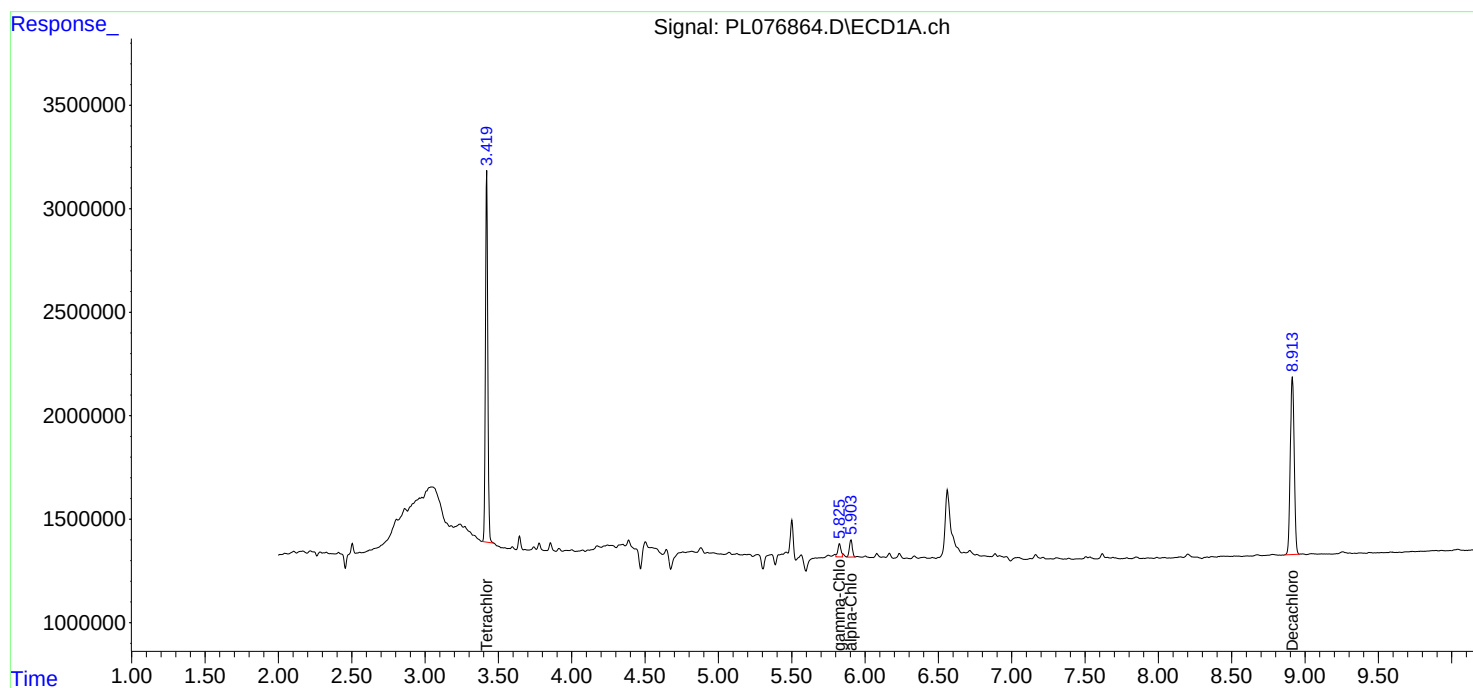


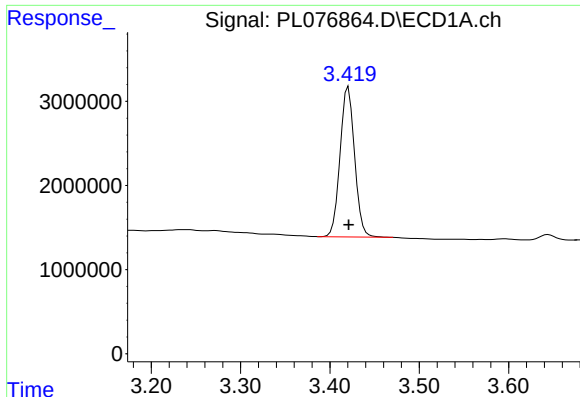

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 20100613
Conc: 21.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-DS

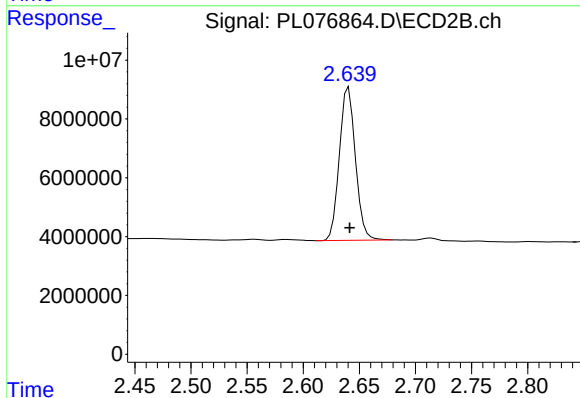


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: 0.000 min
Response: 51825213
Conc: 22.45 ng/ml

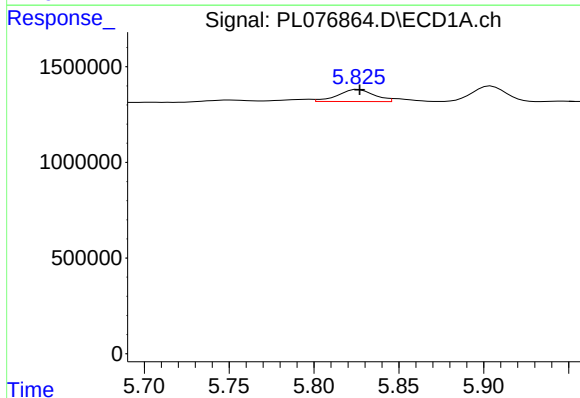


#10 gamma-Chlordane

R.T.: 5.825 min
Delta R.T.: -0.002 min
Response: 919728
Conc: 0.90 ng/ml m

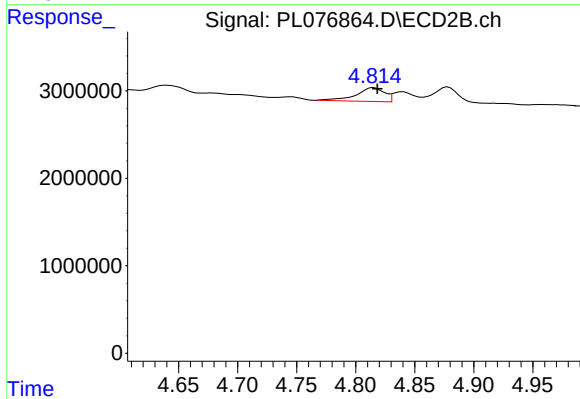

#10 gamma-Chlordane


R.T.: 4.815 min
Delta R.T.: -0.003 min
Response: 2665946
Conc: 1.09 ng/ml

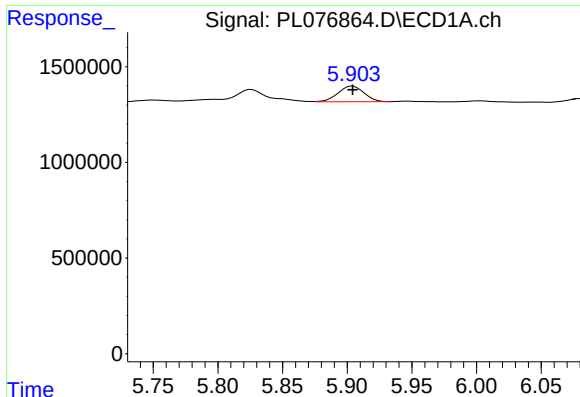

#11 alpha-Chlordane


R.T.: 5.904 min
Delta R.T.: 0.000 min
Response: 1145566
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-DS

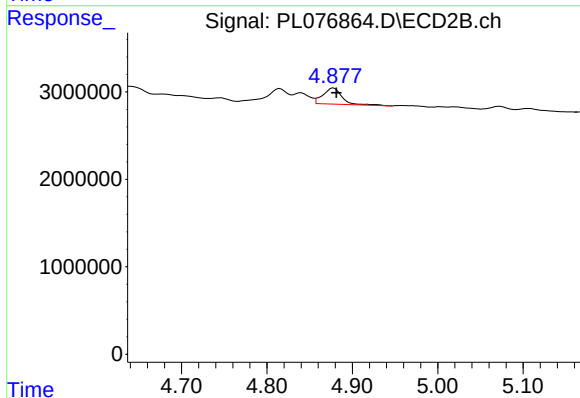


#11 alpha-Chlordane

R.T.: 4.878 min
Delta R.T.: -0.003 min
Response: 2930749
Conc: 1.22 ng/ml

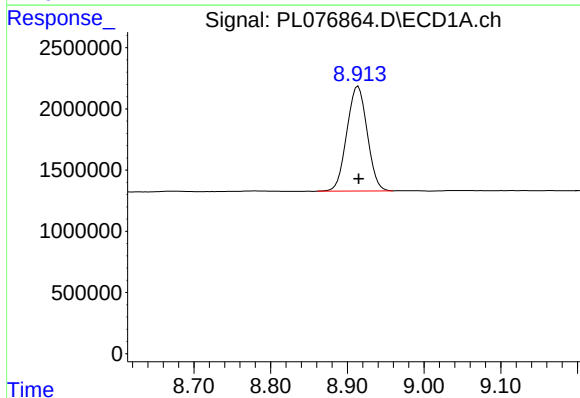

#28 Decachlorobiphenyl

R.T.: 8.914 min
Delta R.T.: 0.000 min
Response: 15869310
Conc: 19.97 ng/ml

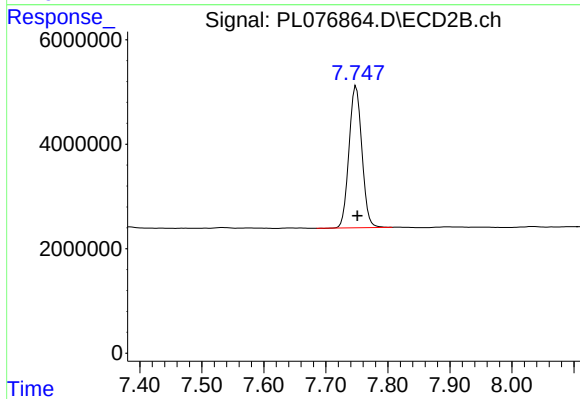

#28 Decachlorobiphenyl

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 39001248
Conc: 20.29 ng/ml