

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080323\
 Data File : PL084455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 09:59
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 11:15:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 11:15:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.686	161.8E6	98962246	74.710	75.577
28)	SA Decachlor...	9.024	7.868	105.9E6	86985305	71.618	72.846
Target Compounds							
23)	Chlordane-1	4.644	3.689	71006804	28432620	740.616	753.704
24)	Chlordane-2	5.176	4.270	80541400	35466646	720.543	731.176
25)	Chlordane-3	5.890	4.903	297.2E6	105.3E6	755.257	759.064
26)	Chlordane-4	5.973	4.965	351.8E6	108.9E6	747.942	763.881
27)	Chlordane-5	6.823	5.864	54267216	37796403	735.331	755.436



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080323\
Data File : PL084455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 09:59
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 11:15:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 11:15:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

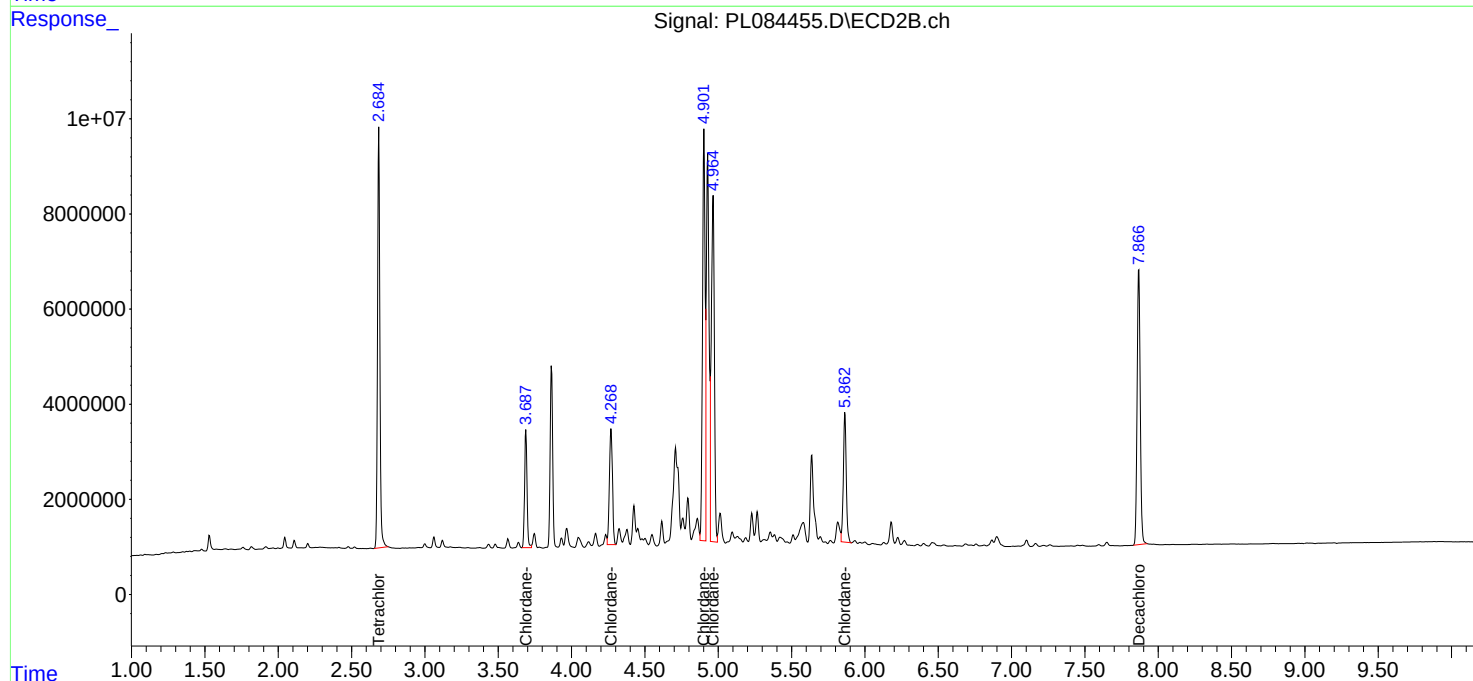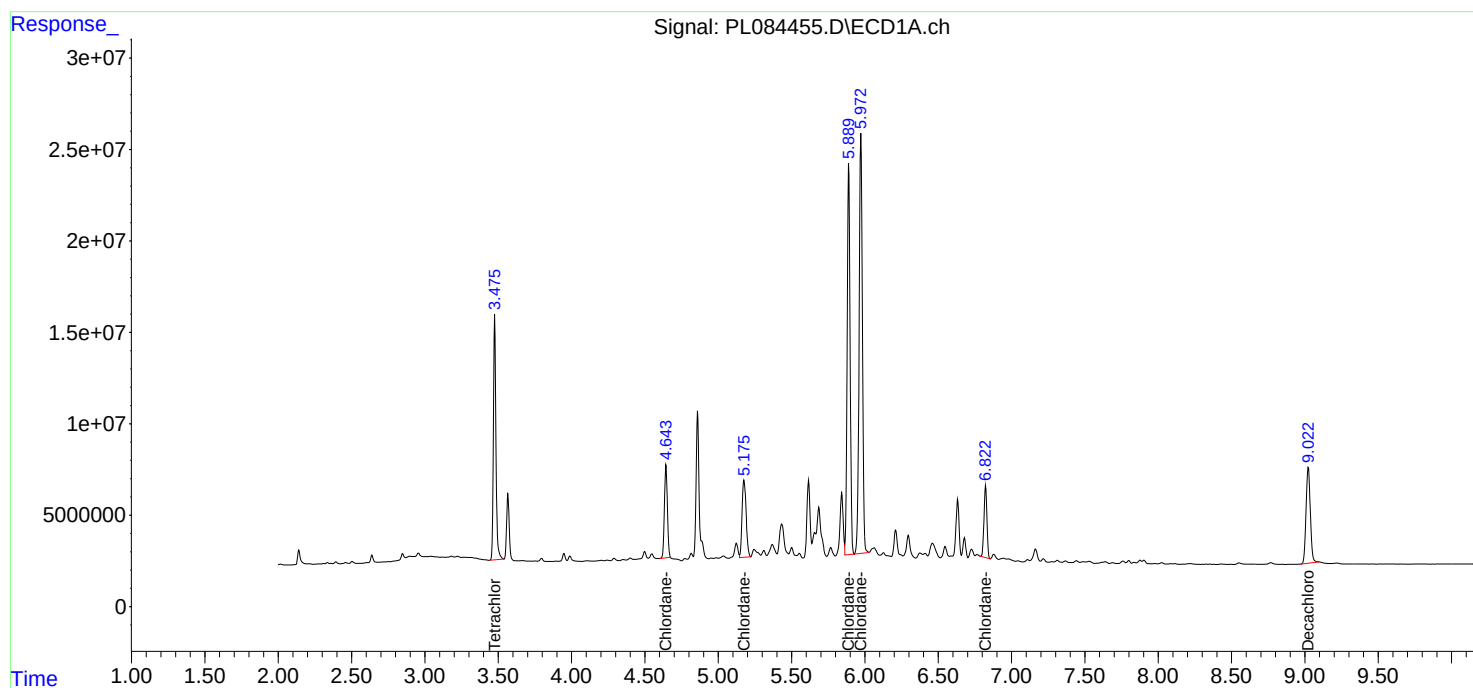


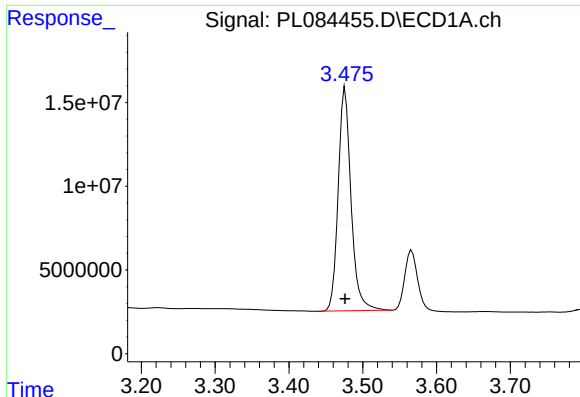

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 161786169
Conc: 74.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

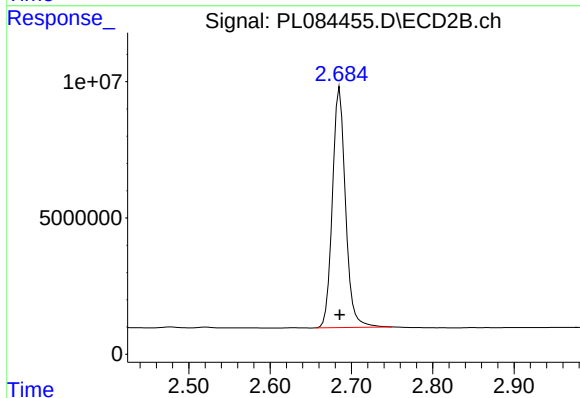


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.000 min
Response: 98962246
Conc: 75.58 ng/ml

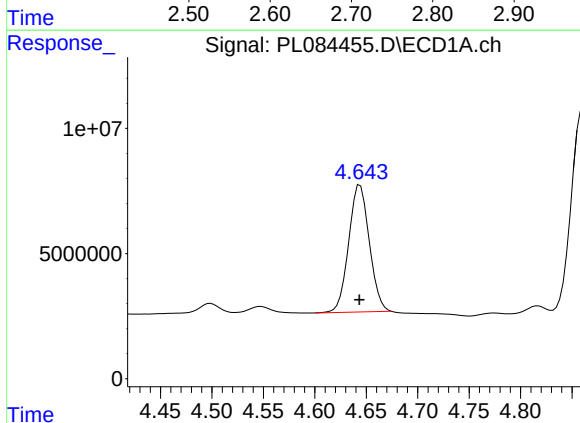


#23 Chlordane-1

R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 71006804
Conc: 740.62 ng/ml

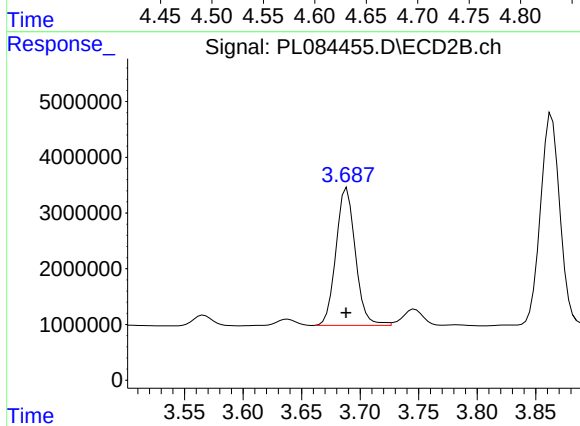

#23 Chlordane-1


R.T.: 3.689 min
Delta R.T.: 0.000 min
Response: 28432620
Conc: 753.70 ng/ml

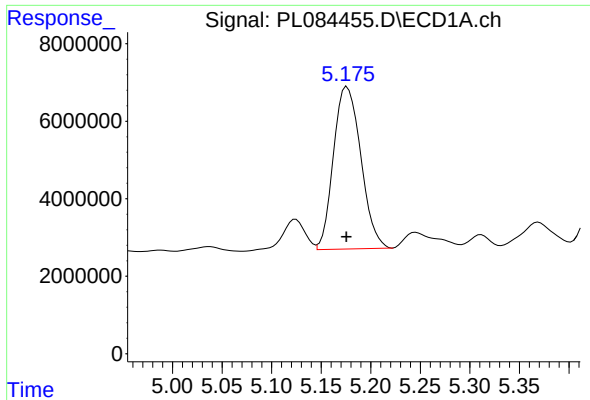

#24 Chlordane-2


R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 80541400
Conc: 720.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

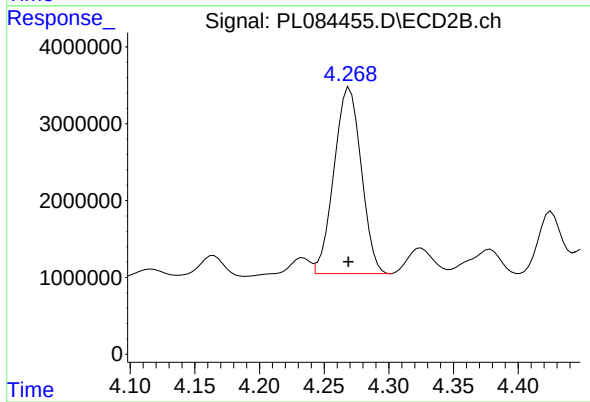


#24 Chlordane-2

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 35466646
Conc: 731.18 ng/ml

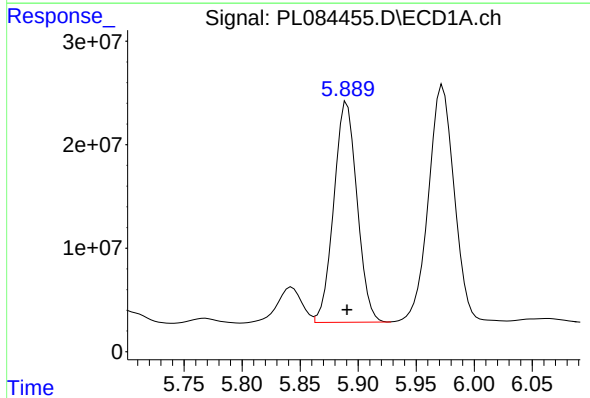


#25 Chlordane-3

R.T.: 5.890 min
Delta R.T.: 0.000 min
Response: 297184045
Conc: 755.26 ng/ml

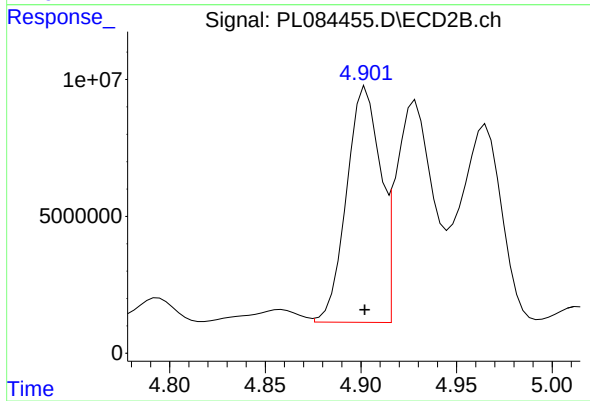

#25 Chlordane-3


R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 105343163
Conc: 759.06 ng/ml

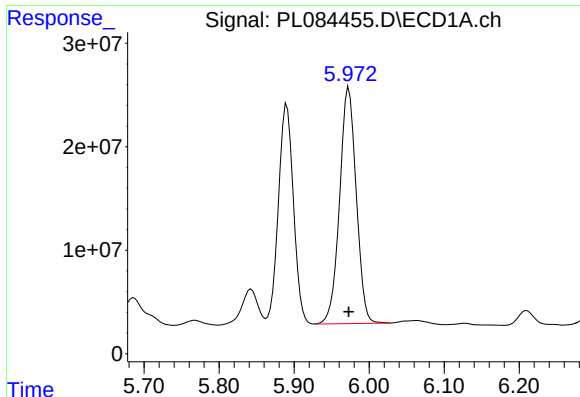

#26 Chlordane-4


R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 351785689
Conc: 747.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

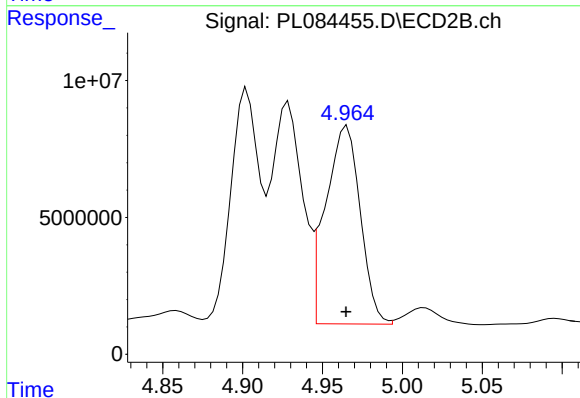


#26 Chlordane-4

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 108870628
Conc: 763.88 ng/ml

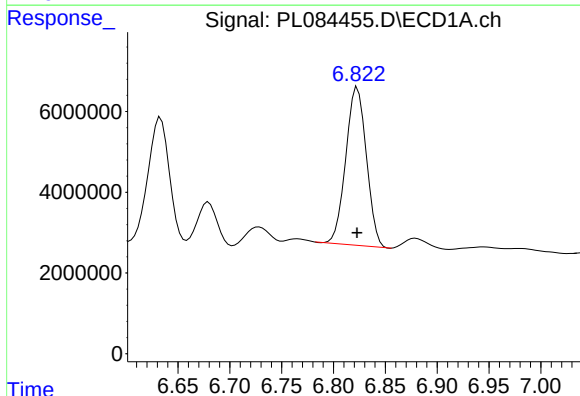


#27 Chlordane-5

R.T.: 6.823 min
Delta R.T.: 0.000 min
Response: 54267216
Conc: 735.33 ng/ml

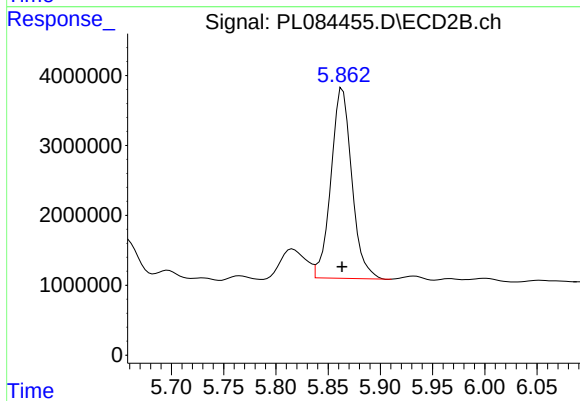

#27 Chlordane-5


R.T.: 5.864 min
Delta R.T.: 0.000 min
Response: 37796403
Conc: 755.44 ng/ml

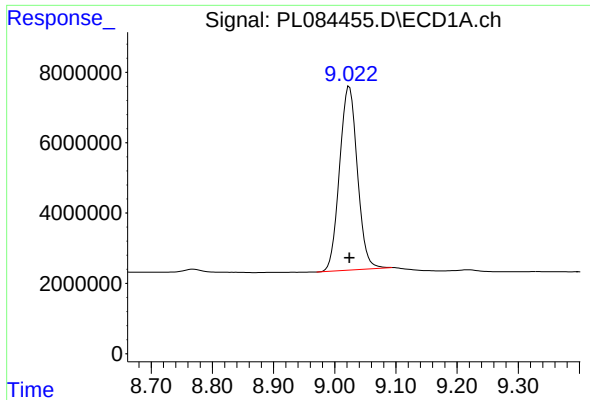

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 105882077
Conc: 71.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

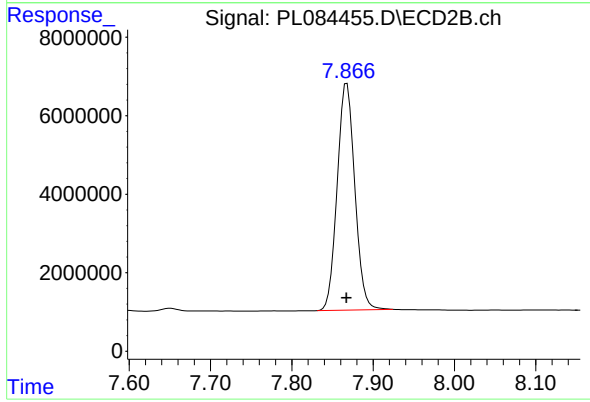

#28 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: 0.000 min
Response: 86985305
Conc: 72.85 ng/ml