

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080323\
 Data File : PL084456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 10:13
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 11:16:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 11:15:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.685	108.3E6	65471417	50.000	50.000
28)	SA Decachlor...	9.024	7.867	73921547	59705337	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.643	3.688	47937689	18861930	500.000	500.000
24)	Chlordane-2	5.176	4.269	55889351	24253147	500.000	500.000
25)	Chlordane-3	5.890	4.902	196.7E6	69390169	500.000	500.000
26)	Chlordane-4	5.973	4.965	235.2E6	71261471	500.000	500.000
27)	Chlordane-5	6.823	5.863	36899851	25016289	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080323\
Data File : PL084456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 10:13
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 11:16:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 11:15:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

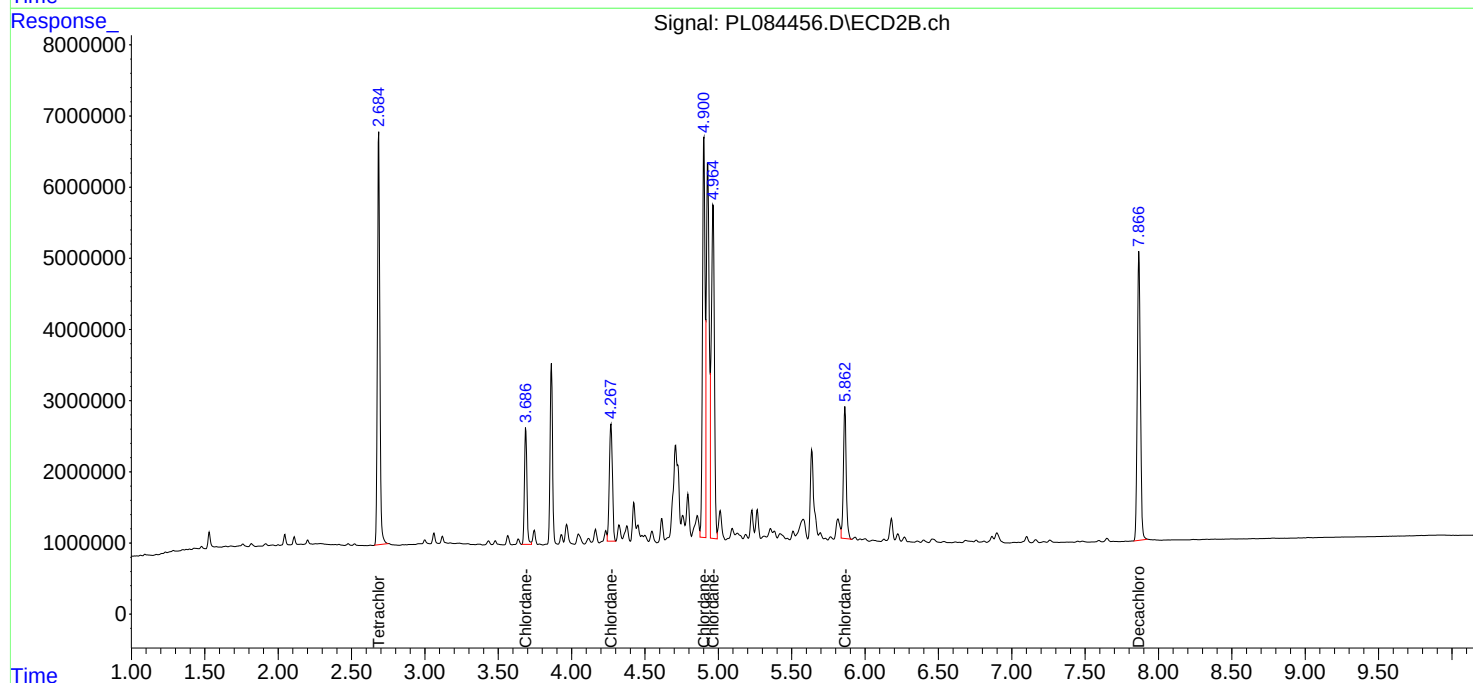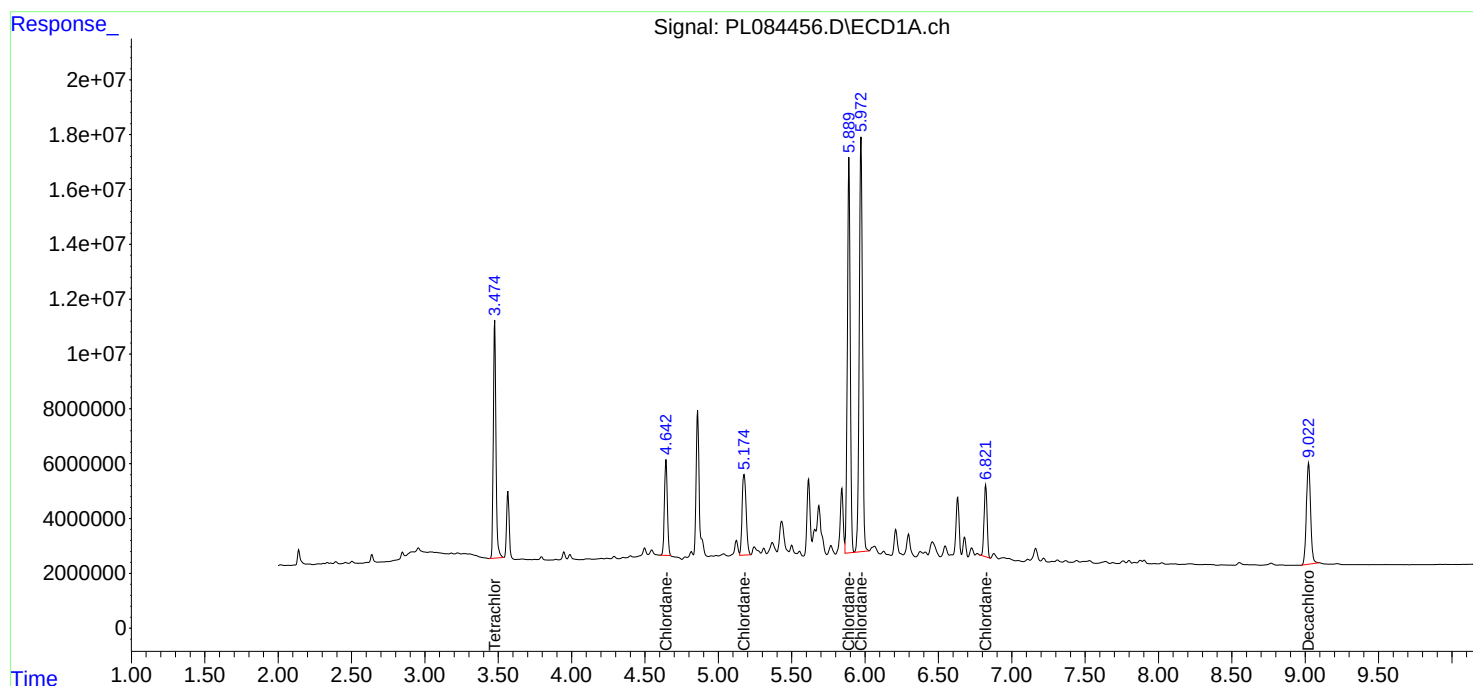


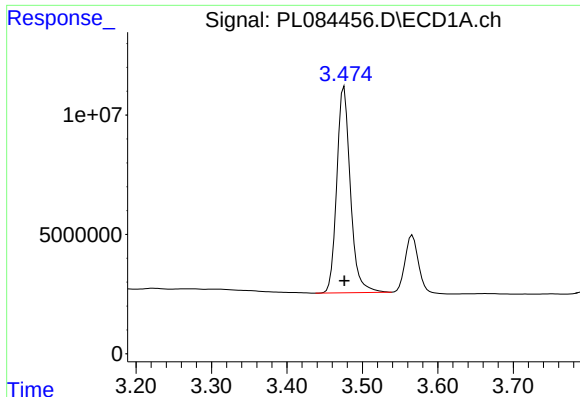

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 108275799
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

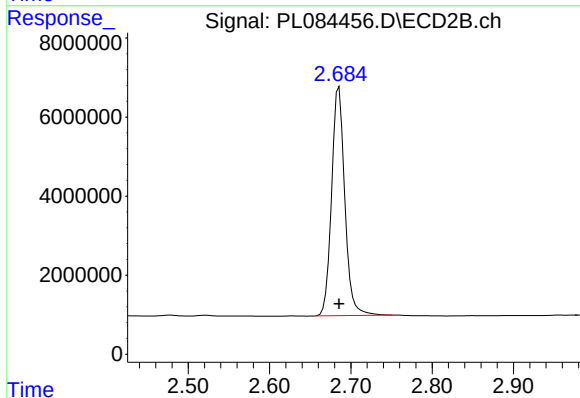


#1 Tetrachloro-m-xylene

R.T.: 2.685 min
Delta R.T.: 0.000 min
Response: 65471417
Conc: 50.00 ng/ml

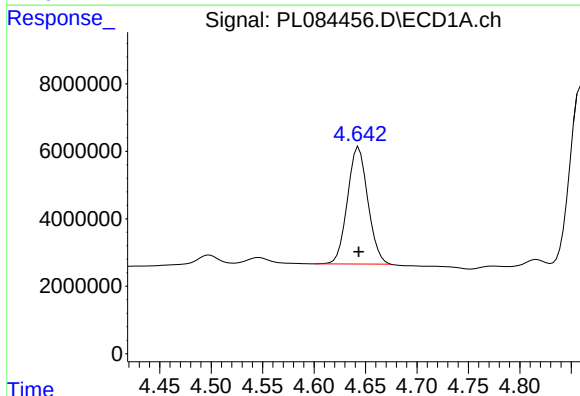


#23 Chlordane-1

R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 47937689
Conc: 500.00 ng/ml

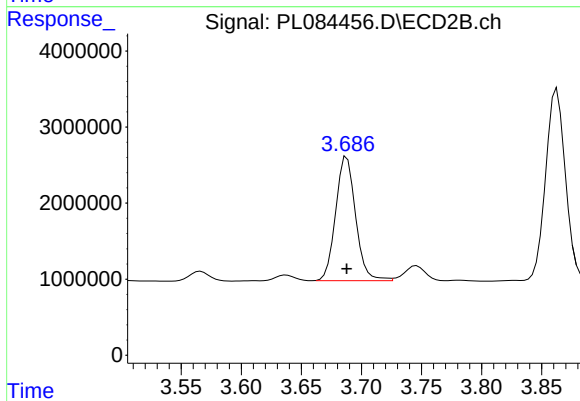

#23 Chlordane-1


R.T.: 3.688 min
Delta R.T.: 0.000 min
Response: 18861930
Conc: 500.00 ng/ml

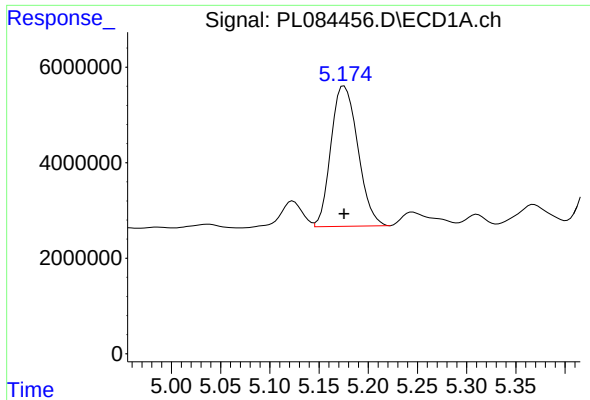

#24 Chlordane-2


R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 55889351
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

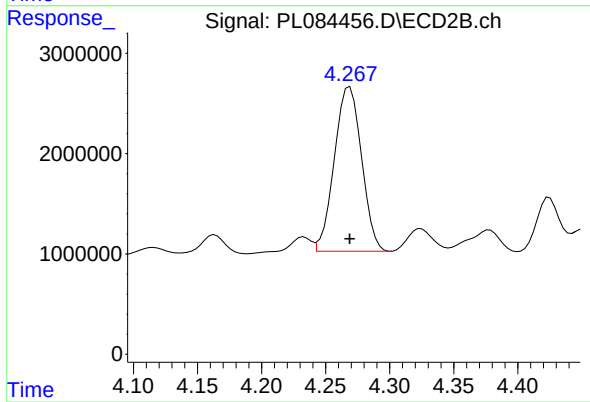


#24 Chlordane-2

R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 24253147
Conc: 500.00 ng/ml

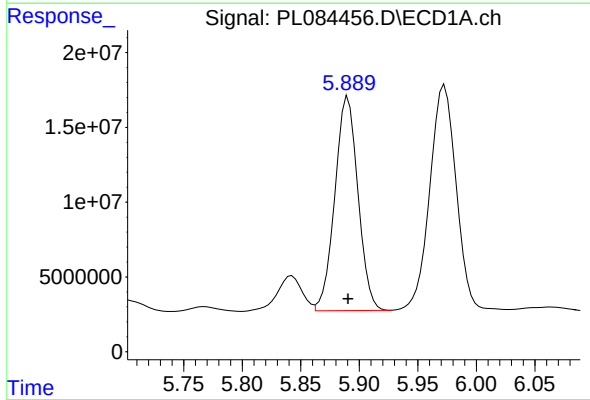


#25 Chlordane-3

R.T.: 5.890 min
Delta R.T.: 0.000 min
Response: 196743550
Conc: 500.00 ng/ml

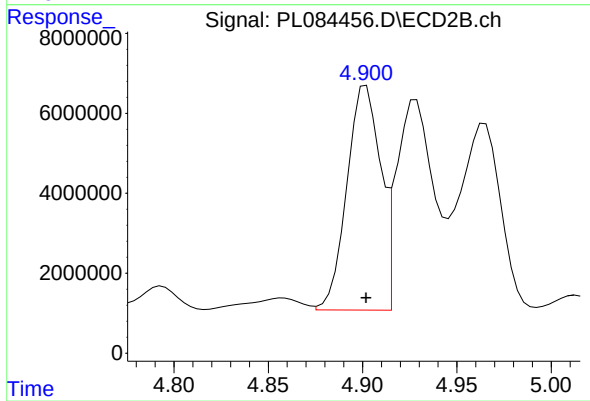

#25 Chlordane-3


R.T.: 4.902 min
Delta R.T.: 0.000 min
Response: 69390169
Conc: 500.00 ng/ml

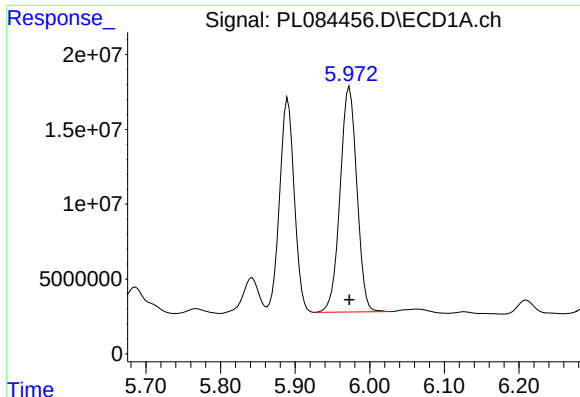

#26 Chlordane-4


R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 235169205
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

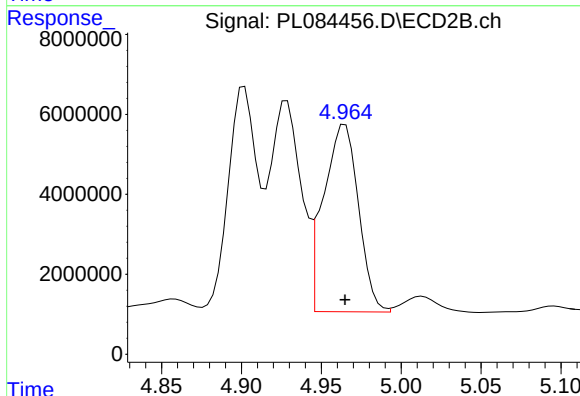


#26 Chlordane-4

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 71261471
Conc: 500.00 ng/ml

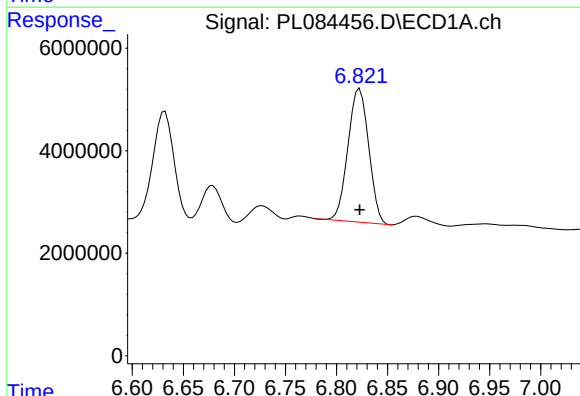


#27 Chlordane-5

R.T.: 6.823 min
Delta R.T.: 0.000 min
Response: 36899851
Conc: 500.00 ng/ml

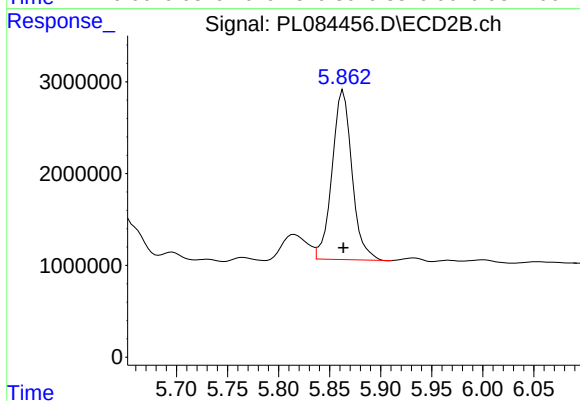

#27 Chlordane-5


R.T.: 5.863 min
Delta R.T.: 0.000 min
Response: 25016289
Conc: 500.00 ng/ml

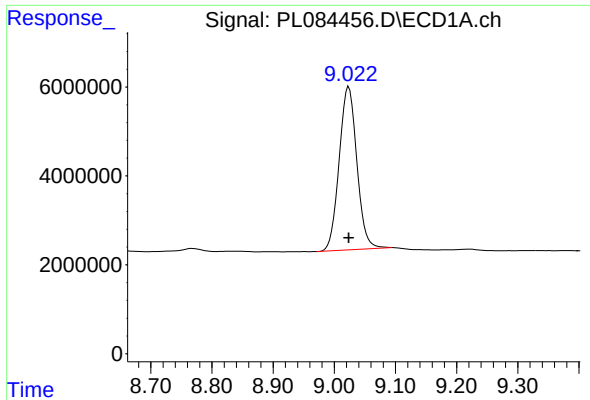

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 73921547
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

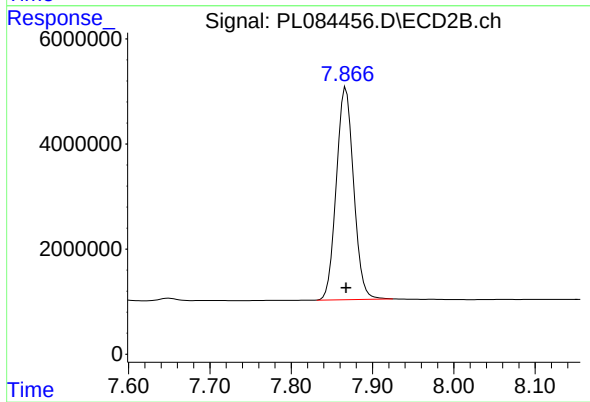

#28 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 59705337
Conc: 50.00 ng/ml