

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080323\
 Data File : PL084457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 10:27
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 11:16:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 11:15:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.686	55983474	33428495	25.852	25.529
28)	SA Decachlor...	9.024	7.867	40960655	32073879	27.705	26.860
Target Compounds							
23)	Chlordane-1	4.642	3.688	25051633	9636274	261.294	255.442
24)	Chlordane-2	5.176	4.269	30026823	12889258	268.627	265.723
25)	Chlordane-3	5.889	4.902	100.5E6	34572133	255.317	249.114
26)	Chlordane-4	5.972	4.965	121.6E6	35848593	258.601	251.529
27)	Chlordane-5	6.822	5.863	19494263	12877267	264.151	257.378



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080323\
Data File : PL084457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 10:27
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 11:16:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 11:15:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

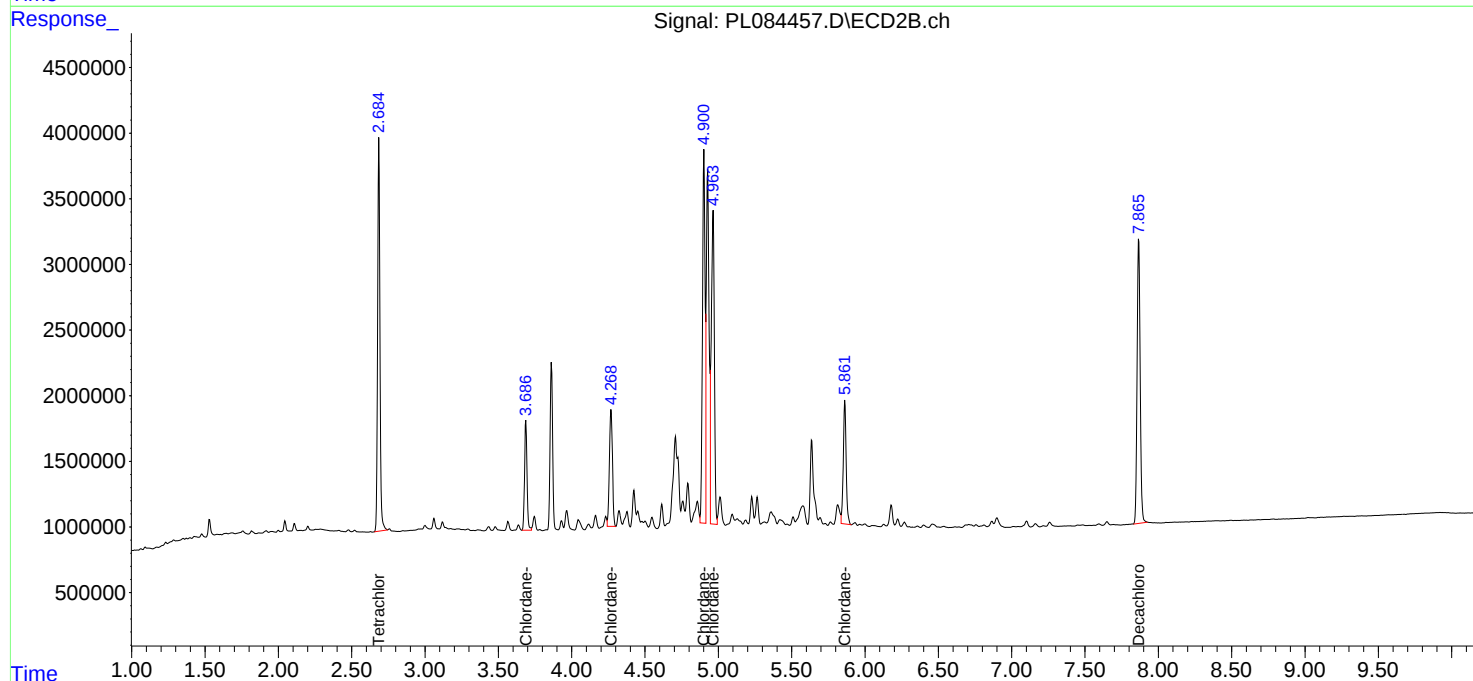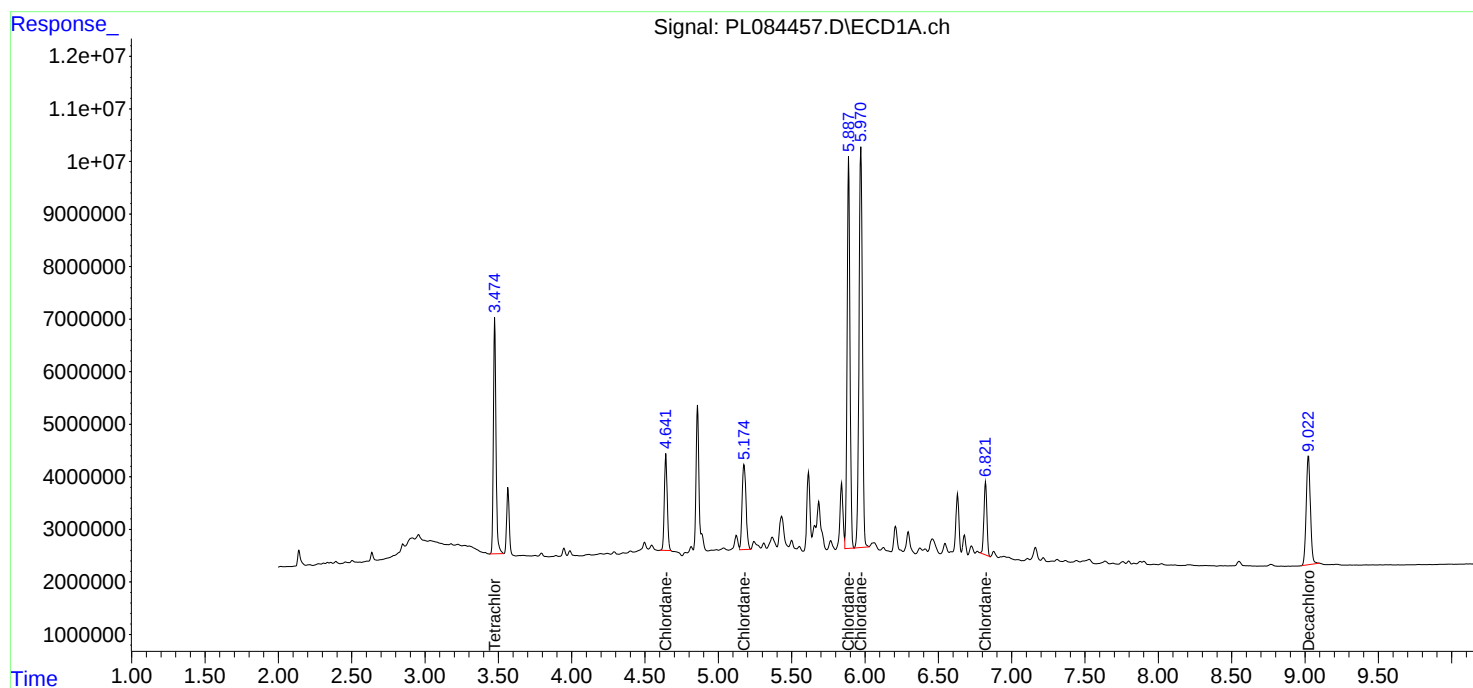


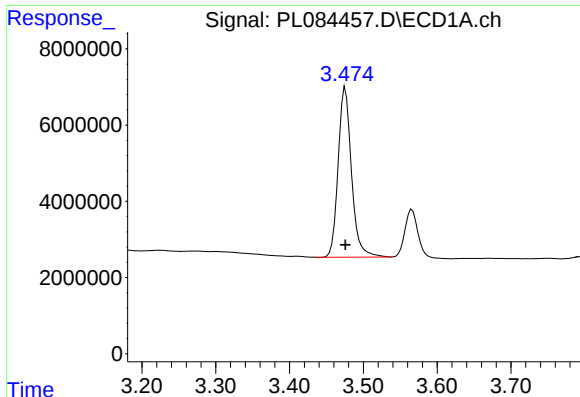

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 55983474
Conc: 25.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

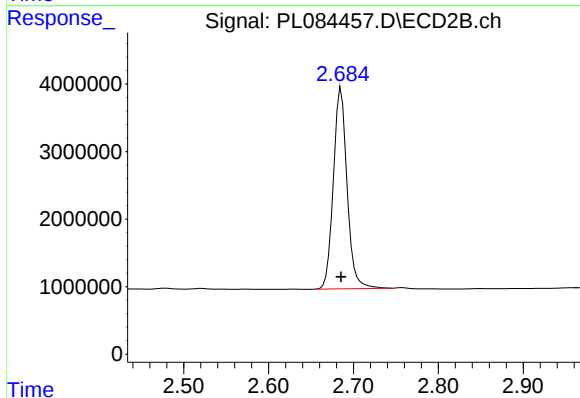


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.000 min
Response: 33428495
Conc: 25.53 ng/ml

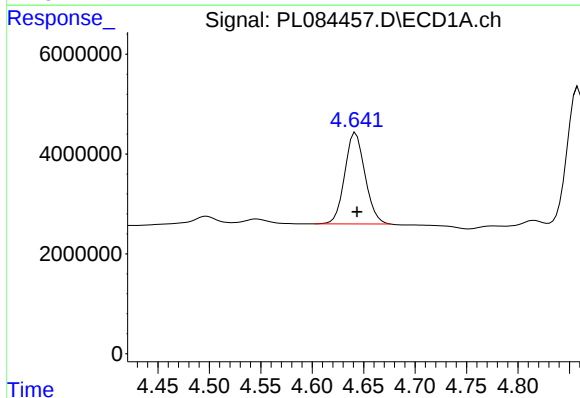


#23 Chlordane-1

R.T.: 4.642 min
Delta R.T.: -0.001 min
Response: 25051633
Conc: 261.29 ng/ml

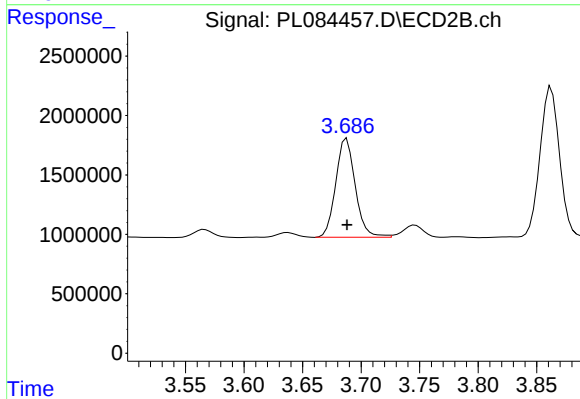

#23 Chlordane-1


R.T.: 3.688 min
Delta R.T.: 0.000 min
Response: 9636274
Conc: 255.44 ng/ml

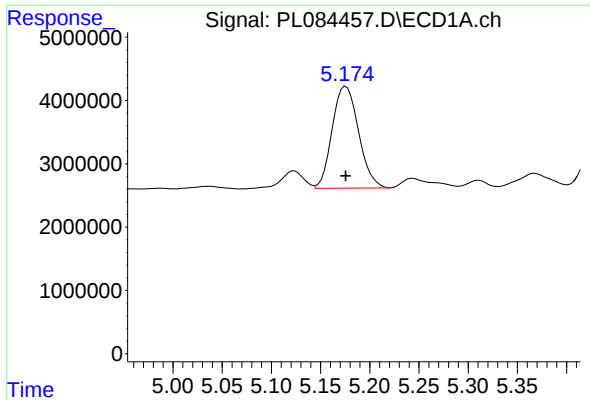

#24 Chlordane-2


R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 30026823
Conc: 268.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

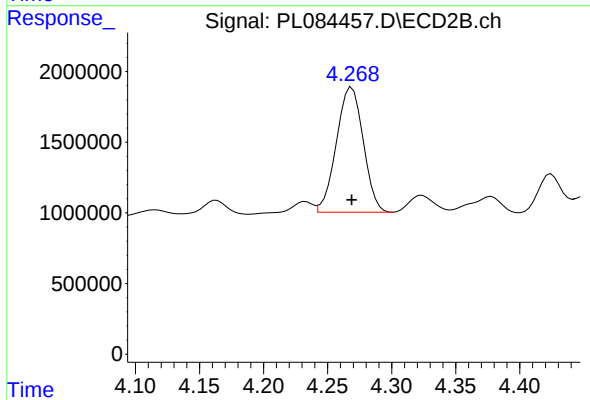


#24 Chlordane-2

R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 12889258
Conc: 265.72 ng/ml

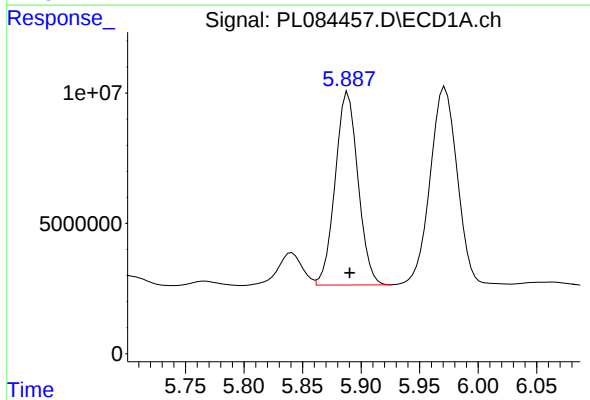


#25 Chlordane-3

R.T.: 5.889 min
Delta R.T.: -0.002 min
Response: 100463936
Conc: 255.32 ng/ml

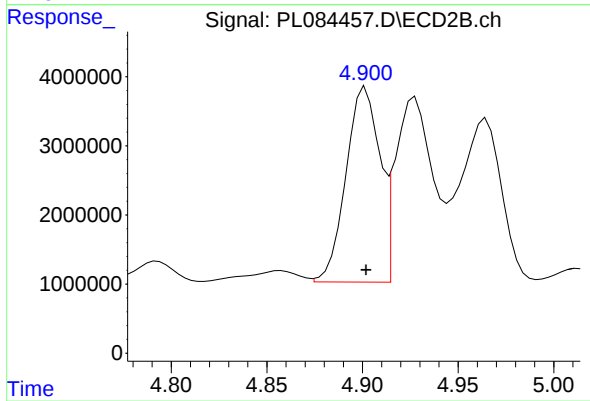

#25 Chlordane-3


R.T.: 4.902 min
Delta R.T.: 0.000 min
Response: 34572133
Conc: 249.11 ng/ml

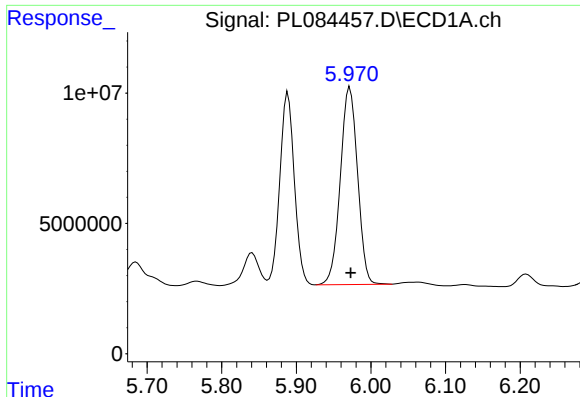

#26 Chlordane-4


R.T.: 5.972 min
Delta R.T.: -0.001 min
Response: 121629951
Conc: 258.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

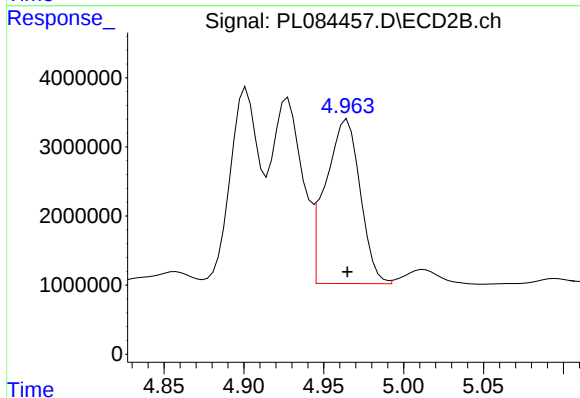


#26 Chlordane-4

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 35848593
Conc: 251.53 ng/ml

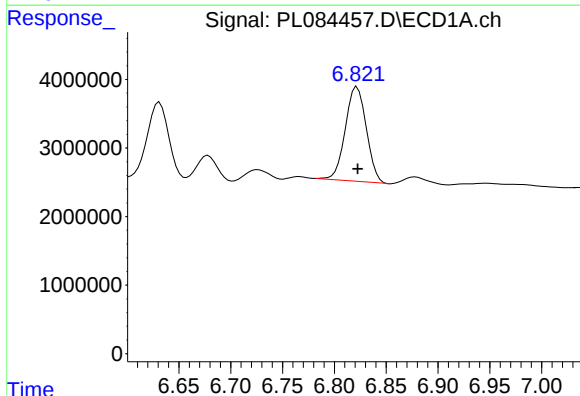


#27 Chlordane-5

R.T.: 6.822 min
Delta R.T.: 0.000 min
Response: 19494263
Conc: 264.15 ng/ml

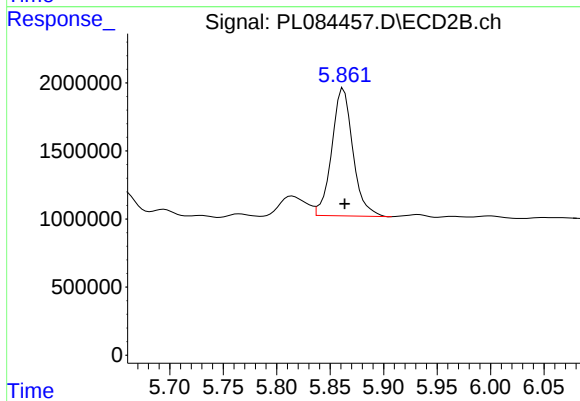

#27 Chlordane-5


R.T.: 5.863 min
Delta R.T.: 0.000 min
Response: 12877267
Conc: 257.38 ng/ml

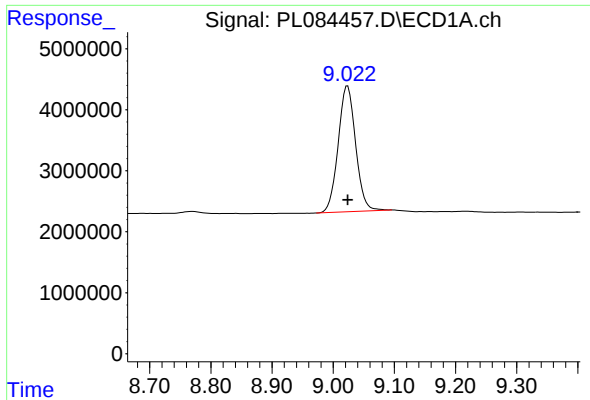

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 40960655
Conc: 27.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

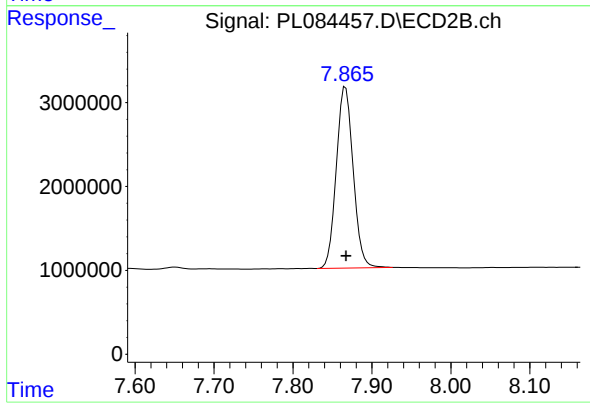

#28 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 32073879
Conc: 26.86 ng/ml