

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080323\
 Data File : PS023925.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 18:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 20:25:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
 Quant Title : 8080.M
 QLast Update : Thu Jul 20 19:21:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.370	6.805	988.8E6	331.5E6	498.728	487.482
Target Compounds							
2) T	3,5-DICHL...	5.711	0.000	2624301	0	<MDL	N.D. #
3) T	4-Nitroph...	6.213	0.000	4541647	0	3.653	N.D. #
5) T	DICAMBA	0.000	6.956	0	478293	N.D.	<MDL
8) T	DICHLORPROP	7.150f	7.601	7332	978667	<MDL	1.295 #
11) T	2,4,5-TP ...	8.050	0.000	1883159	0	<MDL	N.D. #
12) T	2,4,5-T	8.311	9.070	913953	685450	<MDL	<MDL #
13) T	2,4-DB	8.758f	0.000	1369682	0	<MDL	N.D. #
14) T	DINOSEB	9.867	0.000	667582	0	<MDL	N.D. #
15) T	Picloram	9.698	10.819	9375216	4901538	<MDL	<MDL #
16) T	DCPA	10.132	10.819	935541	4901538	<MDL	1.031 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080323\
Data File : PS023925.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 18:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 20:25:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
Quant Title : 8080.M
QLast Update : Thu Jul 20 19:21:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

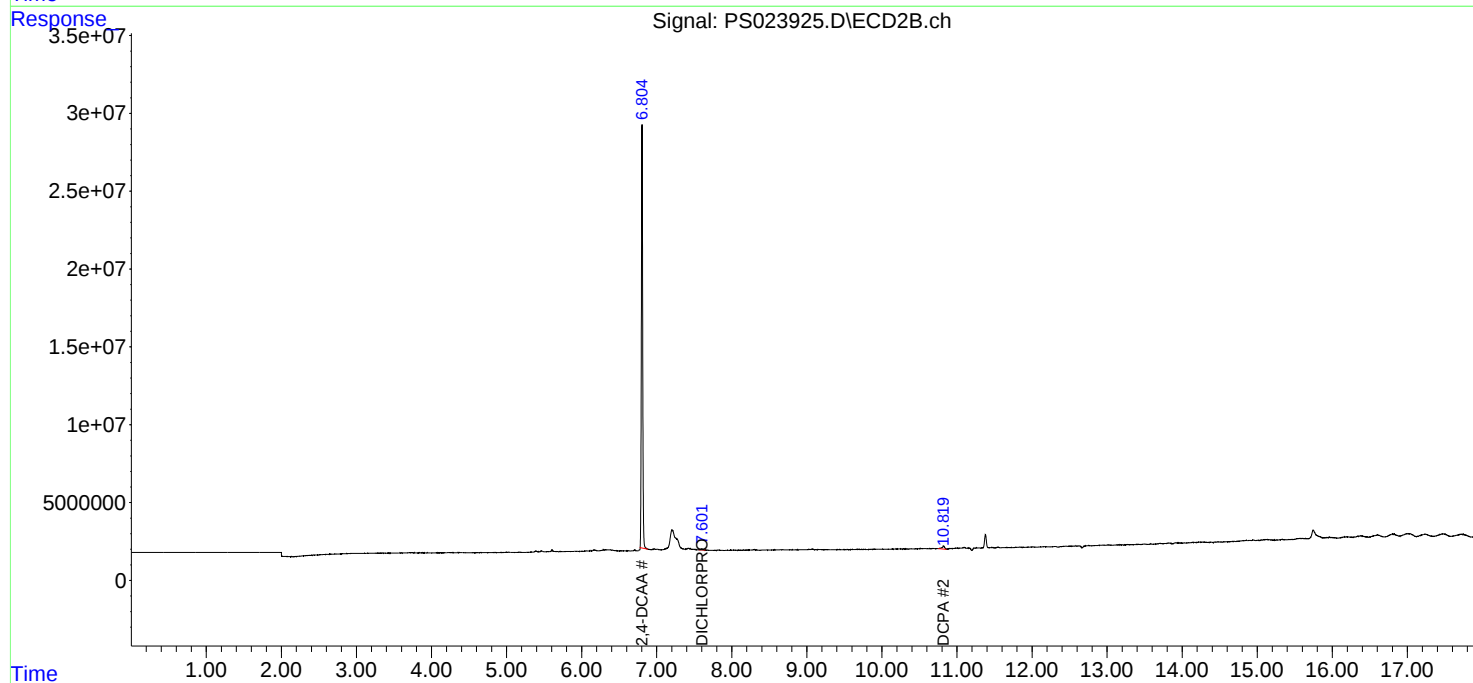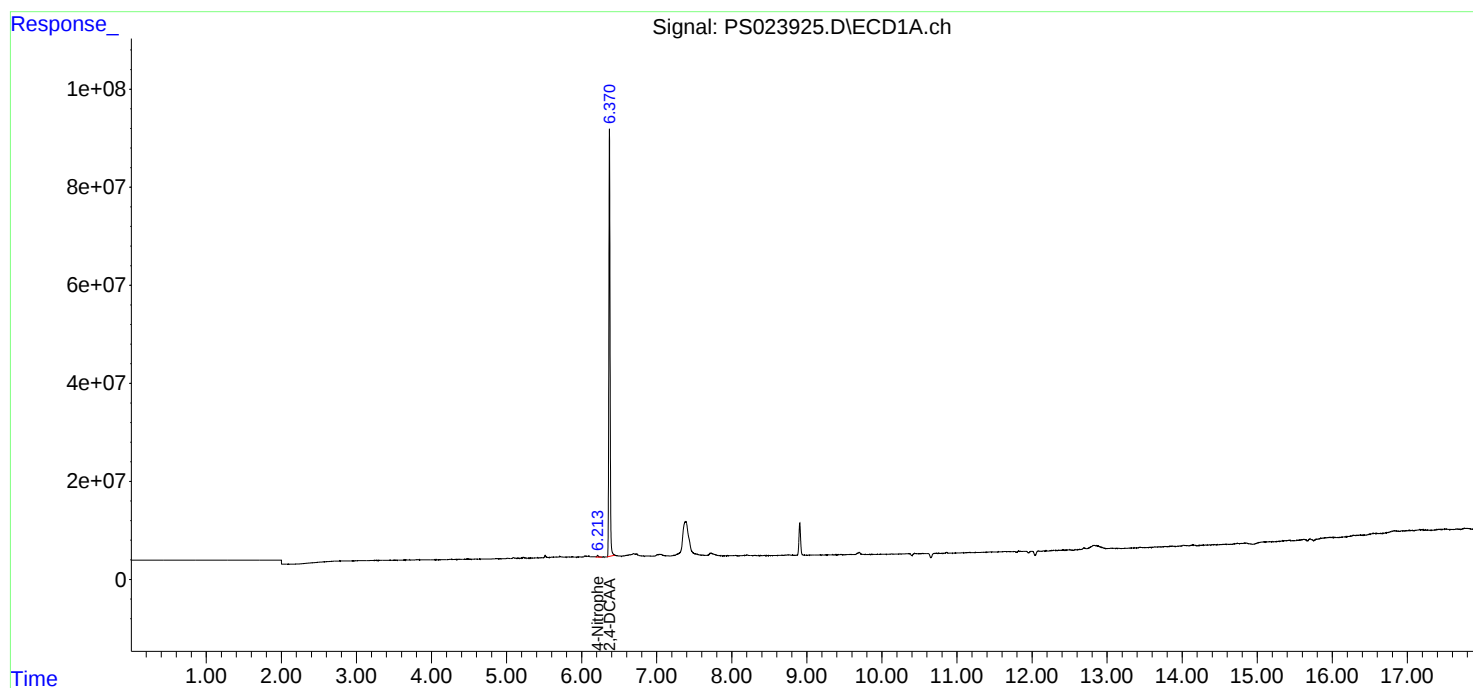


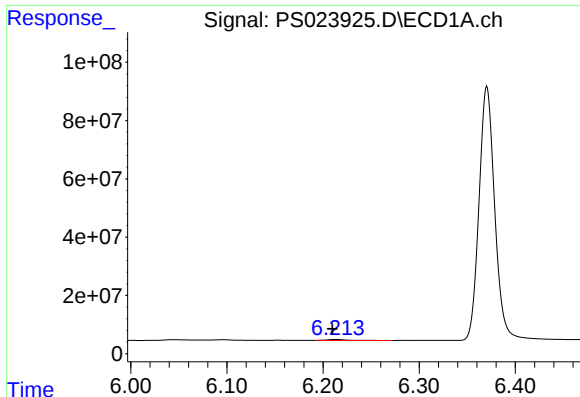

#3 4-Nitrophenol


R.T.: 6.213 min
Delta R.T.: 0.004 min
Response: 4541647
Conc: 3.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

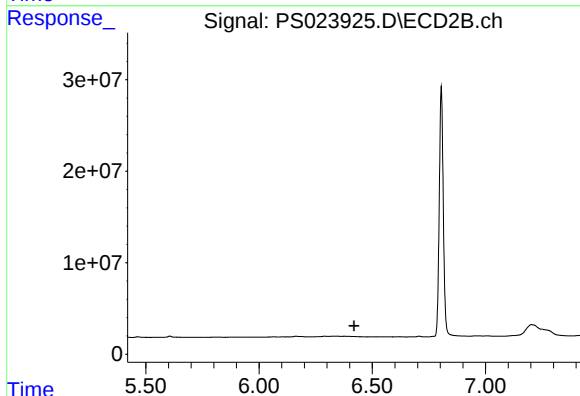


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.419 min
Response: 0
Conc: N.D.

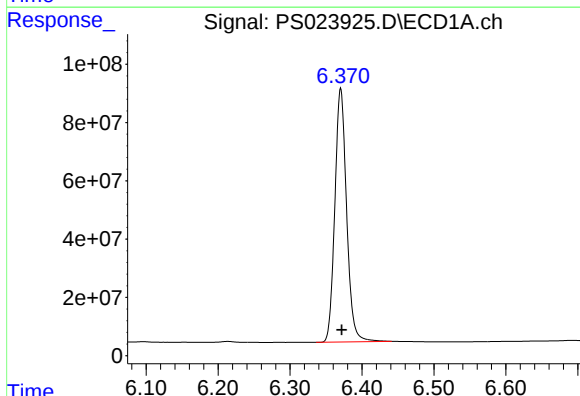


#4 2,4-DCAA

R.T.: 6.370 min
Delta R.T.: -0.002 min
Response: 988795459
Conc: 498.73 ng/ml

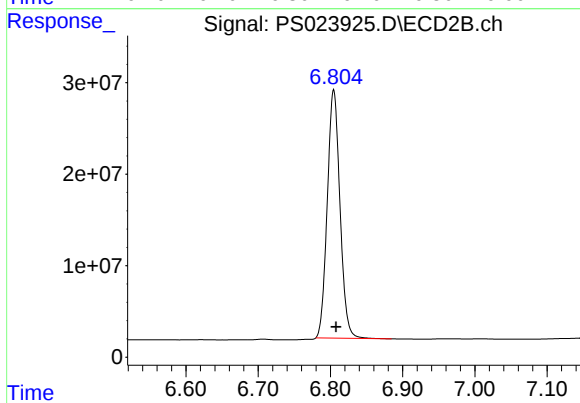

#4 2,4-DCAA


R.T.: 6.805 min
Delta R.T.: -0.003 min
Response: 331535913
Conc: 487.48 ng/ml

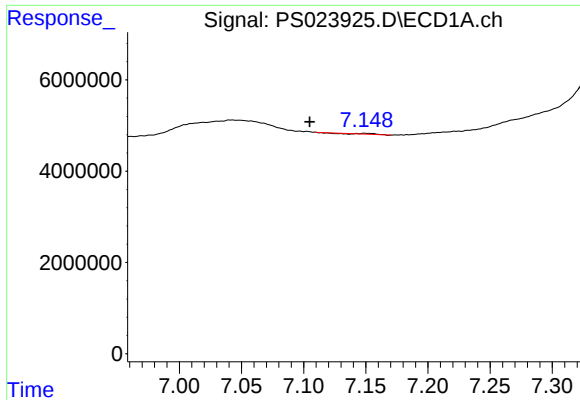

#8 DICHLORPROP


R.T.: 7.150 min
Delta R.T.: 0.045 min
Response: 7332
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

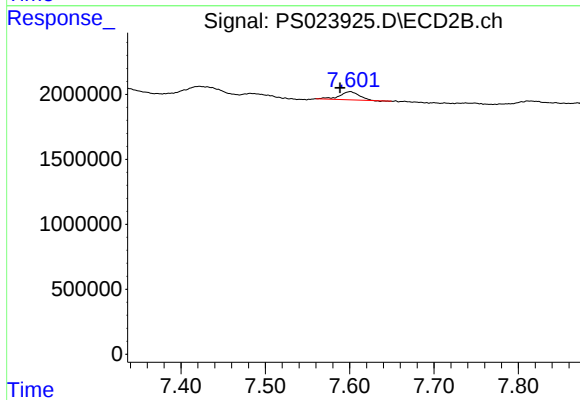


#8 DICHLORPROP

R.T.: 7.601 min
Delta R.T.: 0.012 min
Response: 978667
Conc: 1.30 ng/ml

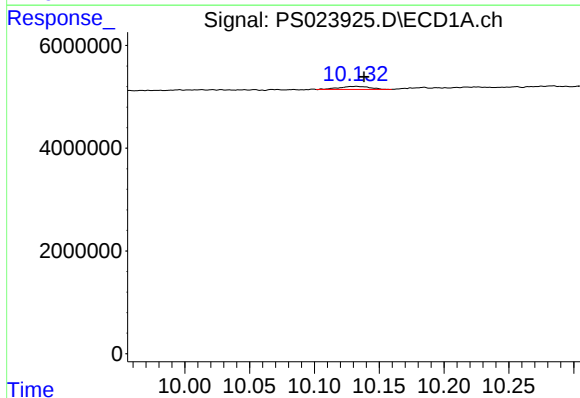

#16 DCPA

R.T.: 10.132 min
Delta R.T.: -0.006 min
Response: 935541
Conc: N.D.

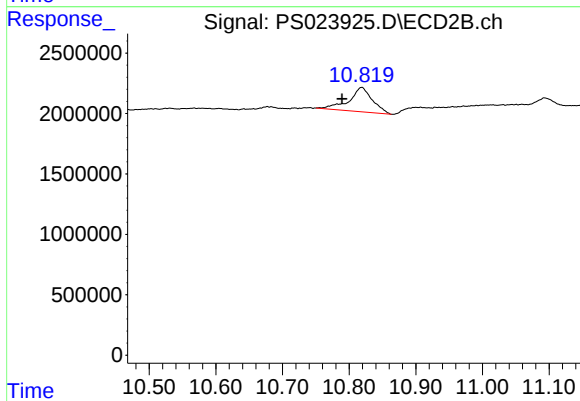

#16 DCPA

R.T.: 10.819 min
Delta R.T.: 0.029 min
Response: 4901538
Conc: 1.03 ng/ml