

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080323\
 Data File : PL084454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 09:45
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 11:15:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 11:15:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.686	218.8E6	133.7E6	101.055	102.118
28)	SA Decachlor...	9.024	7.867	140.1E6	116.0E6	94.779	97.122
Target Compounds							
23)	Chlordane-1	4.644	3.689	95918612	38648440	1000.451	1024.509
24)	Chlordane-2	5.177	4.269	107.0E6	47118885	957.638	971.397
25)	Chlordane-3	5.890	4.902	405.6E6	144.0E6	1030.869	1037.666
26)	Chlordane-4	5.973	4.965	477.9E6	148.4E6	1015.999	1041.156
27)	Chlordane-5	6.824	5.864	73444148	51190266	995.182	1023.139



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080323\
Data File : PL084454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 09:45
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 11:15:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 11:15:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

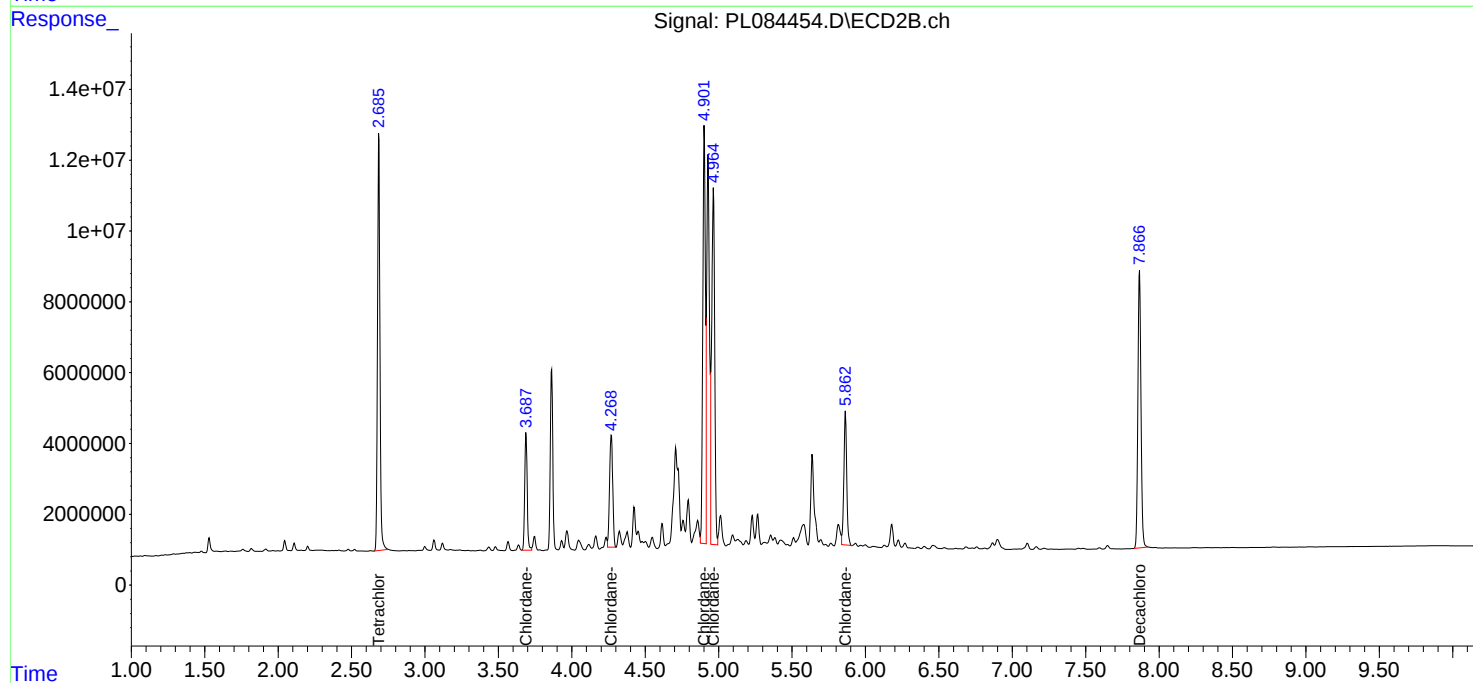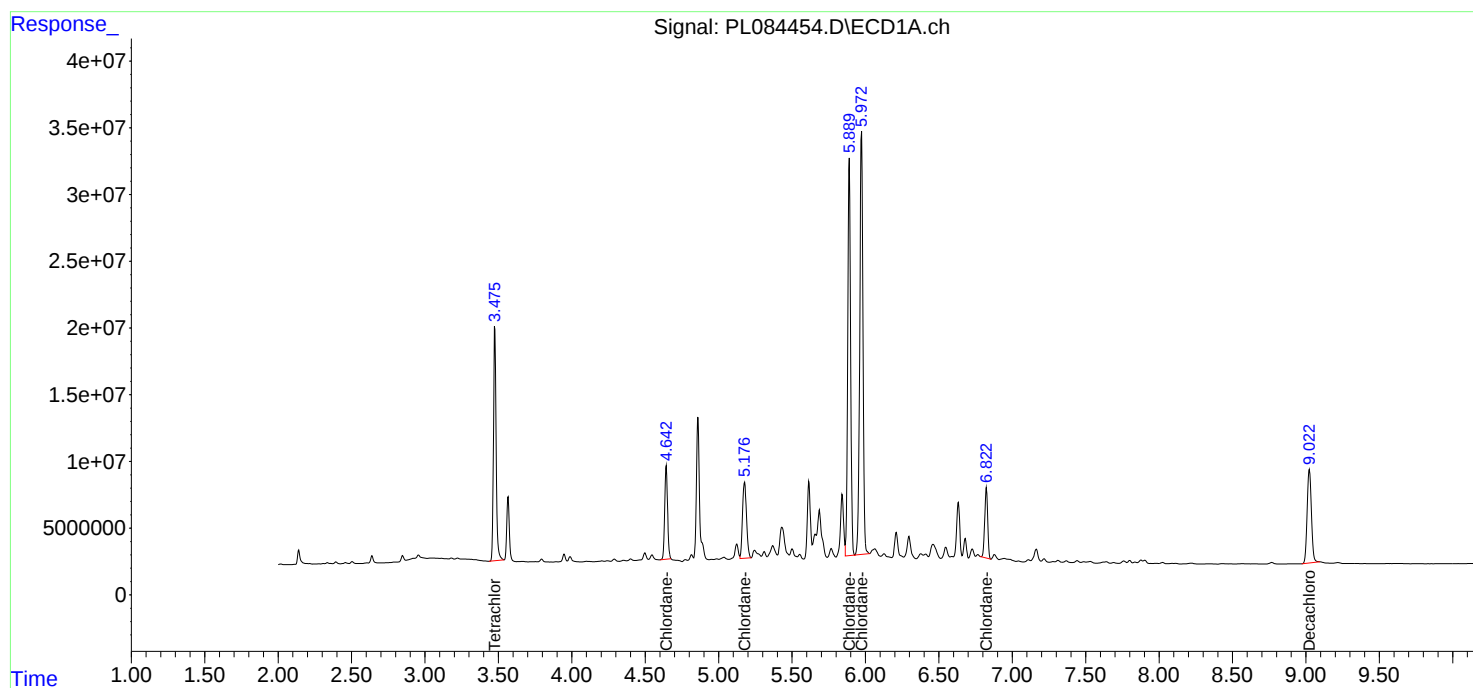


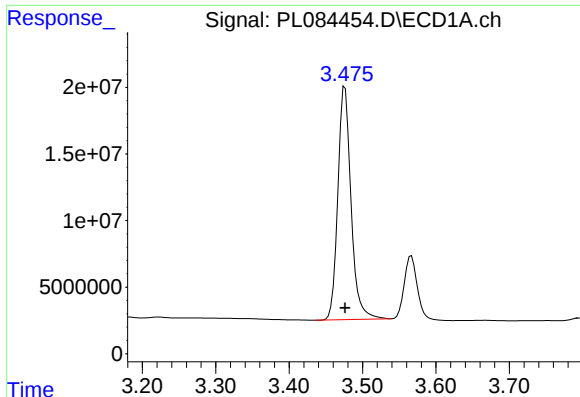

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 218837173
Conc: 101.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

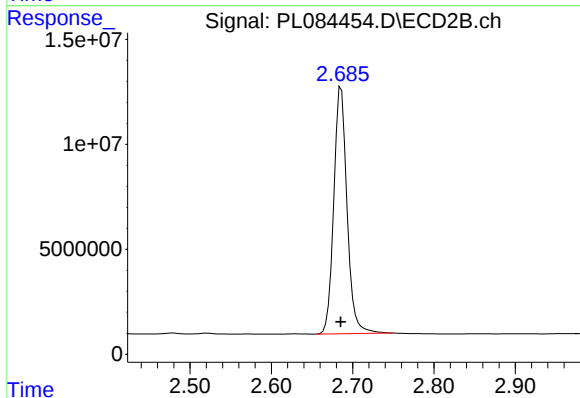


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.000 min
Response: 133715628
Conc: 102.12 ng/ml

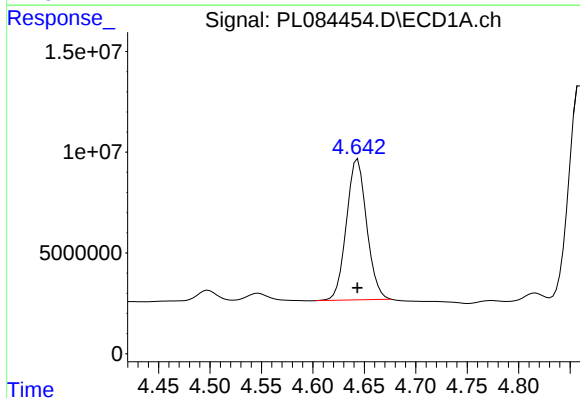


#23 Chlordane-1

R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 95918612
Conc: 1000.45 ng/ml

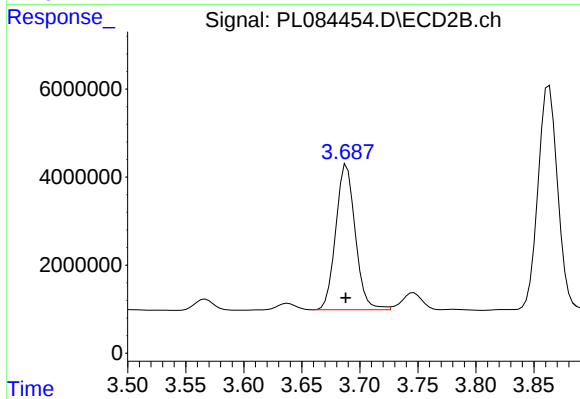

#23 Chlordane-1


R.T.: 3.689 min
Delta R.T.: 0.000 min
Response: 38648440
Conc: 1024.51 ng/ml

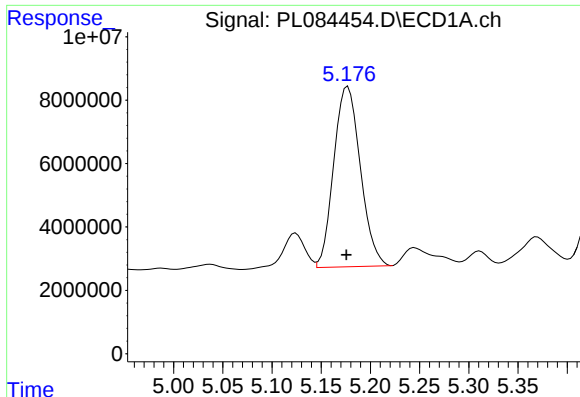

#24 Chlordane-2


R.T.: 5.177 min
Delta R.T.: 0.002 min
Response: 107043479
Conc: 957.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

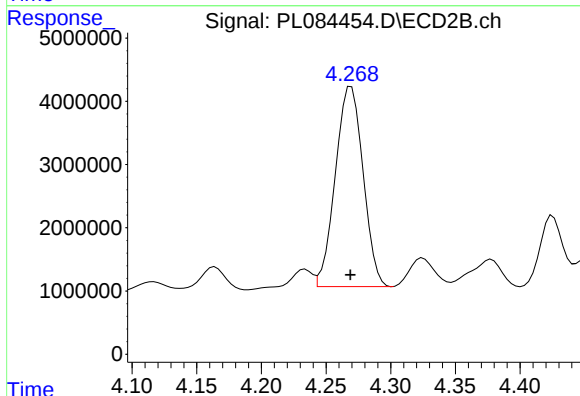


#24 Chlordane-2

R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 47118885
Conc: 971.40 ng/ml

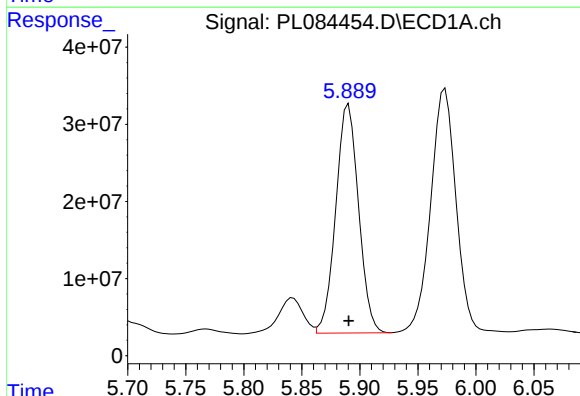


#25 Chlordane-3

R.T.: 5.890 min
Delta R.T.: 0.000 min
Response: 405633719
Conc: 1030.87 ng/ml

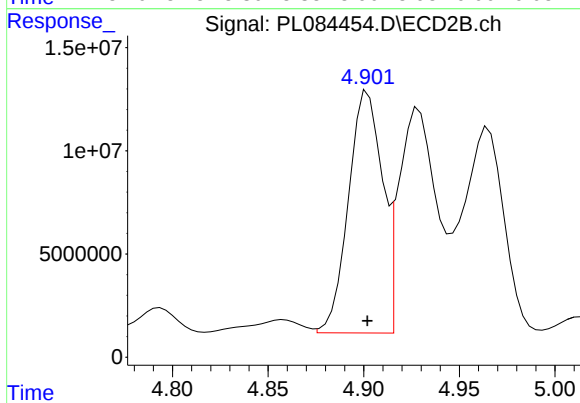

#25 Chlordane-3


R.T.: 4.902 min
Delta R.T.: 0.000 min
Response: 144007707
Conc: 1037.67 ng/ml

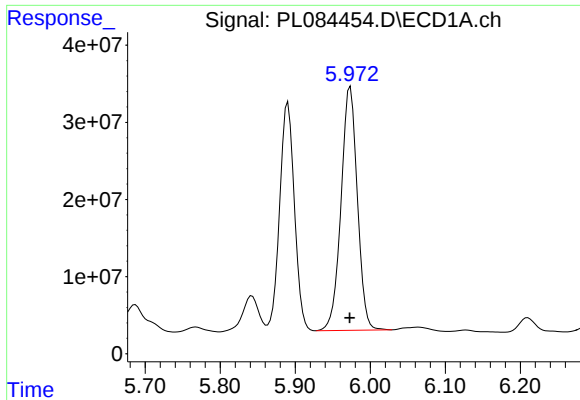

#26 Chlordane-4


R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 477863524
Conc: 1016.00 ng/m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

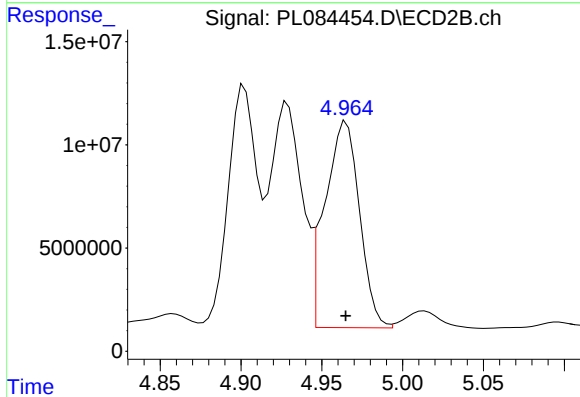


#26 Chlordane-4

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 148388628
Conc: 1041.16 ng/ml

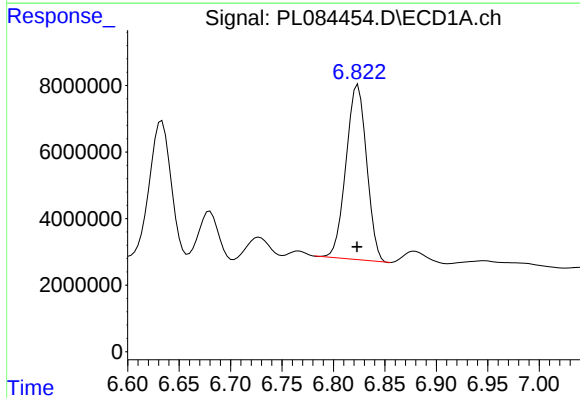


#27 Chlordane-5

R.T.: 6.824 min
Delta R.T.: 0.001 min
Response: 73444148
Conc: 995.18 ng/ml

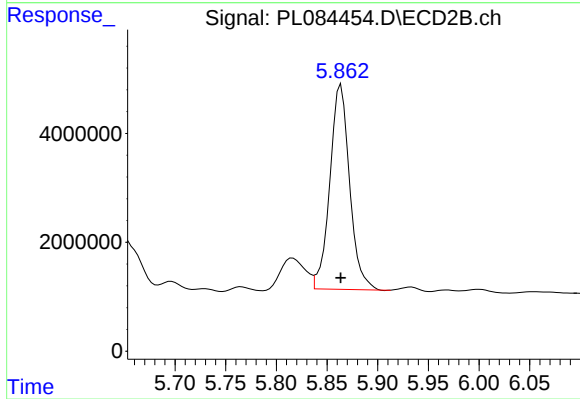

#27 Chlordane-5


R.T.: 5.864 min
Delta R.T.: 0.000 min
Response: 51190266
Conc: 1023.14 ng/ml

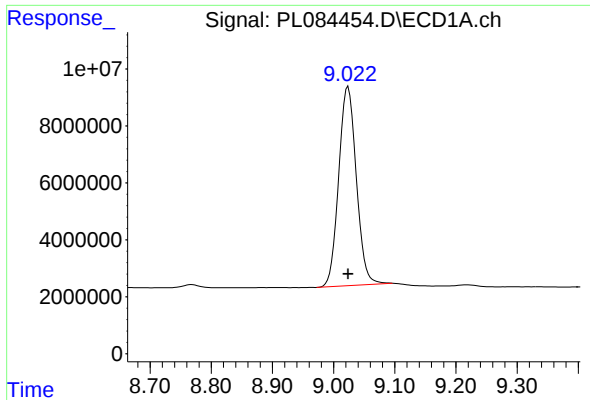

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 140124310
Conc: 94.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

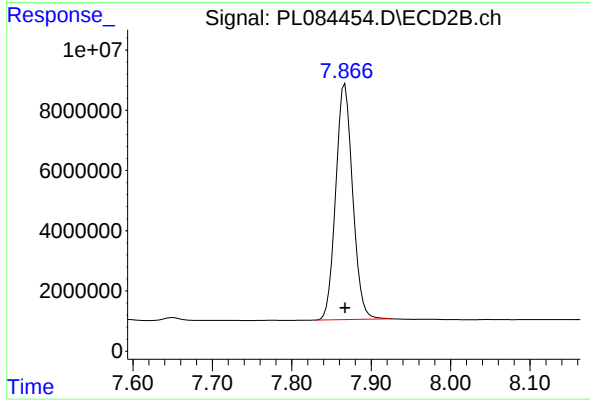

#28 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 115974229
Conc: 97.12 ng/ml