

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080323\
 Data File : PL084478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 16:48
 Operator : AR\AJ
 Sample : 03862-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BUILDING-B-11-(10-15)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 20:24:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 16:21:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.686	46989371	22620868	20.224	20.803
28)	SA Decachlor...	9.024	7.868	32538718	25430871	19.998	20.397

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080323\
Data File : PL084478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 16:48
Operator : AR\AJ
Sample : 03862-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BUILDING-B-11-(10-15)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 20:24:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 16:21:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

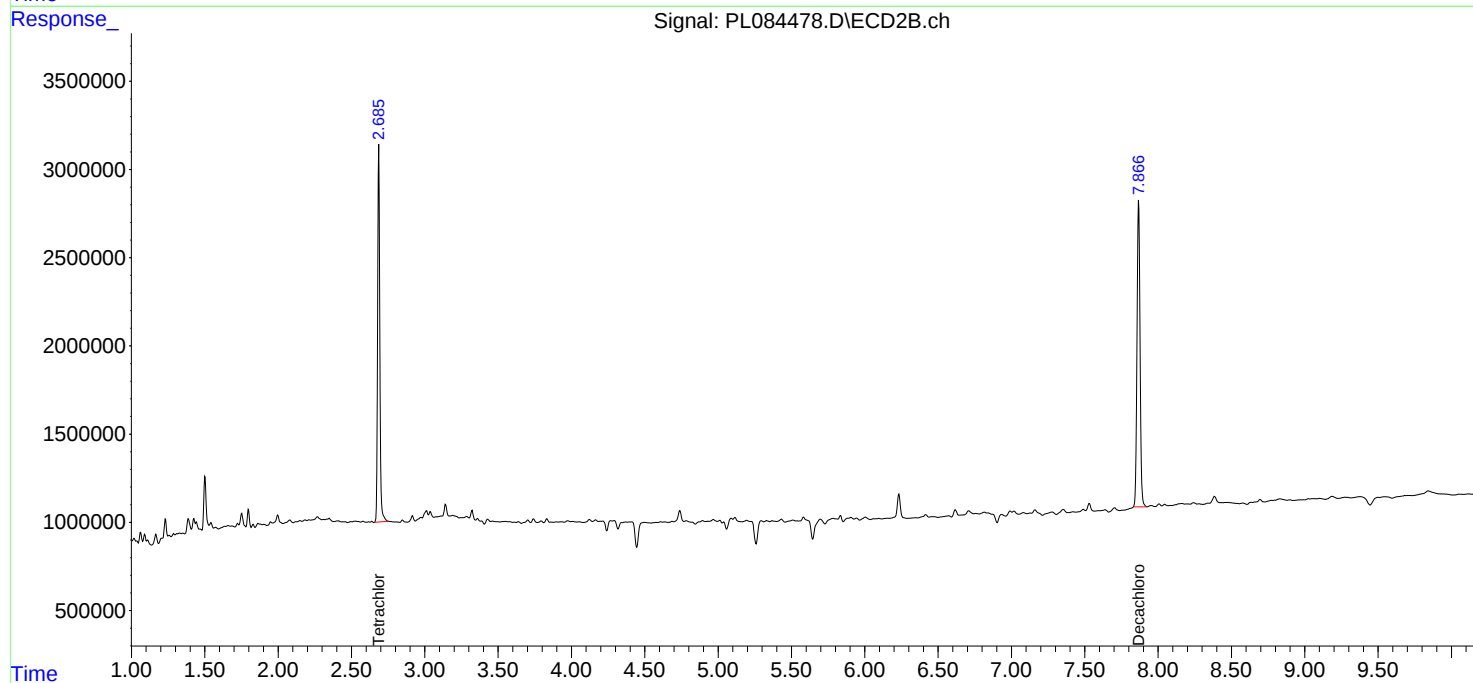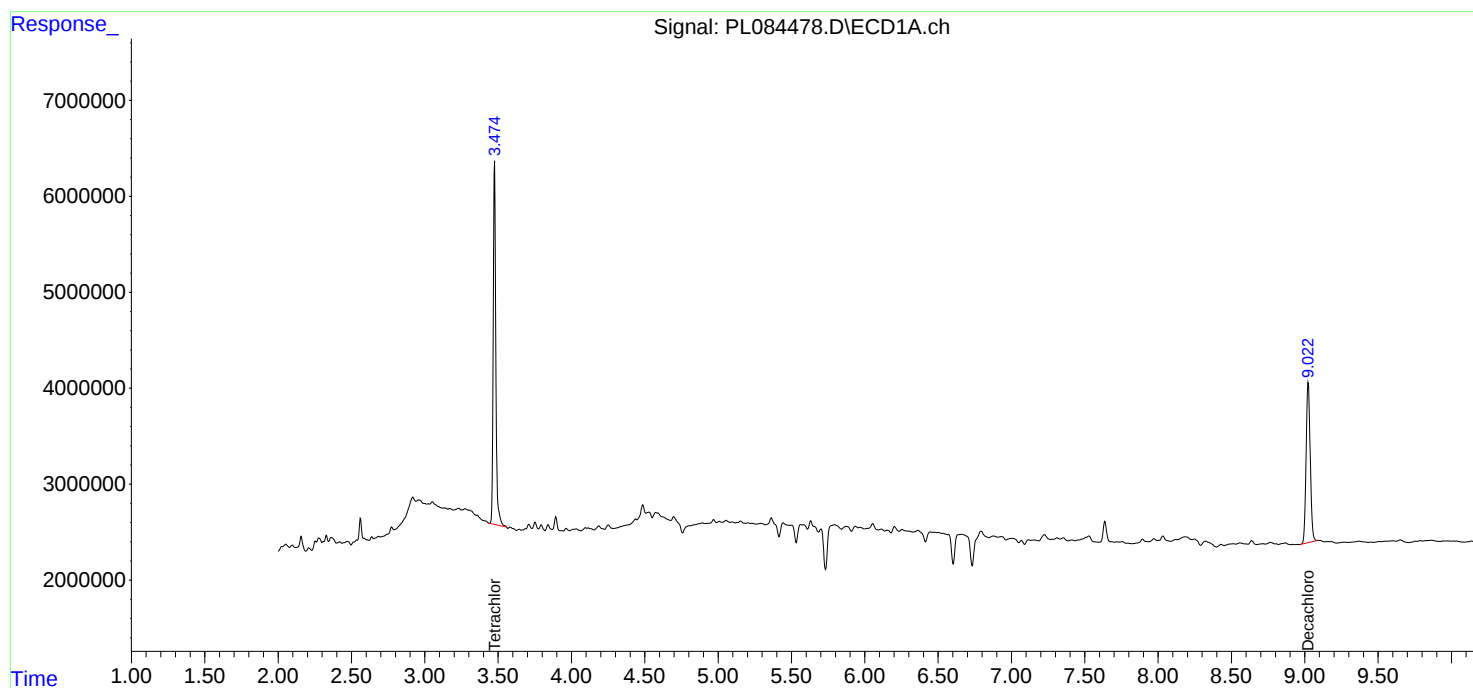


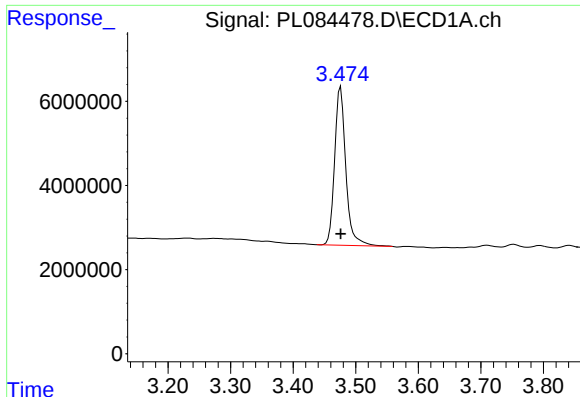

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 46989371
Conc: 20.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUILDING-B-11-(10-15)

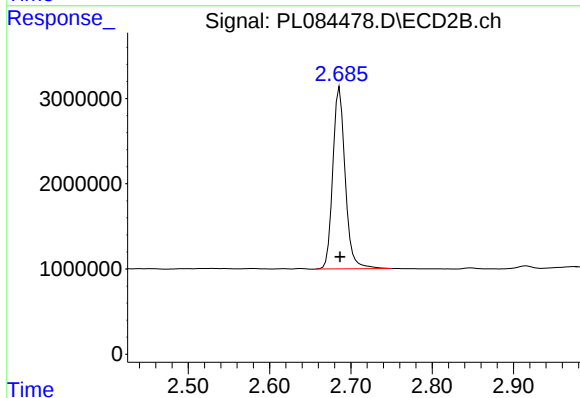


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.000 min
Response: 22620868
Conc: 20.80 ng/ml

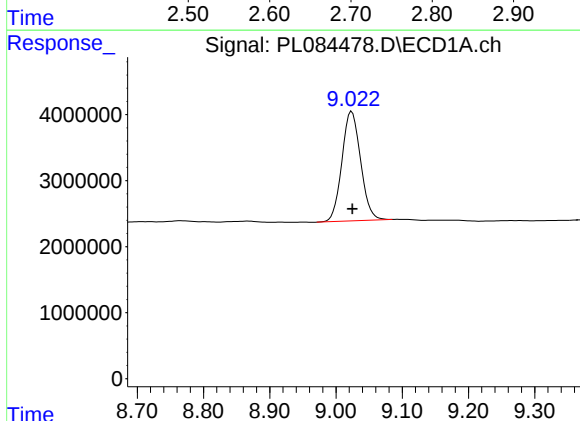

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: -0.001 min
Response: 32538718
Conc: 20.00 ng/ml

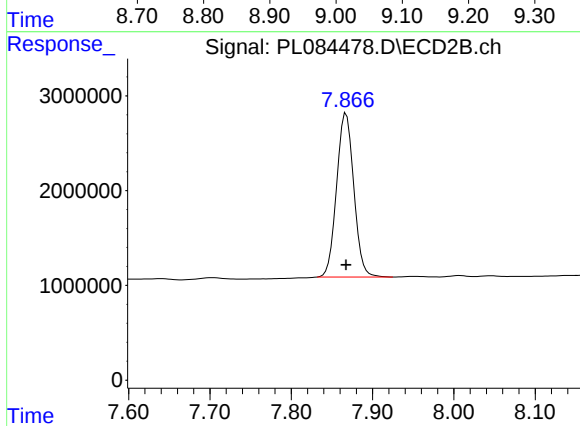

#28 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: 0.000 min
Response: 25430871
Conc: 20.40 ng/ml