

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080323\
 Data File : PL084487.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 18:54
 Operator : AR\AJ
 Sample : 03862-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BUILDING-B-1-(0-5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 20:29:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 16:21:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.476	2.687	24379665	11561436	10.493	10.632
28) SA Decachlor...	9.025	7.867	20150604	15540180	12.384	12.464

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080323\
Data File : PL084487.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 18:54
Operator : AR\AJ
Sample : 03862-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BUILDING-B-1-(0-5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 20:29:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 16:21:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

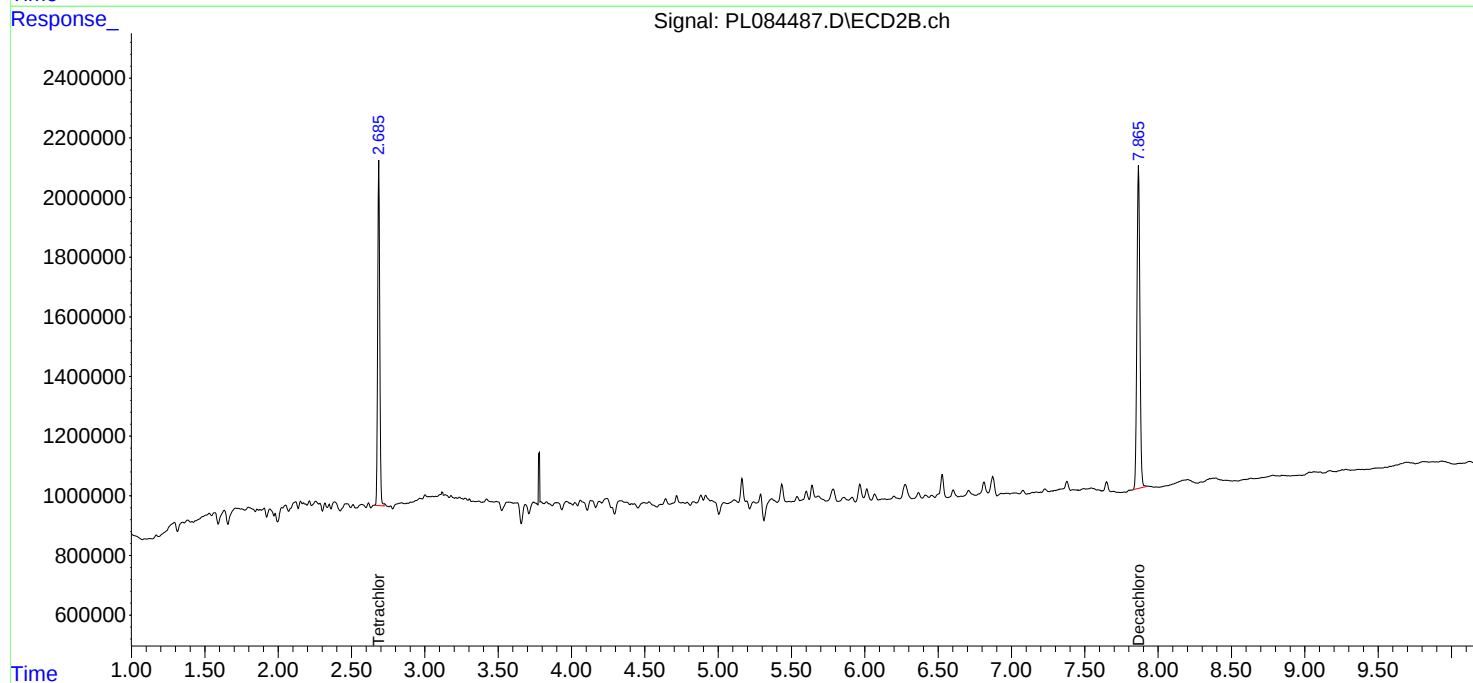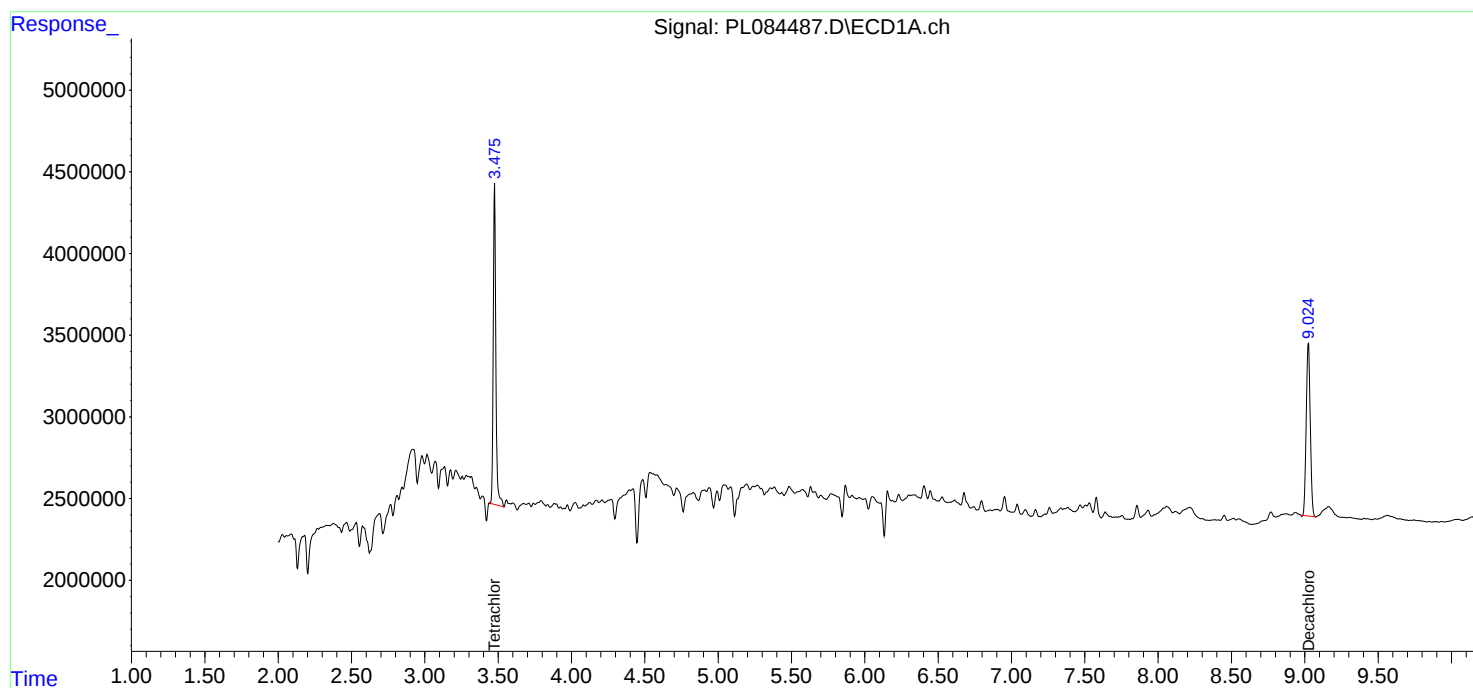


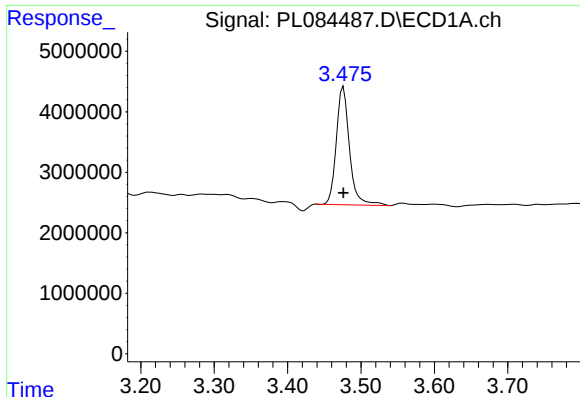

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 24379665
Conc: 10.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUILDING-B-1-(0-5)

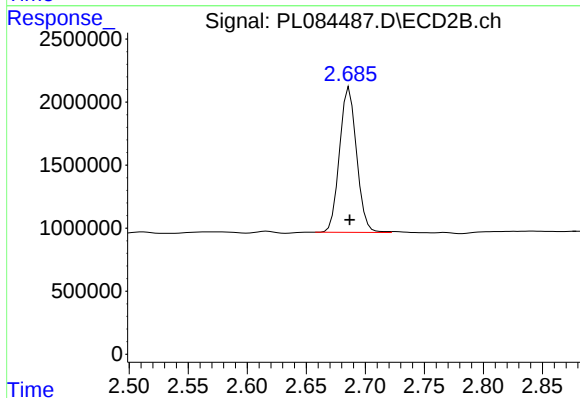


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: 0.000 min
Response: 11561436
Conc: 10.63 ng/ml

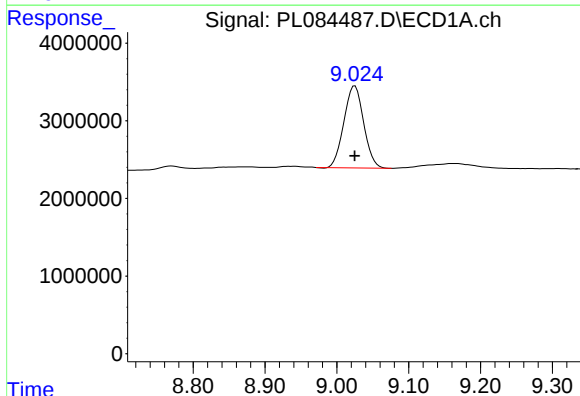

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 20150604
Conc: 12.38 ng/ml

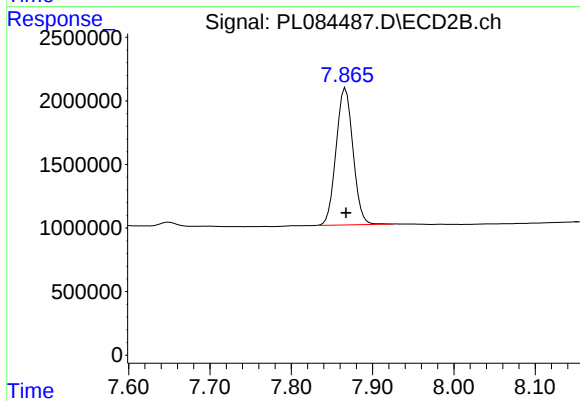

#28 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 15540180
Conc: 12.46 ng/ml