

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080421\
 Data File : PL068664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2021 08:33
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 01:35:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	6.159f	0.000	1390839	0	2.282	N.D.	#
6) B	beta-BHC	6.159	0.000	1390839	0	4.753	N.D.	#
8) B	Heptachlo...	0.000	8.038	0	3030118	N.D.	2.680	#
9) A	Endosulfan I	0.000	8.450	0	88969	N.D.	0.086	#
13) MA	Dieldrin	0.000	8.736	0	478064	N.D.	0.451	#
14) MA	Endrin	8.086	8.965	992047	2505621	1.984	2.802	#
15) B	Endosulfa...	0.000	9.220f	0	241856	N.D.	0.267	#
17) MA	4,4'-DDT	0.000	9.436	0	323580	N.D.	0.343	#
19) B	Endosulfa...	0.000	9.581	0	24302	N.D.	0.027	#
21) B	Endrin ke...	0.000	10.098f	0	160889	N.D.	0.161	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080421\
Data File : PL068664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2021 08:33
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 01:35:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

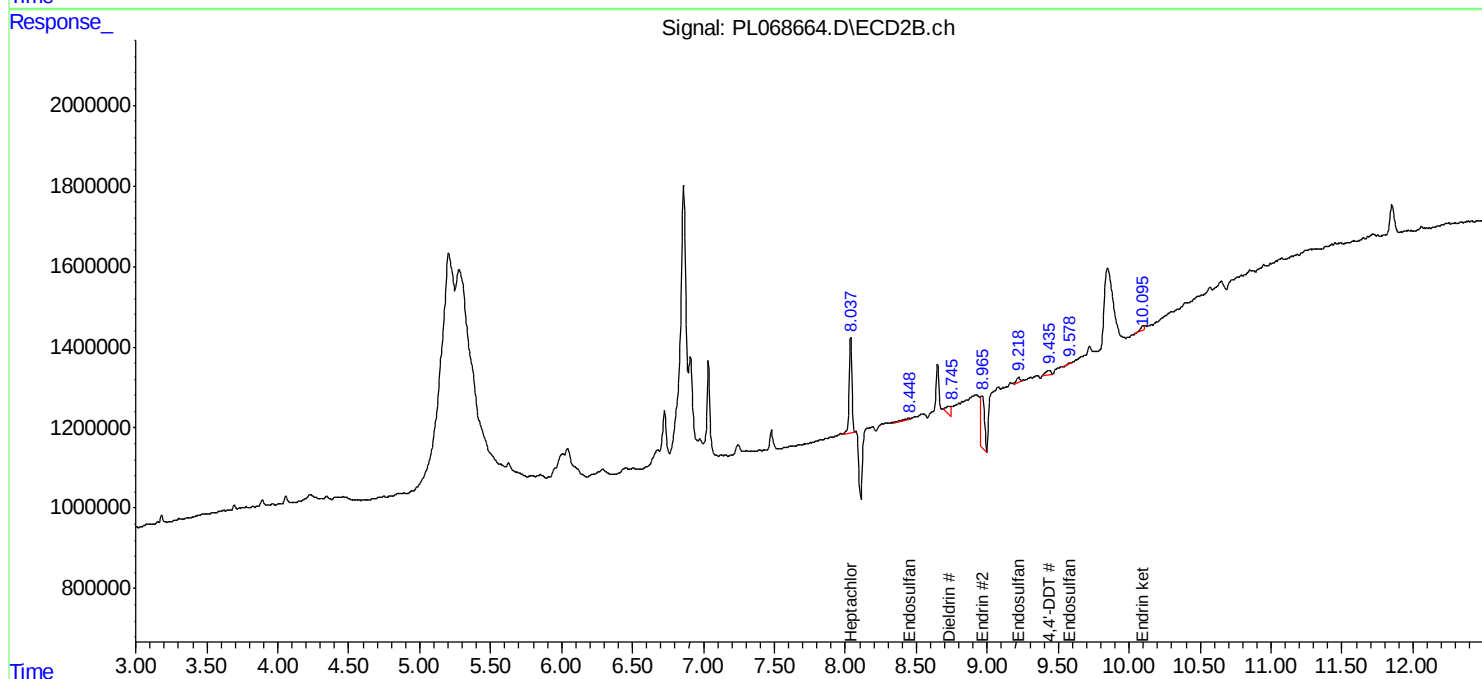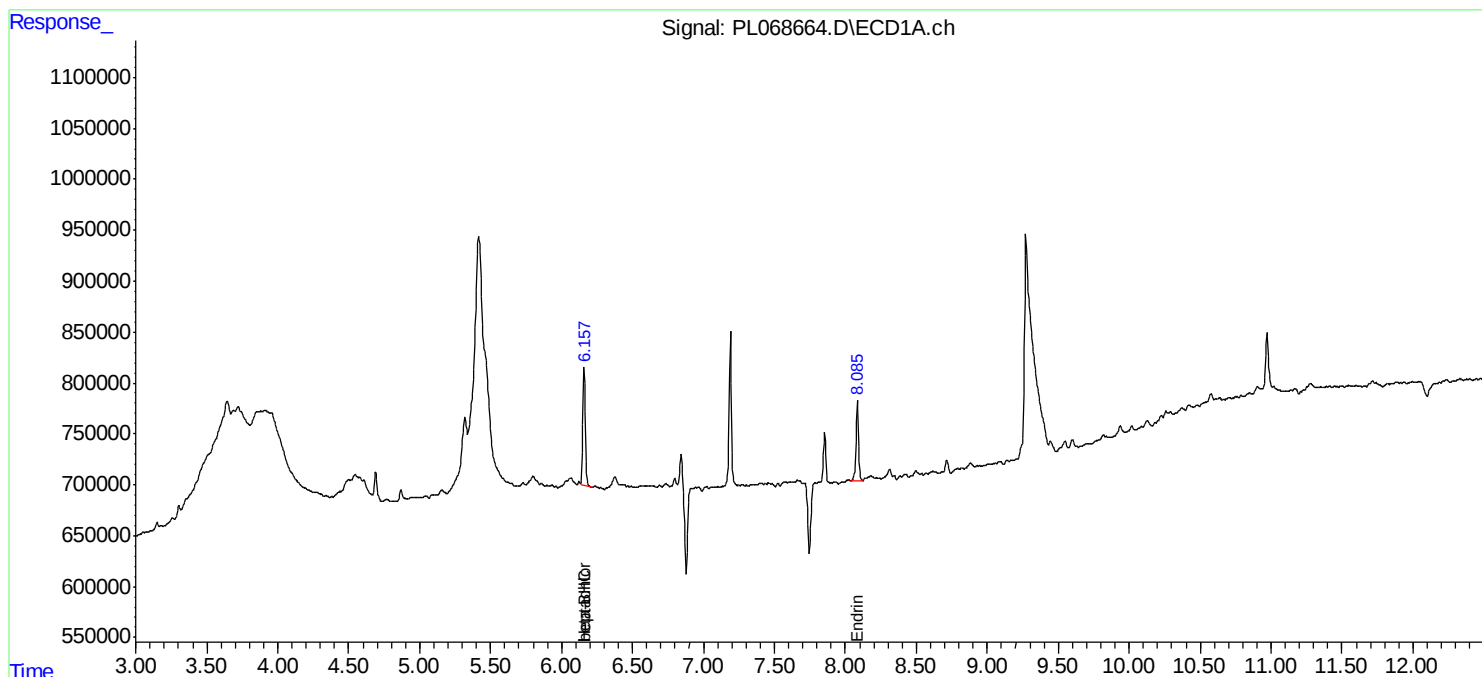


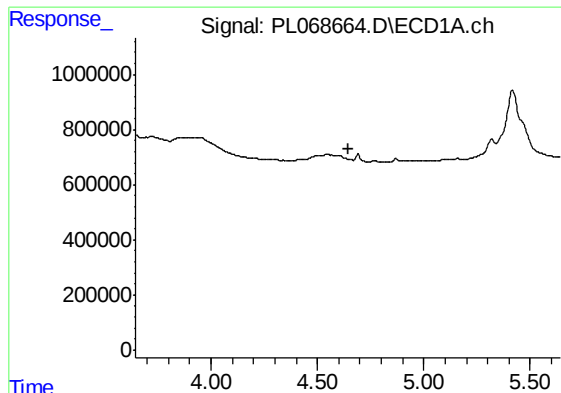

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

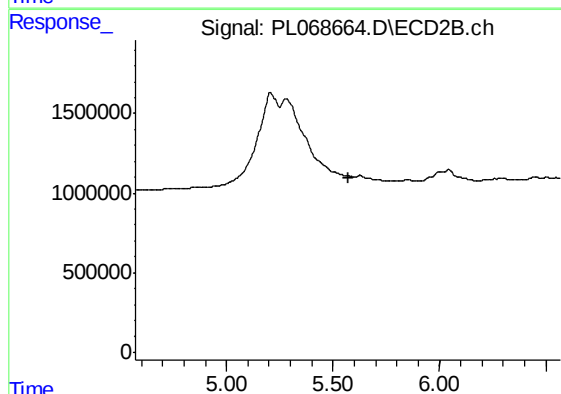


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.571 min
Response: 0
Conc: N.D.

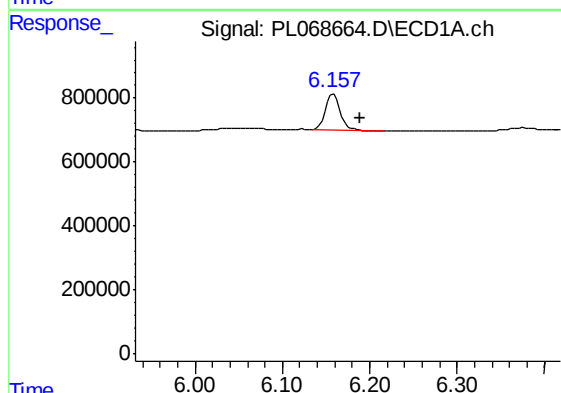


#4 Heptachlor

R.T.: 6.159 min
Delta R.T.: -0.030 min
Response: 1390839
Conc: 2.28 ng/ml

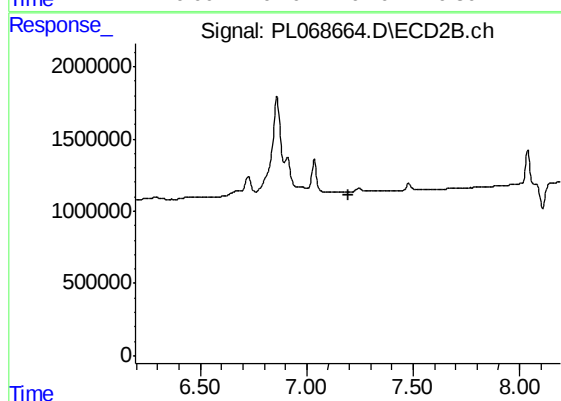

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.195 min
Response: 0
Conc: N.D.

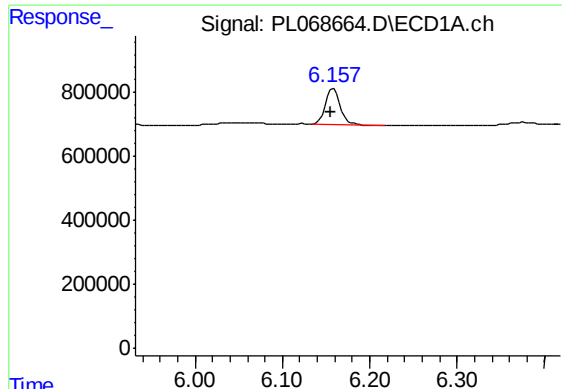

#6 beta-BHC


R.T.: 6.159 min
Delta R.T.: 0.004 min
Response: 1390839
Conc: 4.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

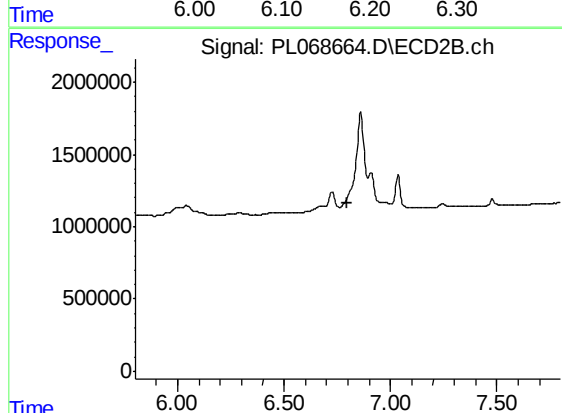


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

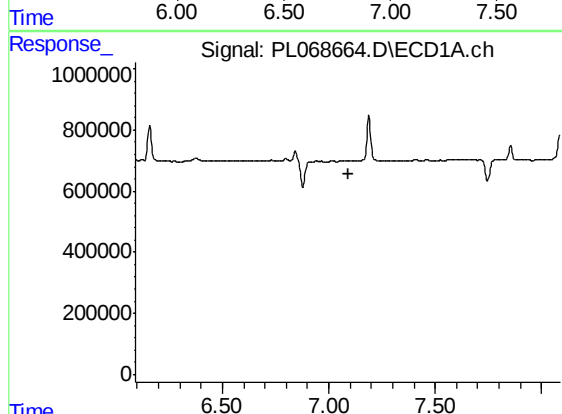


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

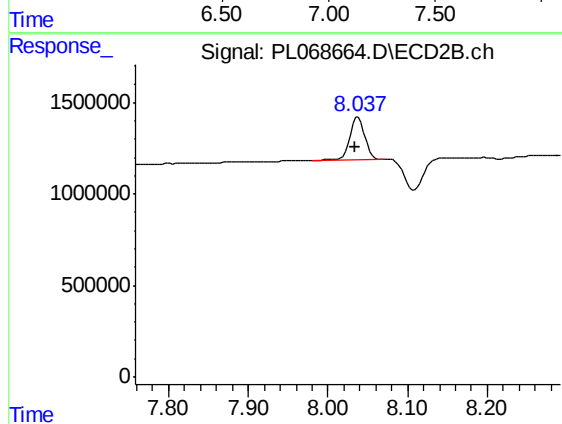

#8 Heptachlor epoxide


R.T.: 8.038 min
Delta R.T.: 0.005 min
Response: 3030118
Conc: 2.68 ng/ml

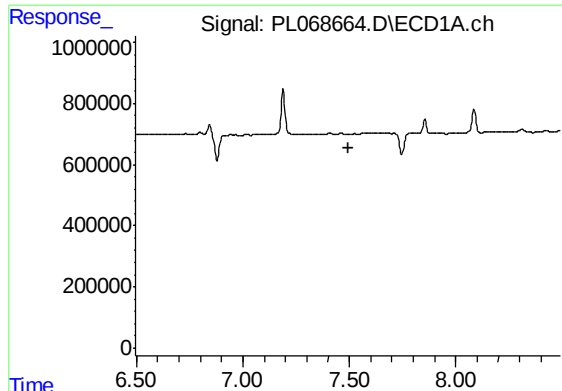

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

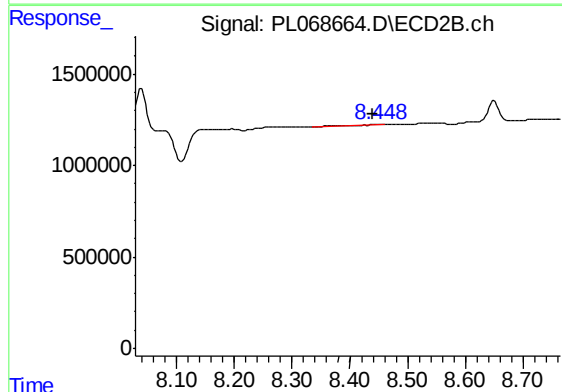


#9 Endosulfan I

R.T.: 8.450 min
Delta R.T.: 0.011 min
Response: 88969
Conc: 0.09 ng/ml

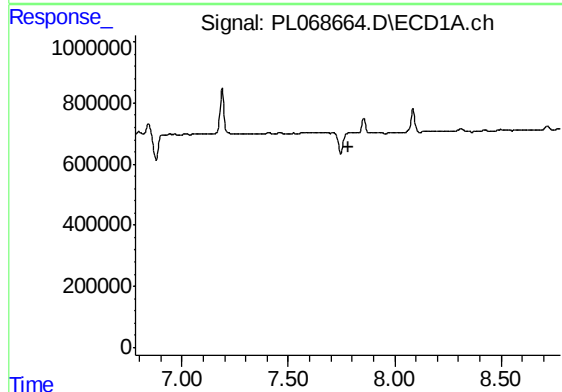


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 7.781 min
Response: 0
Conc: N.D.

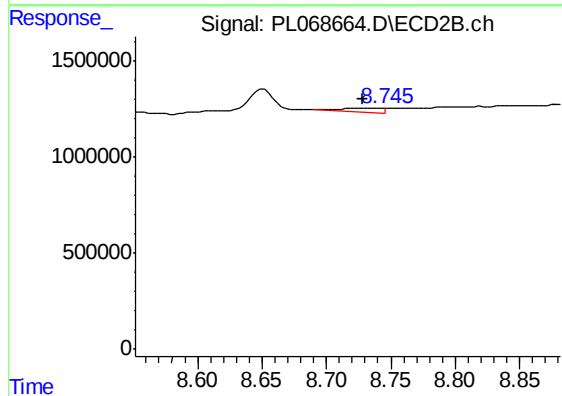

#13 Dieldrin


R.T.: 8.736 min
Delta R.T.: 0.008 min
Response: 478064
Conc: 0.45 ng/ml

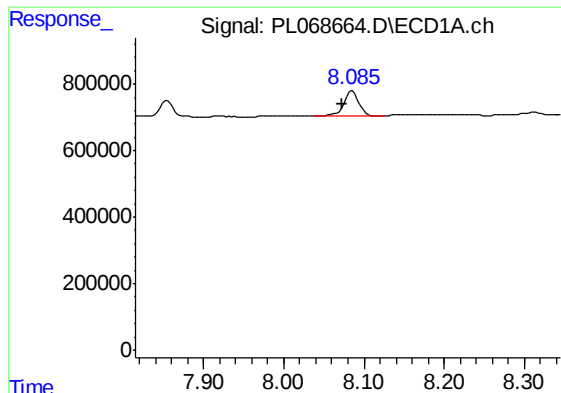

#14 Endrin


R.T.: 8.086 min
Delta R.T.: 0.014 min
Response: 992047
Conc: 1.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

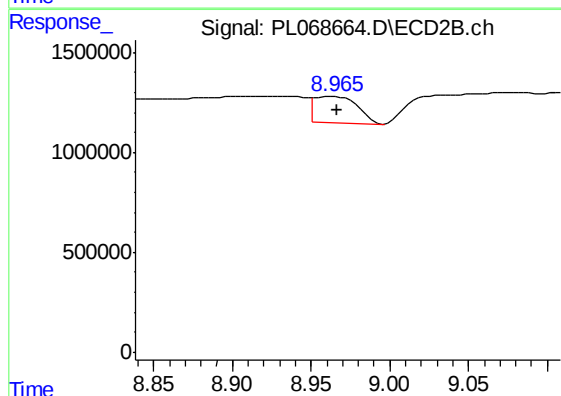


#14 Endrin

R.T.: 8.965 min
Delta R.T.: -0.001 min
Response: 2505621
Conc: 2.80 ng/ml

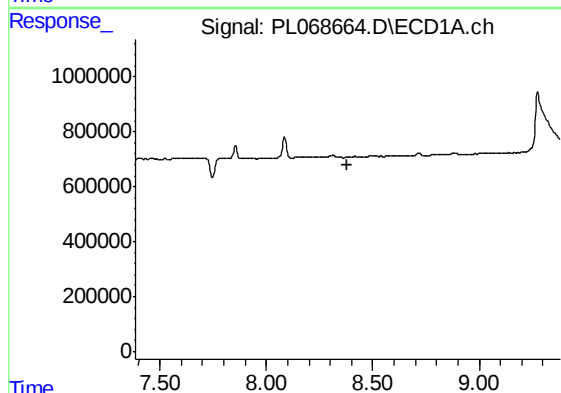


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

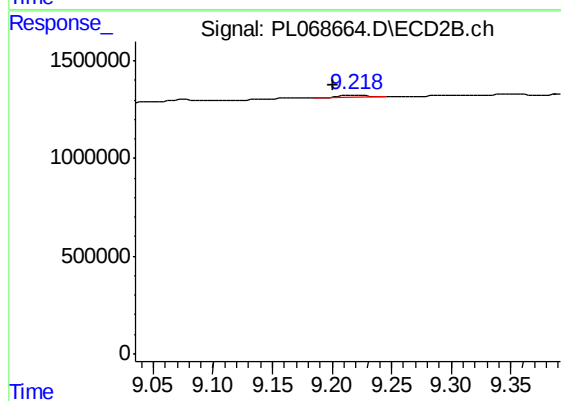

#15 Endosulfan II


R.T.: 9.220 min
Delta R.T.: 0.019 min
Response: 241856
Conc: 0.27 ng/ml

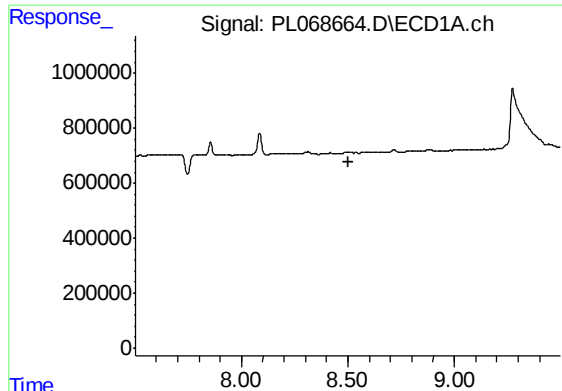

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 8.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

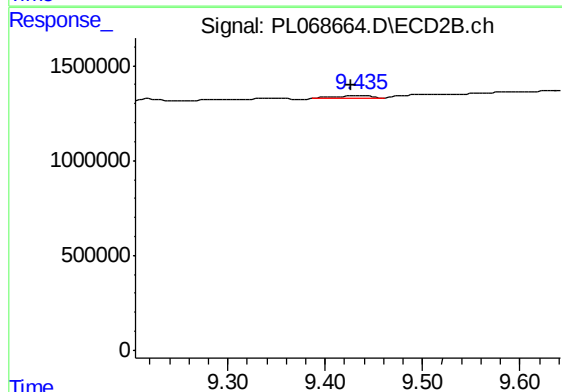


#17 4,4'-DDT

R.T.: 9.436 min
Delta R.T.: 0.009 min
Response: 323580
Conc: 0.34 ng/ml

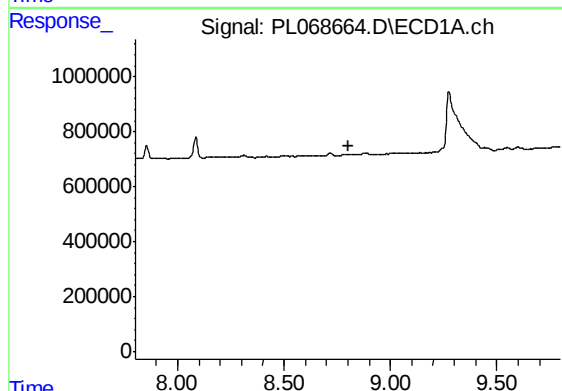


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 8.801 min
Response: 0
Conc: N.D.

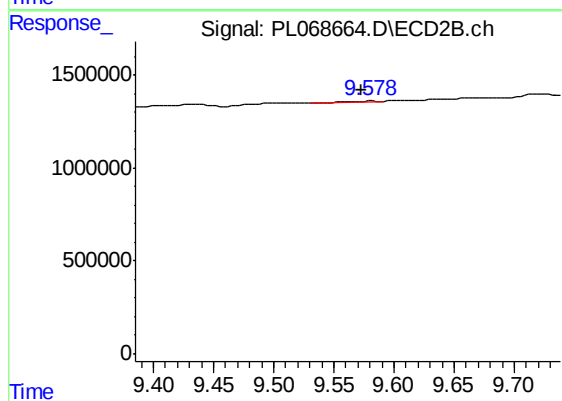

#19 Endosulfan Sulfate


R.T.: 9.581 min
Delta R.T.: 0.008 min
Response: 24302
Conc: 0.03 ng/ml

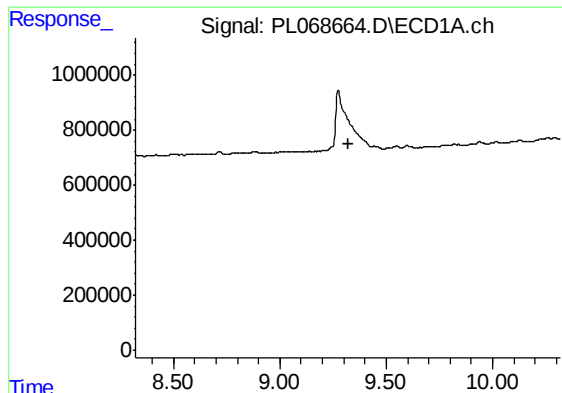

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

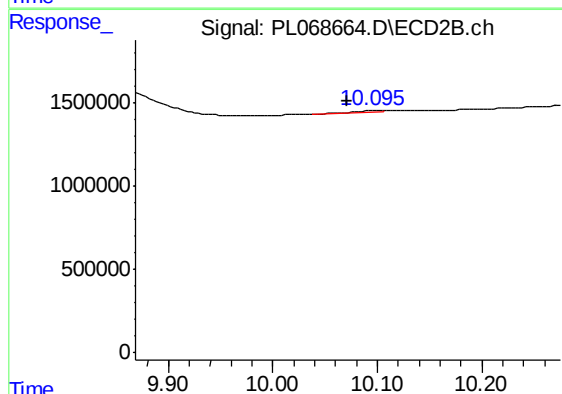


#21 Endrin ketone

R.T.: 10.098 min
Delta R.T.: 0.027 min
Response: 160889
Conc: 0.16 ng/ml

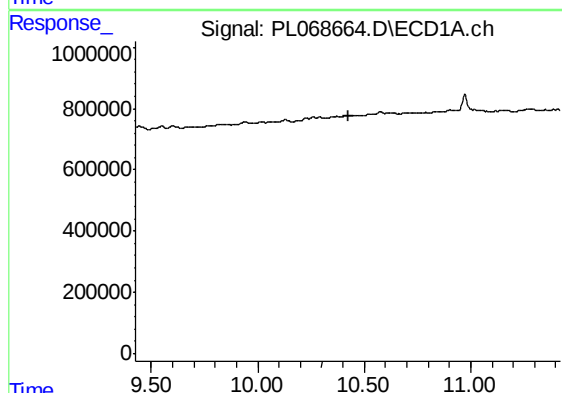

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.424 min
Response: 0
Conc: N.D.

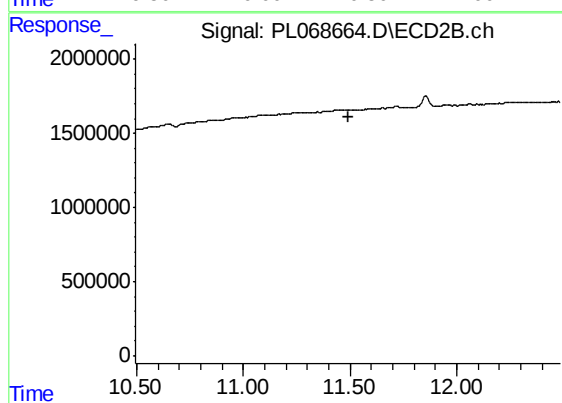

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.492 min
Response: 0
Conc: N.D.