

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080422\
 Data File : PL076893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2022 17:23
 Operator : AR\AJ
 Sample : PB146748BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 05:04:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:34:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.639	17092113	44162559	17.954	19.134
28)	SA Decachlor...	8.908	7.743	16117313	40474493	20.282	21.052
Target Compounds							
2)	A alpha-BHC	3.878	0.000	406801	0	0.296	N.D. #
3)	MA gamma-BHC...	4.205f	0.000	32351	0	0.026	N.D. #
10)	B gamma-Chl...	0.000	4.807	0	83486	N.D.	0.034 #
14)	MA Endrin	0.000	5.488f	0	48197	N.D.	0.022 #
25)	Chlordane-3	0.000	4.807	0	83486	N.D.	0.303 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080422\
Data File : PL076893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2022 17:23
Operator : AR\AJ
Sample : PB146748BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 05:04:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:34:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

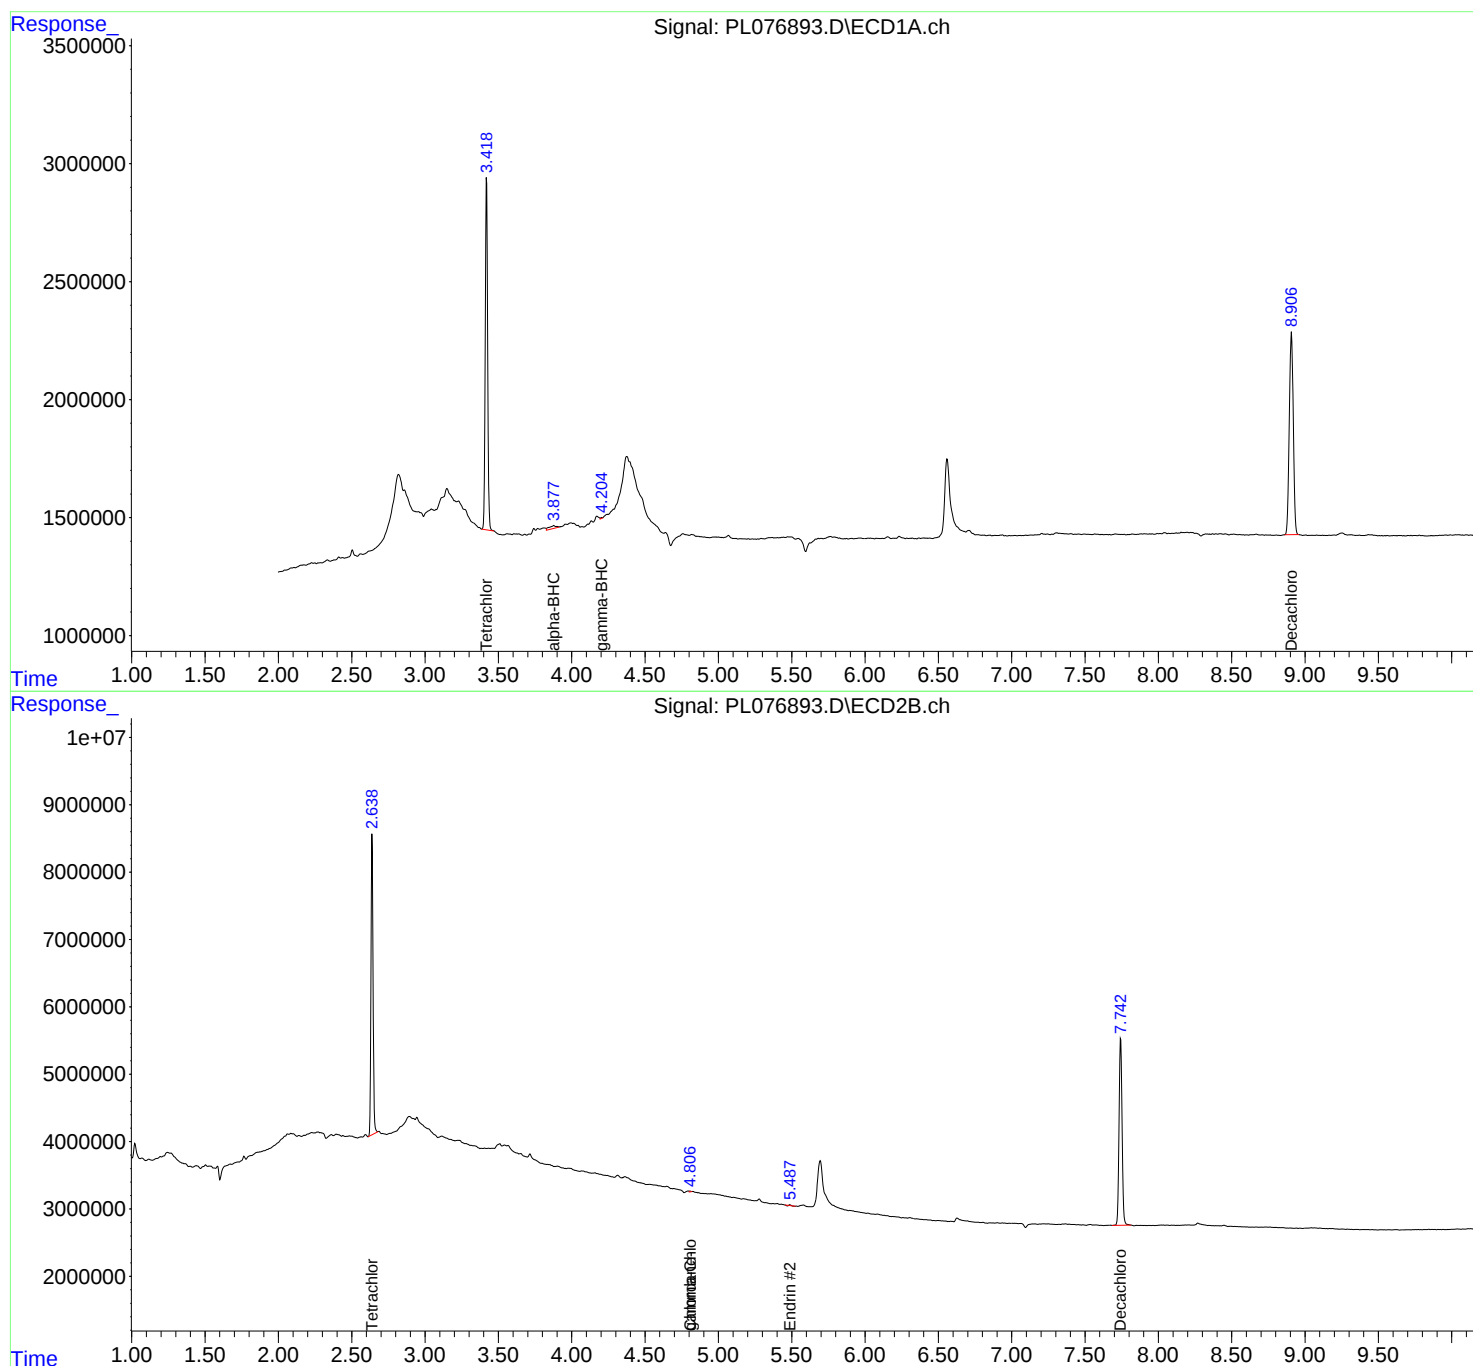


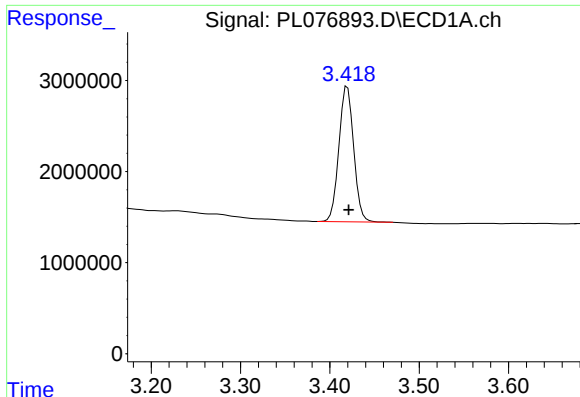

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: -0.001 min
Response: 17092113
Conc: 17.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

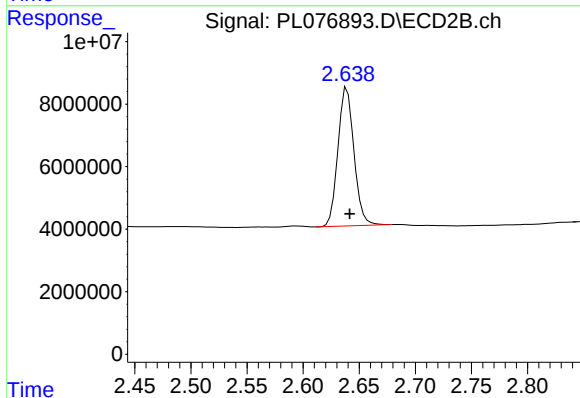


#1 Tetrachloro-m-xylene

R.T.: 2.639 min
Delta R.T.: -0.002 min
Response: 44162559
Conc: 19.13 ng/ml

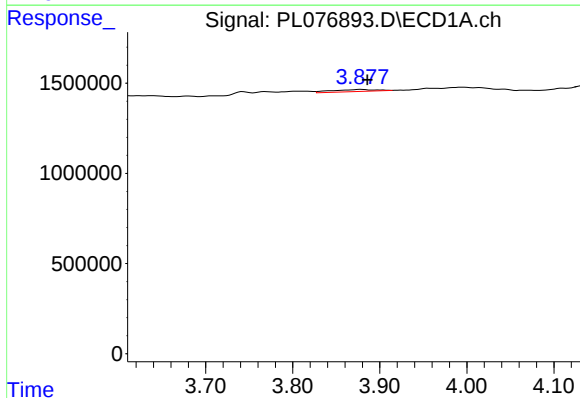


#2 alpha-BHC

R.T.: 3.878 min
Delta R.T.: -0.007 min
Response: 406801
Conc: 0.30 ng/ml

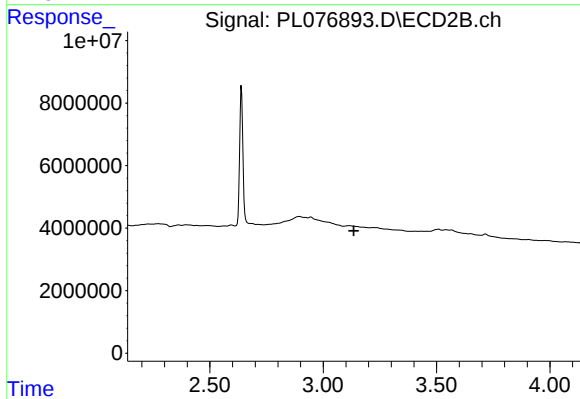

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.136 min
Response: 0
Conc: N.D.

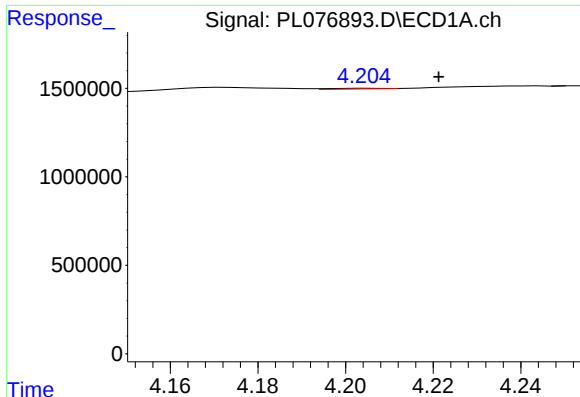

#3 gamma-BHC (Lindane)


R.T.: 4.205 min
Delta R.T.: -0.016 min
Response: 32351
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

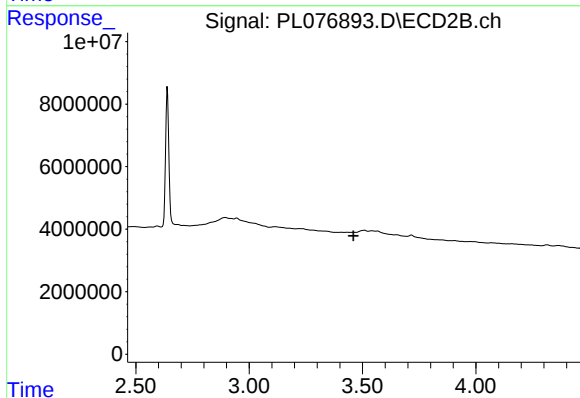


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.460 min
Response: 0
Conc: N.D.

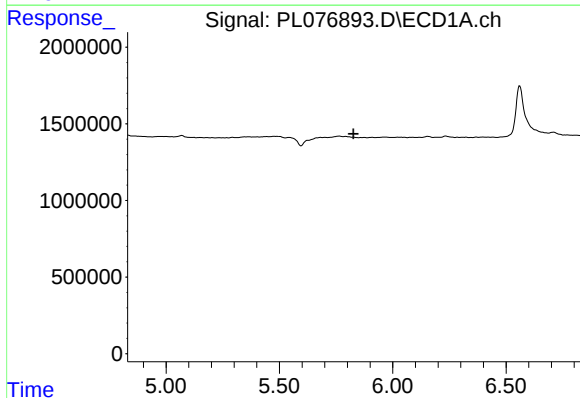


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.827 min
Response: 0
Conc: N.D.

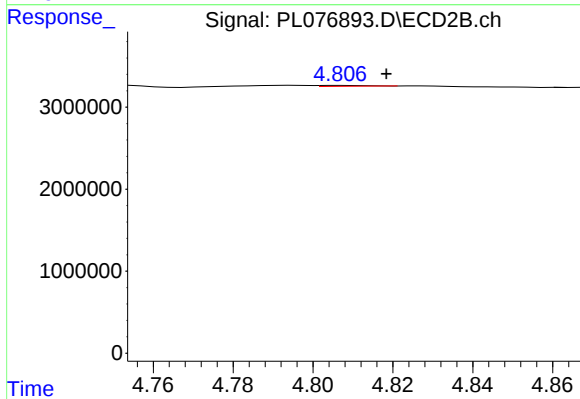

#10 gamma-Chlordane


R.T.: 4.807 min
Delta R.T.: -0.011 min
Response: 83486
Conc: 0.03 ng/ml

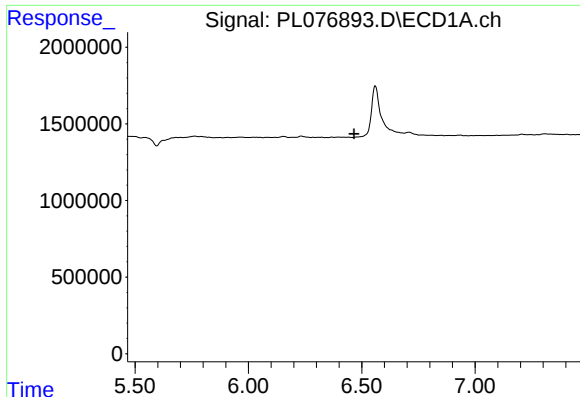

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

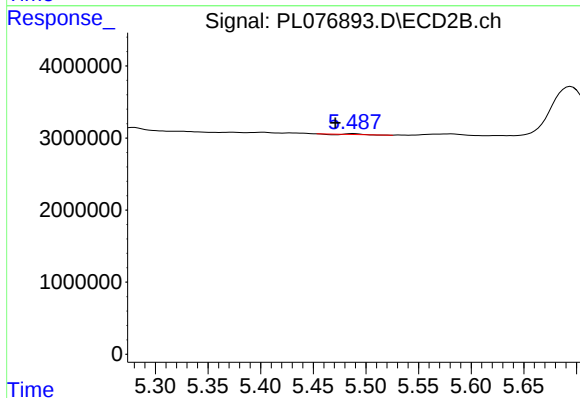


#14 Endrin

R.T.: 5.488 min
Delta R.T.: 0.017 min
Response: 48197
Conc: 0.02 ng/ml

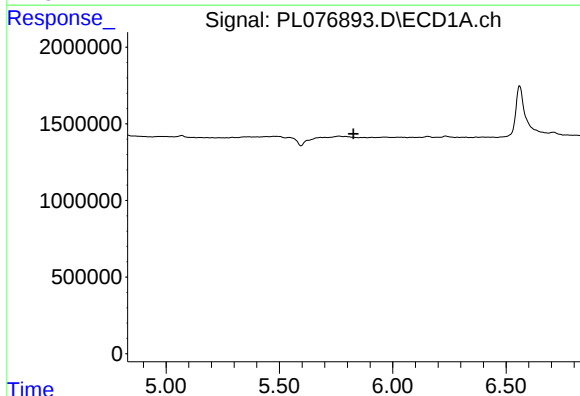


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.827 min
Response: 0
Conc: N.D.

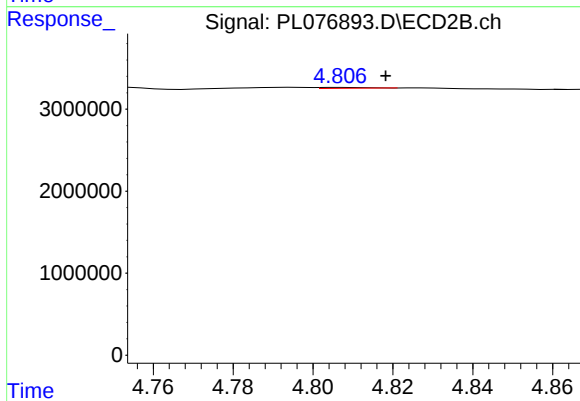

#25 Chlordane-3


R.T.: 4.807 min
Delta R.T.: -0.011 min
Response: 83486
Conc: 0.30 ng/ml

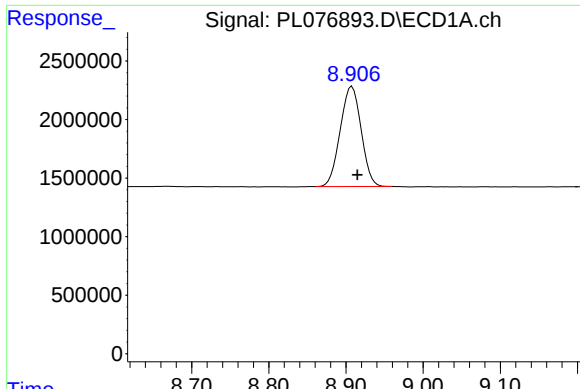

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: -0.007 min
Response: 16117313
Conc: 20.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

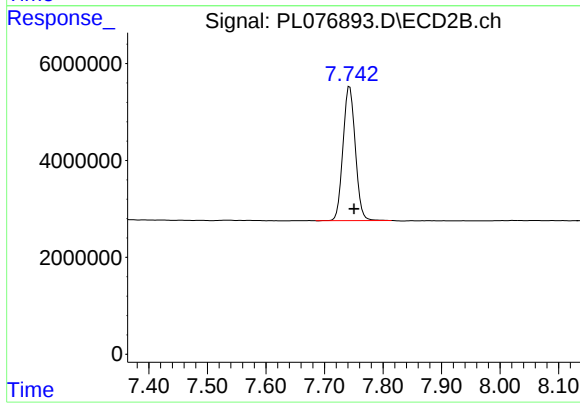

#28 Decachlorobiphenyl

R.T.: 7.743 min
Delta R.T.: -0.008 min
Response: 40474493
Conc: 21.05 ng/ml