

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080422\
 Data File : PL076875.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2022 12:29
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 04:59:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:34:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	2.639	48540993	137.2E6	50.989	59.433
28)	SA Decachlor...	8.915	7.750	37760347	93145768	47.518	48.449
Target Compounds							
23)	Chlordane-1	4.584	3.621	17114985	35949945	455.774	450.577
24)	Chlordane-2	5.116	4.192	18548867	42471235	445.501	431.219
25)	Chlordane-3	5.829	4.817	70532654	117.1E6	436.874	424.501
26)	Chlordane-4	5.907	4.878	85364346	120.5E6	435.029	417.680
27)	Chlordane-5	6.766	5.543	15110101	31862584	433.165	417.434



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080422\
Data File : PL076875.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2022 12:29
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 04:59:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:34:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

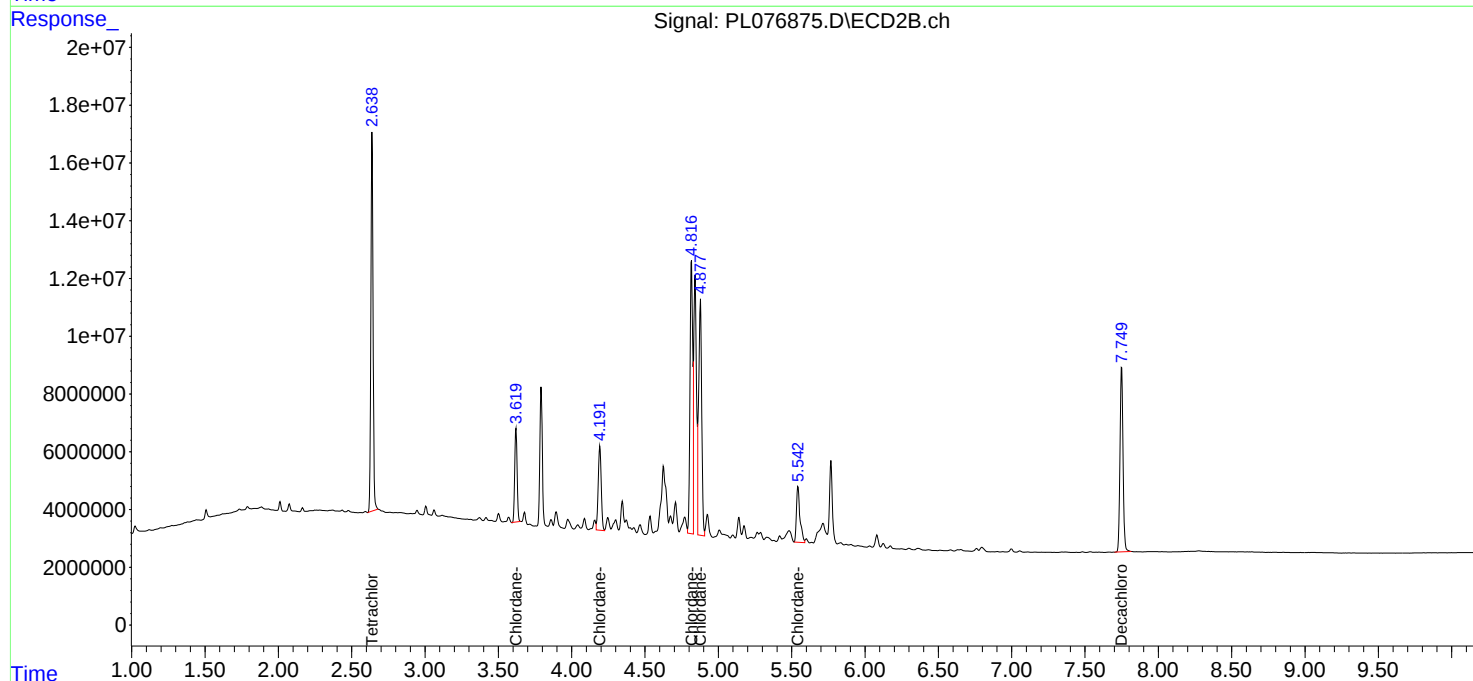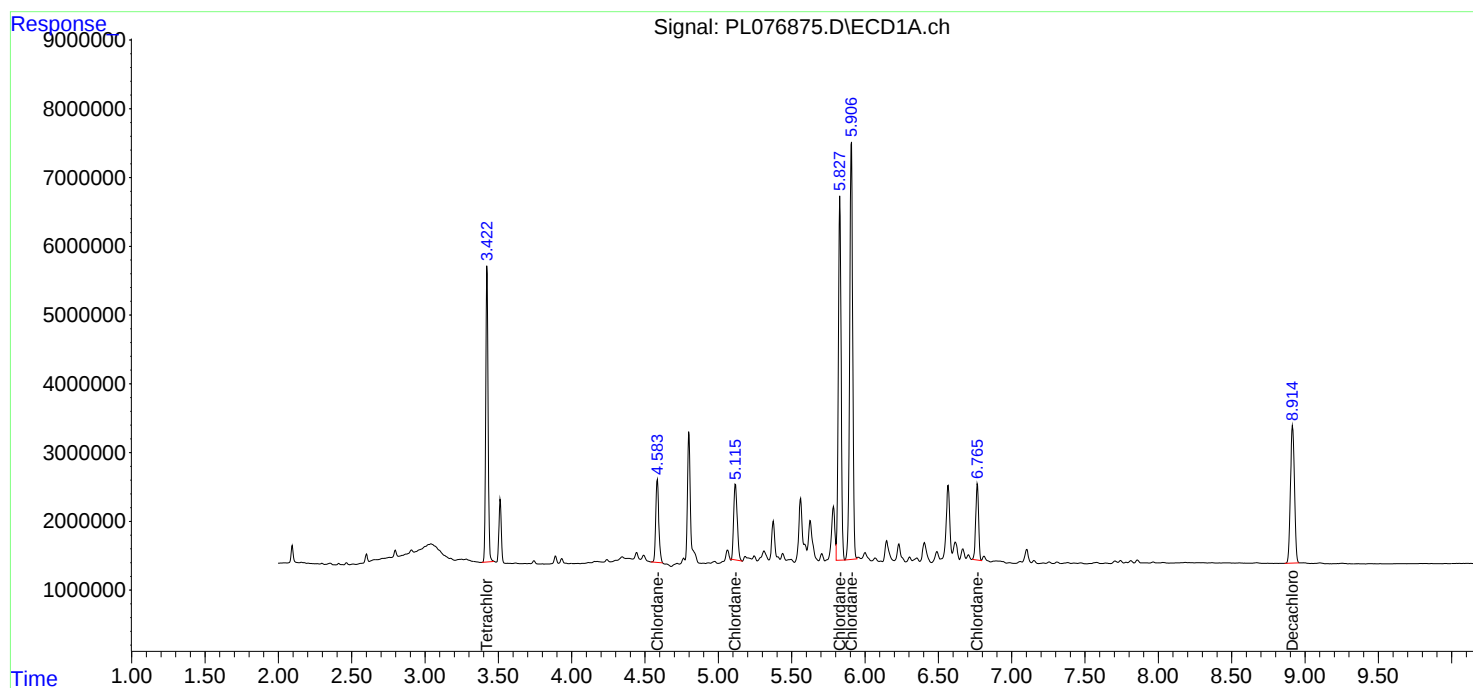


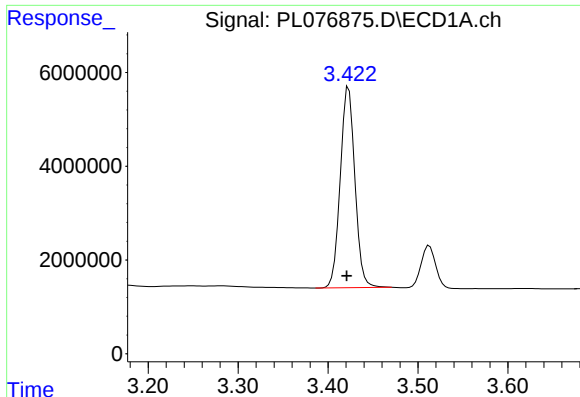

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: 0.002 min
Response: 48540993
Conc: 50.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

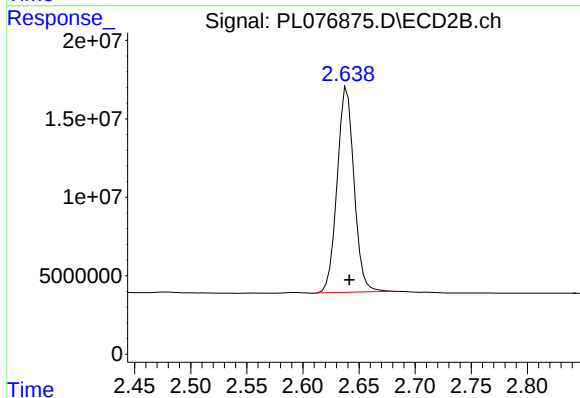


#1 Tetrachloro-m-xylene

R.T.: 2.639 min
Delta R.T.: -0.002 min
Response: 137177966
Conc: 59.43 ng/ml

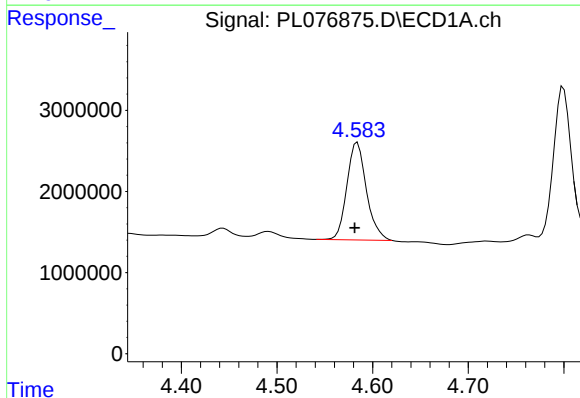


#23 Chlordane-1

R.T.: 4.584 min
Delta R.T.: 0.003 min
Response: 17114985
Conc: 455.77 ng/ml

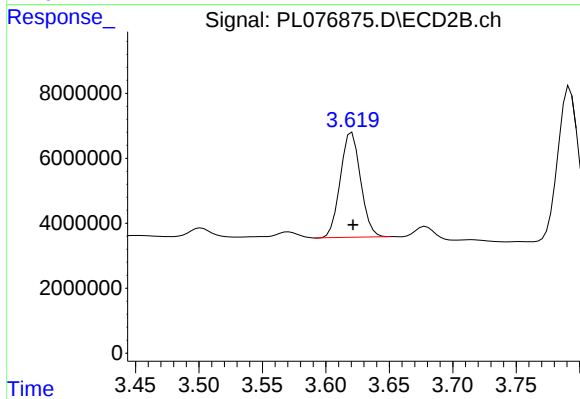

#23 Chlordane-1


R.T.: 3.621 min
Delta R.T.: 0.000 min
Response: 35949945
Conc: 450.58 ng/ml

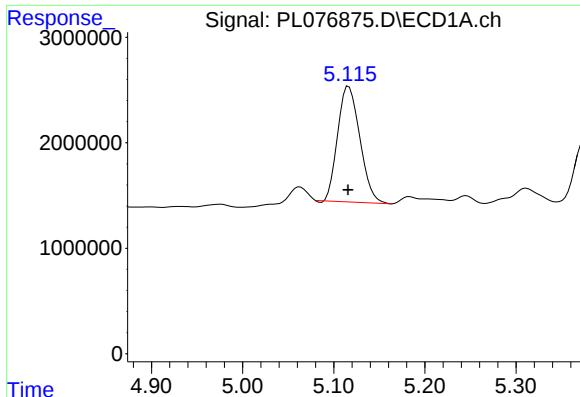

#24 Chlordane-2


R.T.: 5.116 min
Delta R.T.: 0.000 min
Response: 18548867
Conc: 445.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

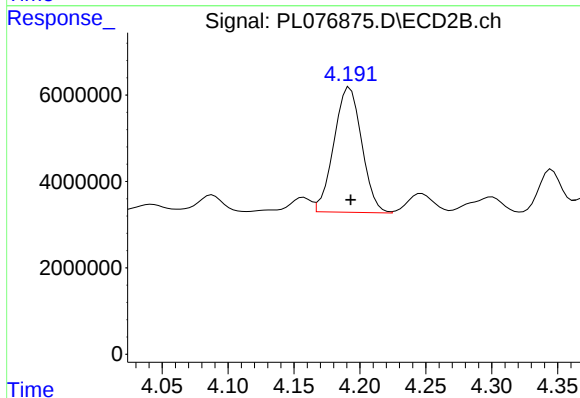


#24 Chlordane-2

R.T.: 4.192 min
Delta R.T.: 0.000 min
Response: 42471235
Conc: 431.22 ng/ml

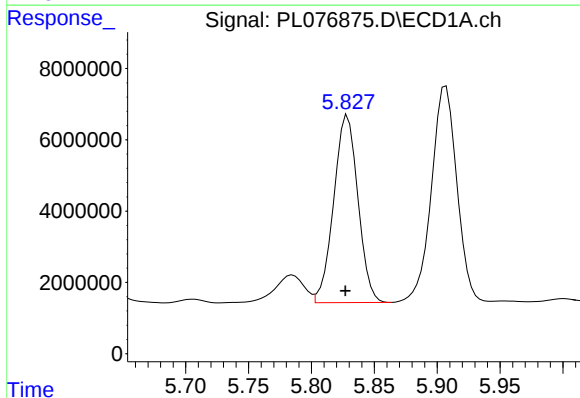


#25 Chlordane-3

R.T.: 5.829 min
Delta R.T.: 0.002 min
Response: 70532654
Conc: 436.87 ng/ml

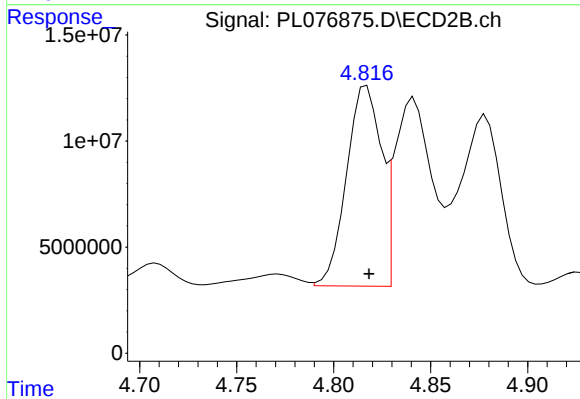

#25 Chlordane-3


R.T.: 4.817 min
Delta R.T.: -0.001 min
Response: 117064148
Conc: 424.50 ng/ml

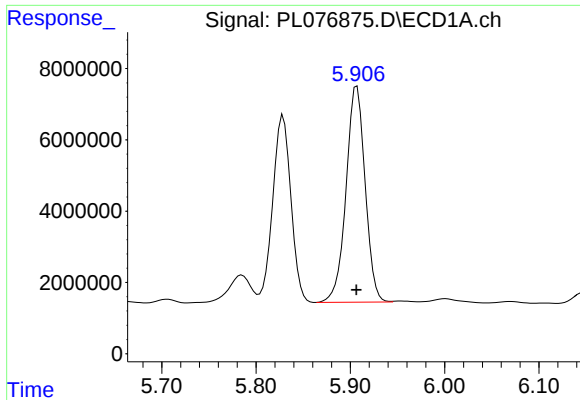

#26 Chlordane-4


R.T.: 5.907 min
Delta R.T.: 0.000 min
Response: 85364346
Conc: 435.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

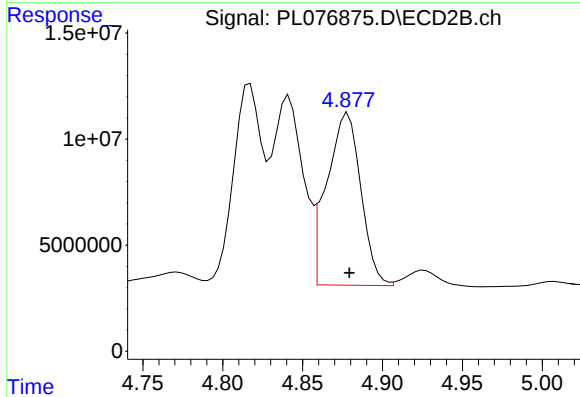


#26 Chlordane-4

R.T.: 4.878 min
Delta R.T.: 0.000 min
Response: 120485131
Conc: 417.68 ng/ml

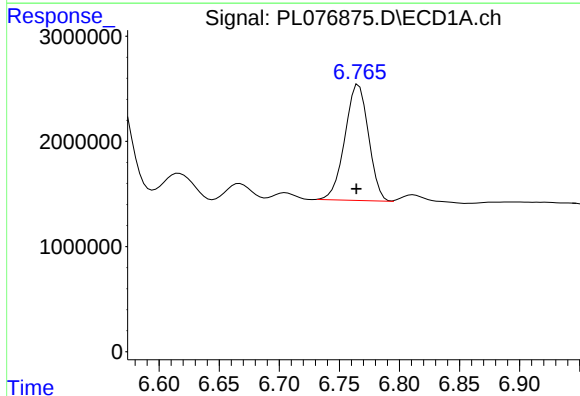


#27 Chlordane-5

R.T.: 6.766 min
Delta R.T.: 0.002 min
Response: 15110101
Conc: 433.17 ng/ml

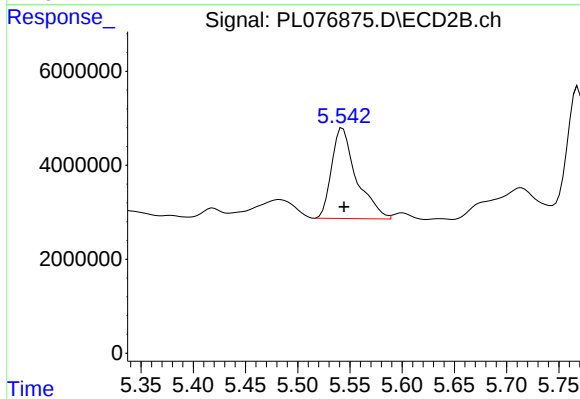

#27 Chlordane-5


R.T.: 5.543 min
Delta R.T.: -0.001 min
Response: 31862584
Conc: 417.43 ng/ml

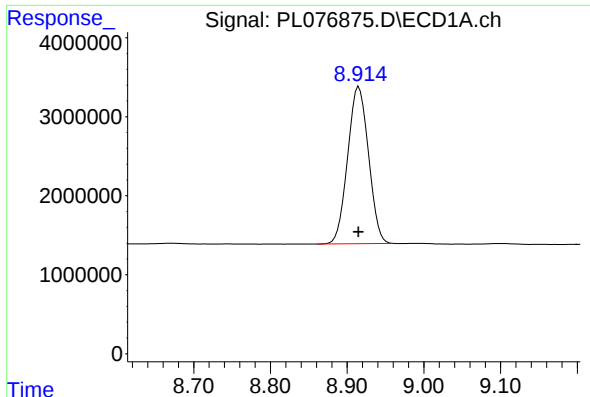

#28 Decachlorobiphenyl

R.T.: 8.915 min
Delta R.T.: 0.000 min
Response: 37760347
Conc: 47.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

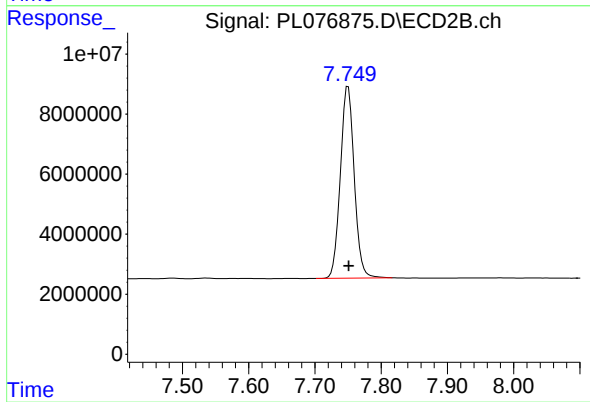

#28 Decachlorobiphenyl

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 93145768
Conc: 48.45 ng/ml