

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080422\
 Data File : PL076887.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2022 15:59
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 05:03:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:34:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.639	46805444	138.0E6	49.166	59.793
28)	SA Decachlor...	8.913	7.749	37361794	96439470	47.016	50.162
Target Compounds							
23)	Chlordane-1	4.582	3.620	16864176	36878630	449.095	462.217
24)	Chlordane-2	5.116	4.191	18361836	43632914	441.009	443.014
25)	Chlordane-3	5.827	4.816	68931968	120.7E6	426.960	437.821
26)	Chlordane-4	5.906	4.878	83555169	123.8E6	425.809	429.200
27)	Chlordane-5	6.765	5.543	14666339	32978891	420.444	432.059



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080422\
Data File : PL076887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2022 15:59
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 05:03:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:34:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

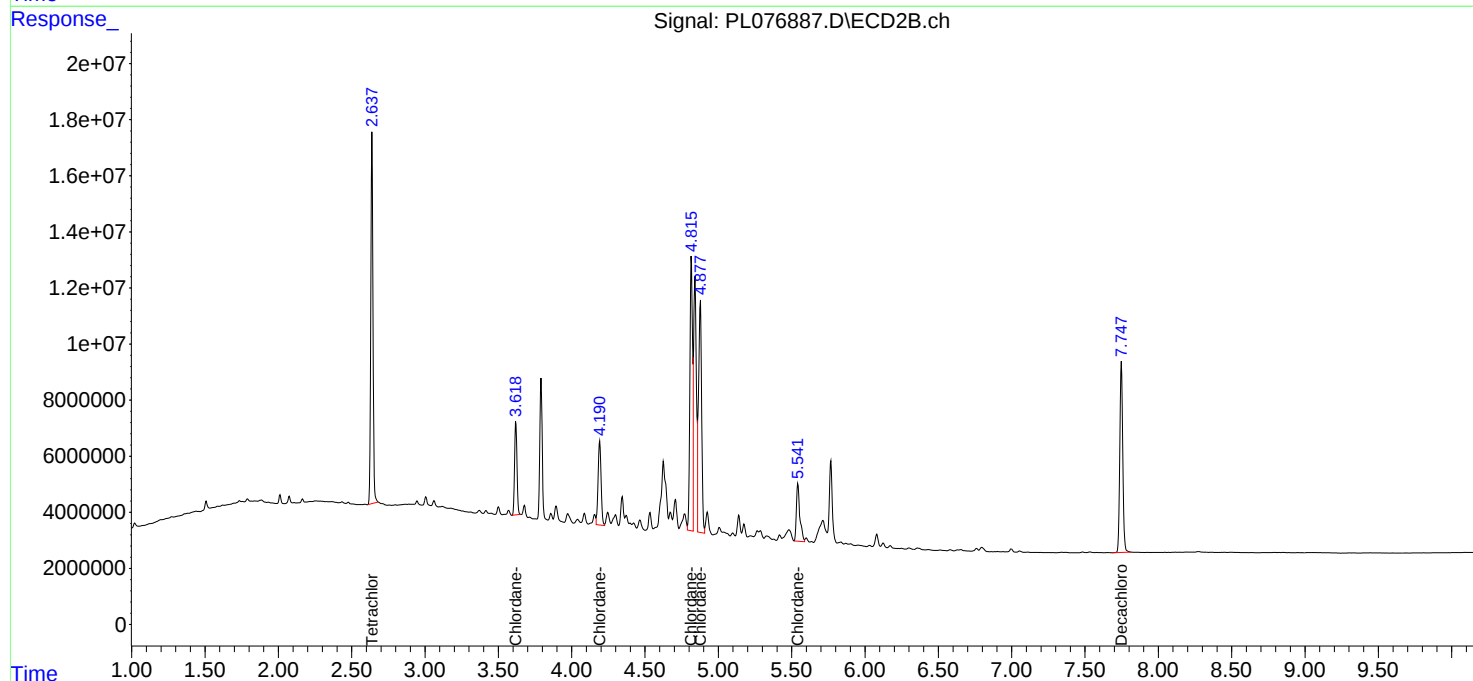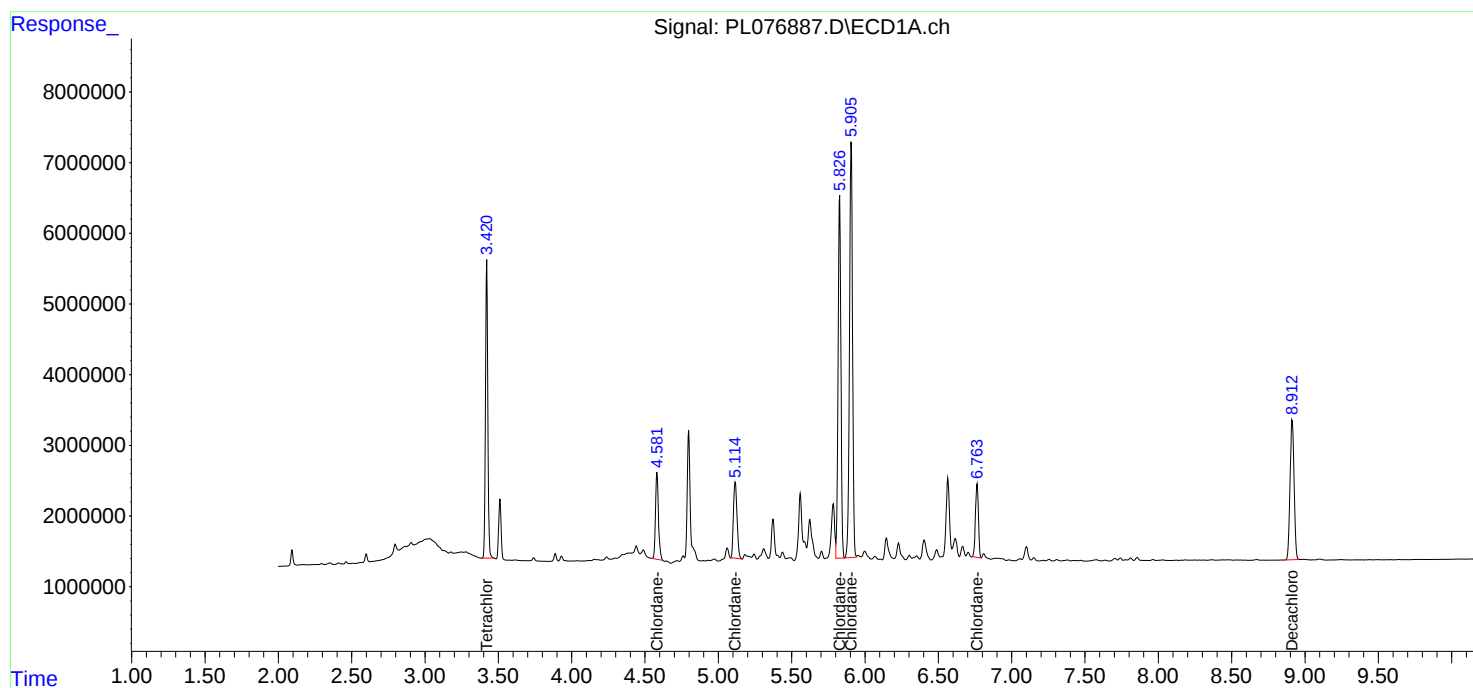


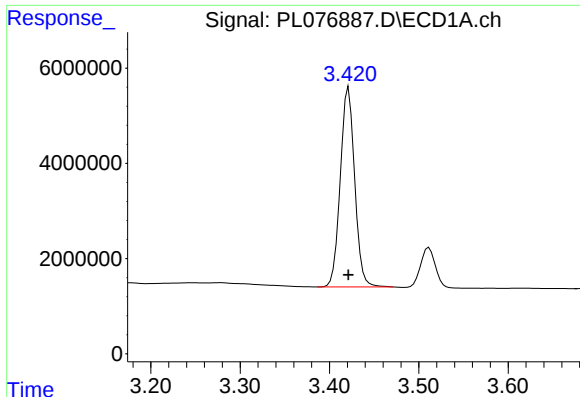

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 46805444
Conc: 49.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

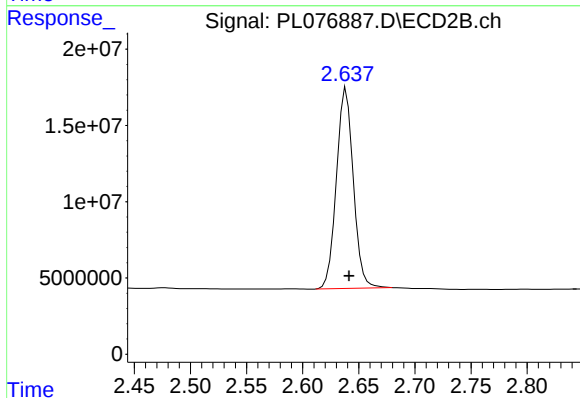


#1 Tetrachloro-m-xylene

R.T.: 2.639 min
Delta R.T.: -0.003 min
Response: 138009803
Conc: 59.79 ng/ml

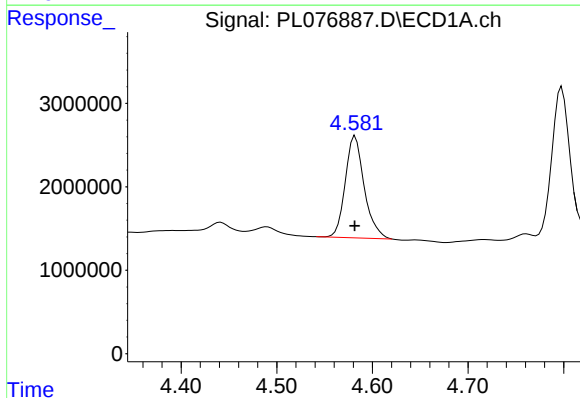


#23 Chlordane-1

R.T.: 4.582 min
Delta R.T.: 0.000 min
Response: 16864176
Conc: 449.10 ng/ml

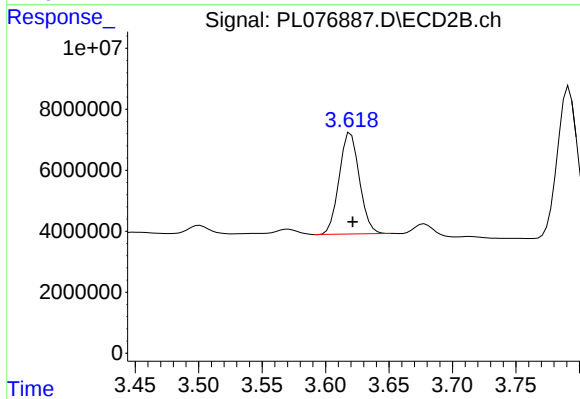

#23 Chlordane-1


R.T.: 3.620 min
Delta R.T.: -0.002 min
Response: 36878630
Conc: 462.22 ng/ml

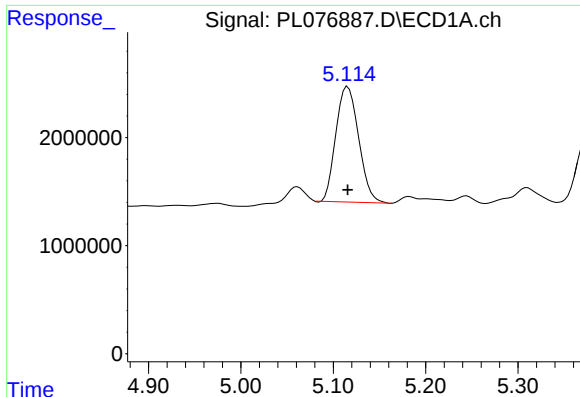

#24 Chlordane-2


R.T.: 5.116 min
Delta R.T.: 0.000 min
Response: 18361836
Conc: 441.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

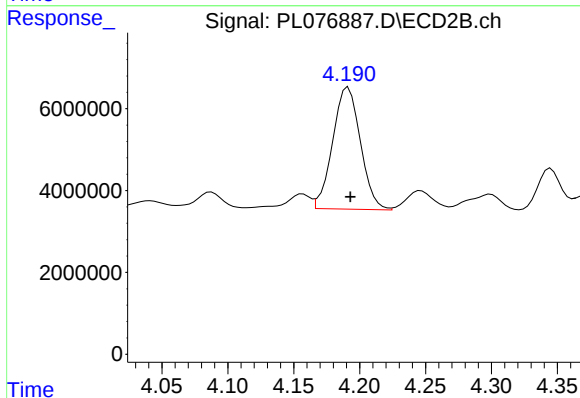


#24 Chlordane-2

R.T.: 4.191 min
Delta R.T.: -0.002 min
Response: 43632914
Conc: 443.01 ng/ml

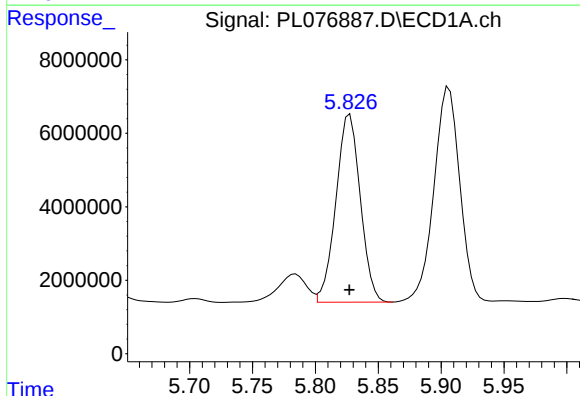


#25 Chlordane-3

R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 68931968
Conc: 426.96 ng/ml

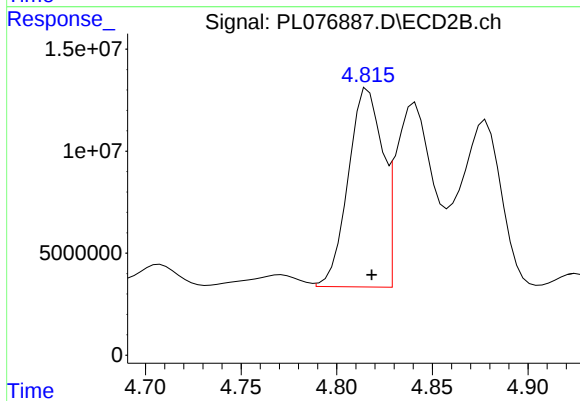

#25 Chlordane-3


R.T.: 4.816 min
Delta R.T.: -0.002 min
Response: 120737545
Conc: 437.82 ng/ml

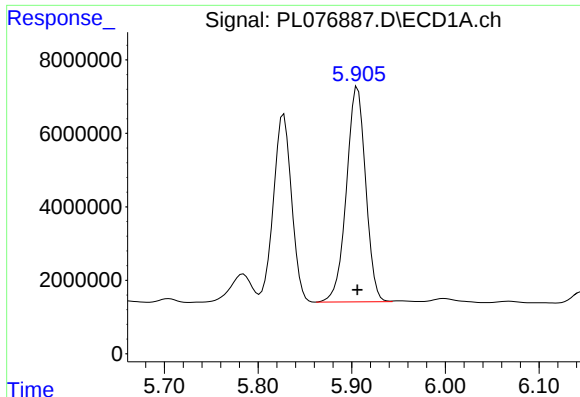

#26 Chlordane-4


R.T.: 5.906 min
Delta R.T.: 0.000 min
Response: 83555169
Conc: 425.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

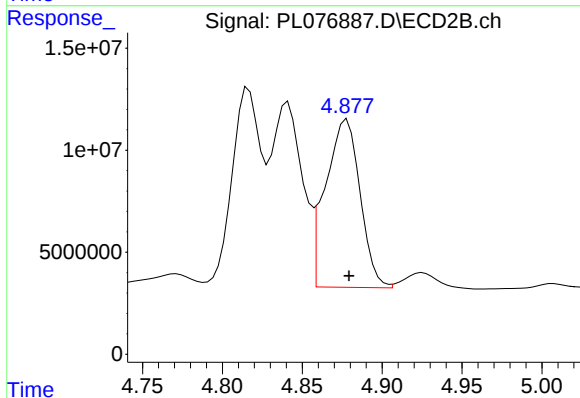


#26 Chlordane-4

R.T.: 4.878 min
Delta R.T.: -0.001 min
Response: 123808183
Conc: 429.20 ng/ml

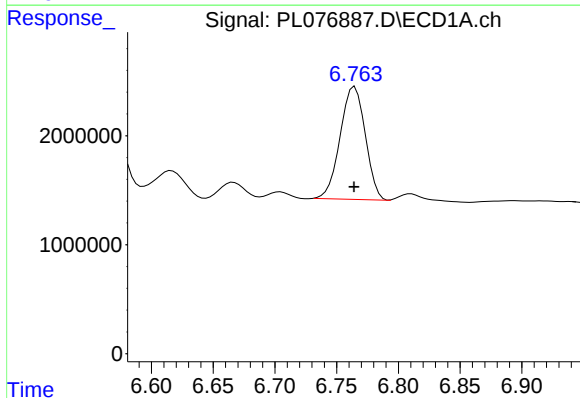


#27 Chlordane-5

R.T.: 6.765 min
Delta R.T.: 0.000 min
Response: 14666339
Conc: 420.44 ng/ml

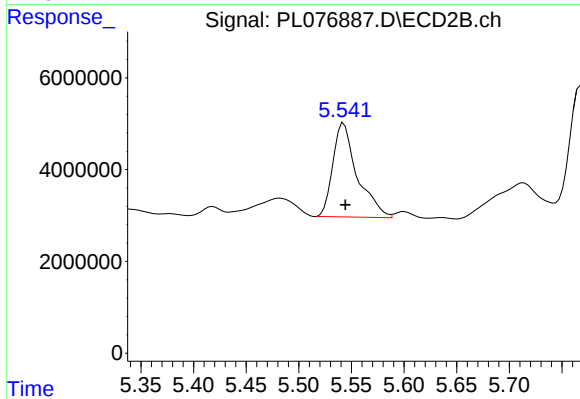

#27 Chlordane-5


R.T.: 5.543 min
Delta R.T.: -0.002 min
Response: 32978891
Conc: 432.06 ng/ml

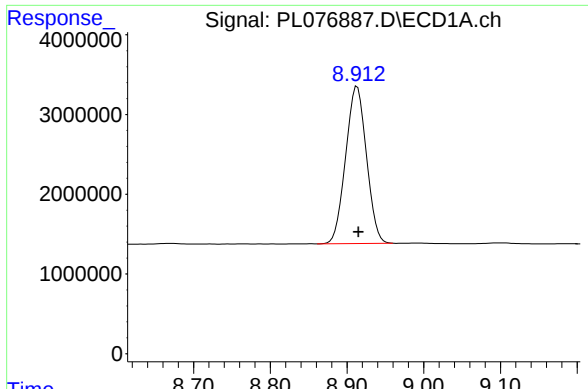

#28 Decachlorobiphenyl

R.T.: 8.913 min
Delta R.T.: -0.002 min
Response: 37361794
Conc: 47.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

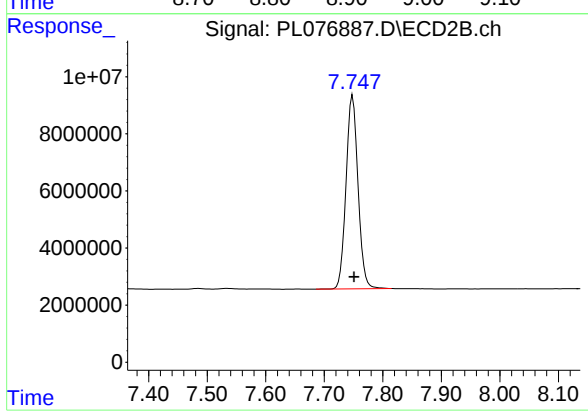

#28 Decachlorobiphenyl

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 96439470
Conc: 50.16 ng/ml