

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080422\
 Data File : PL076900.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2022 19:01
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 05:06:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:34:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.637	45710120	143.4E6	48.015	62.144 #
28)	SA Decachlor...	8.905	7.742	37208232	101.4E6	46.823	52.761
Target Compounds							
23)	Chlordane-1	4.579	3.616	16925455	38760215	450.727	485.800
24)	Chlordane-2	5.112	4.188	18136691	45547618	435.601	462.455
25)	Chlordane-3	5.824	4.811	67017562	125.6E6	415.102	455.444
26)	Chlordane-4	5.902	4.872	82042163	130.6E6	418.099	452.904
27)	Chlordane-5	6.760	5.537	13970281	34863467	400.490	456.749



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080422\
Data File : PL076900.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2022 19:01
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 05:06:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:34:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

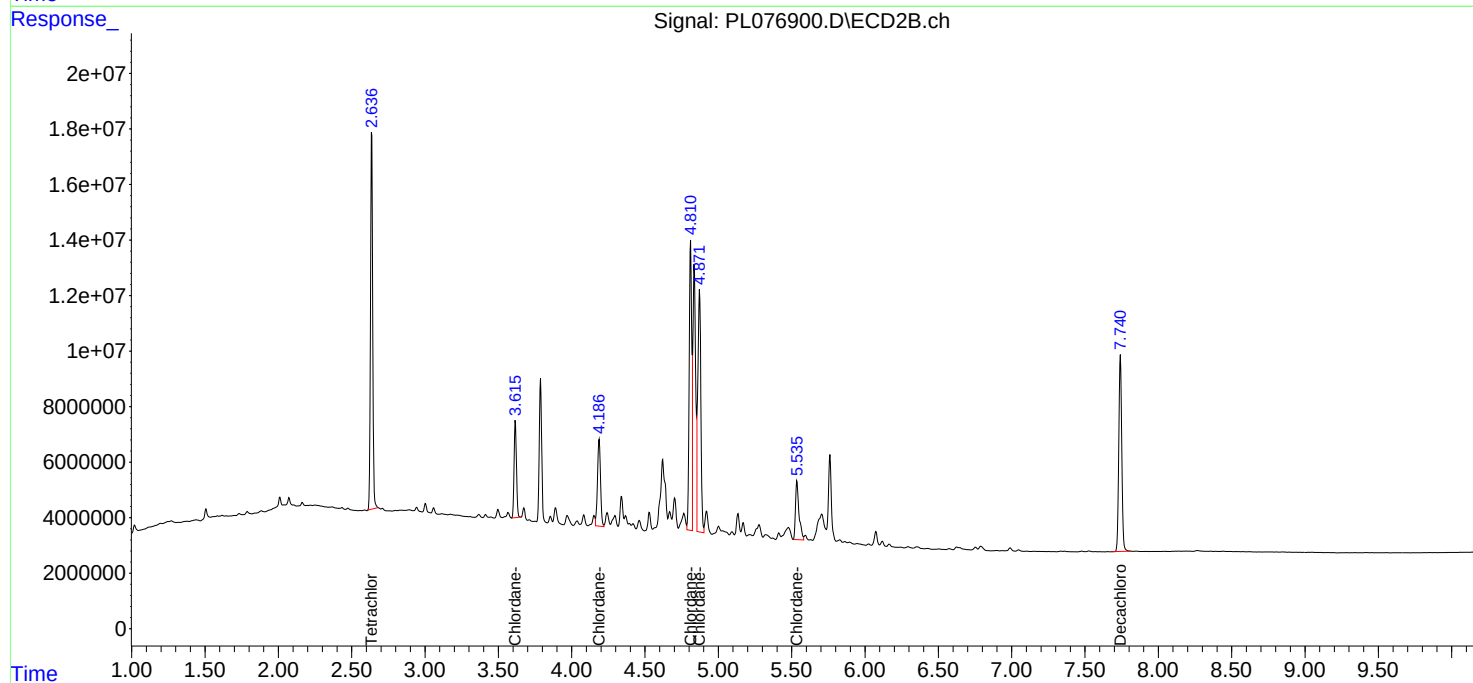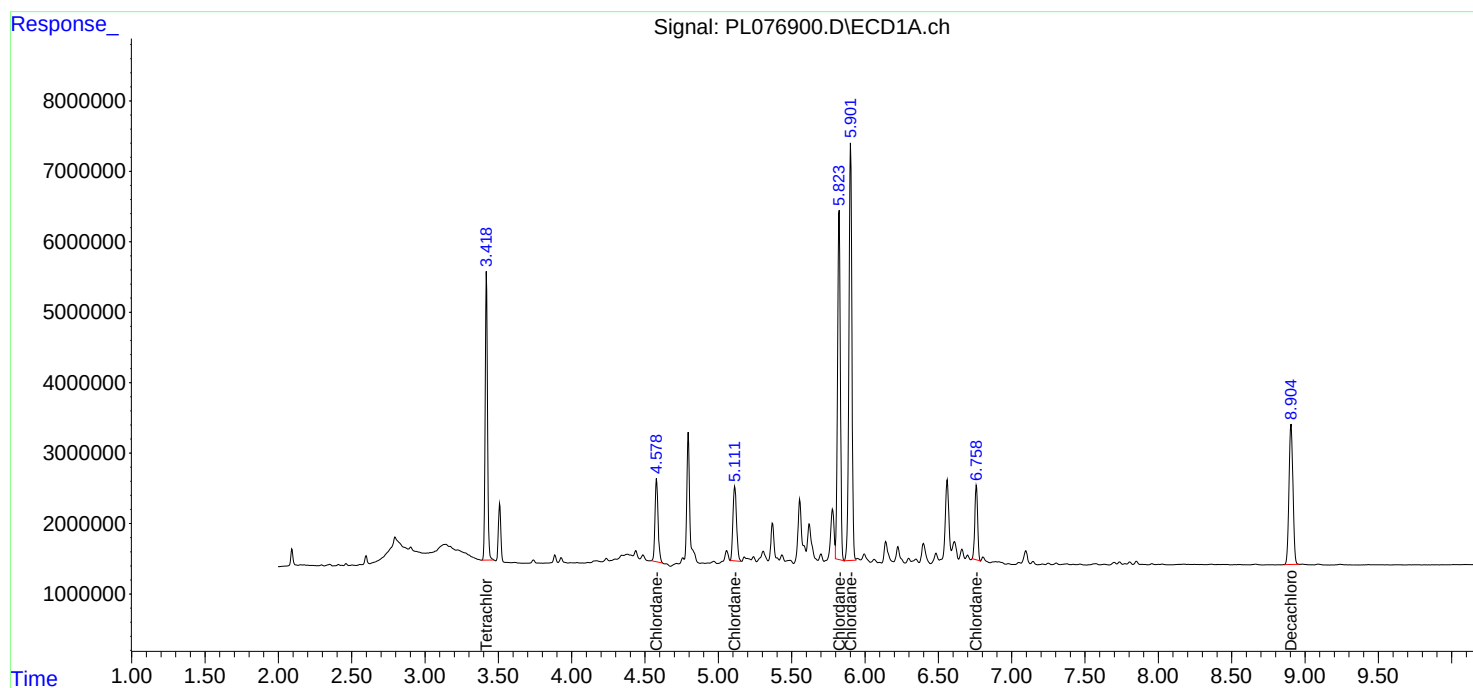


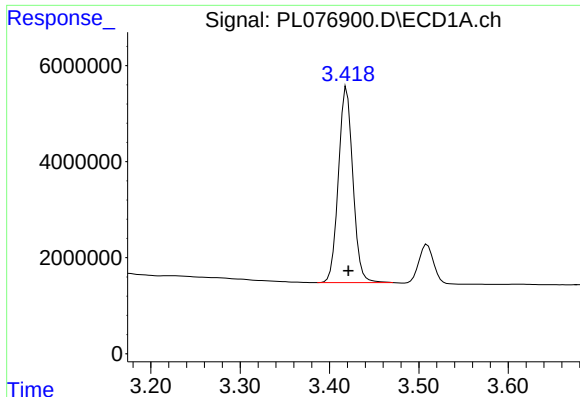

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: -0.002 min
Response: 45710120
Conc: 48.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

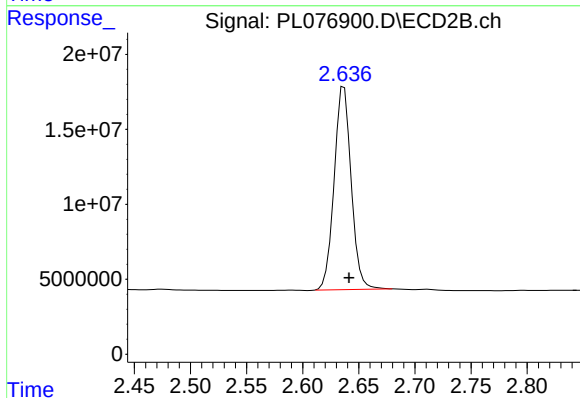


#1 Tetrachloro-m-xylene

R.T.: 2.637 min
Delta R.T.: -0.005 min
Response: 143436802
Conc: 62.14 ng/ml

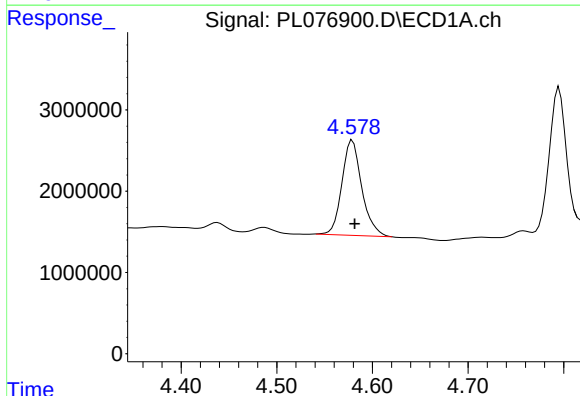


#23 Chlordane-1

R.T.: 4.579 min
Delta R.T.: -0.002 min
Response: 16925455
Conc: 450.73 ng/ml

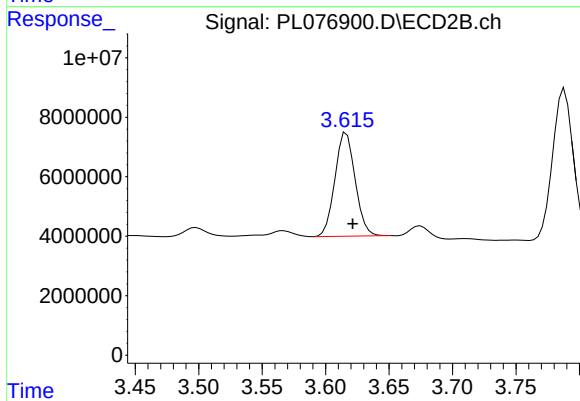

#23 Chlordane-1


R.T.: 3.616 min
Delta R.T.: -0.005 min
Response: 38760215
Conc: 485.80 ng/ml

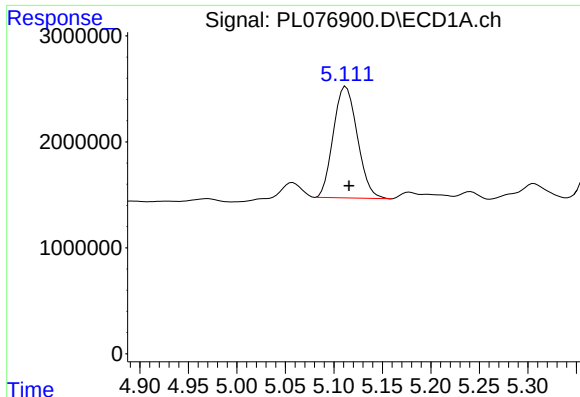

#24 Chlordane-2


R.T.: 5.112 min
Delta R.T.: -0.003 min
Response: 18136691
Conc: 435.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

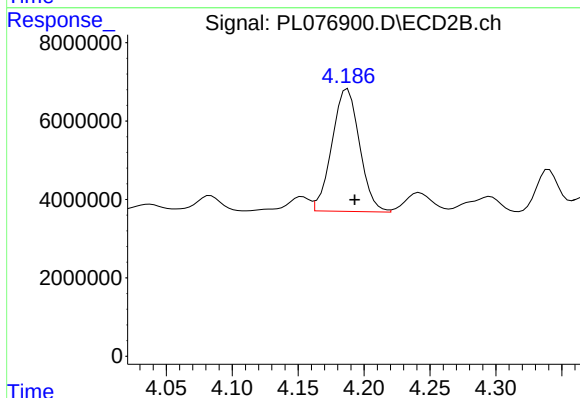


#24 Chlordane-2

R.T.: 4.188 min
Delta R.T.: -0.005 min
Response: 45547618
Conc: 462.45 ng/ml

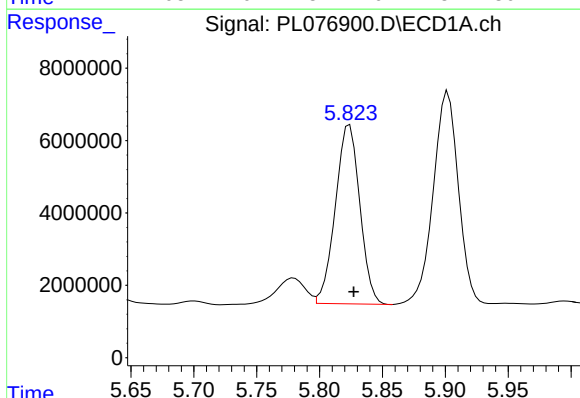


#25 Chlordane-3

R.T.: 5.824 min
Delta R.T.: -0.003 min
Response: 67017562
Conc: 415.10 ng/ml

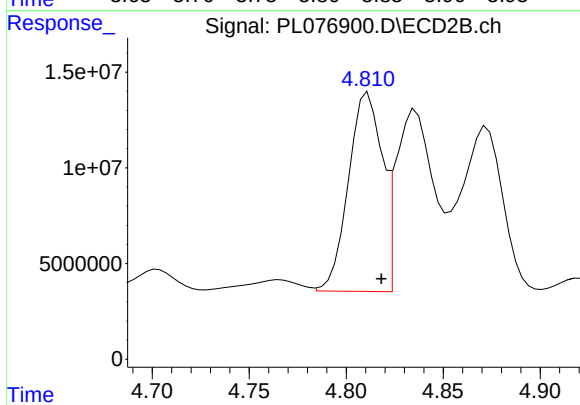

#25 Chlordane-3


R.T.: 4.811 min
Delta R.T.: -0.007 min
Response: 125597322
Conc: 455.44 ng/ml

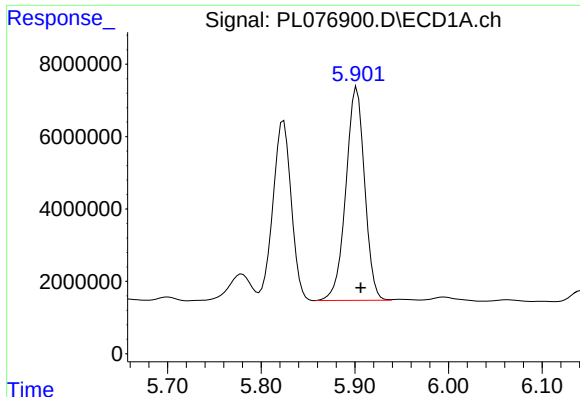

#26 Chlordane-4


R.T.: 5.902 min
Delta R.T.: -0.004 min
Response: 82042163
Conc: 418.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

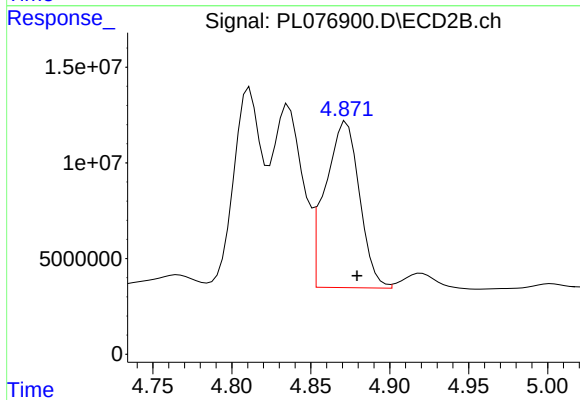


#26 Chlordane-4

R.T.: 4.872 min
Delta R.T.: -0.007 min
Response: 130645920
Conc: 452.90 ng/ml

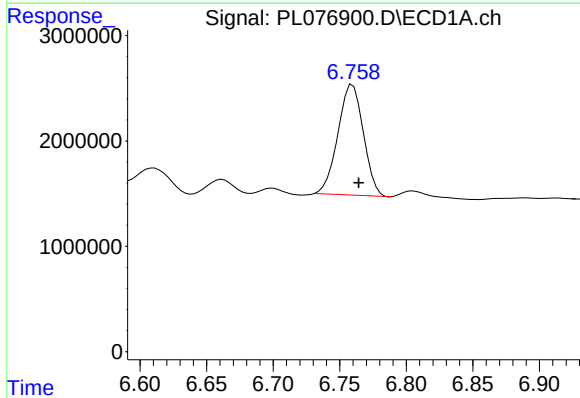


#27 Chlordane-5

R.T.: 6.760 min
Delta R.T.: -0.005 min
Response: 13970281
Conc: 400.49 ng/ml

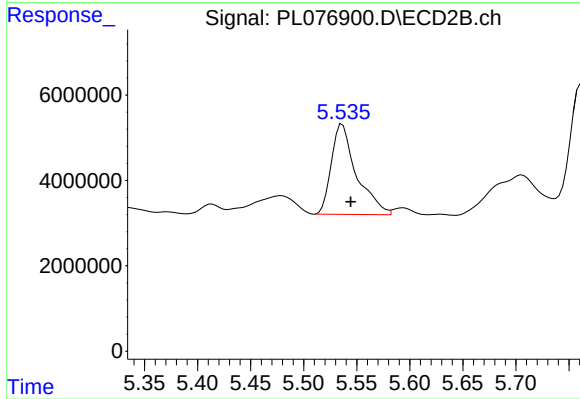

#27 Chlordane-5


R.T.: 5.537 min
Delta R.T.: -0.008 min
Response: 34863467
Conc: 456.75 ng/ml

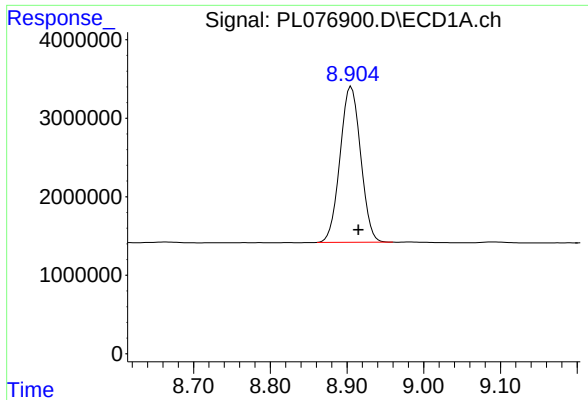

#28 Decachlorobiphenyl

R.T.: 8.905 min
Delta R.T.: -0.009 min
Response: 37208232
Conc: 46.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

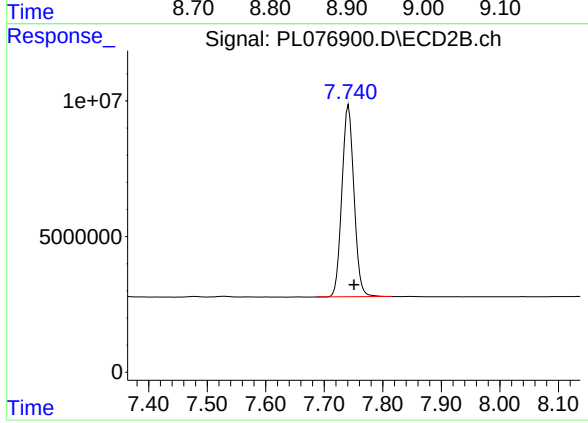

#28 Decachlorobiphenyl

R.T.: 7.742 min
Delta R.T.: -0.009 min
Response: 101436472
Conc: 52.76 ng/ml