

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080423\
 Data File : PL084543.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2023 18:22
 Operator : AR\AJ
 Sample : 03862-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EQUIPMENT-BLANK-1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/07/2023
 Supervised By :Ankita Jodhani 08/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 00:54:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 16:21:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.477	2.687	38442474	18638188	16.545	17.140
2) SA Decachlor...	9.025	7.867	6458077	5237200	3.969m	4.201

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080423\
Data File : PL084543.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2023 18:22
Operator : AR\AJ
Sample : 03862-09
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EQUIPMENT-BLANK-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/07/2023
Supervised By : Ankita Jodhani 08/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 00:54:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 16:21:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

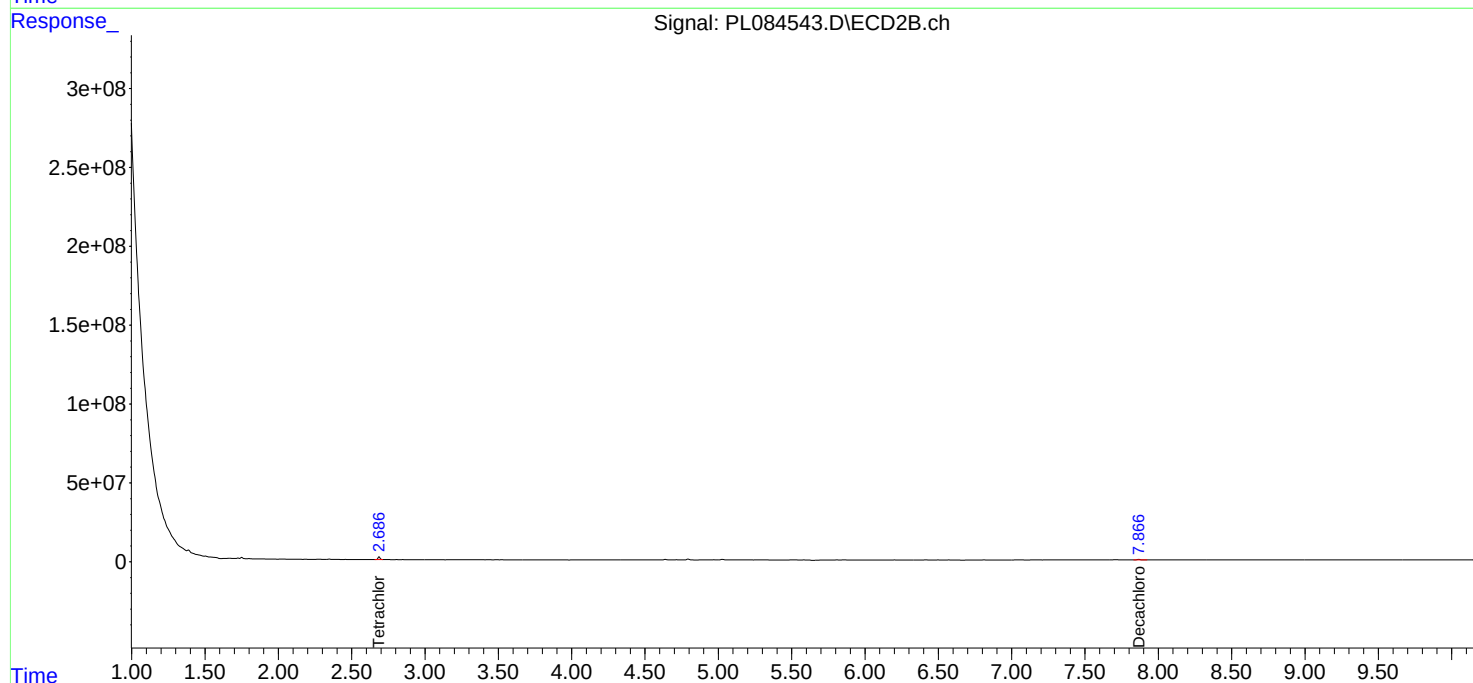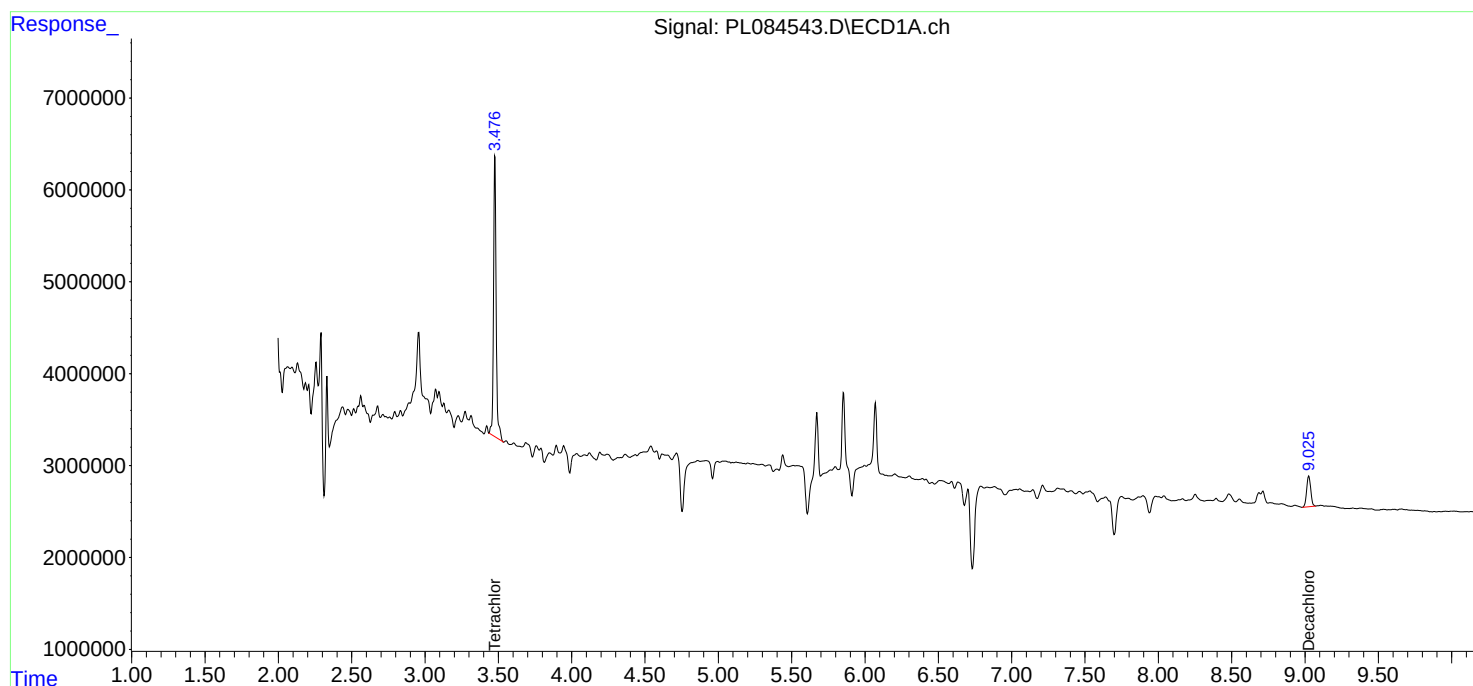

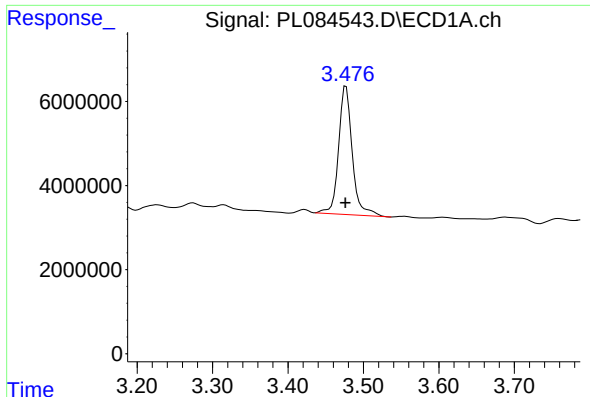


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: 0.000 min
Response: 38442474
Conc: 16.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
EQUIPMENT-BLANK-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/07/2023
Supervised By :Ankita Jodhani 08/07/2023

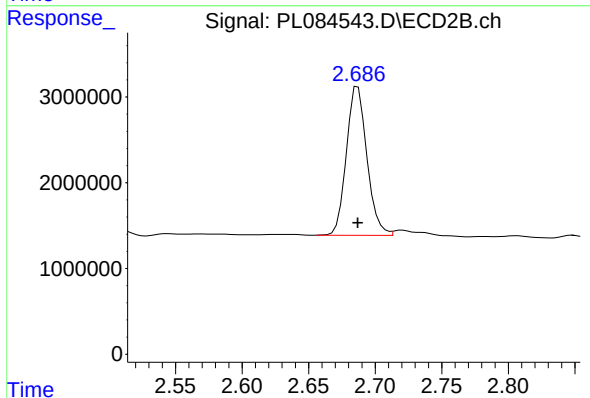


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: 0.000 min
Response: 18638188
Conc: 17.14 ng/ml

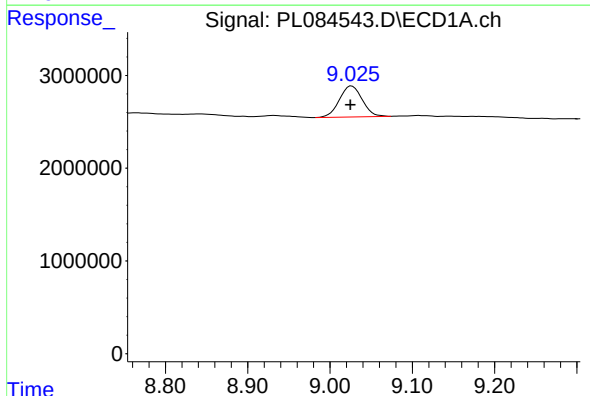

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 6458077
Conc: 3.97 ng/ml m

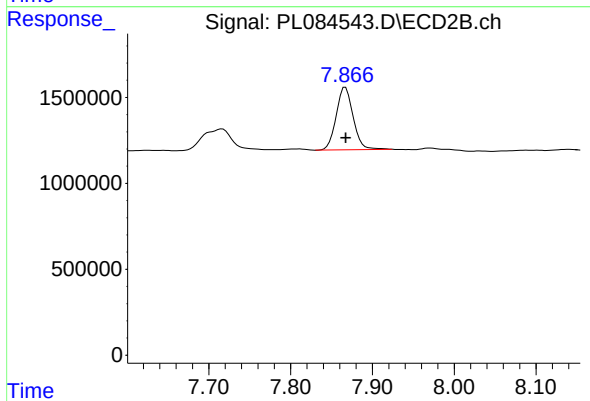

#28 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 5237200
Conc: 4.20 ng/ml