

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080519\
 Data File : PL051076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 03:24
 Operator : SM\AJ
 Sample : K4135-26
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 1S-A1-A4-COMP-(30)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 03:56:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.928	234.7E6	65374188	23.363	22.913
28)	SA Decachlor...	7.978	8.956	227.5E6	60702712	22.471	21.466
Target Compounds							
6)	B beta-BHC	0.000	4.802f	0	3062260	N.D.	1.771 #
11)	B alpha-Chl...	5.264	0.000	10488347	0	0.687	N.D. #
15)	B Endosulfa...	0.000	6.848	0	1012918	N.D.	0.319 #
26)	Chlordane-4	5.264	0.000	10488347	0	7.952	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080519\
Data File : PL051076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 03:24
Operator : SM\AJ
Sample : K4135-26
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
1S-A1-A4-COMP-(30)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 03:56:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

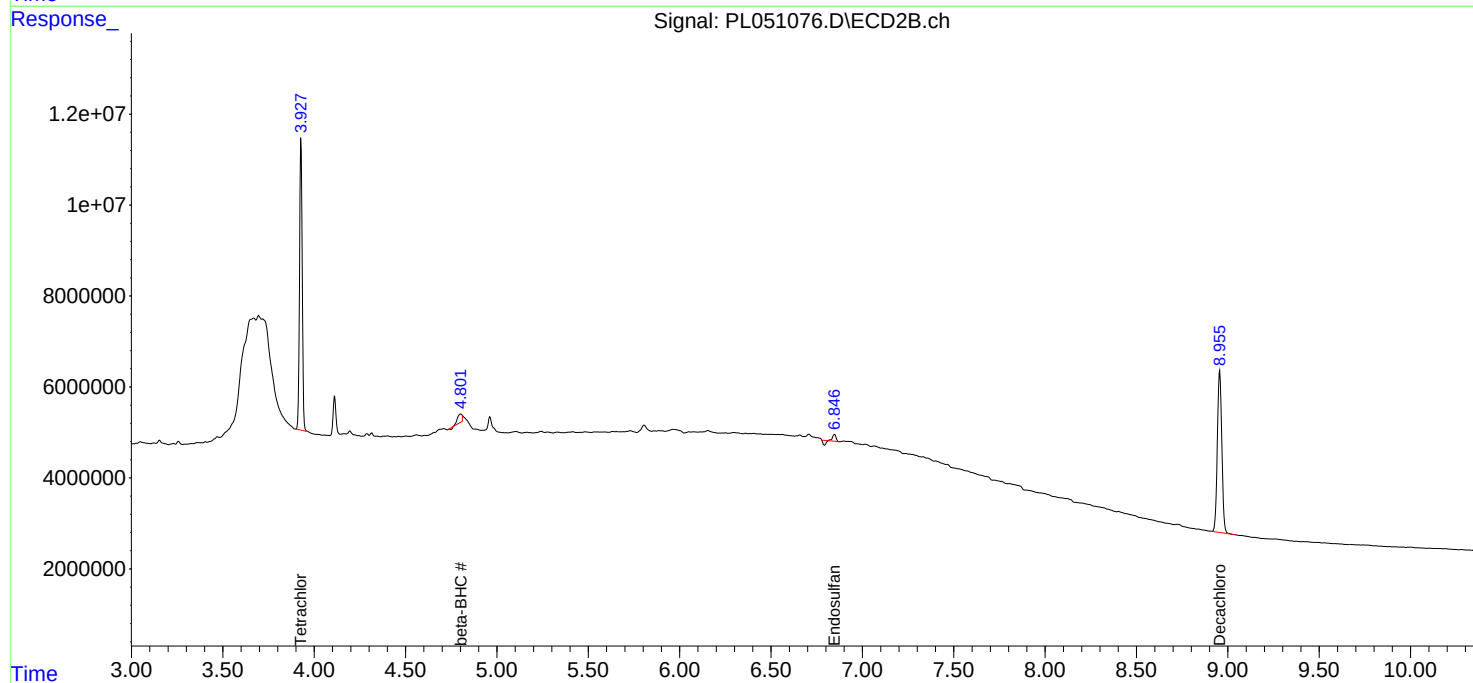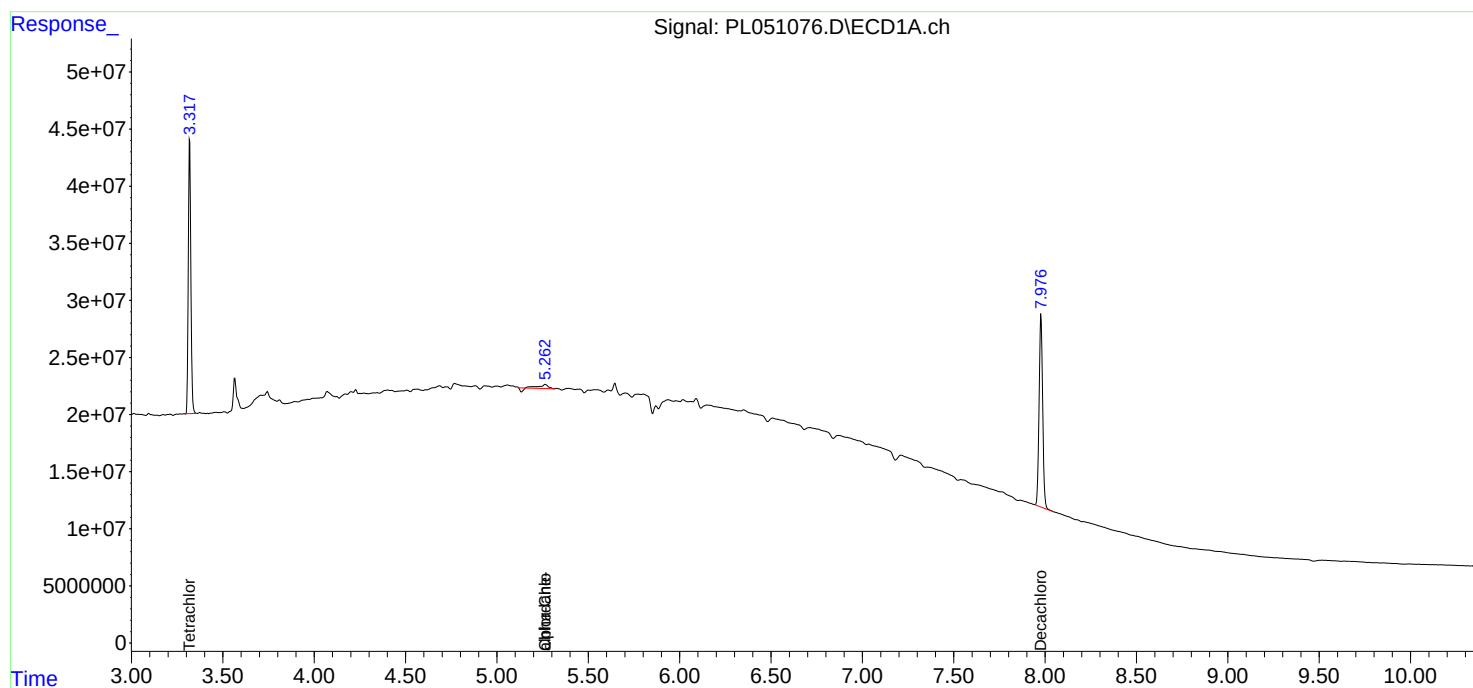


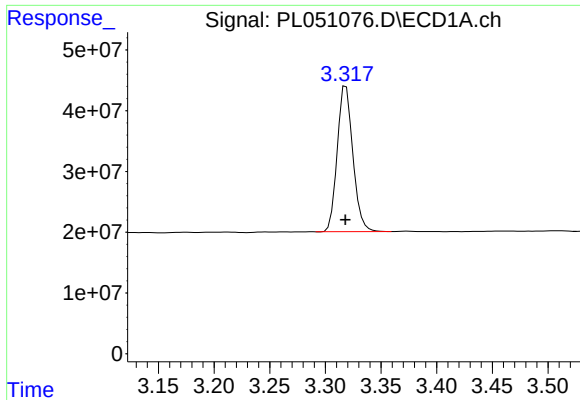

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 234743651
Conc: 23.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
1S-A1-A4-COMP-(30)

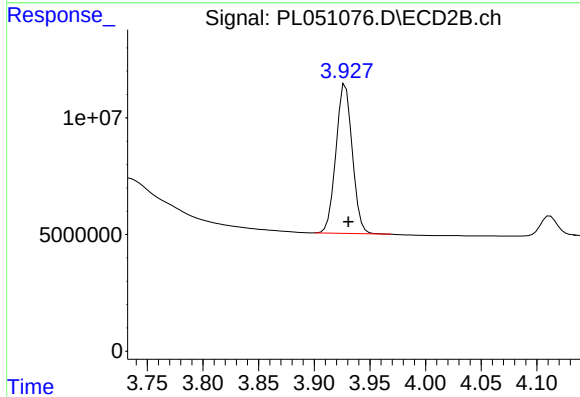


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.003 min
Response: 65374188
Conc: 22.91 ng/ml

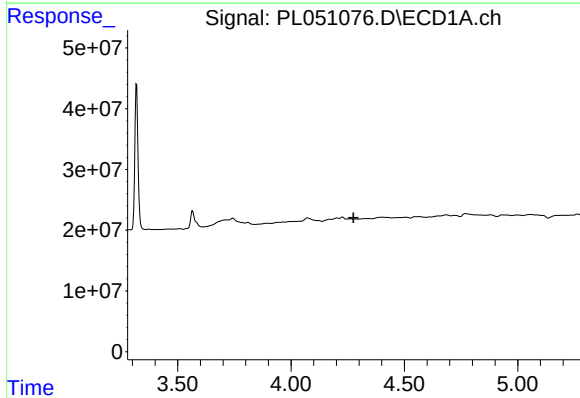


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

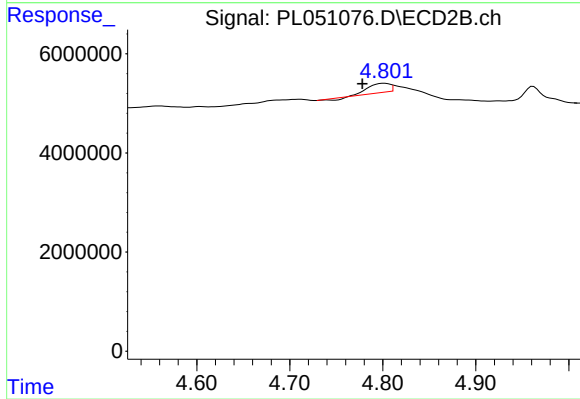

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.024 min
Response: 3062260
Conc: 1.77 ng/ml

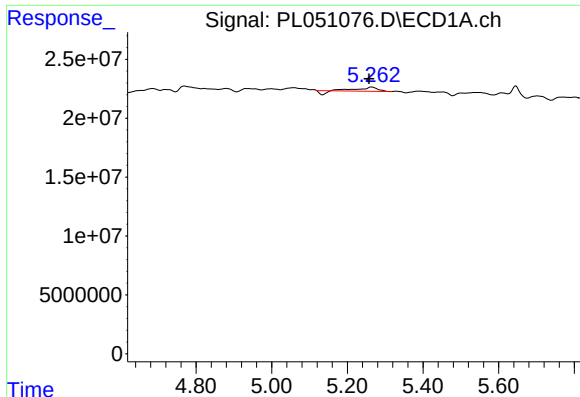

#11 alpha-Chlordane


R.T.: 5.264 min
Delta R.T.: 0.007 min
Response: 10488347
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
1S-A1-A4-COMP-(30)

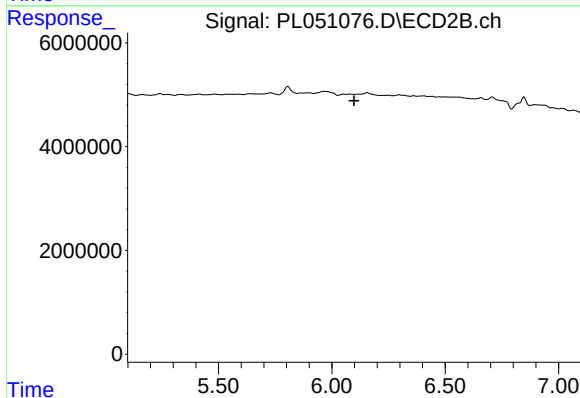


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

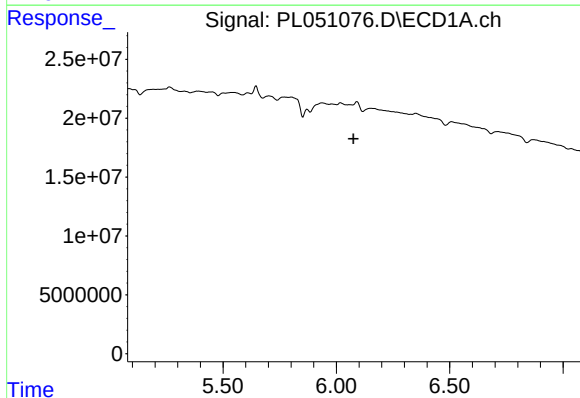


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

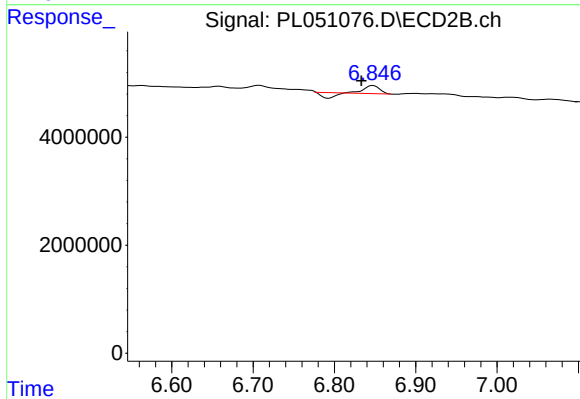

#15 Endosulfan II


R.T.: 6.848 min
Delta R.T.: 0.015 min
Response: 1012918
Conc: 0.32 ng/ml

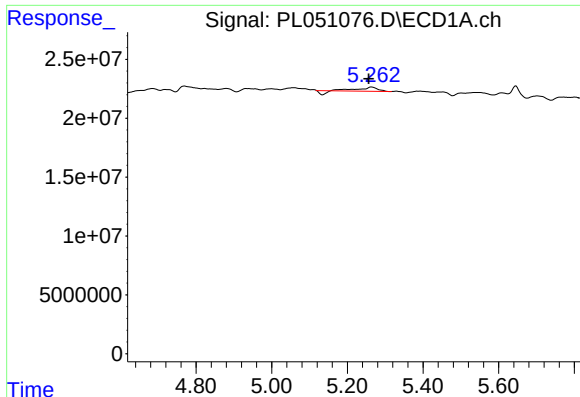

#26 Chlordane-4


R.T.: 5.264 min
Delta R.T.: 0.007 min
Response: 10488347
Conc: 7.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
1S-A1-A4-COMP-(30)

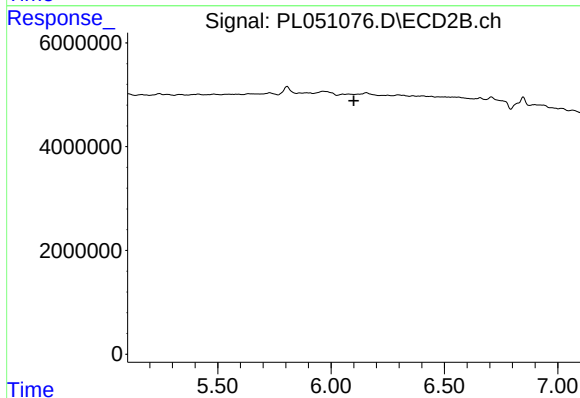


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

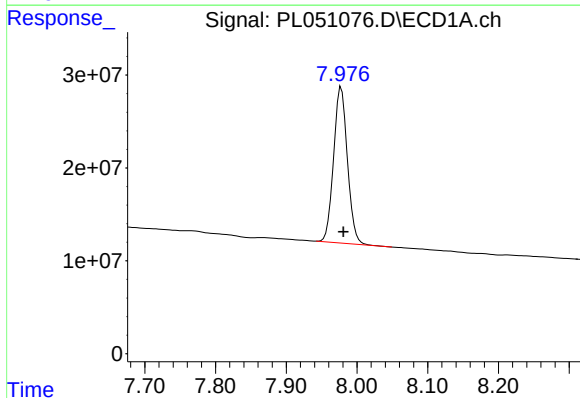

#28 Decachlorobiphenyl

R.T.: 7.978 min
Delta R.T.: -0.003 min
Response: 227522852
Conc: 22.47 ng/ml

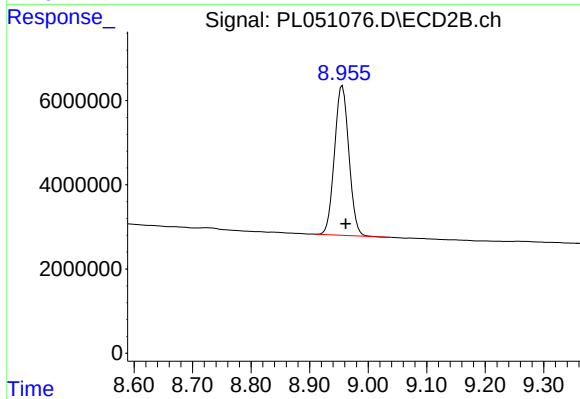

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: -0.006 min
Response: 60702712
Conc: 21.47 ng/ml