

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080519\
 Data File : PL051037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2019 17:35
 Operator : SM\AJ
 Sample : K4156-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RT1494

Manual Integrations
 APPROVED

Ankita
 8/7/2019 4:17:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 00:51:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.929	223.4E6	57435675	22.232	20.130
28)	SA Decachlor...	7.979	8.957	182.9E6	50128017	18.063	17.726
Target Compounds							
10)	B gamma-Chl...	5.200	6.017	8961560	5614627	0.568m	1.519m#
11)	B alpha-Chl...	5.255	6.095	20452833	5169538	1.341m	1.410

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080519\
Data File : PL051037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2019 17:35
Operator : SM\AJ
Sample : K4156-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
RT1494


Manual Integrations
APPROVED

Ankita
8/7/2019 4:17:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 00:51:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

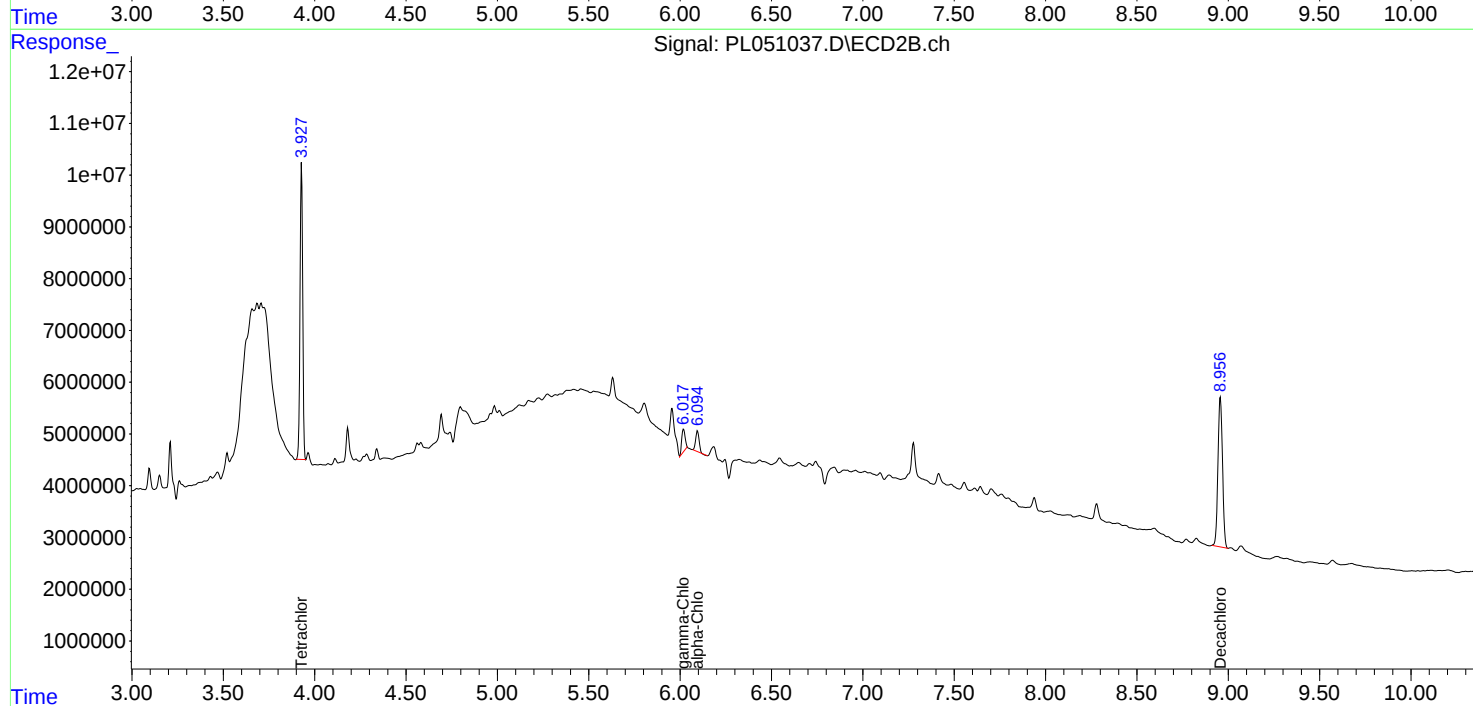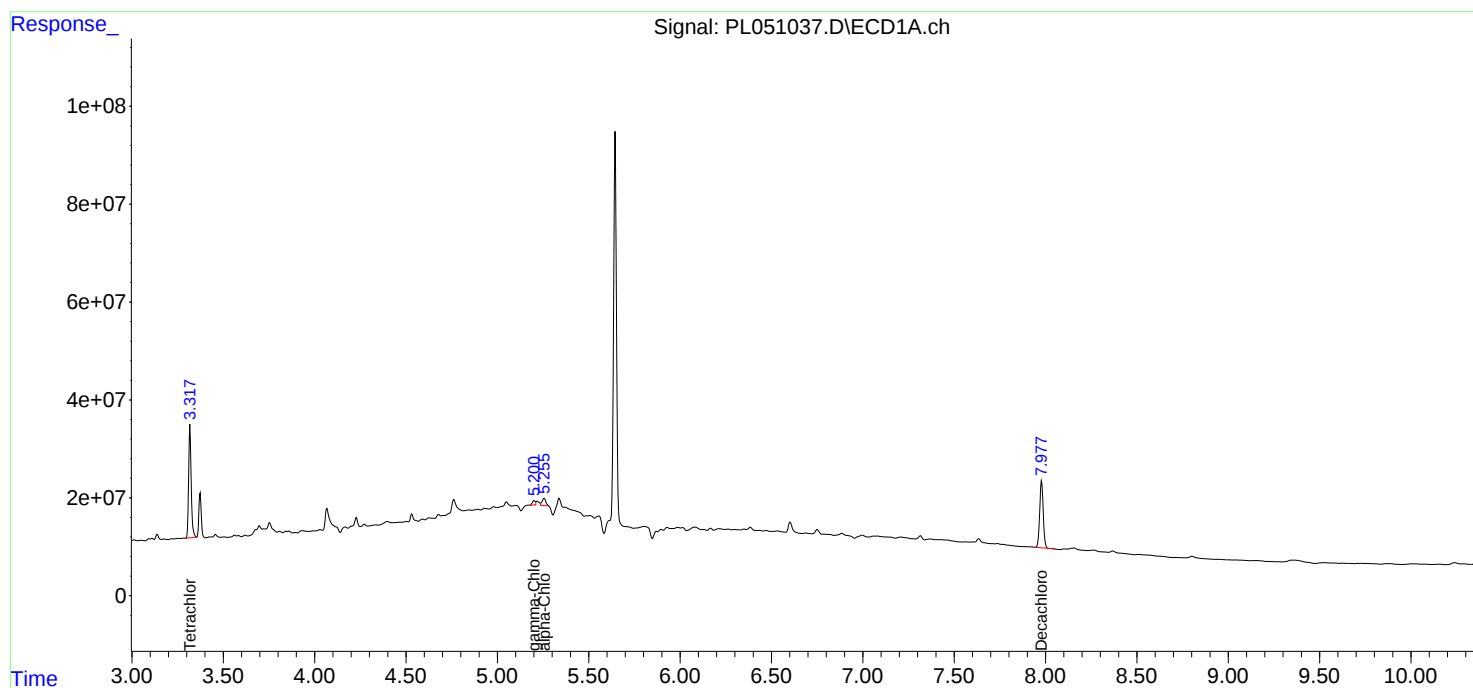

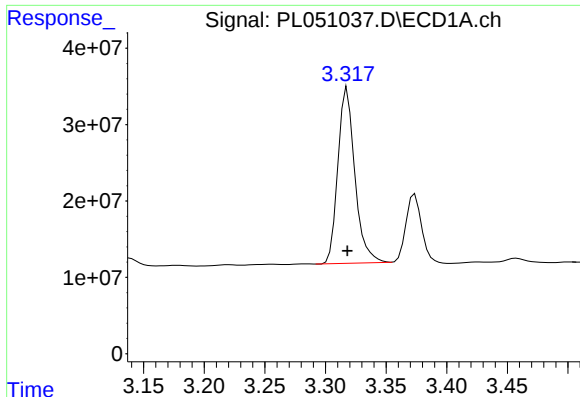


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 223383021
Conc: 22.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT1494


Manual Integrations
APPROVED

Ankita
8/7/2019 4:17:19 PM

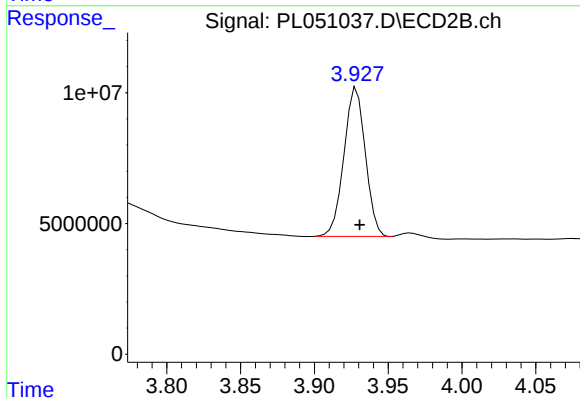


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 57435675
Conc: 20.13 ng/ml

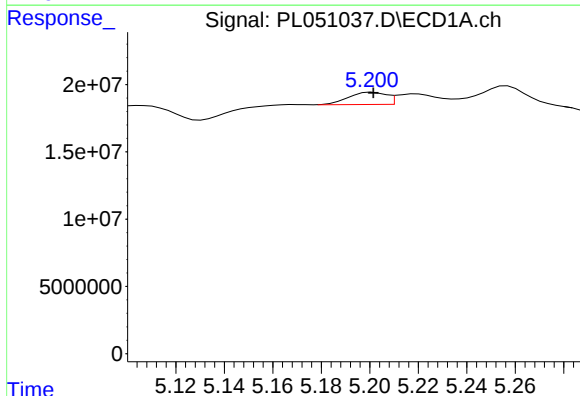


#10 gamma-Chlordane

R.T.: 5.200 min
Delta R.T.: -0.002 min
Response: 8961560
Conc: 0.57 ng/ml m

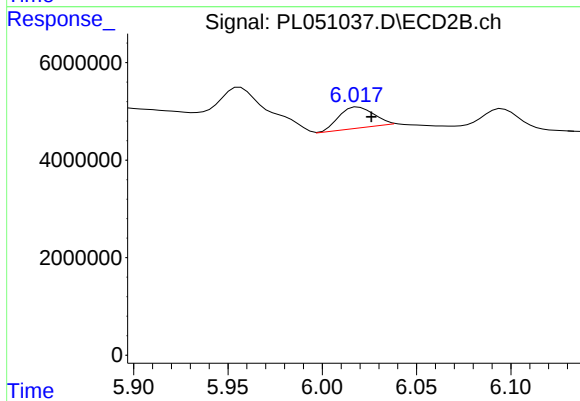

#10 gamma-Chlordane

R.T.: 6.017 min
Delta R.T.: -0.009 min
Response: 5614627
Conc: 1.52 ng/ml m

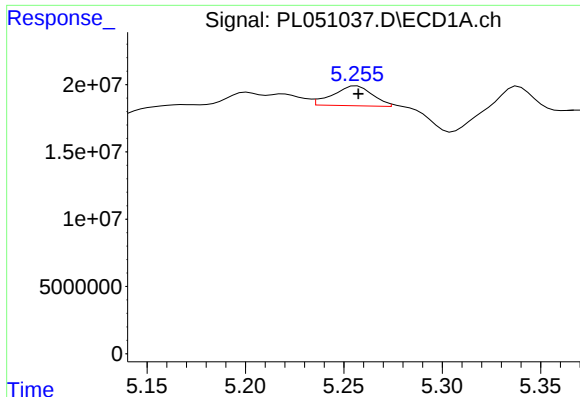


#11 alpha-Chlordane

R.T.: 5.255 min
Delta R.T.: -0.002 min
Response: 20452833
Conc: 1.34 ng/ml m

Instrument :
ECD_L
ClientSampleId :
RT1494


Manual Integrations
APPROVED

Ankita
8/7/2019 4:17:19 PM

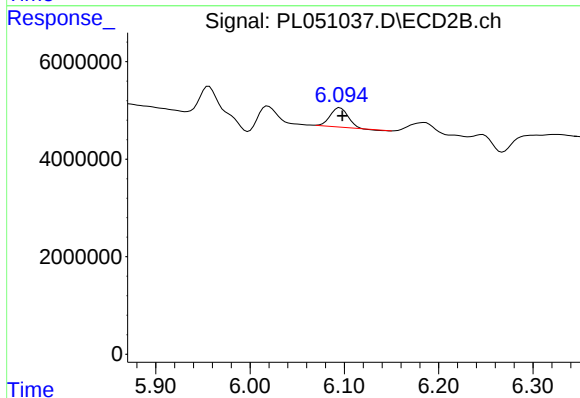


#11 alpha-Chlordane

R.T.: 6.095 min
Delta R.T.: -0.002 min
Response: 5169538
Conc: 1.41 ng/ml

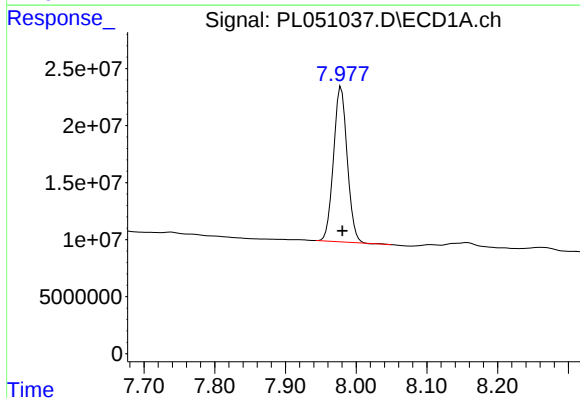

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.002 min
Response: 182890517
Conc: 18.06 ng/ml

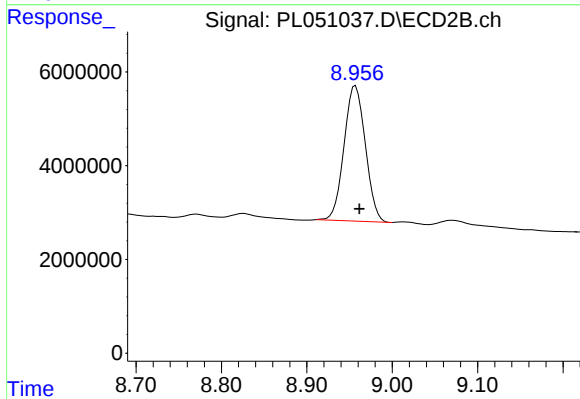

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.005 min
Response: 50128017
Conc: 17.73 ng/ml