

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080519\
 Data File : PL051041.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2019 18:36
 Operator : SM\AJ
 Sample : K4158-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-055

Manual Integrations
 APPROVED

Ankita
 8/6/2019 3:14:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 00:53:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.929	149.4E6	40488251	14.873	14.190
28)	SA Decachlor...	7.979	8.958	74901746	20468938	7.397	7.238
Target Compounds							
10)	B gamma-Chl...	5.200	6.023	18893934	4588771	1.197m	1.242
11)	B alpha-Chl...	5.256	6.097	21817371	7774659	1.430	2.121 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080519\
Data File : PL051041.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2019 18:36
Operator : SM\AJ
Sample : K4158-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-PS-01-055


Manual Integrations
APPROVED

Ankita
8/6/2019 3:14:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 00:53:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

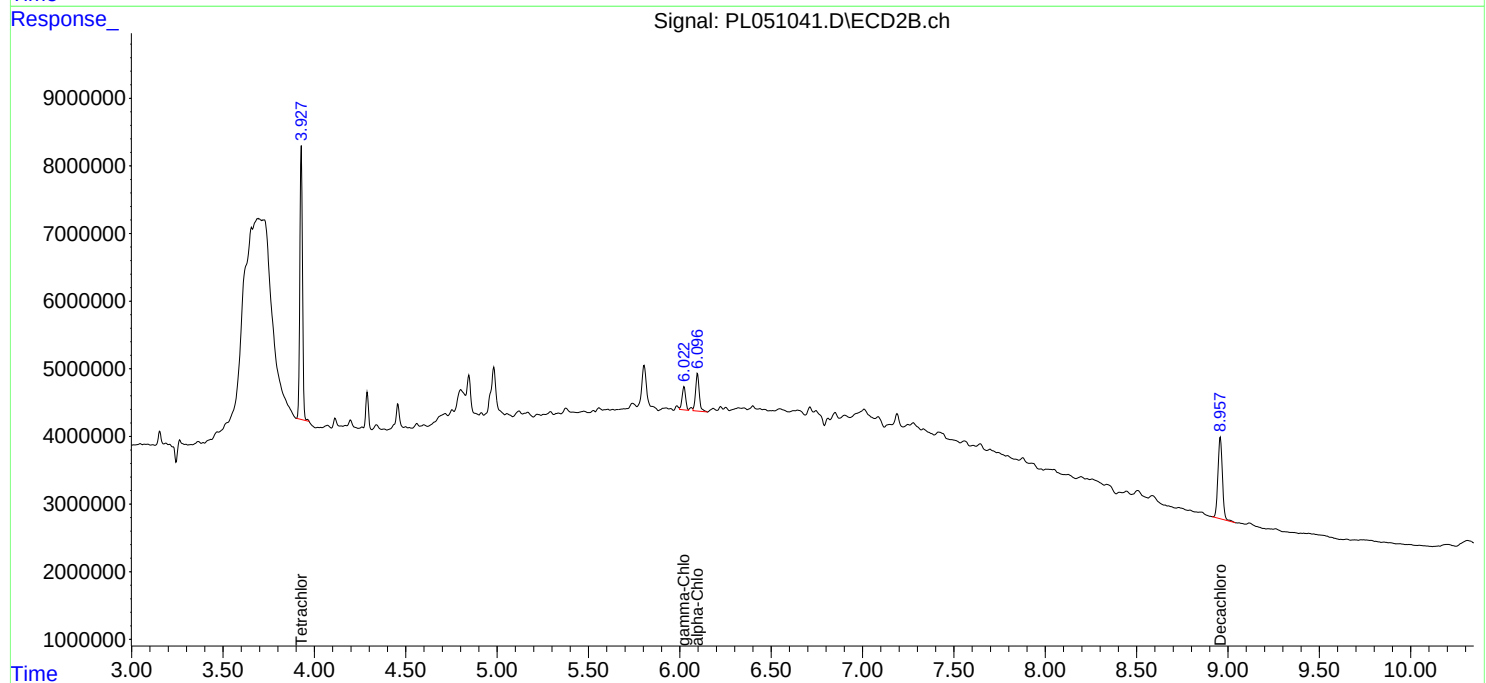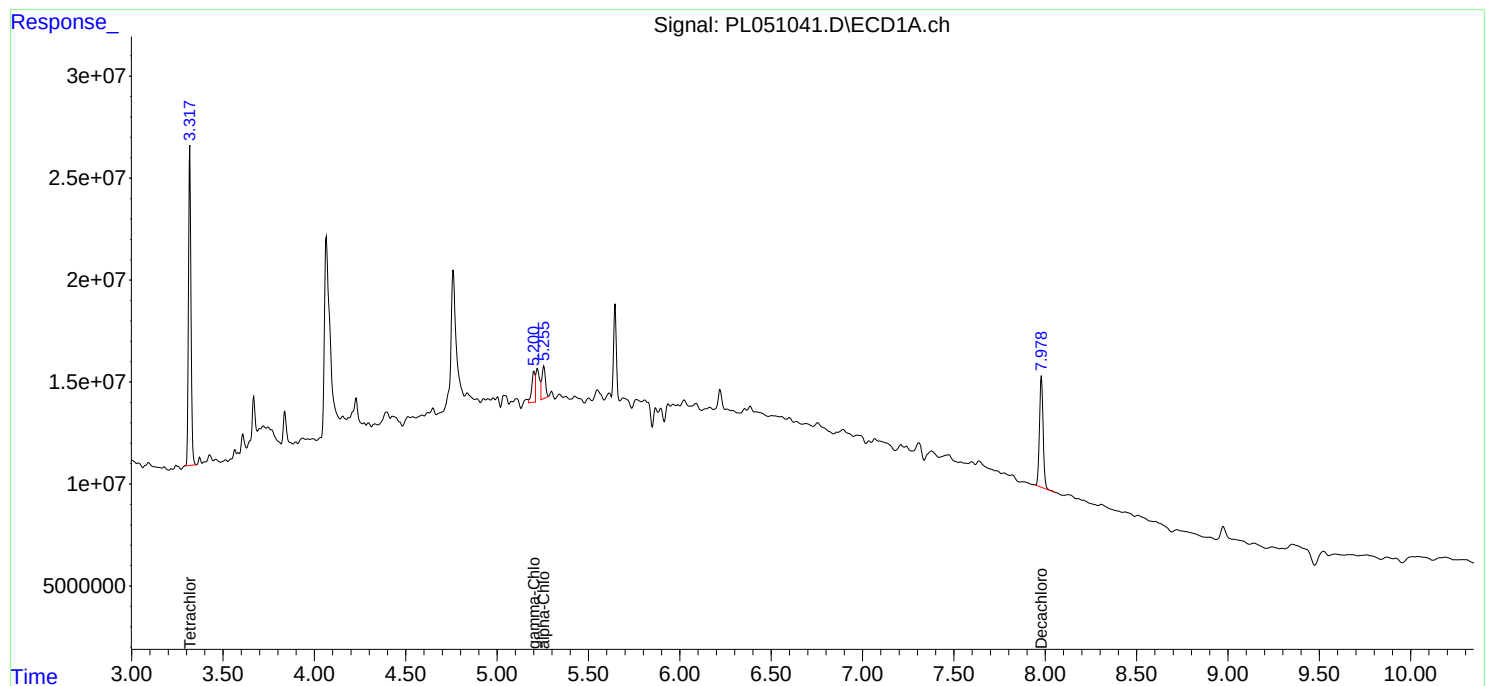

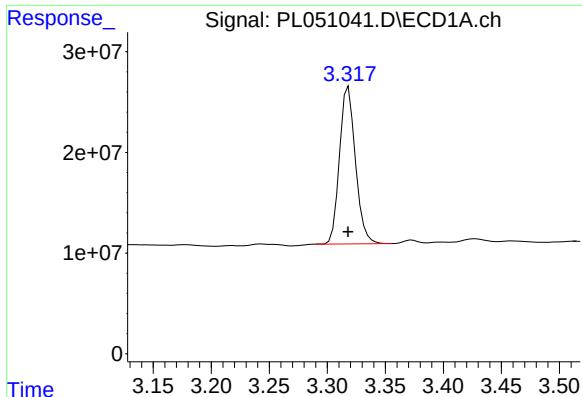


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 149443892
Conc: 14.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-055


Manual Integrations
APPROVED

Ankita
8/6/2019 3:14:58 PM

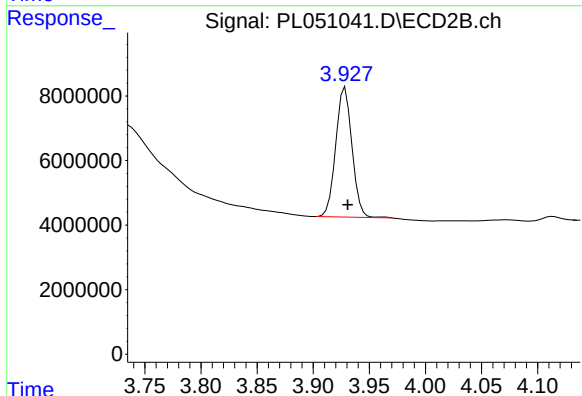


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 40488251
Conc: 14.19 ng/ml

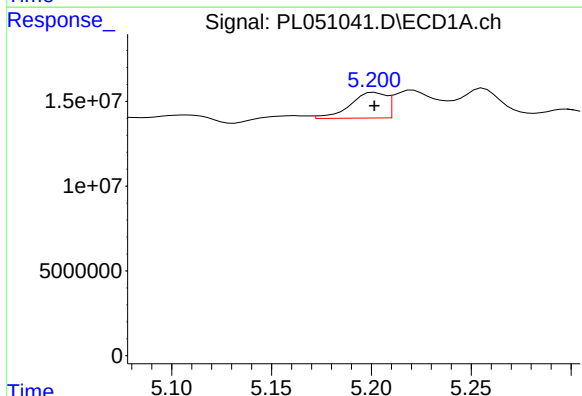


#10 gamma-Chlordane

R.T.: 5.200 min
Delta R.T.: -0.002 min
Response: 18893934
Conc: 1.20 ng/ml m

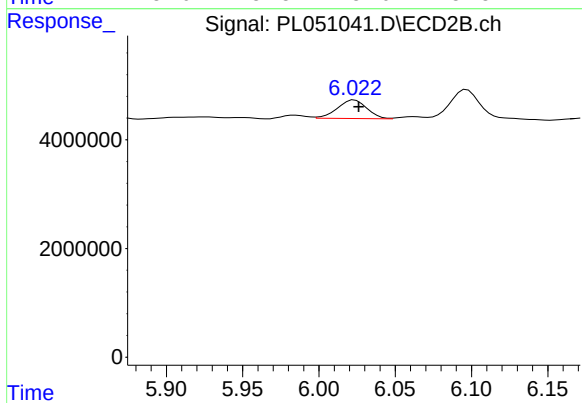

#10 gamma-Chlordane

R.T.: 6.023 min
Delta R.T.: -0.003 min
Response: 4588771
Conc: 1.24 ng/ml

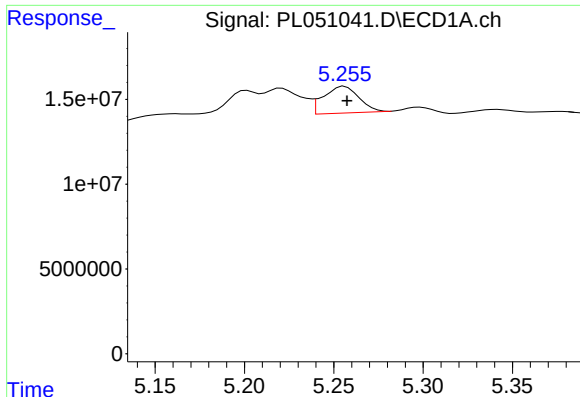


#11 alpha-Chlordane

R.T.: 5.256 min
Delta R.T.: -0.001 min
Response: 21817371
Conc: 1.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-055


Manual Integrations
APPROVED

Ankita
8/6/2019 3:14:58 PM

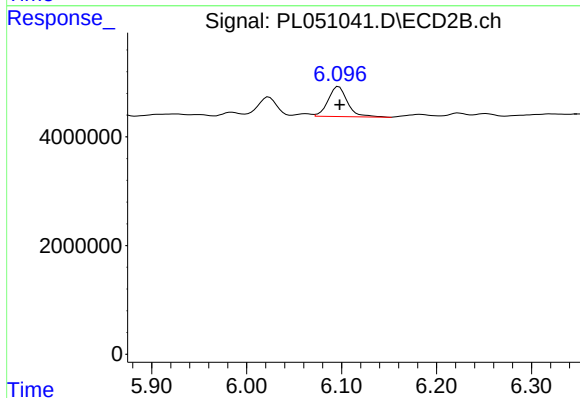


#11 alpha-Chlordane

R.T.: 6.097 min
Delta R.T.: 0.000 min
Response: 7774659
Conc: 2.12 ng/ml

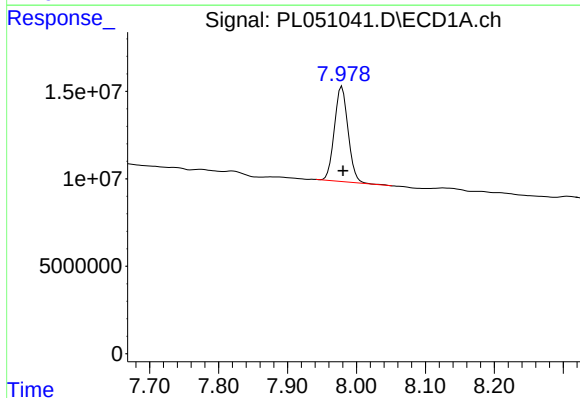

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.002 min
Response: 74901746
Conc: 7.40 ng/ml

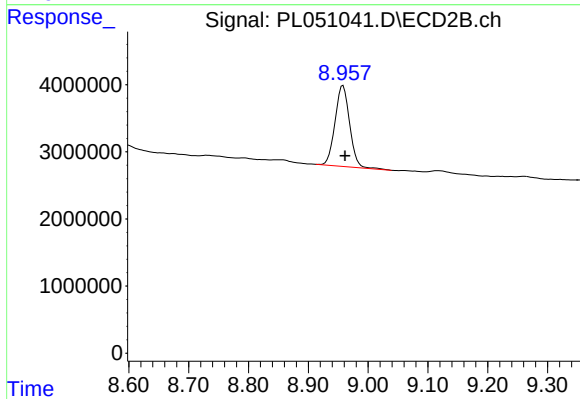

#28 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.004 min
Response: 20468938
Conc: 7.24 ng/ml