

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080521\
 Data File : PL068697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2021 09:39
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 03:05:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	8.041	0	424144	N.D. 0.367 #
9) A	Endosulfan I	0.000	8.455f	0	59773	N.D. 0.057 #
10) B	gamma-Chl...	0.000	8.294	0	237755	N.D. 0.208 #
11) B	alpha-Chl...	0.000	8.412f	0	244250	N.D. 0.213 #
15) B	Endosulfa...	8.348f	9.219f	1479755	293949	3.085 0.320 #
17) MA	4,4'-DDT	0.000	9.404f	0	226215	N.D. 0.239 #
21) B	Endrin ke...	0.000	10.095f	0	103328	N.D. 0.101 #
25)	Chlordane-3	0.000	8.294	0	237755	N.D. 1.455 #
26)	Chlordane-4	0.000	8.412f	0	244250	N.D. 1.232 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080521\
Data File : PL068697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2021 09:39
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 03:05:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

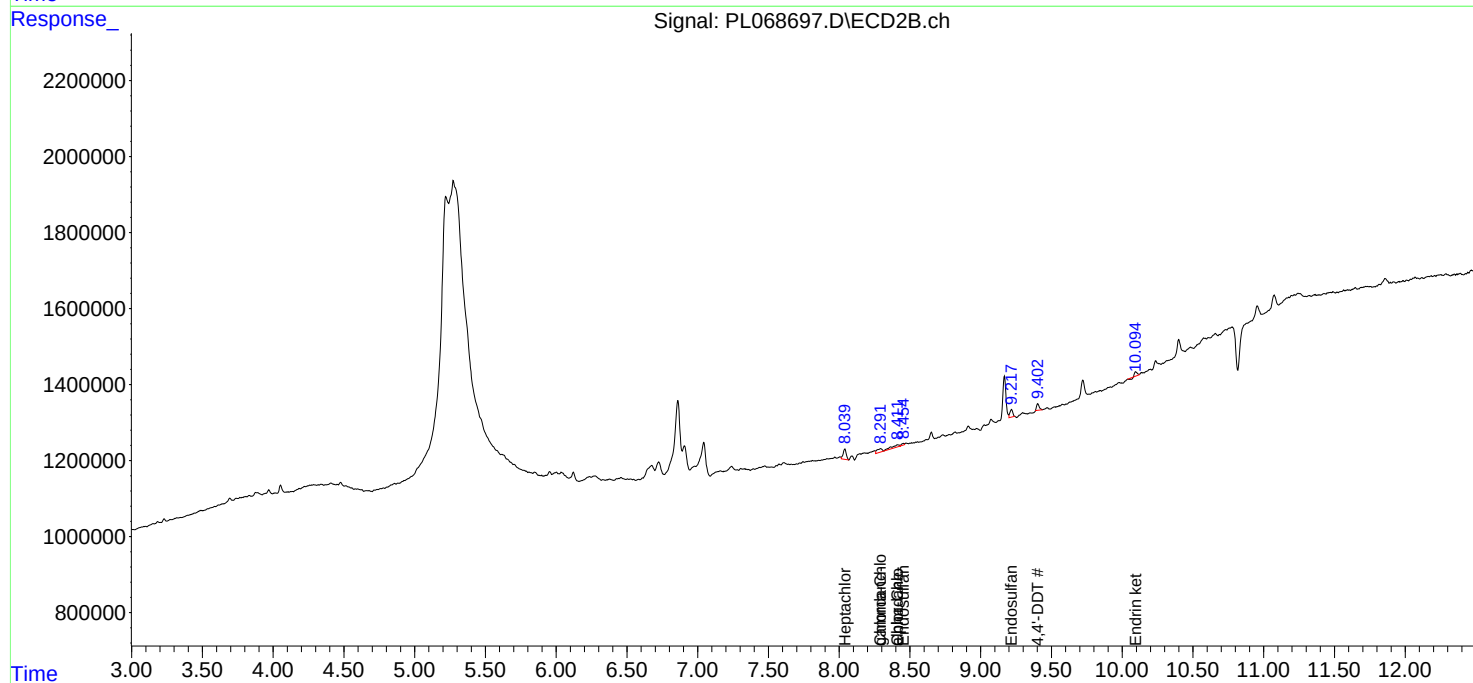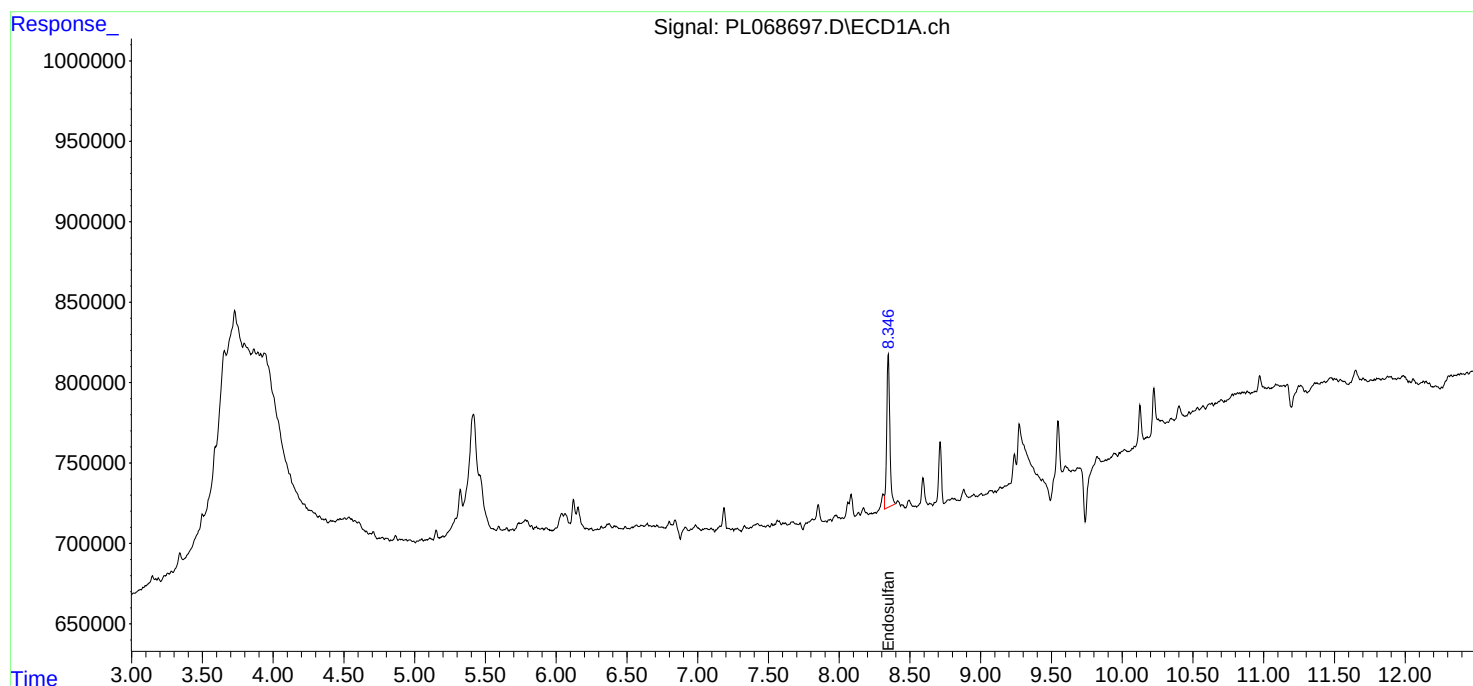


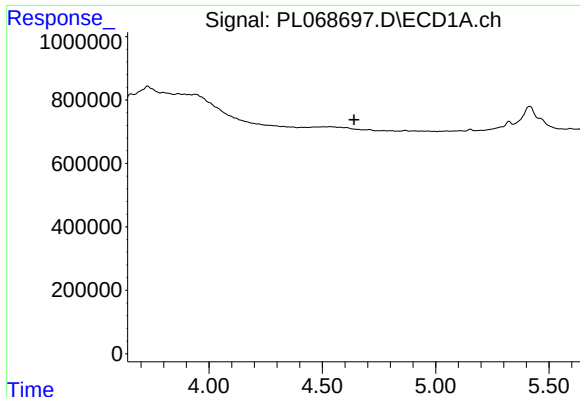

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

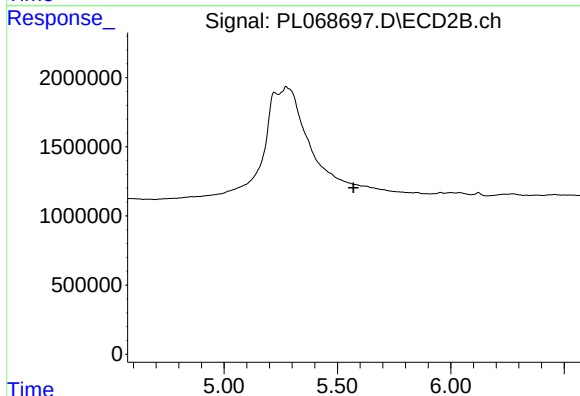


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.571 min
Response: 0
Conc: N.D.

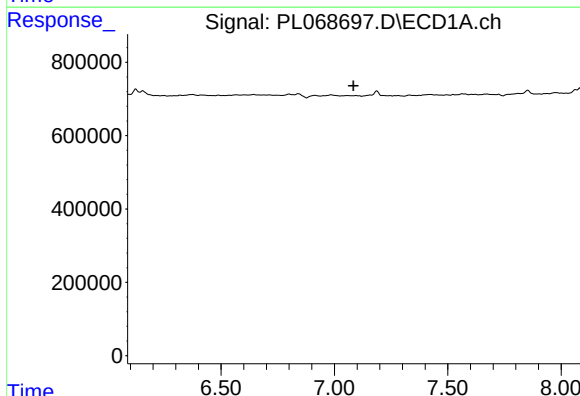


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

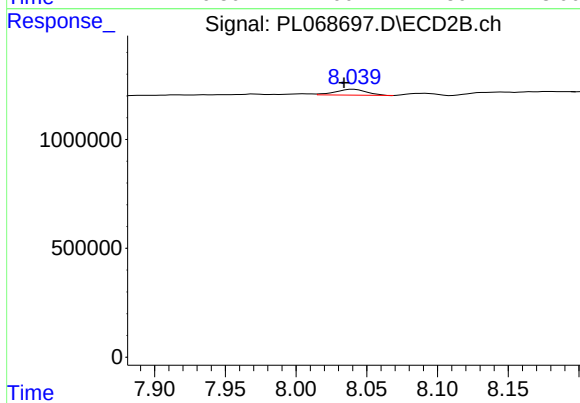

#8 Heptachlor epoxide


R.T.: 8.041 min
Delta R.T.: 0.007 min
Response: 424144
Conc: 0.37 ng/ml

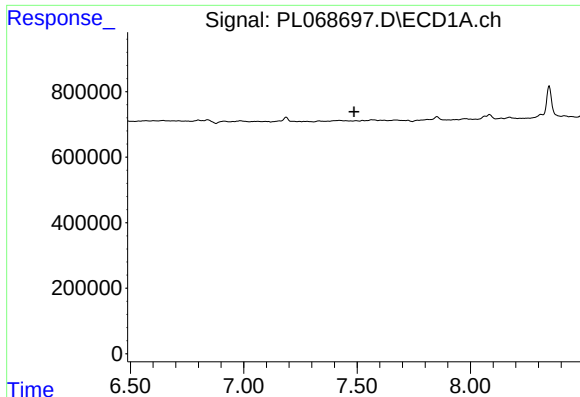

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

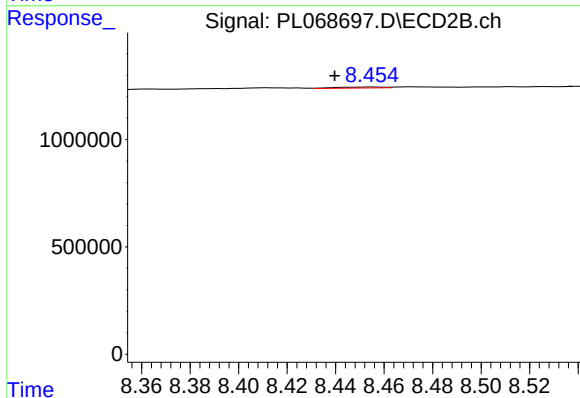


#9 Endosulfan I

R.T.: 8.455 min
Delta R.T.: 0.016 min
Response: 59773
Conc: 0.06 ng/ml

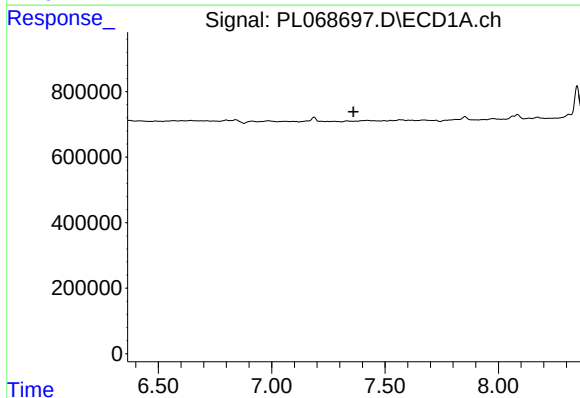


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.361 min
Response: 0
Conc: N.D.

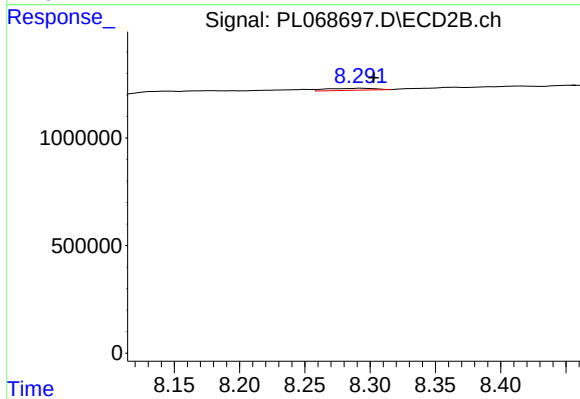

#10 gamma-Chlordane


R.T.: 8.294 min
Delta R.T.: -0.009 min
Response: 237755
Conc: 0.21 ng/ml

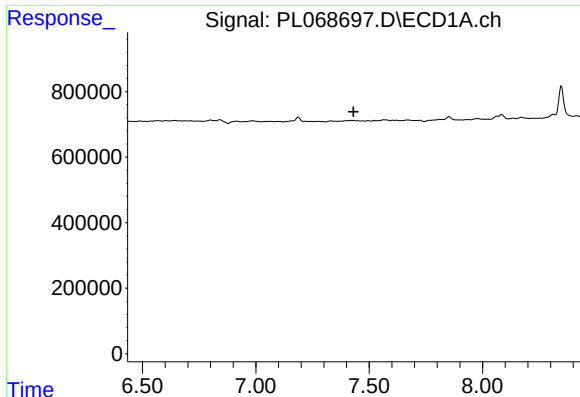

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

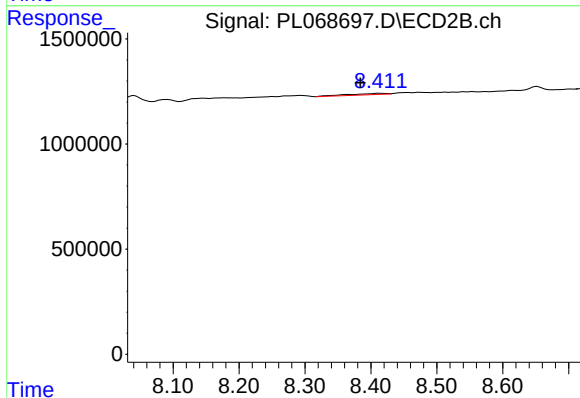


#11 alpha-Chlordane

R.T.: 8.412 min
Delta R.T.: 0.028 min
Response: 244250
Conc: 0.21 ng/ml

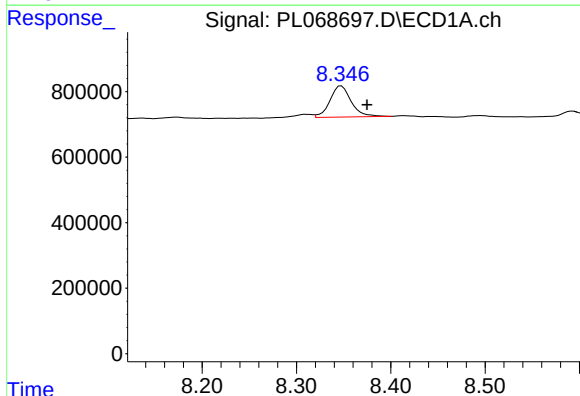


#15 Endosulfan II

R.T.: 8.348 min
Delta R.T.: -0.027 min
Response: 1479755
Conc: 3.08 ng/ml

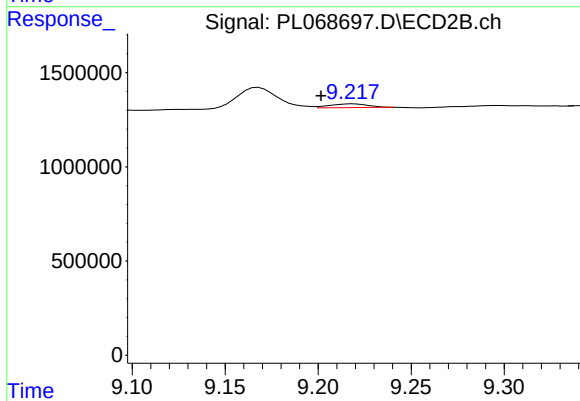

#15 Endosulfan II


R.T.: 9.219 min
Delta R.T.: 0.017 min
Response: 293949
Conc: 0.32 ng/ml

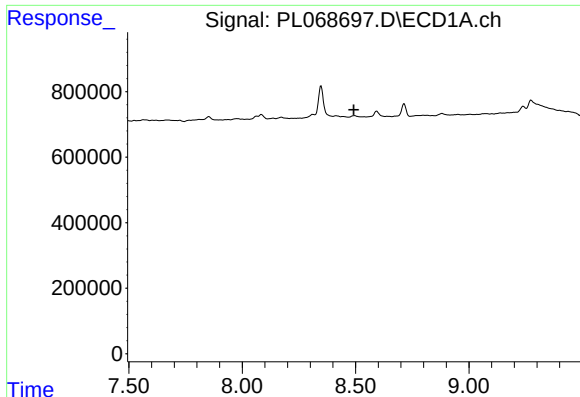

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

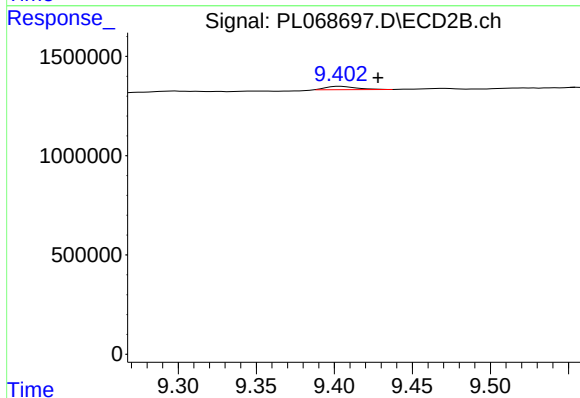


#17 4,4'-DDT

R.T.: 9.404 min
Delta R.T.: -0.024 min
Response: 226215
Conc: 0.24 ng/ml

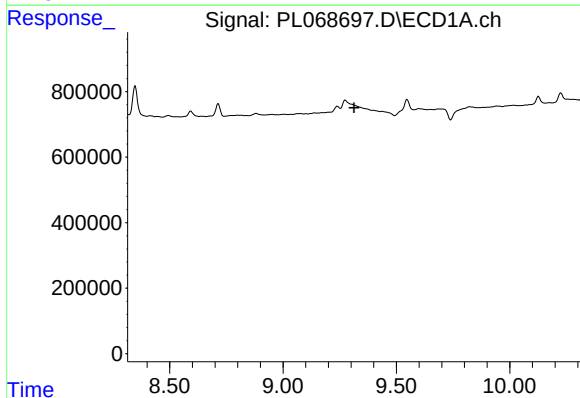


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.313 min
Response: 0
Conc: N.D.

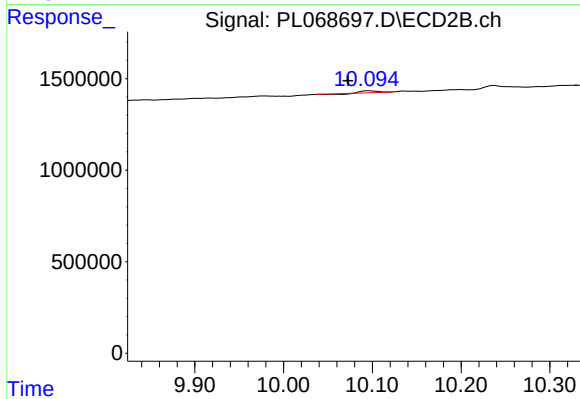

#21 Endrin ketone


R.T.: 10.095 min
Delta R.T.: 0.023 min
Response: 103328
Conc: 0.10 ng/ml

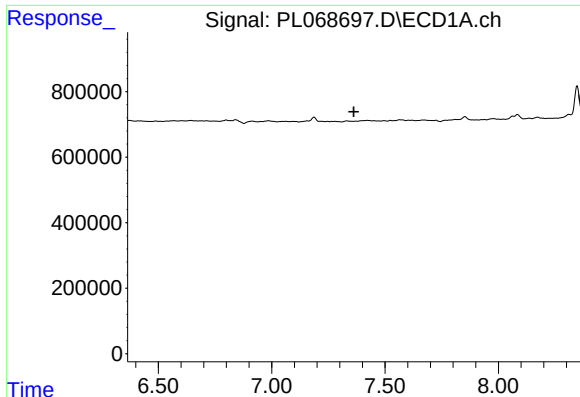

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

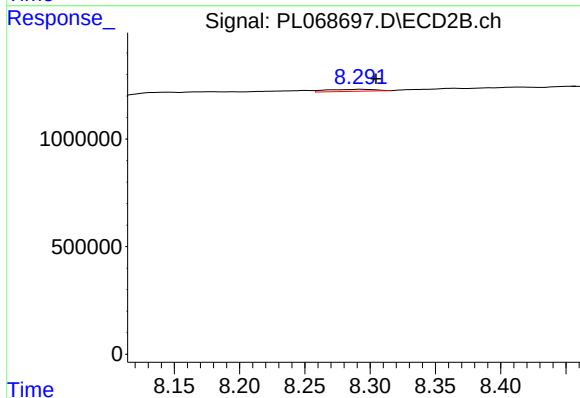


#25 Chlordane-3

R.T.: 8.294 min
Delta R.T.: -0.011 min
Response: 237755
Conc: 1.46 ng/ml

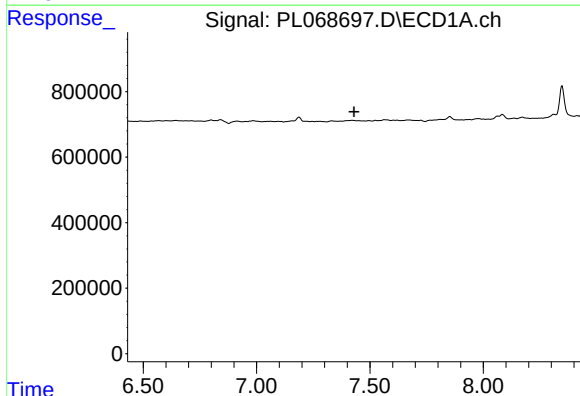


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

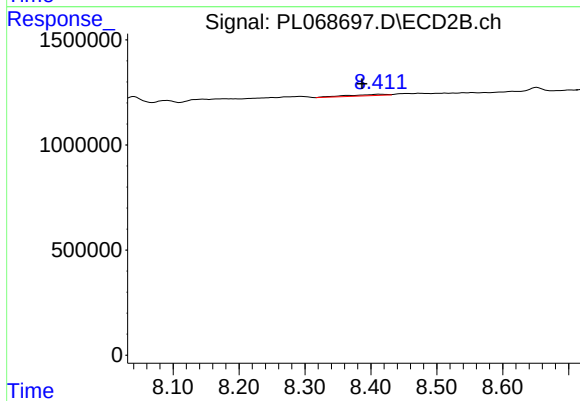

#26 Chlordane-4


R.T.: 8.412 min
Delta R.T.: 0.026 min
Response: 244250
Conc: 1.23 ng/ml

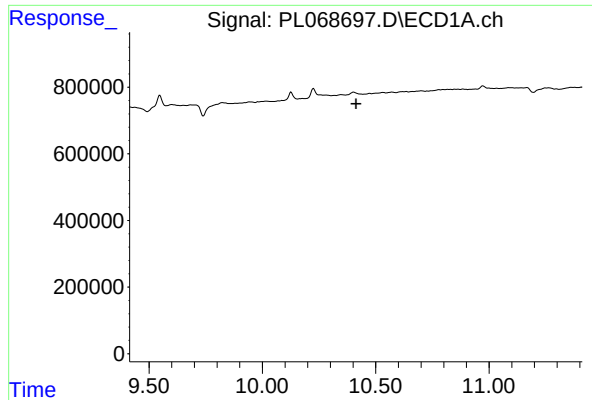

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

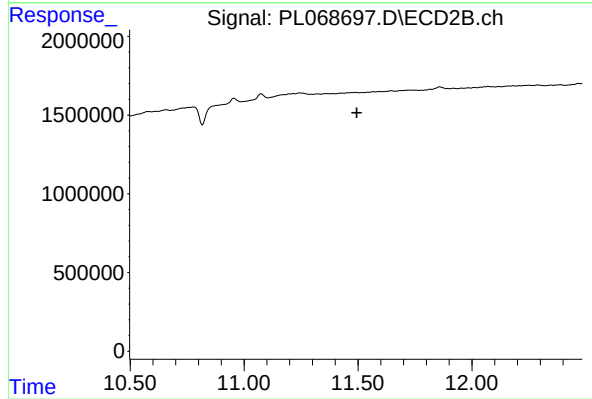

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.