

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080521\
 Data File : PL068719.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2021 15:45
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 03:07:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.572	8243883	20942315	19.930	20.626
28)	SA Decachlor...	10.414	11.496	12083303	20294396	21.026	20.917
Target Compounds							
4)	MA Heptachlor	6.159f	0.000	376909	0	0.642	N.D. #
6)	B beta-BHC	6.159	0.000	376909	0	1.337	N.D. #
10)	B gamma-Chl...	0.000	8.277f	0	95740	N.D.	0.084 #
11)	B alpha-Chl...	0.000	8.409f	0	67496	N.D.	0.059 #
15)	B Endosulfa...	0.000	9.220f	0	291339	N.D.	0.318 #
21)	B Endrin ke...	0.000	10.096f	0	178431	N.D.	0.175 #
22)	Mirex	0.000	10.567f	0	132426	N.D.	0.167 #
25)	Chlordane-3	0.000	8.277f	0	95740	N.D.	0.586 #
26)	Chlordane-4	0.000	8.409f	0	67496	N.D.	0.340 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080521\
Data File : PL068719.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2021 15:45
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 03:07:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

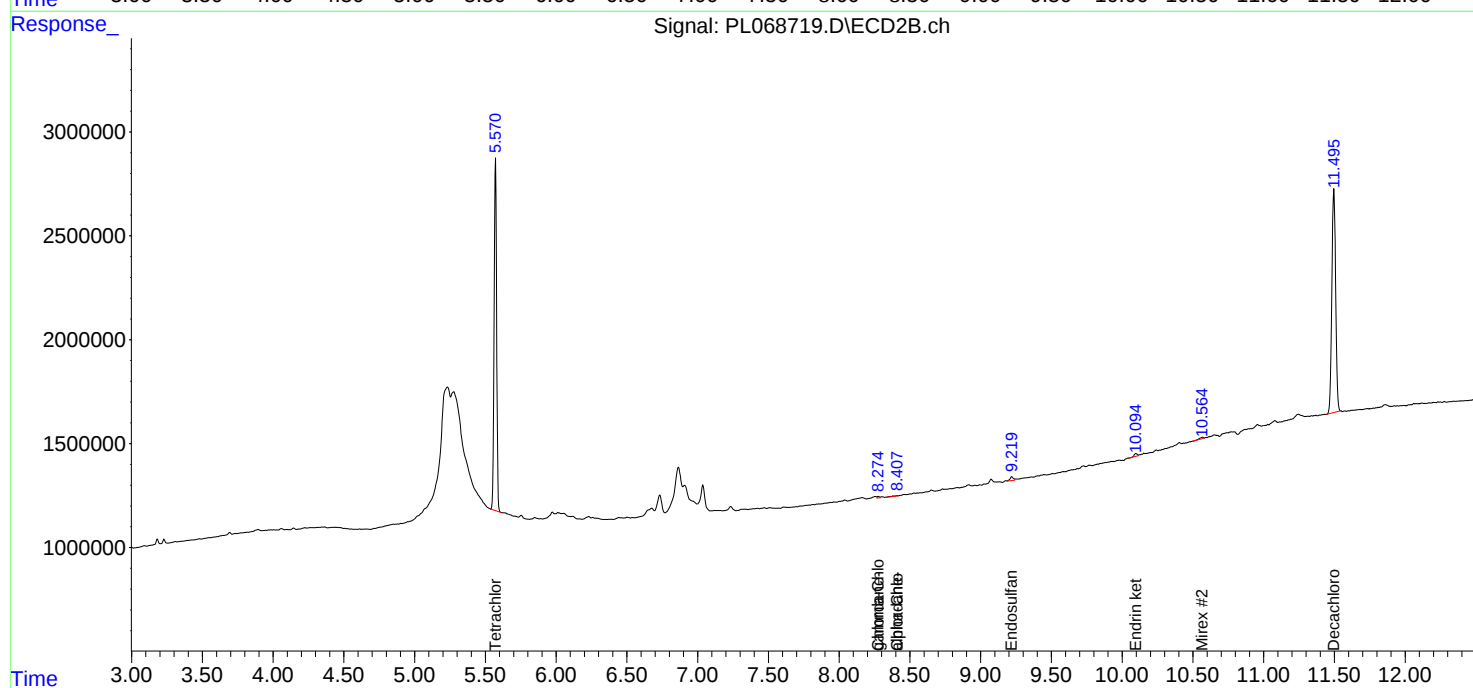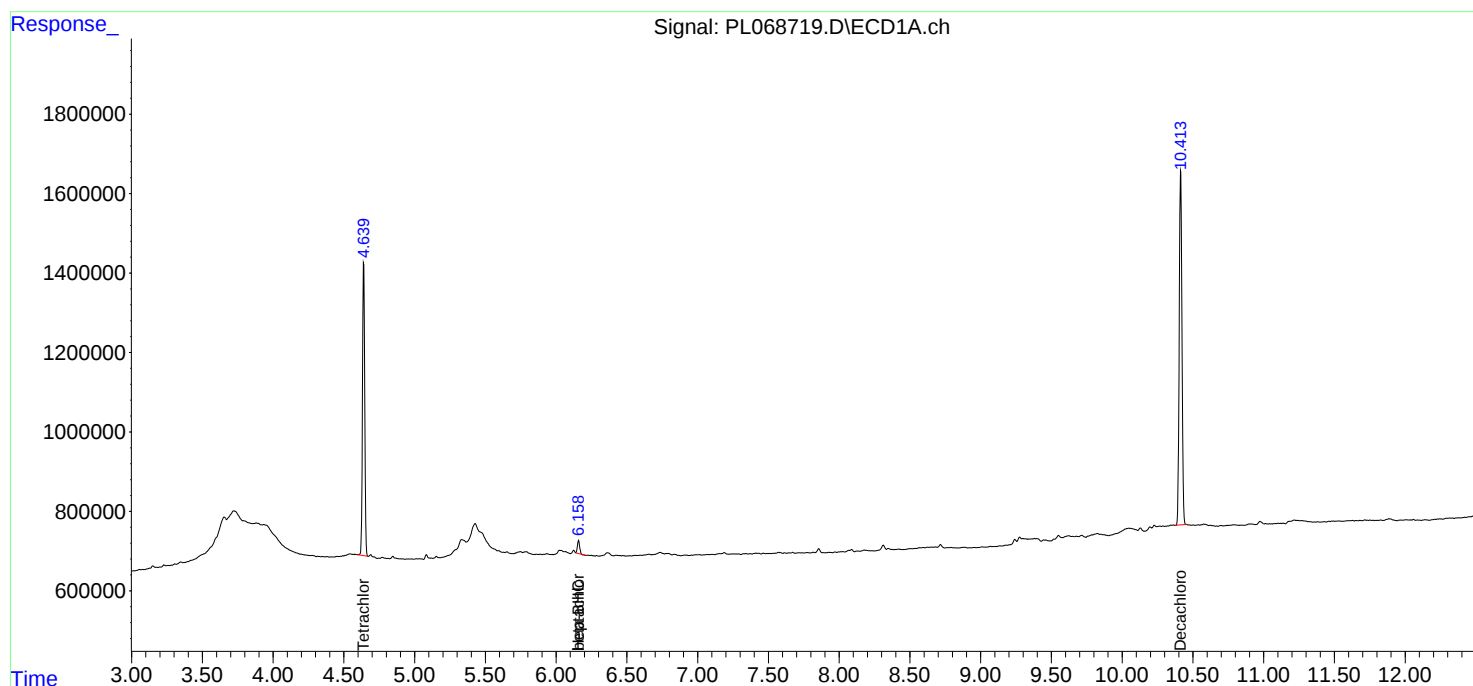


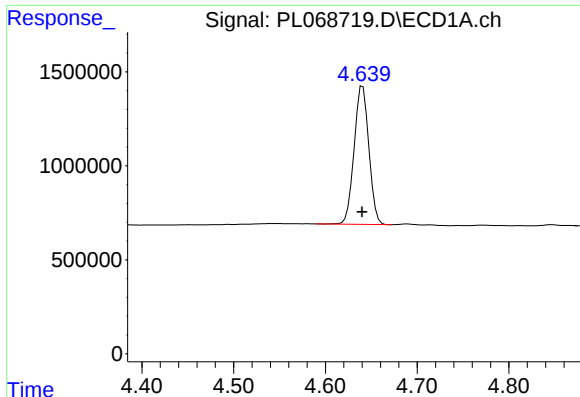

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 8243883
Conc: 19.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

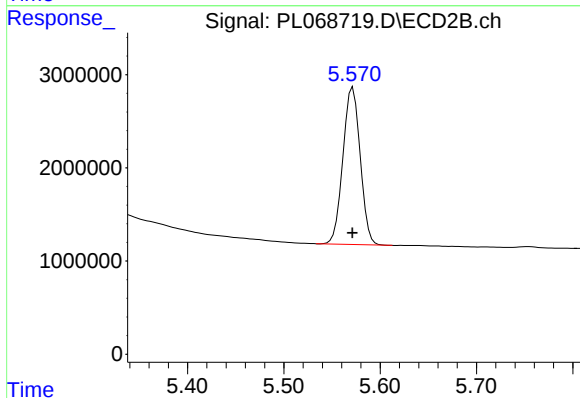


#1 Tetrachloro-m-xylene

R.T.: 5.572 min
Delta R.T.: 0.000 min
Response: 20942315
Conc: 20.63 ng/ml

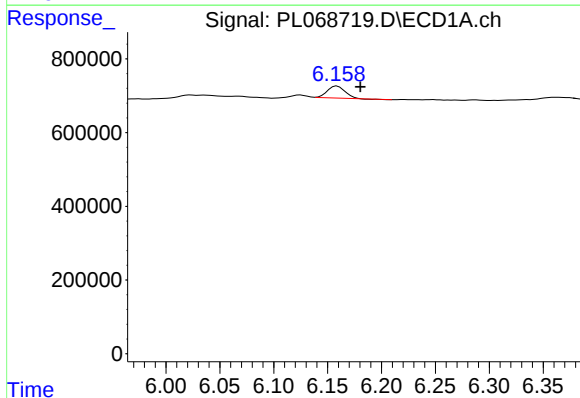


#4 Heptachlor

R.T.: 6.159 min
Delta R.T.: -0.021 min
Response: 376909
Conc: 0.64 ng/ml

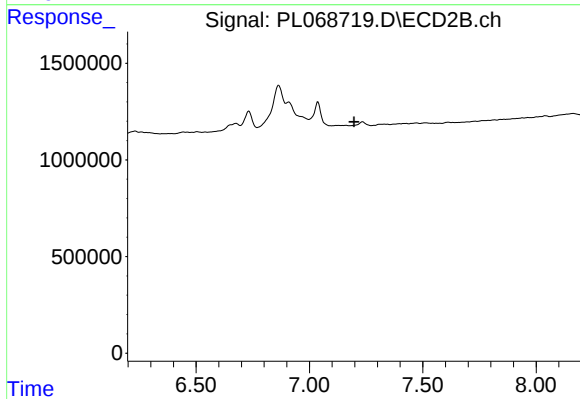

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.197 min
Response: 0
Conc: N.D.

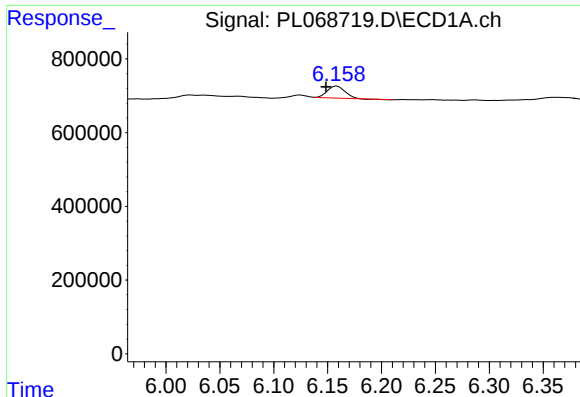

#6 beta-BHC


R.T.: 6.159 min
Delta R.T.: 0.010 min
Response: 376909
Conc: 1.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

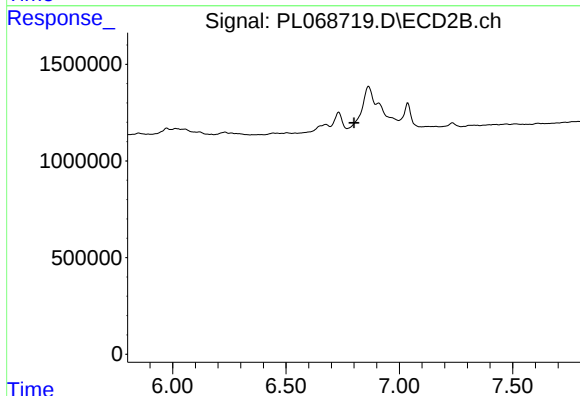


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

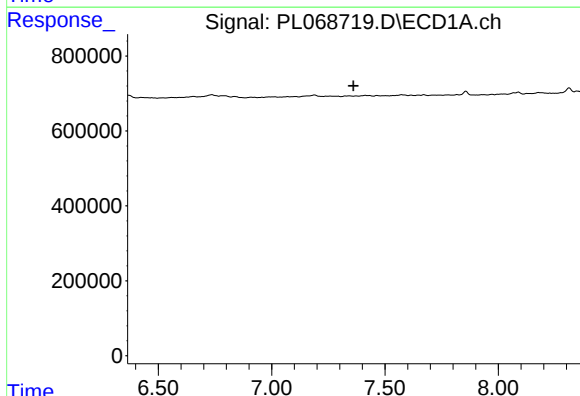


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.361 min
Response: 0
Conc: N.D.

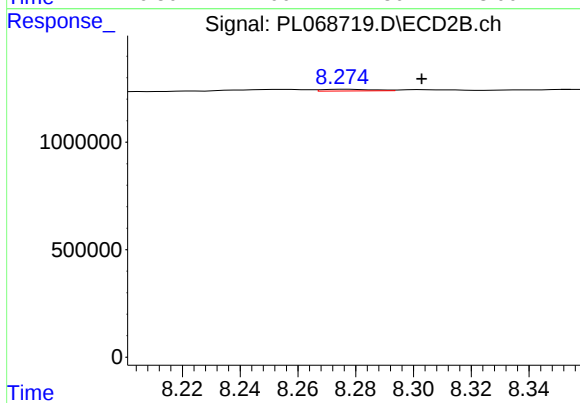

#10 gamma-Chlordane


R.T.: 8.277 min
Delta R.T.: -0.026 min
Response: 95740
Conc: 0.08 ng/ml

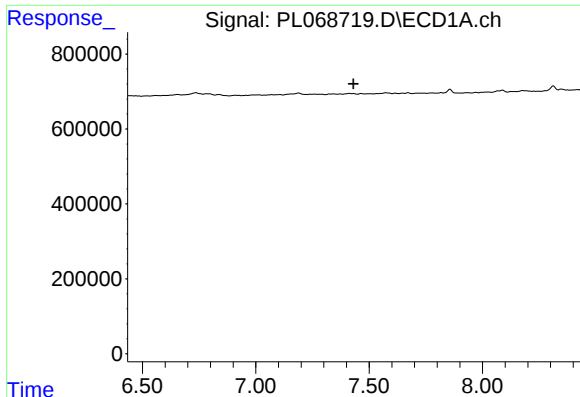

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

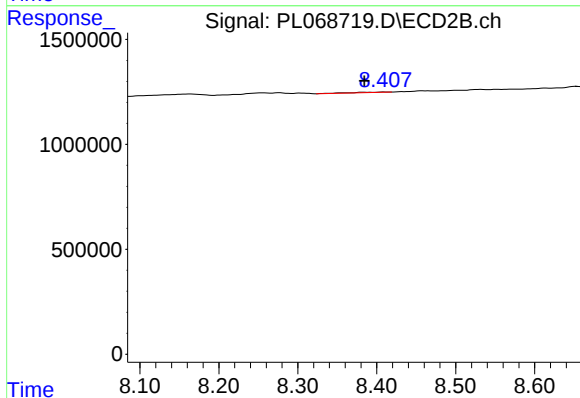


#11 alpha-Chlordane

R.T.: 8.409 min
Delta R.T.: 0.024 min
Response: 67496
Conc: 0.06 ng/ml

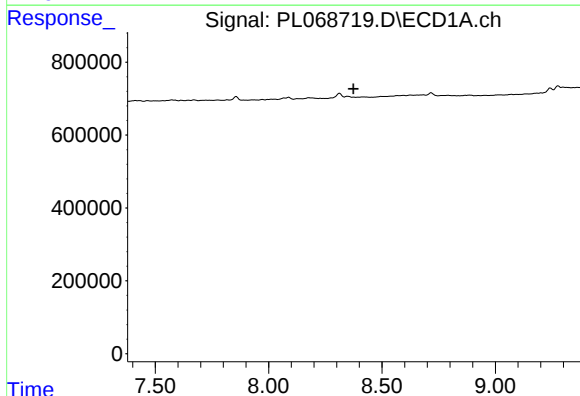


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

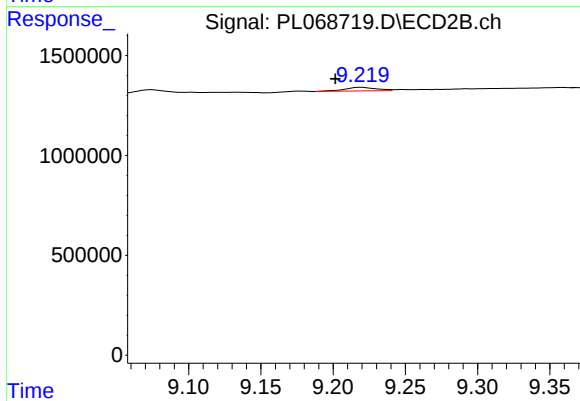

#15 Endosulfan II


R.T.: 9.220 min
Delta R.T.: 0.018 min
Response: 291339
Conc: 0.32 ng/ml

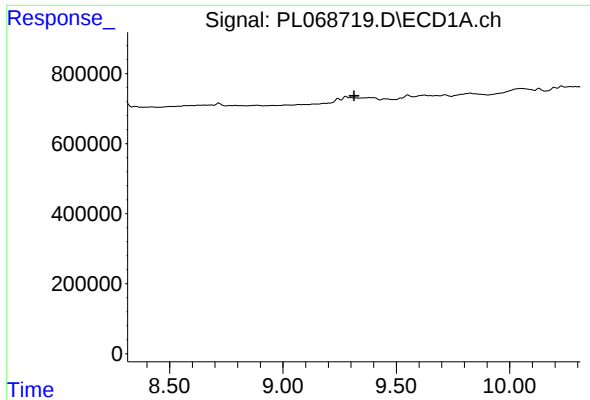

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.313 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

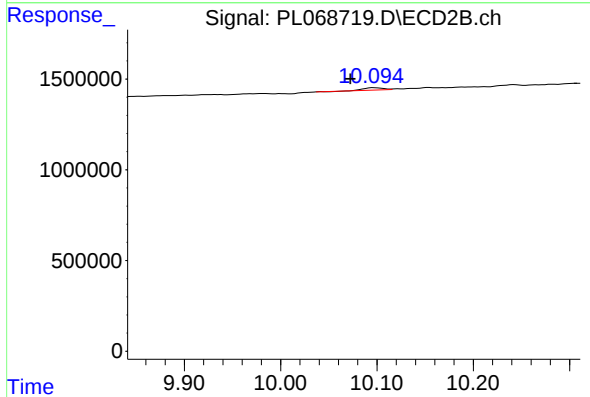


#21 Endrin ketone

R.T.: 10.096 min
Delta R.T.: 0.024 min
Response: 178431
Conc: 0.18 ng/ml

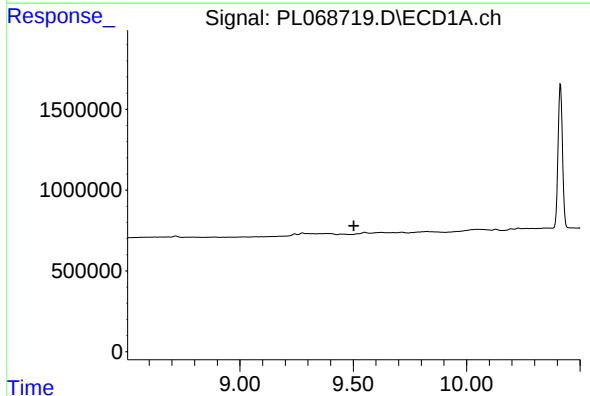


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.502 min
Response: 0
Conc: N.D.

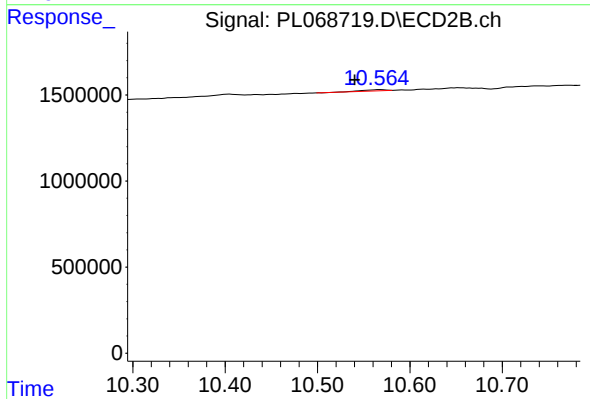

#22 Mirex


R.T.: 10.567 min
Delta R.T.: 0.026 min
Response: 132426
Conc: 0.17 ng/ml

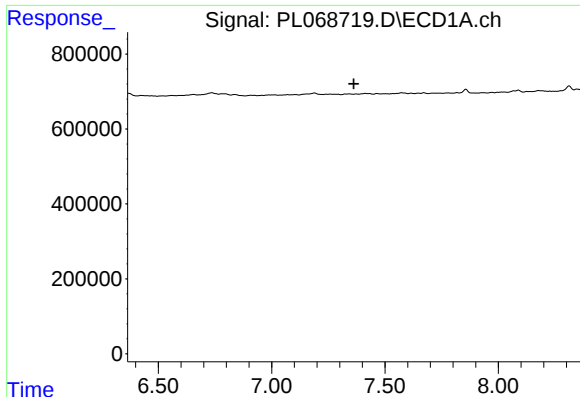

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

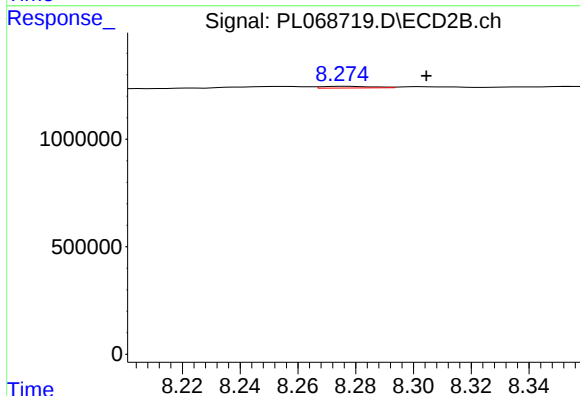


#25 Chlordane-3

R.T.: 8.277 min
Delta R.T.: -0.028 min
Response: 95740
Conc: 0.59 ng/ml

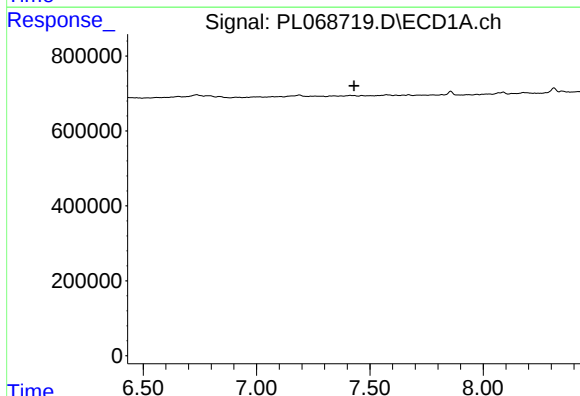


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

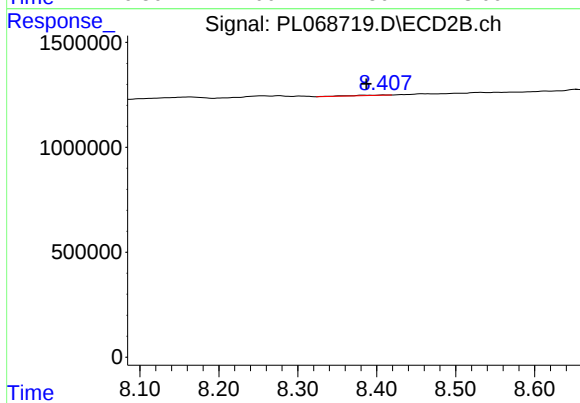

#26 Chlordane-4


R.T.: 8.409 min
Delta R.T.: 0.022 min
Response: 67496
Conc: 0.34 ng/ml

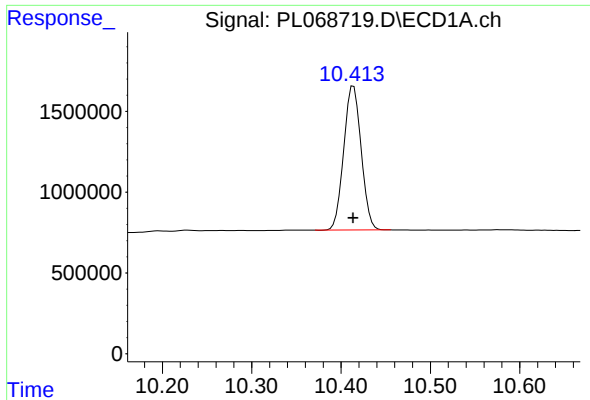

#28 Decachlorobiphenyl

R.T.: 10.414 min
Delta R.T.: 0.000 min
Response: 12083303
Conc: 21.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

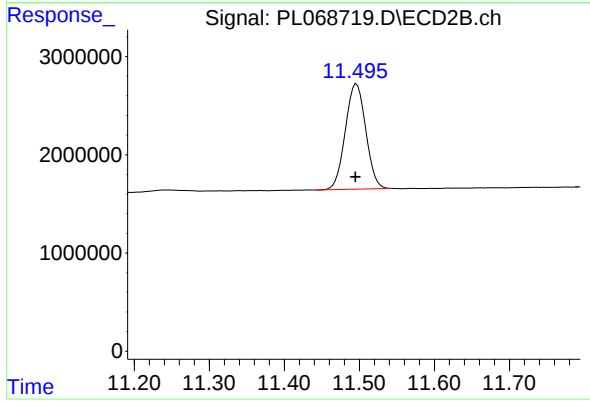

#28 Decachlorobiphenyl

R.T.: 11.496 min
Delta R.T.: 0.002 min
Response: 20294396
Conc: 20.92 ng/ml