

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080521\
 Data File : PL068746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2021 23:15
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 03:17:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.639	5.568	8376899	21689919	20.252	21.362
28)	SA Decachlor...	10.409	11.488	12011147	20130346	20.900	20.748
Target Compounds							
4)	MA Heptachlor	6.156f	0.000	277356	0	0.472	N.D. #
6)	B beta-BHC	6.156	0.000	277356	0	0.984	N.D. #
8)	B Heptachlo...	0.000	8.036	0	403181	N.D.	0.349 #
9)	A Endosulfan I	0.000	8.429	0	89896	N.D.	0.085 #
10)	B gamma-Chl...	0.000	8.328f	0	201375	N.D.	0.176 #
15)	B Endosulfa...	0.000	9.218f	0	325569	N.D.	0.355 #
21)	B Endrin ke...	0.000	10.093f	0	222426	N.D.	0.218 #
22)	Mirex	0.000	10.563f	0	206647	N.D.	0.261 #
25)	Chlordane-3	0.000	8.328f	0	201375	N.D.	1.233 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080521\
Data File : PL068746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2021 23:15
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 03:17:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

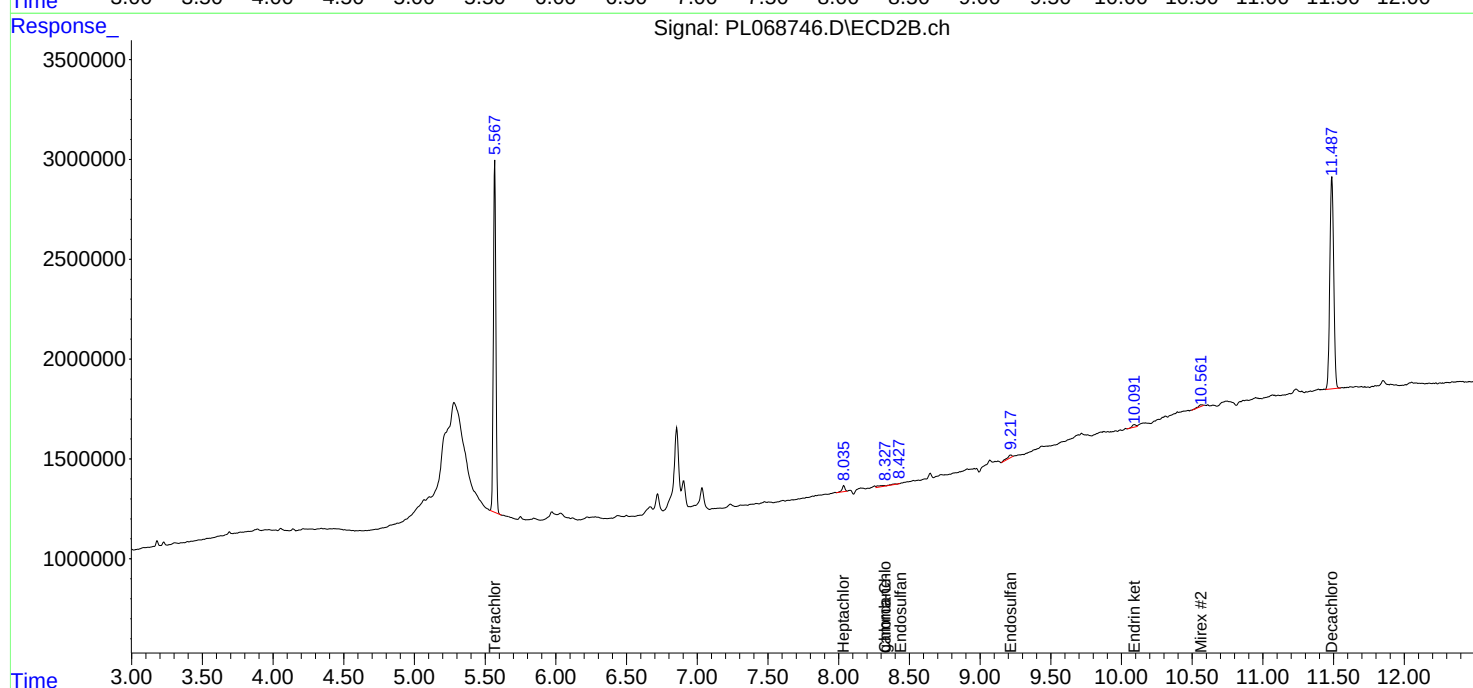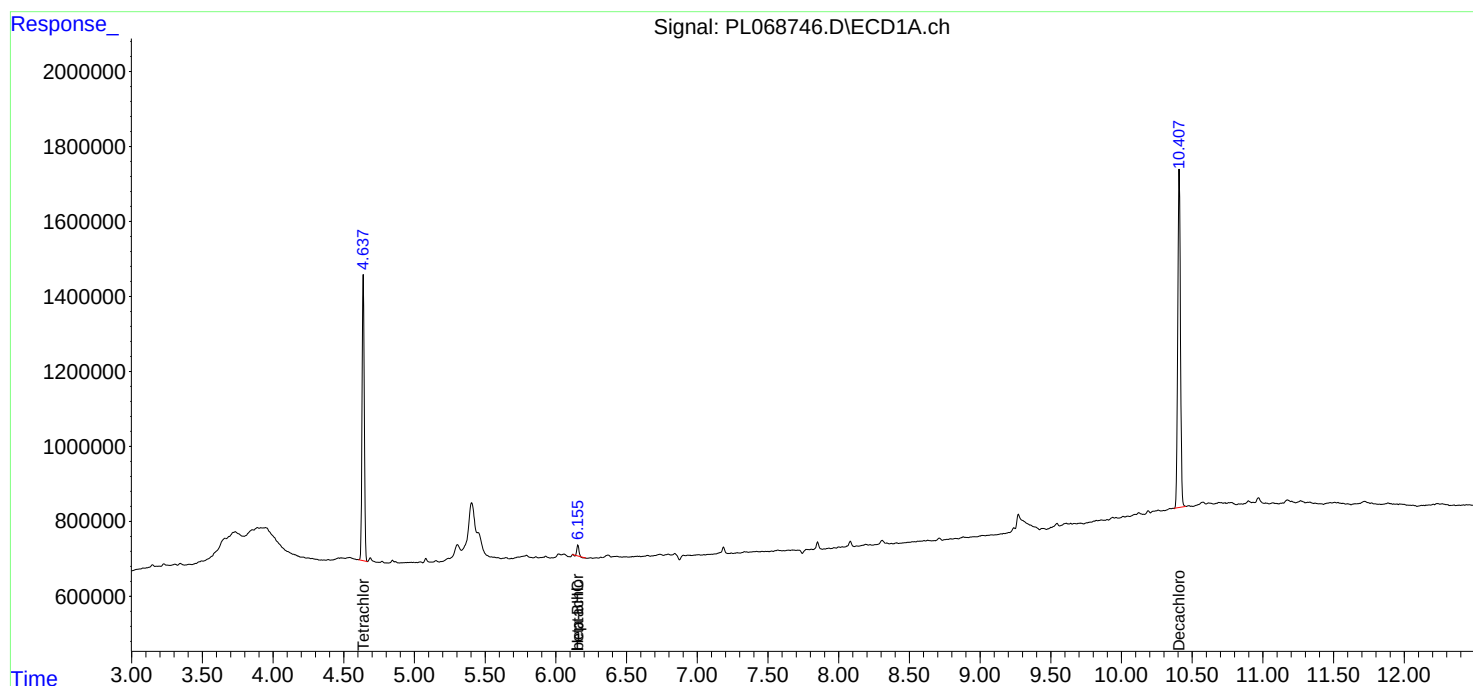


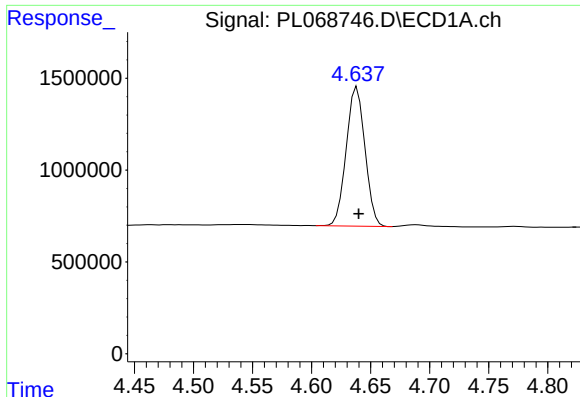

#1 Tetrachloro-m-xylene


R.T.: 4.639 min
Delta R.T.: -0.001 min
Response: 8376899
Conc: 20.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

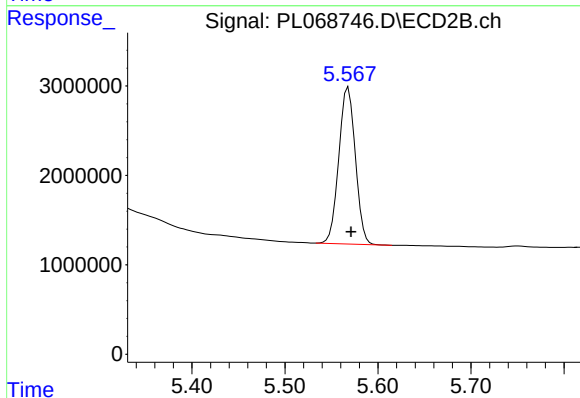


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 21689919
Conc: 21.36 ng/ml

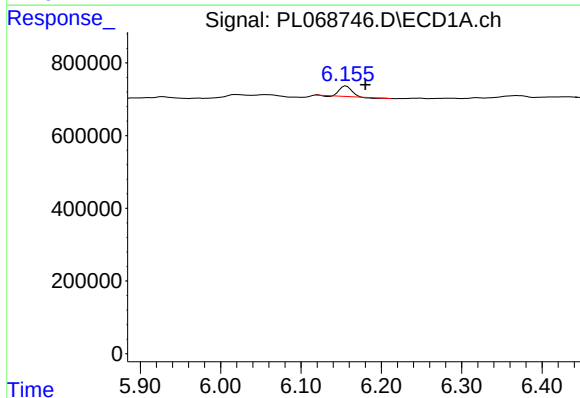


#4 Heptachlor

R.T.: 6.156 min
Delta R.T.: -0.024 min
Response: 277356
Conc: 0.47 ng/ml

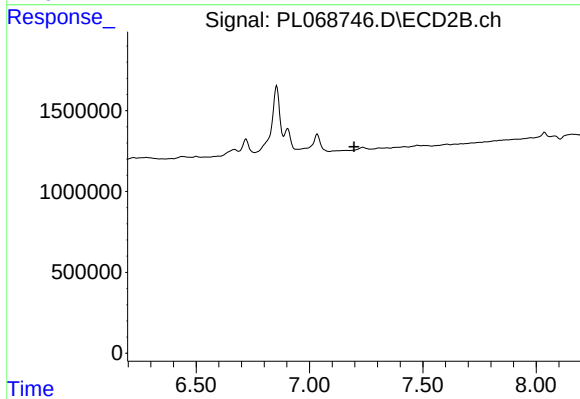

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.197 min
Response: 0
Conc: N.D.

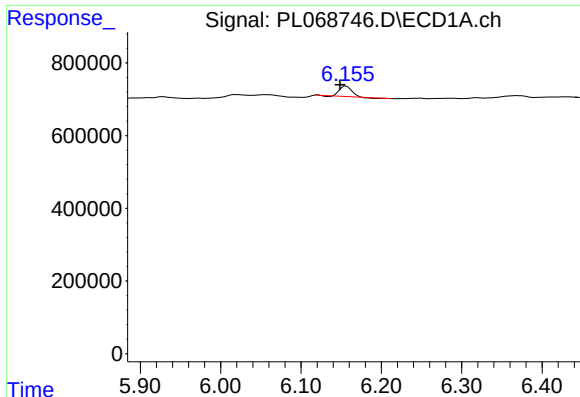

#6 beta-BHC


R.T.: 6.156 min
Delta R.T.: 0.008 min
Response: 277356
Conc: 0.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

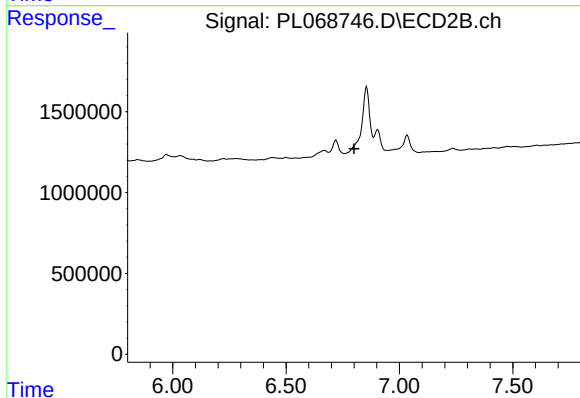


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

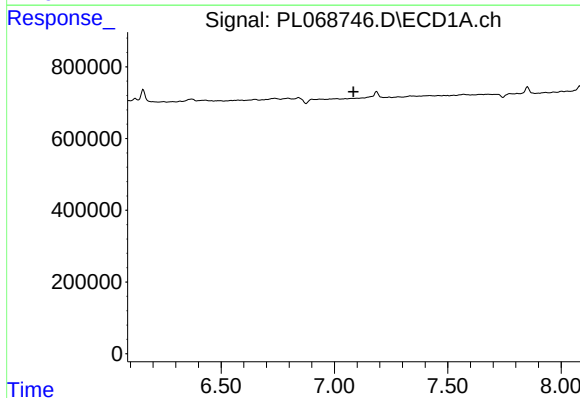


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

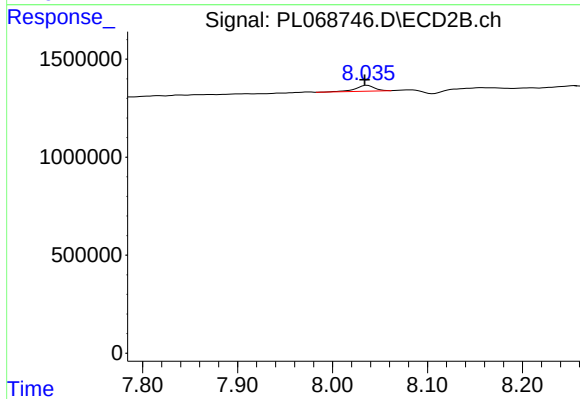

#8 Heptachlor epoxide


R.T.: 8.036 min
Delta R.T.: 0.002 min
Response: 403181
Conc: 0.35 ng/ml

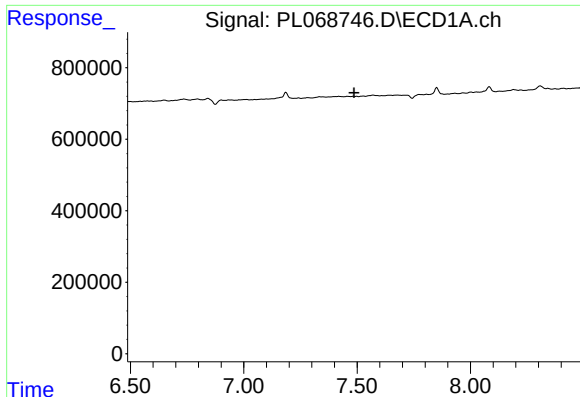

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

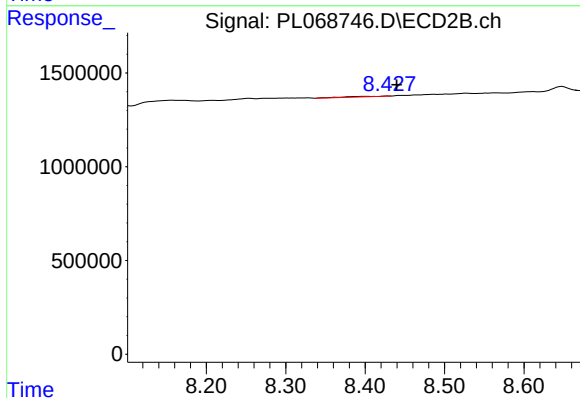


#9 Endosulfan I

R.T.: 8.429 min
Delta R.T.: -0.011 min
Response: 89896
Conc: 0.09 ng/ml

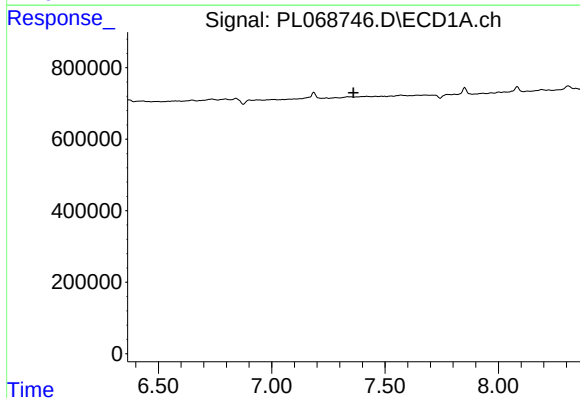


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.361 min
Response: 0
Conc: N.D.

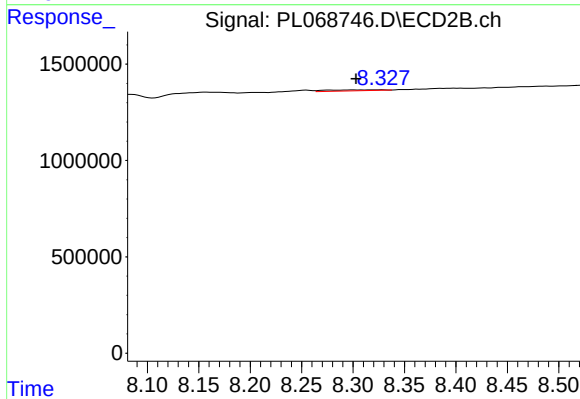

#10 gamma-Chlordane


R.T.: 8.328 min
Delta R.T.: 0.025 min
Response: 201375
Conc: 0.18 ng/ml

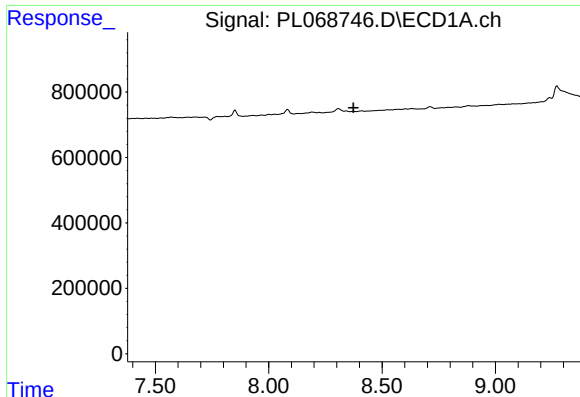

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

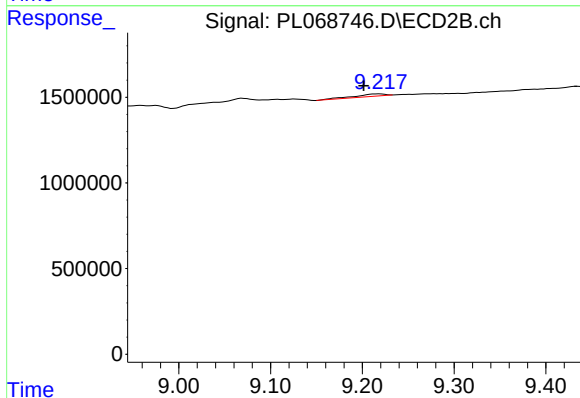


#15 Endosulfan II

R.T.: 9.218 min
Delta R.T.: 0.017 min
Response: 325569
Conc: 0.35 ng/ml

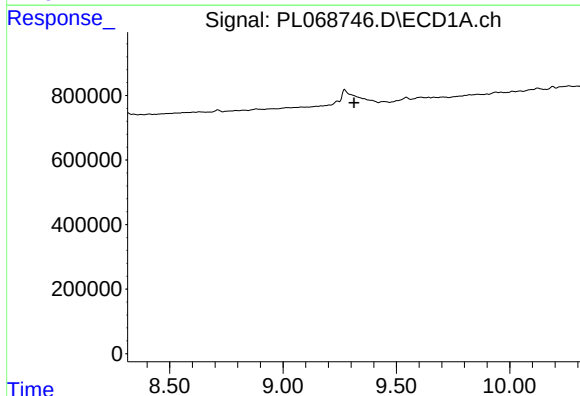


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.313 min
Response: 0
Conc: N.D.

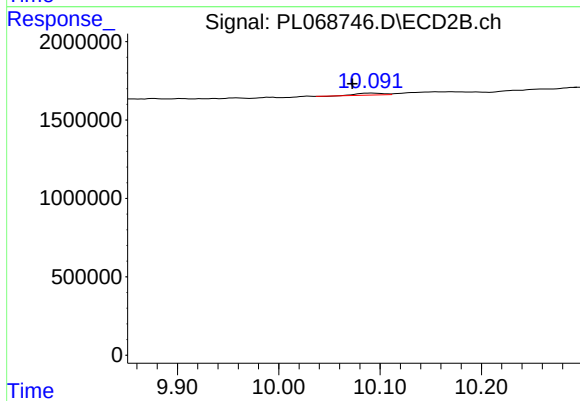

#21 Endrin ketone


R.T.: 10.093 min
Delta R.T.: 0.020 min
Response: 222426
Conc: 0.22 ng/ml

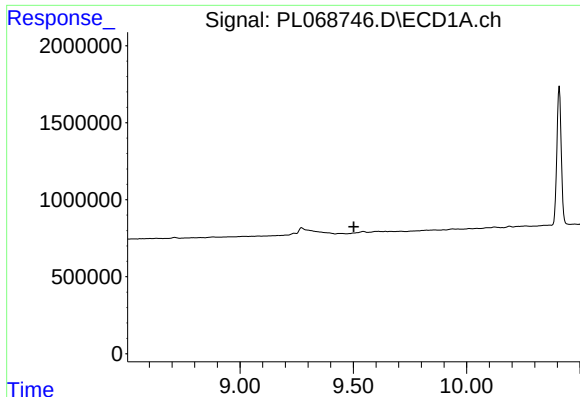

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

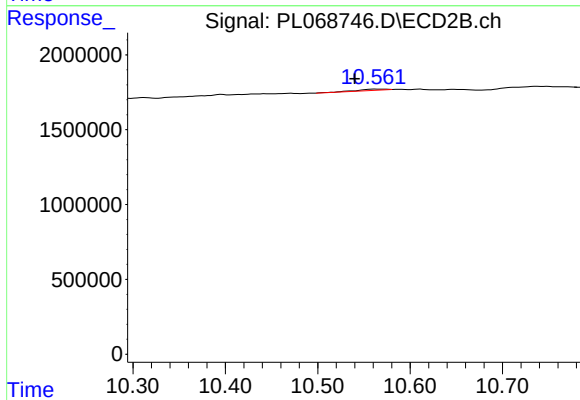


#22 Mirex

R.T.: 10.563 min
Delta R.T.: 0.023 min
Response: 206647
Conc: 0.26 ng/ml

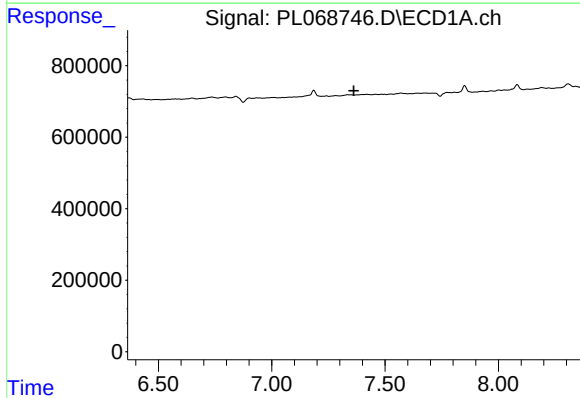


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

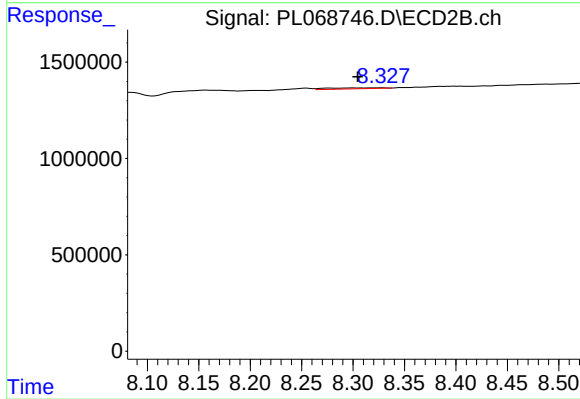

#25 Chlordane-3


R.T.: 8.328 min
Delta R.T.: 0.023 min
Response: 201375
Conc: 1.23 ng/ml

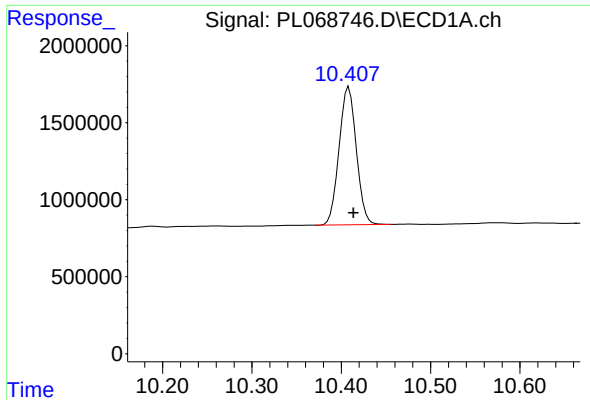

#28 Decachlorobiphenyl

R.T.: 10.409 min
Delta R.T.: -0.005 min
Response: 12011147
Conc: 20.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

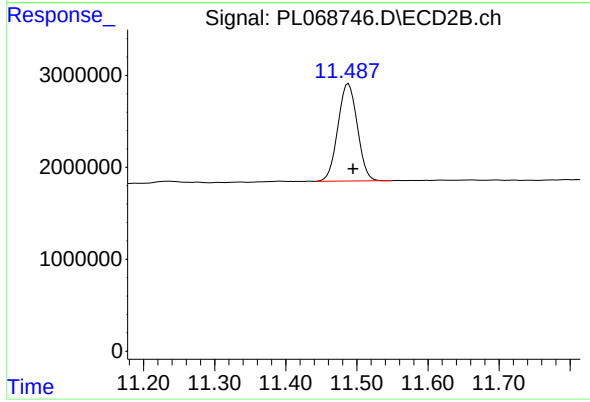

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: -0.007 min
Response: 20130346
Conc: 20.75 ng/ml