

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080521\
 Data File : PL068751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 00:38
 Operator : AR\AJ
 Sample : M3279-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20210568-COM-41

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 03:19:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.638	5.568	7336893	18292194	17.737	18.016
28)	SA Decachlor...	10.408	11.487	7005003	11749688	12.189	12.110
Target Compounds							
8)	B Heptachlo...	0.000	8.030	0	151886	N.D.	0.131 #
10)	B gamma-Chl...	0.000	8.321f	0	314555	N.D.	0.275 #
11)	B alpha-Chl...	0.000	8.383	0	37777	N.D.	0.033 #
15)	B Endosulfa...	0.000	9.216	0	534189	N.D.	0.582 #
21)	B Endrin ke...	0.000	10.092f	0	15873	N.D.	0.016 #
22)	Mirex	0.000	10.565f	0	57687	N.D.	0.073 #
25)	Chlordane-3	0.000	8.321f	0	314555	N.D.	1.926 #
26)	Chlordane-4	0.000	8.383	0	37777	N.D.	0.190 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080521\
Data File : PL068751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 00:38
Operator : AR\AJ
Sample : M3279-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20210568-COM-41

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 03:19:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

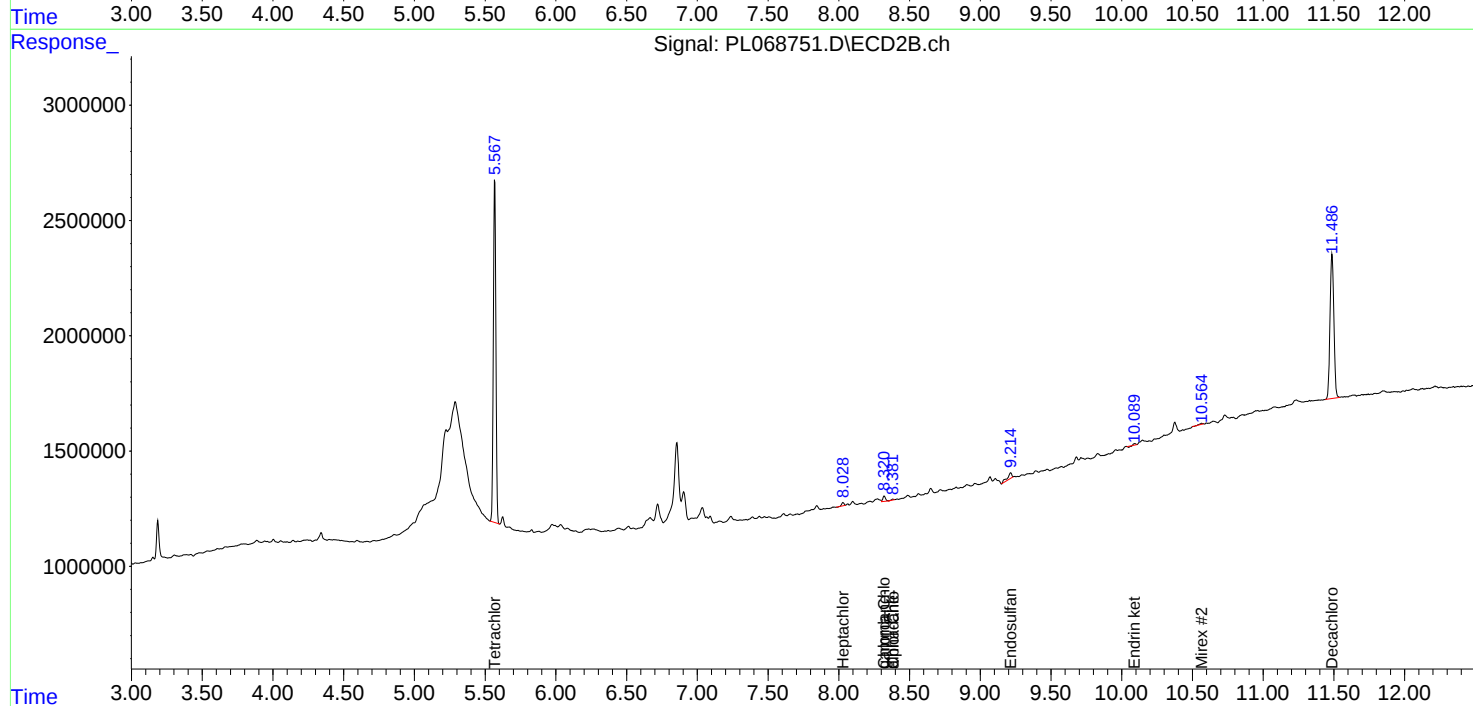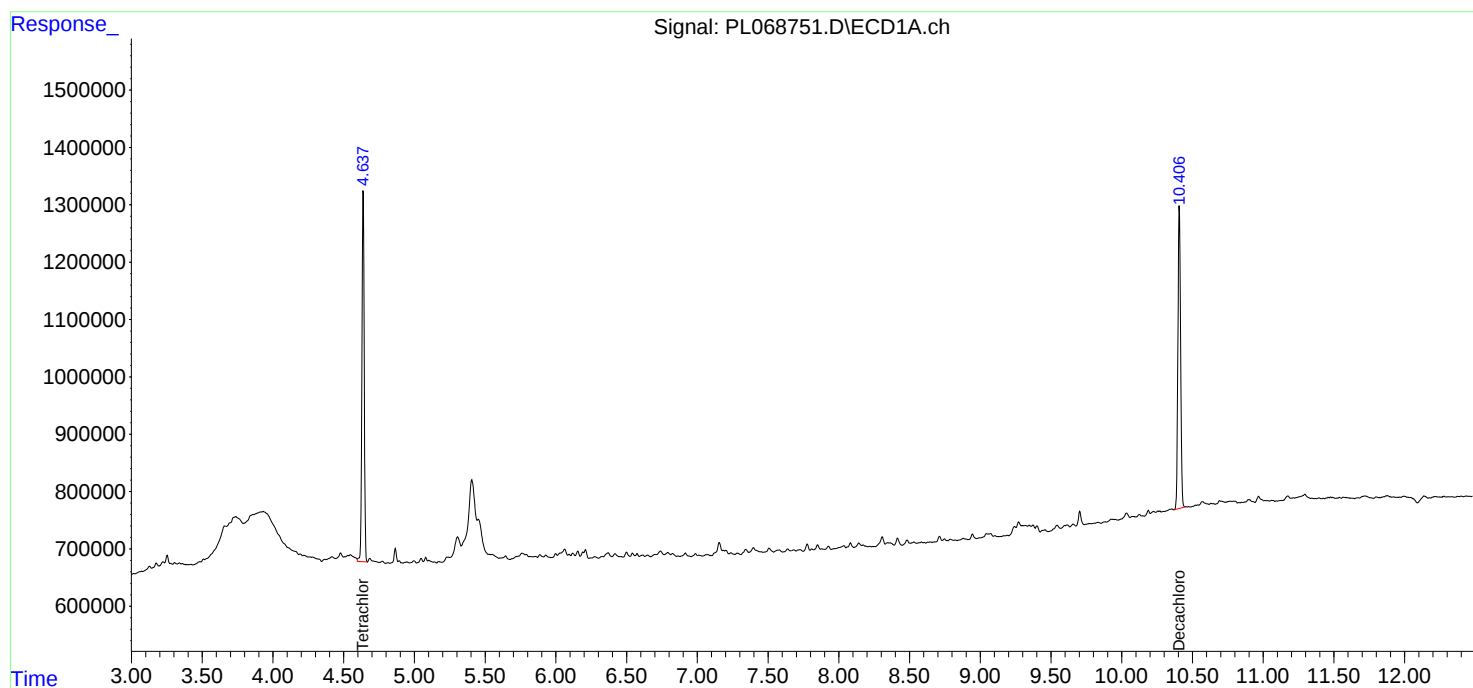


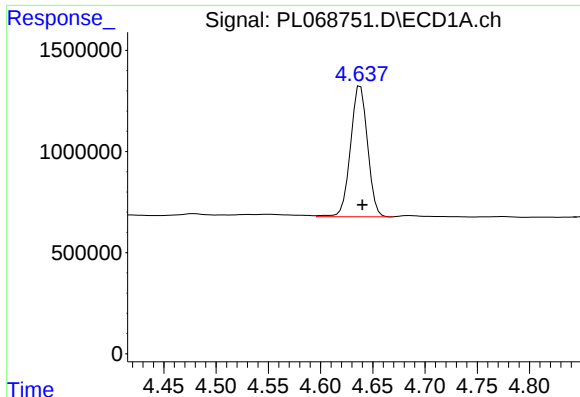

#1 Tetrachloro-m-xylene


R.T.: 4.638 min
Delta R.T.: -0.002 min
Response: 7336893
Conc: 17.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210568-COM-41

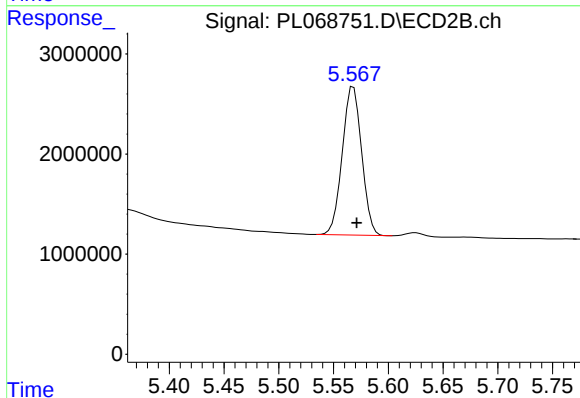


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 18292194
Conc: 18.02 ng/ml

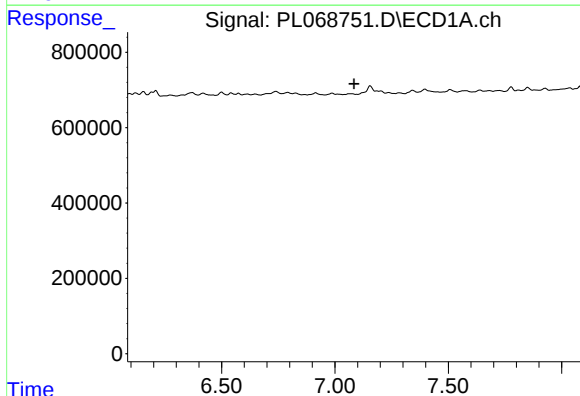


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

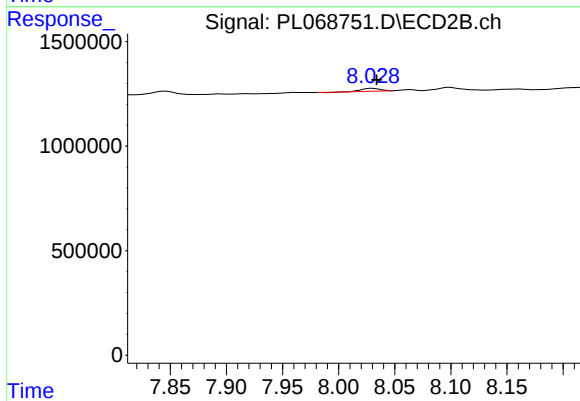

#8 Heptachlor epoxide


R.T.: 8.030 min
Delta R.T.: -0.004 min
Response: 151886
Conc: 0.13 ng/ml

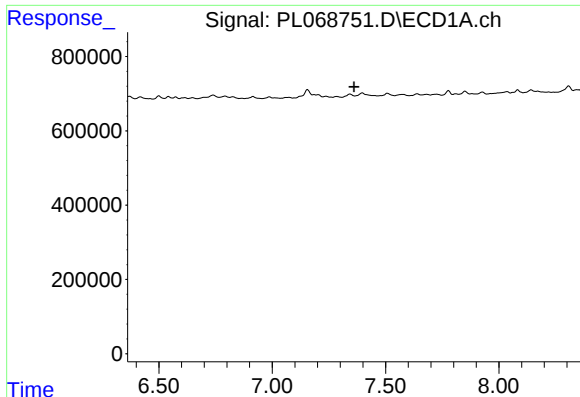

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210568-COM-41

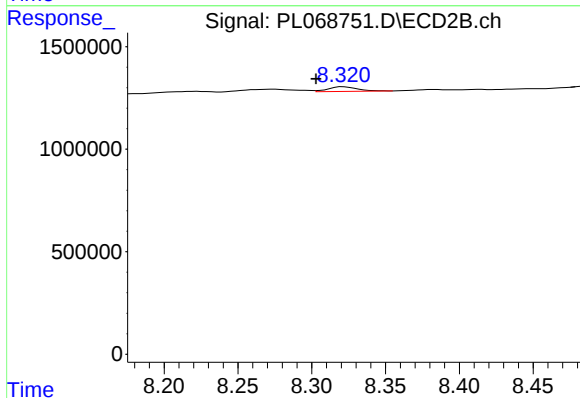


#10 gamma-Chlordane

R.T.: 8.321 min
Delta R.T.: 0.018 min
Response: 314555
Conc: 0.27 ng/ml

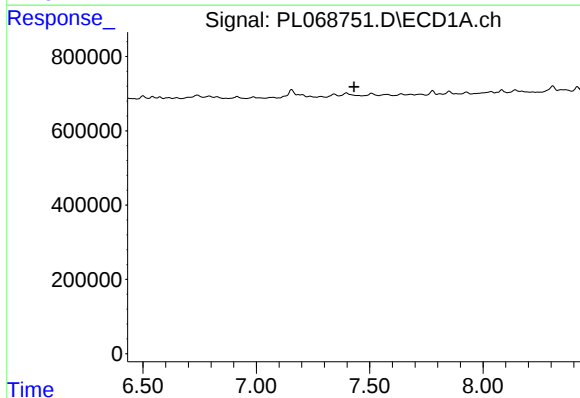


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

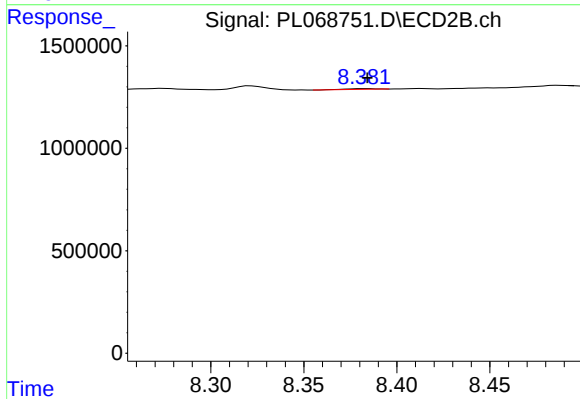

#11 alpha-Chlordane


R.T.: 8.383 min
Delta R.T.: -0.002 min
Response: 37777
Conc: 0.03 ng/ml

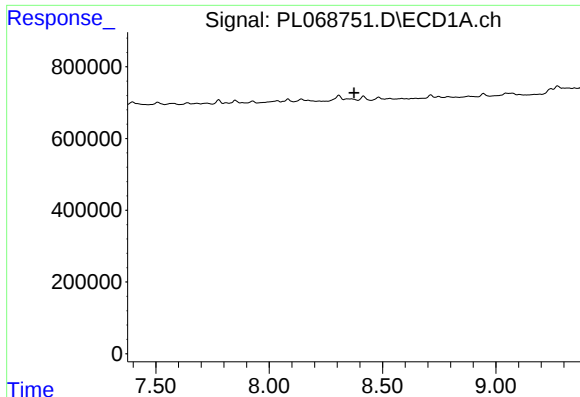

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210568-COM-41

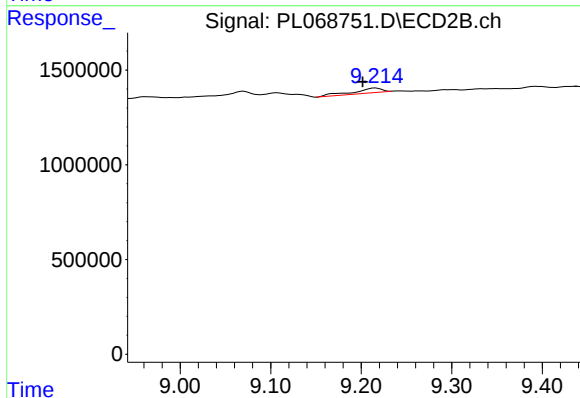


#15 Endosulfan II

R.T.: 9.216 min
Delta R.T.: 0.014 min
Response: 534189
Conc: 0.58 ng/ml

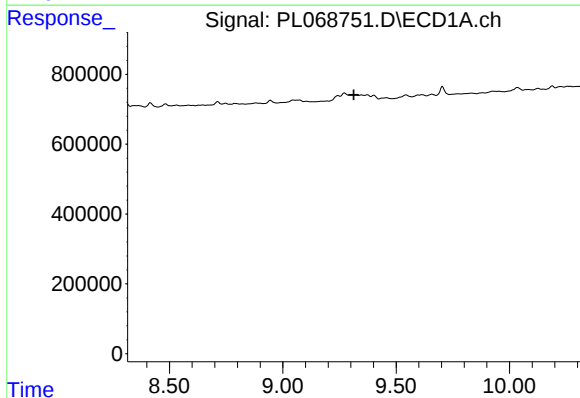


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.313 min
Response: 0
Conc: N.D.

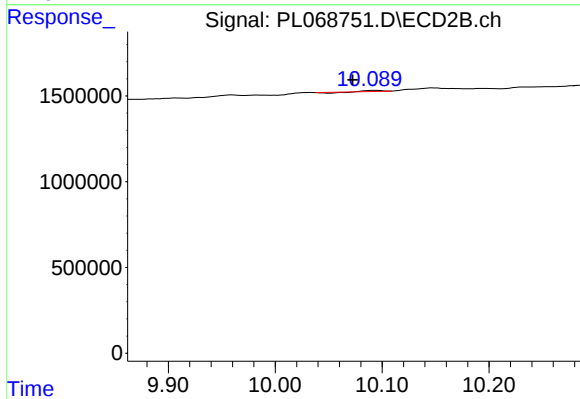

#21 Endrin ketone


R.T.: 10.092 min
Delta R.T.: 0.019 min
Response: 15873
Conc: 0.02 ng/ml

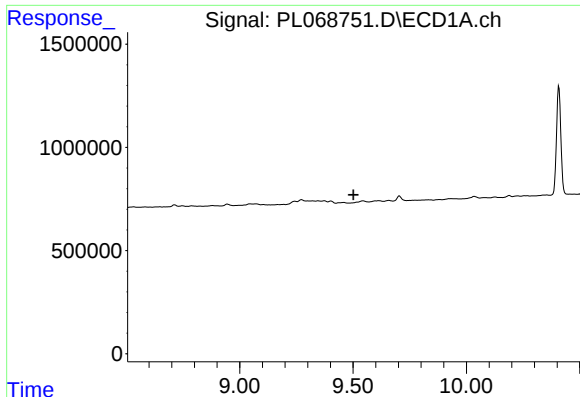

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210568-COM-41

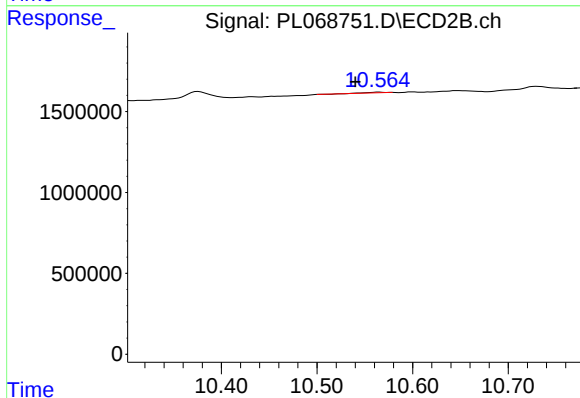


#22 Mirex

R.T.: 10.565 min
Delta R.T.: 0.025 min
Response: 57687
Conc: 0.07 ng/ml

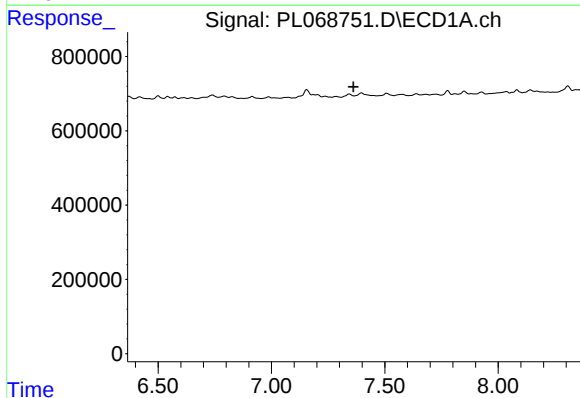


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

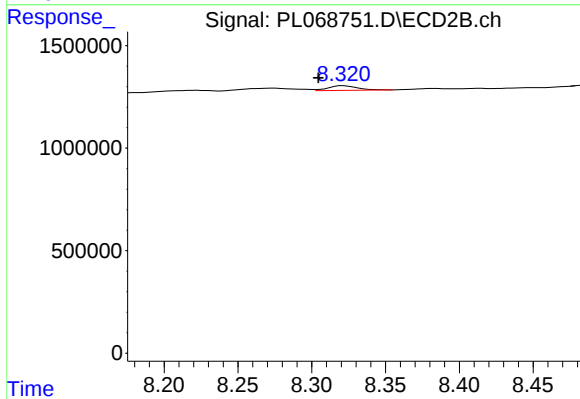

#25 Chlordane-3


R.T.: 8.321 min
Delta R.T.: 0.017 min
Response: 314555
Conc: 1.93 ng/ml

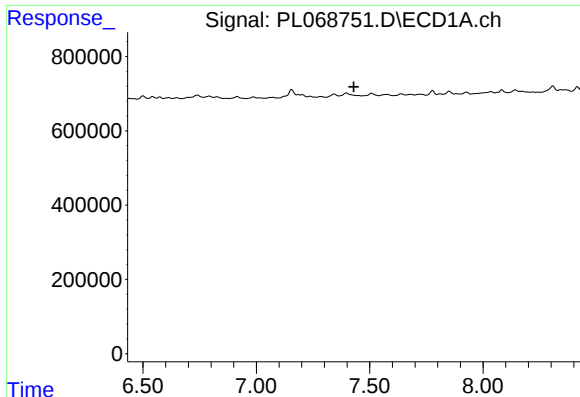

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210568-COM-41

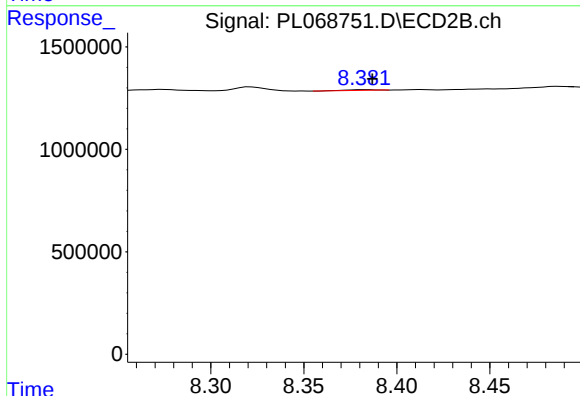


#26 Chlordane-4

R.T.: 8.383 min
Delta R.T.: -0.004 min
Response: 37777
Conc: 0.19 ng/ml

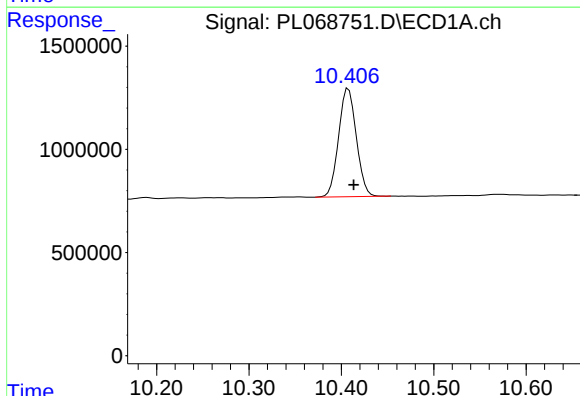

#28 Decachlorobiphenyl

R.T.: 10.408 min
Delta R.T.: -0.006 min
Response: 7005003
Conc: 12.19 ng/ml

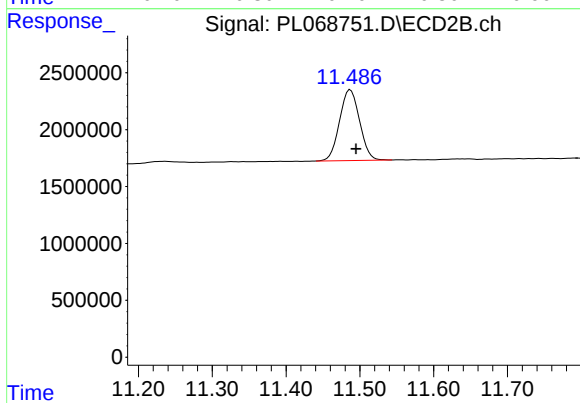

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.007 min
Response: 11749688
Conc: 12.11 ng/ml