

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080521\
 Data File : PL068757.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 02:17
 Operator : AR\AJ
 Sample : M3279-07
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20210577-COM-50

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 03:33:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.638	5.569	8111873	20816074	19.611	20.502
28)	SA Decachlor...	10.409	11.488	10419037	17842219	18.130	18.389
Target Compounds							
7)	B delta-BHC	0.000	7.091f	0	151203	N.D.	0.120 #
8)	B Heptachlo...	0.000	8.031	0	229709	N.D.	0.199 #
10)	B gamma-Chl...	0.000	8.324f	0	207774	N.D.	0.181 #
12)	B 4,4'-DDE	0.000	8.567	0	243491	N.D.	0.230 #
15)	B Endosulfa...	0.000	9.216	0	420496	N.D.	0.458 #
22)	Mirex	0.000	10.560f	0	67069	N.D.	0.085 #
23)	Chlordane-1	0.000	6.983f	0	182776	N.D.	4.334 #
25)	Chlordane-3	0.000	8.324f	0	207774	N.D.	1.272 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080521\
Data File : PL068757.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 02:17
Operator : AR\AJ
Sample : M3279-07
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20210577-COM-50

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 03:33:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

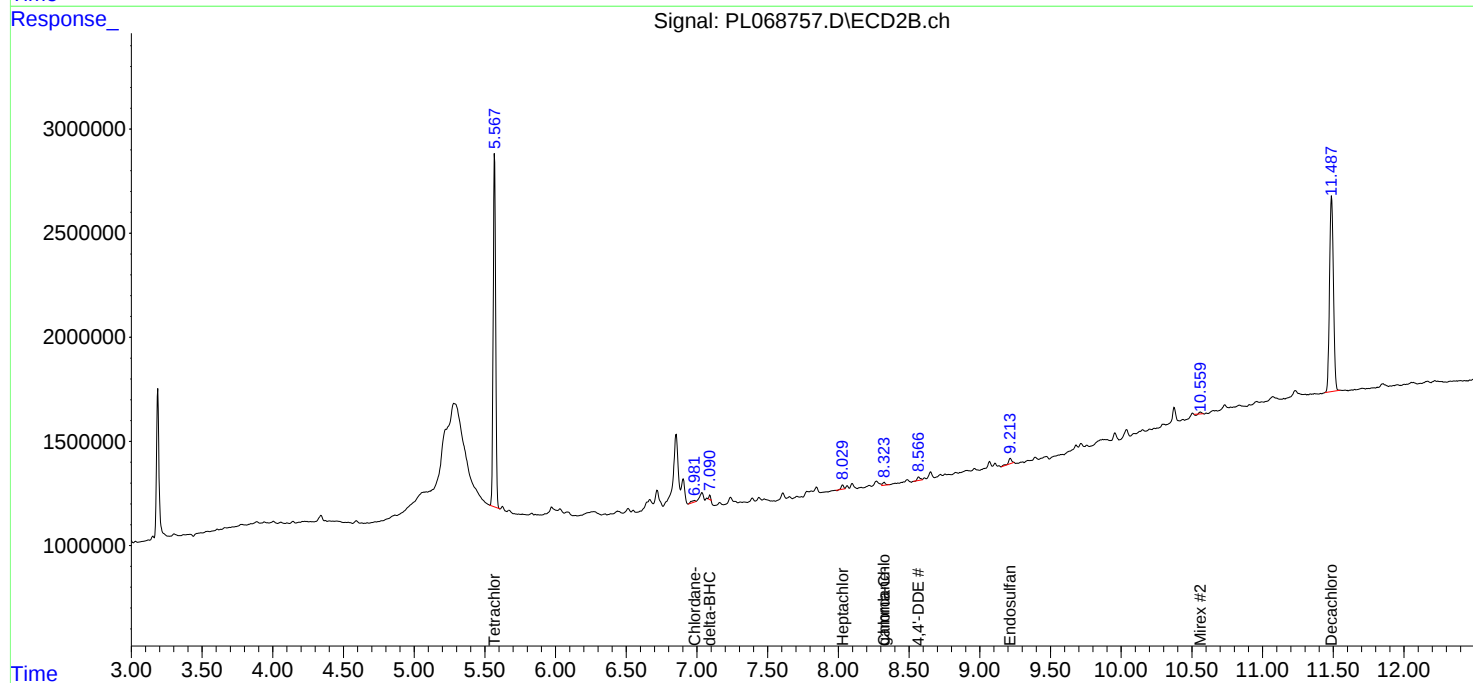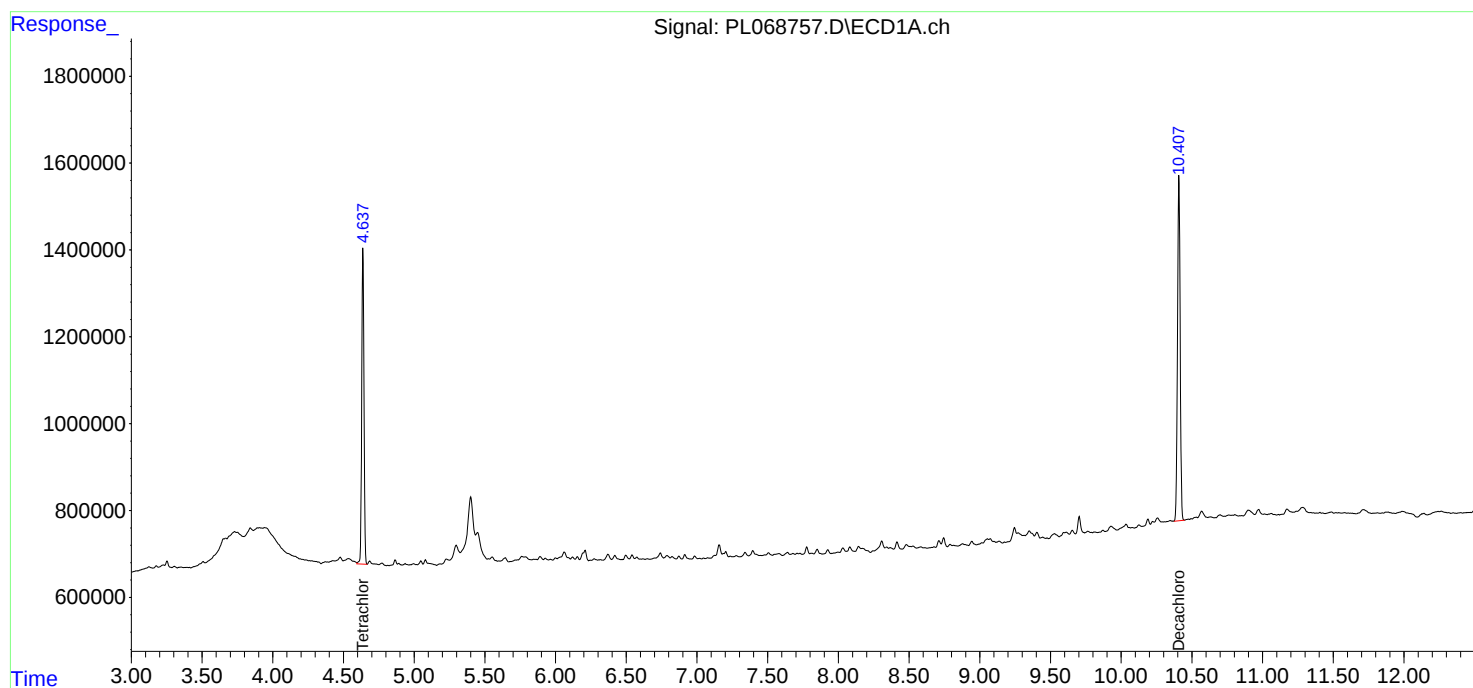


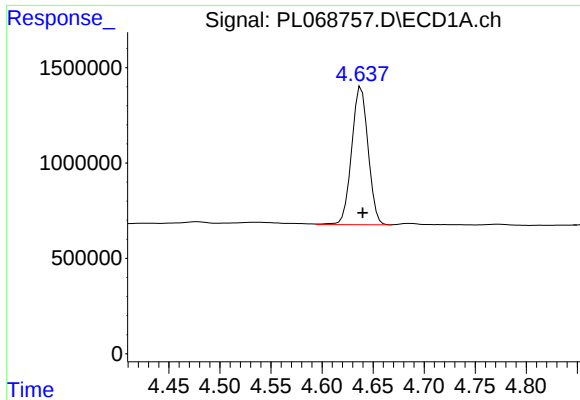

#1 Tetrachloro-m-xylene


R.T.: 4.638 min
Delta R.T.: -0.002 min
Response: 8111873
Conc: 19.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210577-COM-50

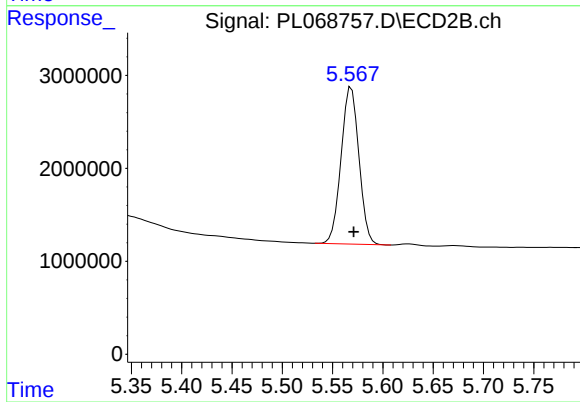


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 20816074
Conc: 20.50 ng/ml

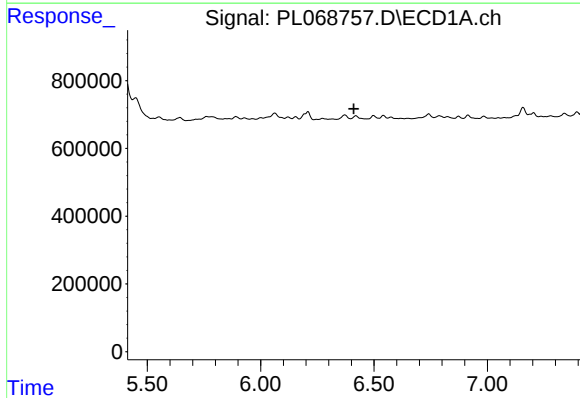


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.411 min
Response: 0
Conc: N.D.

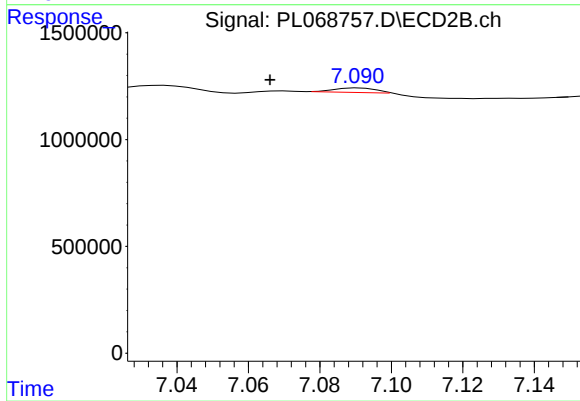

#7 delta-BHC


R.T.: 7.091 min
Delta R.T.: 0.025 min
Response: 151203
Conc: 0.12 ng/ml

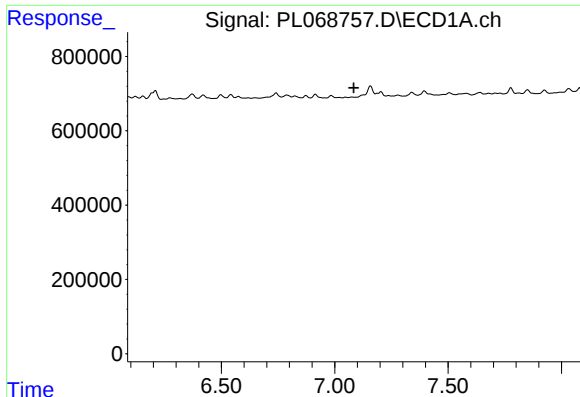

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210577-COM-50

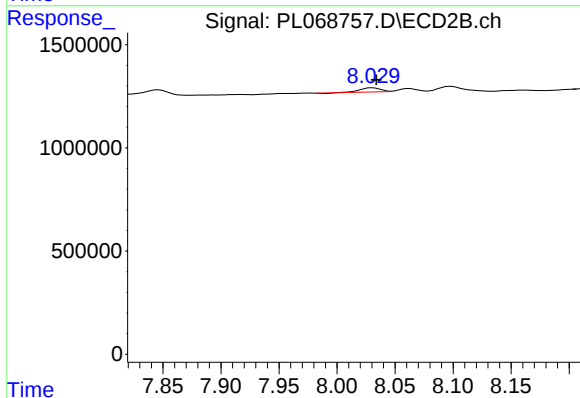


#8 Heptachlor epoxide

R.T.: 8.031 min
Delta R.T.: -0.003 min
Response: 229709
Conc: 0.20 ng/ml

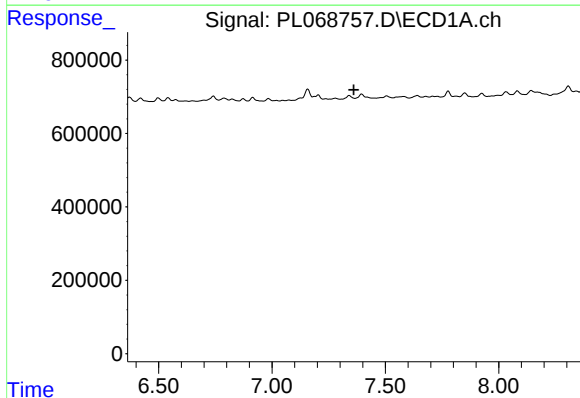


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.361 min
Response: 0
Conc: N.D.

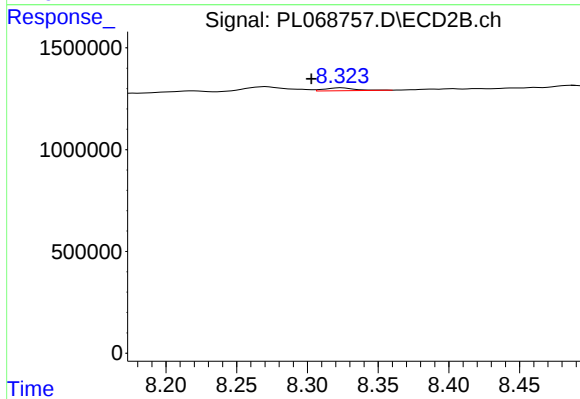

#10 gamma-Chlordane


R.T.: 8.324 min
Delta R.T.: 0.021 min
Response: 207774
Conc: 0.18 ng/ml

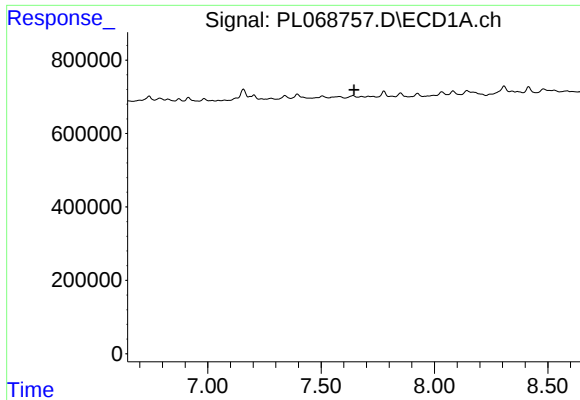

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210577-COM-50

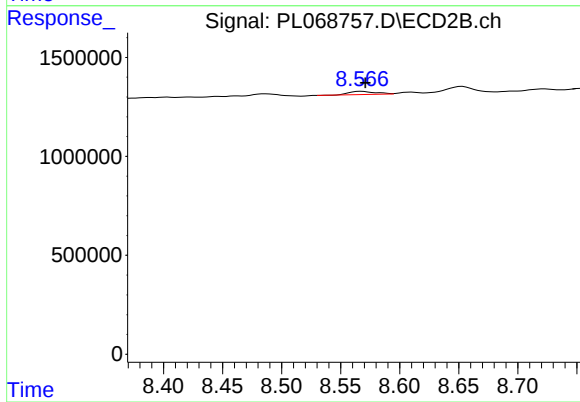


#12 4,4'-DDE

R.T.: 8.567 min
Delta R.T.: -0.004 min
Response: 243491
Conc: 0.23 ng/ml

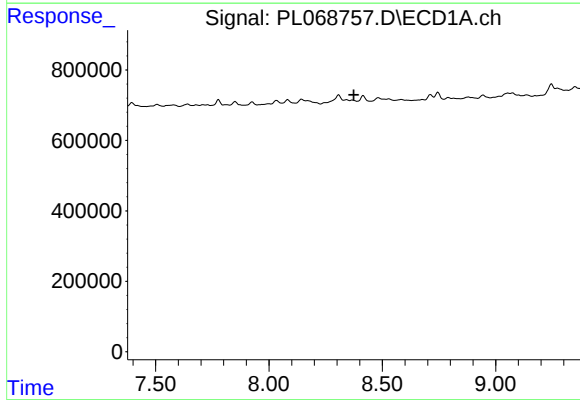


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

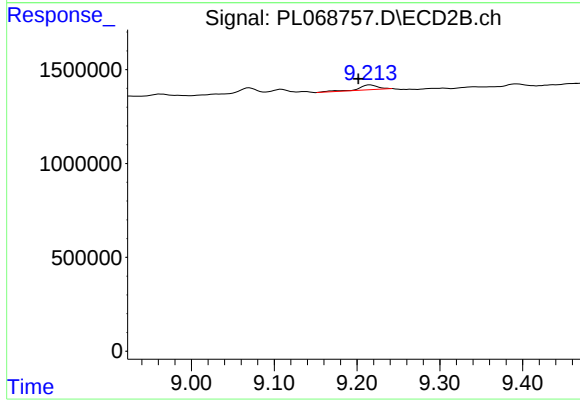

#15 Endosulfan II


R.T.: 9.216 min
Delta R.T.: 0.014 min
Response: 420496
Conc: 0.46 ng/ml

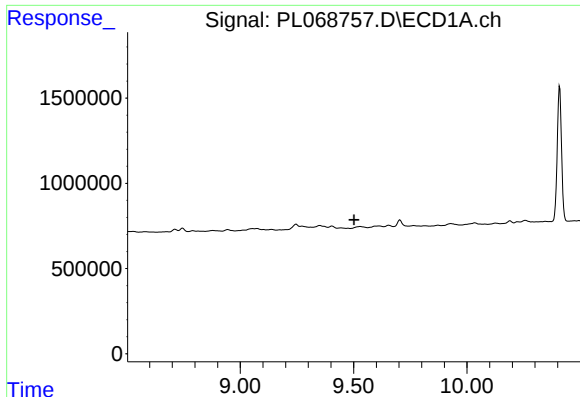

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210577-COM-50

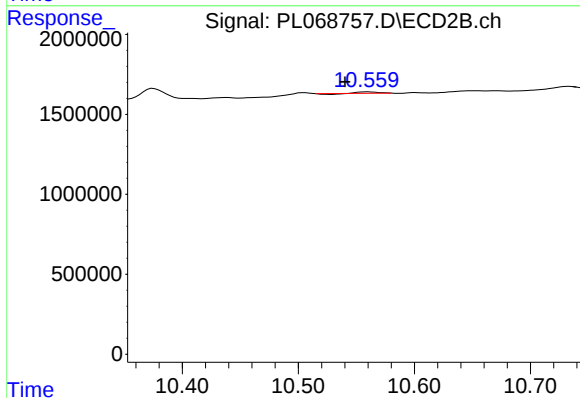


#22 Mirex

R.T.: 10.560 min
Delta R.T.: 0.020 min
Response: 67069
Conc: 0.08 ng/ml

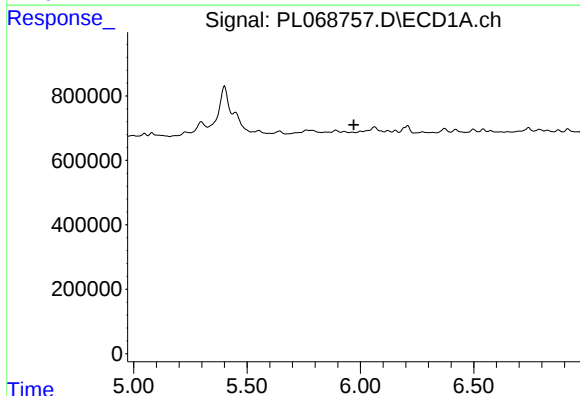


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

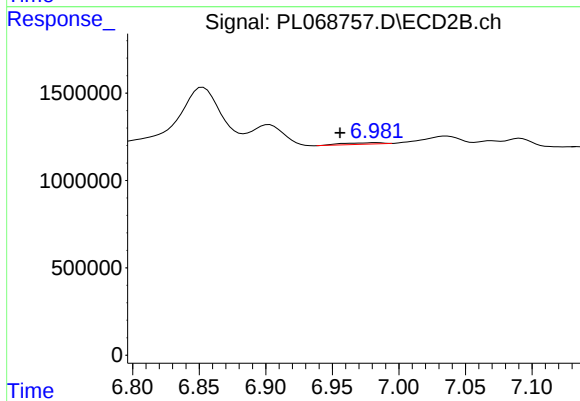

#23 Chlordane-1


R.T.: 6.983 min
Delta R.T.: 0.027 min
Response: 182776
Conc: 4.33 ng/ml

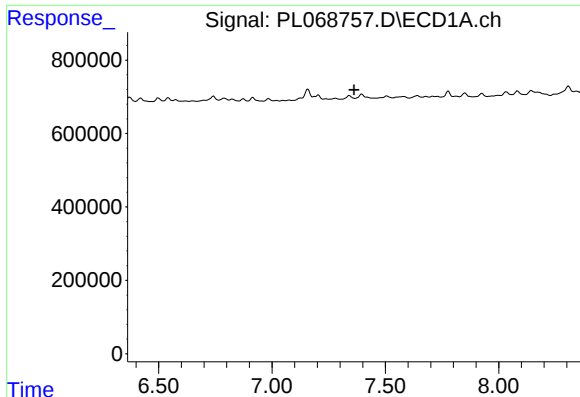

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210577-COM-50

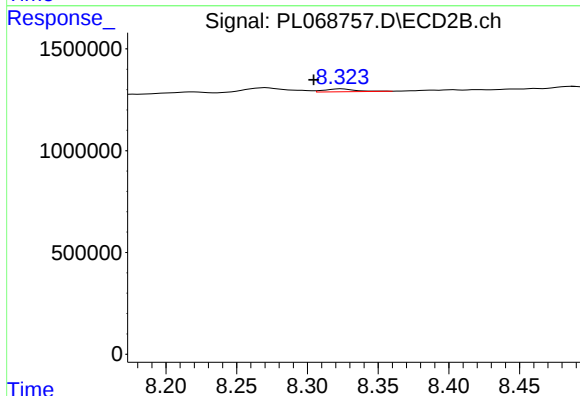


#25 Chlordane-3

R.T.: 8.324 min
Delta R.T.: 0.020 min
Response: 207774
Conc: 1.27 ng/ml

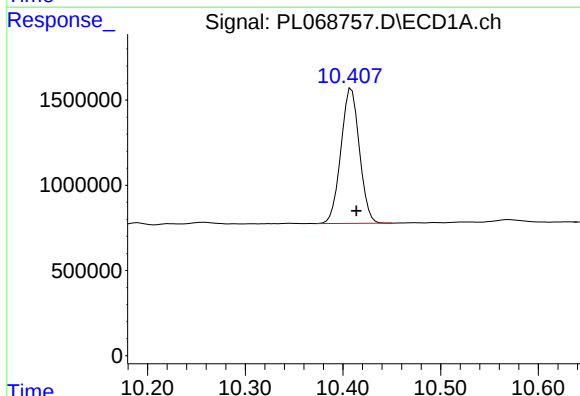

#28 Decachlorobiphenyl

R.T.: 10.409 min
Delta R.T.: -0.005 min
Response: 10419037
Conc: 18.13 ng/ml

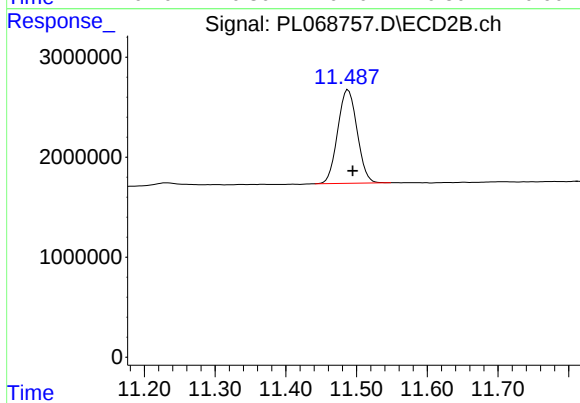

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: -0.007 min
Response: 17842219
Conc: 18.39 ng/ml