

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080521\
 Data File : PL068758.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 02:34
 Operator : AR\AJ
 Sample : M3279-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20210580-COM-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 03:34:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.638	5.569	8343130	21423938	20.170	21.100
28)	SA Decachlor...	10.409	11.489	10869802	18633971	18.914	19.205
Target Compounds							
7)	B delta-BHC	0.000	7.092f	0	104117	N.D.	0.083 #
8)	B Heptachlo...	0.000	8.031	0	244085	N.D.	0.211 #
10)	B gamma-Chl...	0.000	8.295	0	174540	N.D.	0.152 #
12)	B 4,4'-DDE	0.000	8.565	0	158291	N.D.	0.150 #
13)	MA Dieldrin	0.000	8.720	0	140076	N.D.	0.129 #
14)	MA Endrin	0.000	8.963	0	157073	N.D.	0.173 #
15)	B Endosulfa...	0.000	9.217f	0	305007	N.D.	0.333 #
25)	Chlordane-3	0.000	8.295	0	174540	N.D.	1.068 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080521\
Data File : PL068758.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 02:34
Operator : AR\AJ
Sample : M3279-08
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20210580-COM-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 03:34:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

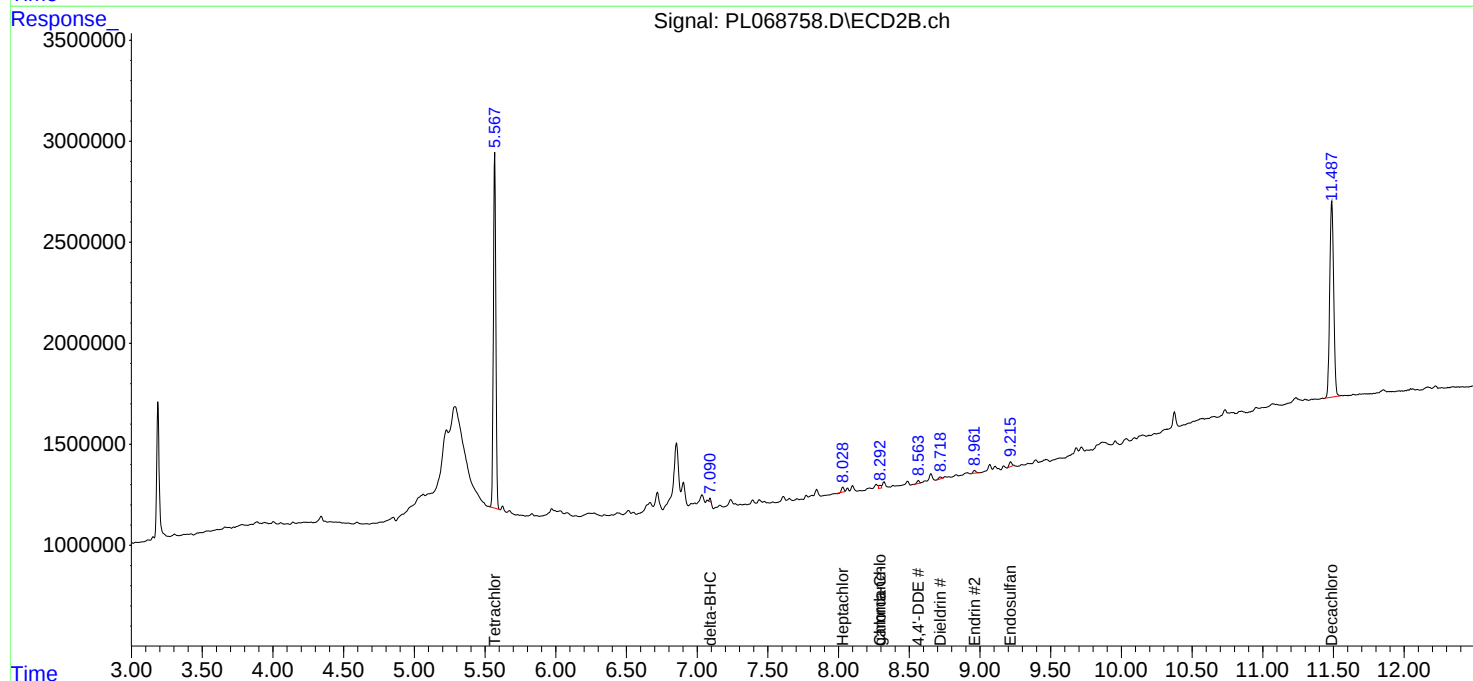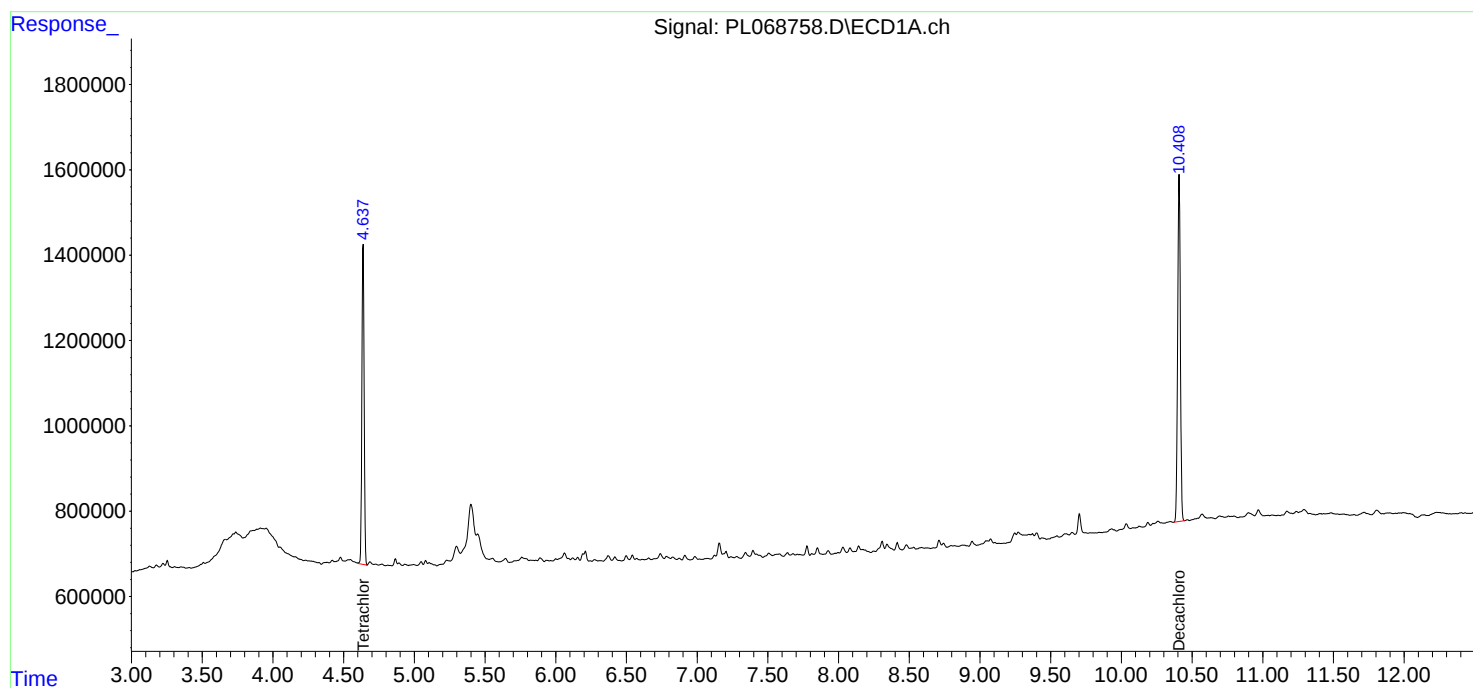


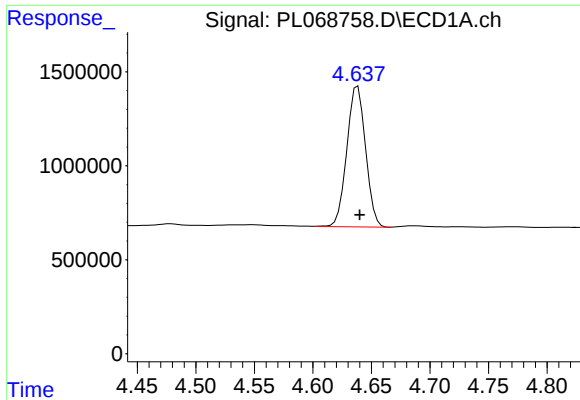

#1 Tetrachloro-m-xylene


R.T.: 4.638 min
Delta R.T.: -0.002 min
Response: 8343130
Conc: 20.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210580-COM-3

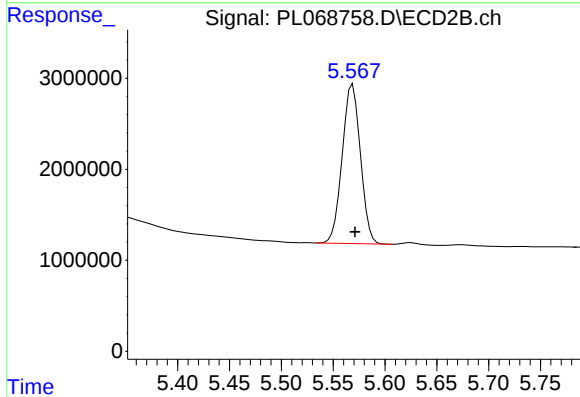


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 21423938
Conc: 21.10 ng/ml

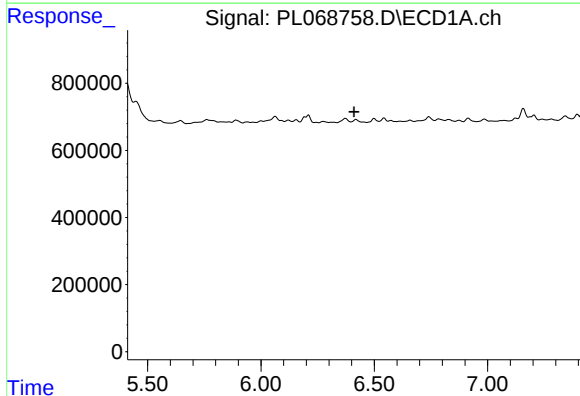


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.411 min
Response: 0
Conc: N.D.

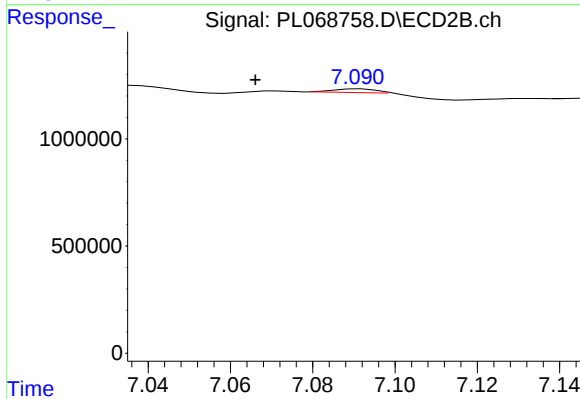

#7 delta-BHC


R.T.: 7.092 min
Delta R.T.: 0.025 min
Response: 104117
Conc: 0.08 ng/ml

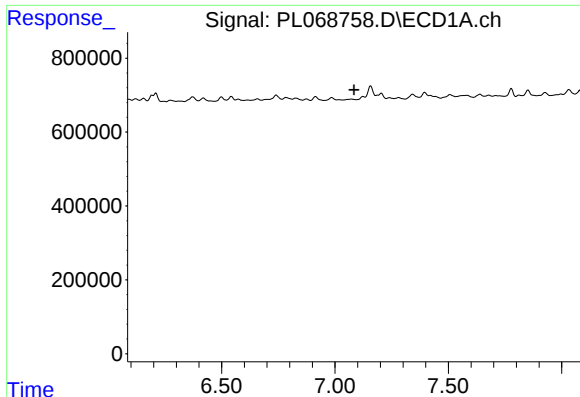

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210580-COM-3

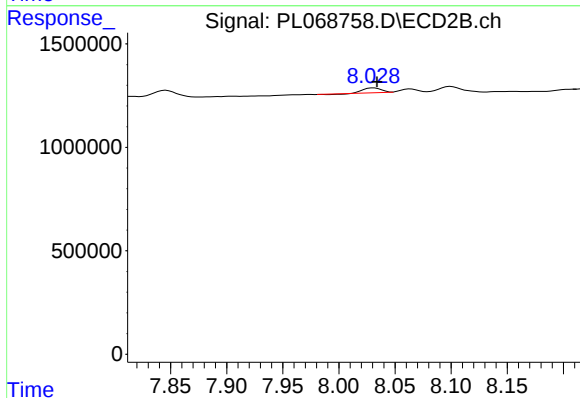


#8 Heptachlor epoxide

R.T.: 8.031 min
Delta R.T.: -0.003 min
Response: 244085
Conc: 0.21 ng/ml

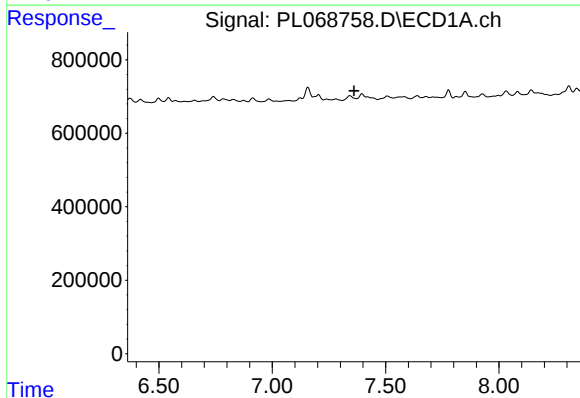


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.361 min
Response: 0
Conc: N.D.

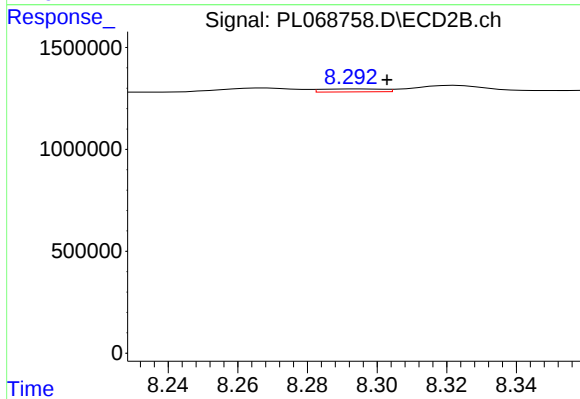

#10 gamma-Chlordane


R.T.: 8.295 min
Delta R.T.: -0.008 min
Response: 174540
Conc: 0.15 ng/ml

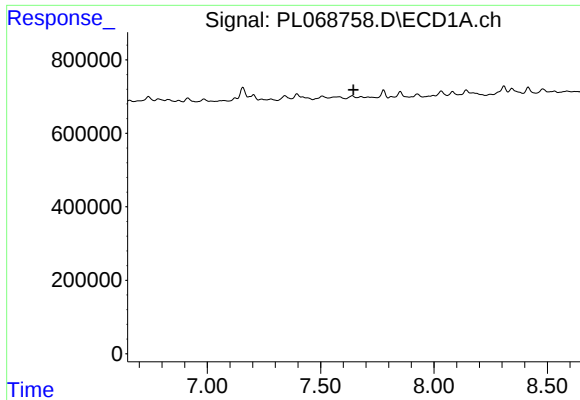

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210580-COM-3

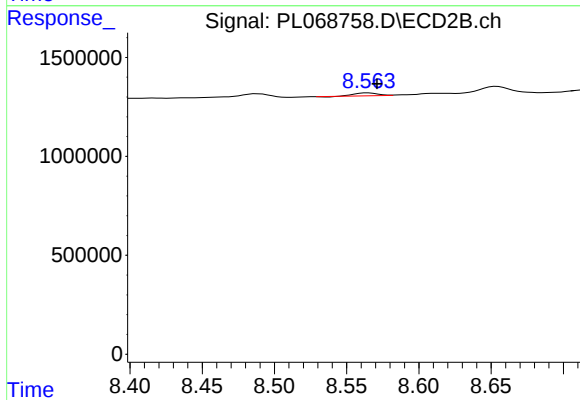


#12 4,4'-DDE

R.T.: 8.565 min
Delta R.T.: -0.006 min
Response: 158291
Conc: 0.15 ng/ml

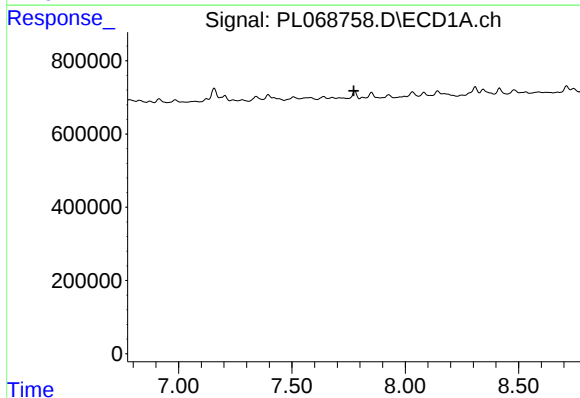


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.774 min
Response: 0
Conc: N.D.

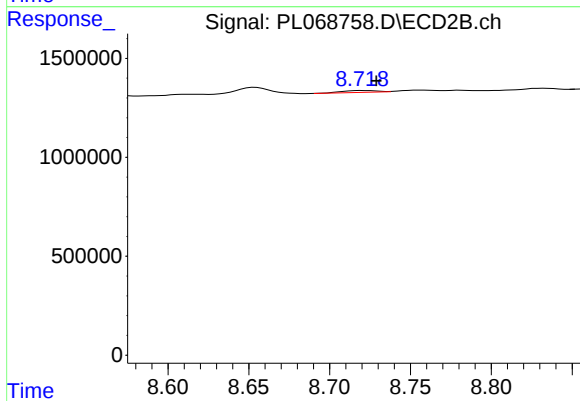

#13 Dieldrin


R.T.: 8.720 min
Delta R.T.: -0.009 min
Response: 140076
Conc: 0.13 ng/ml

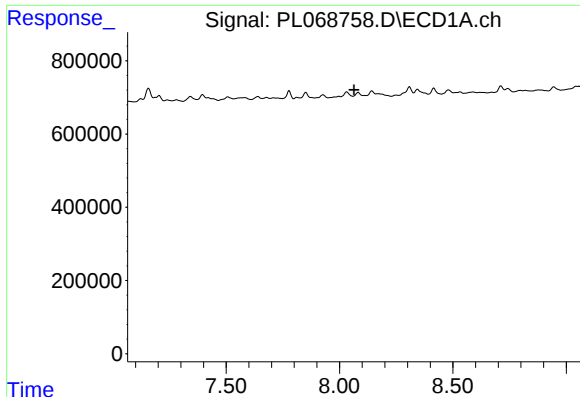

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210580-COM-3

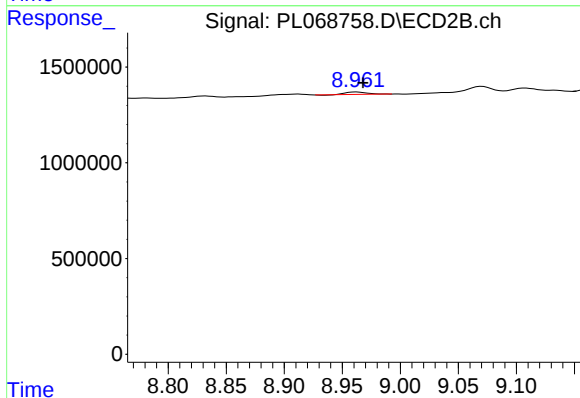


#14 Endrin

R.T.: 8.963 min
Delta R.T.: -0.005 min
Response: 157073
Conc: 0.17 ng/ml

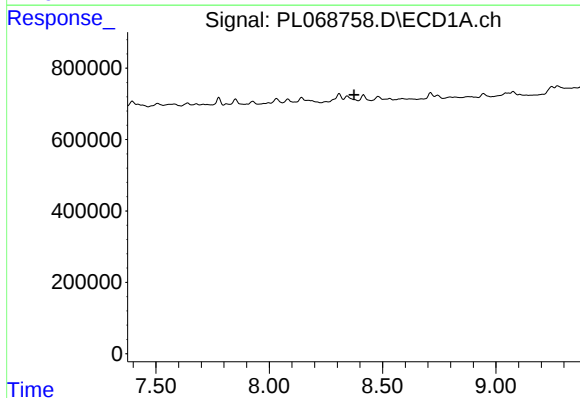


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

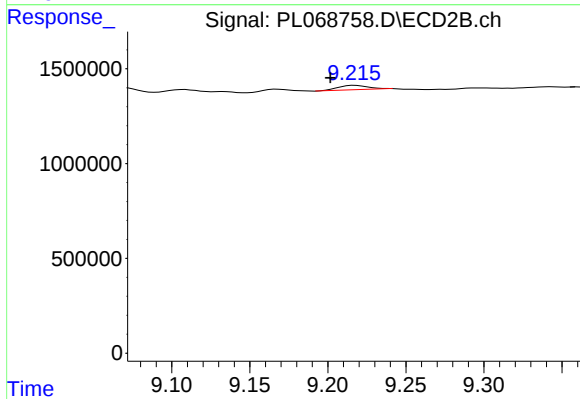

#15 Endosulfan II


R.T.: 9.217 min
Delta R.T.: 0.016 min
Response: 305007
Conc: 0.33 ng/ml

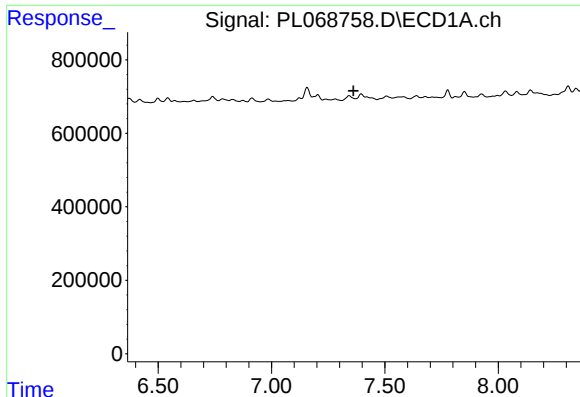

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210580-COM-3

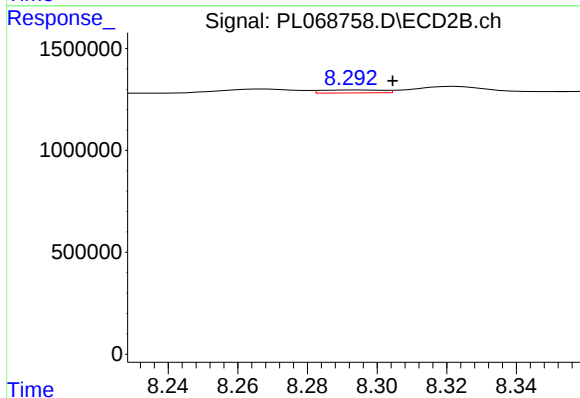


#25 Chlordane-3

R.T.: 8.295 min
Delta R.T.: -0.010 min
Response: 174540
Conc: 1.07 ng/ml

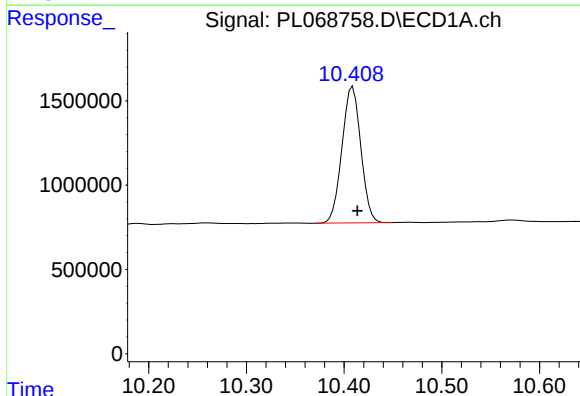

#28 Decachlorobiphenyl

R.T.: 10.409 min
Delta R.T.: -0.005 min
Response: 10869802
Conc: 18.91 ng/ml

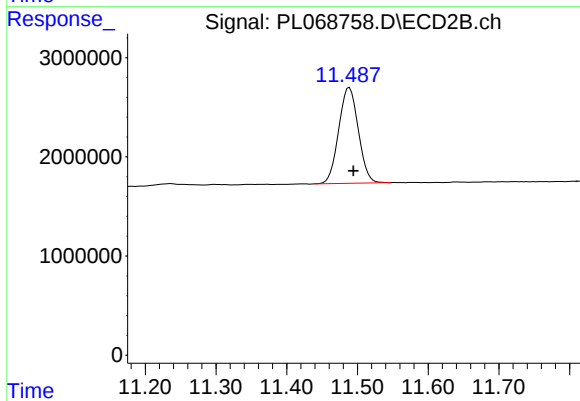

#28 Decachlorobiphenyl

R.T.: 11.489 min
Delta R.T.: -0.006 min
Response: 18633971
Conc: 19.21 ng/ml