

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080522\
 Data File : PL076916.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2022 11:41
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 22:24:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:34:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.424	2.640	46712225	133.7E6	49.068	57.939
28)	SA Decachlor...	8.914	7.748	36478527	90333567	45.905	46.986
Target Compounds							
23)	Chlordane-1	4.585	3.620	16922002	36163868	450.635	453.259
24)	Chlordane-2	5.117	4.192	18334056	42720542	440.342	433.751
25)	Chlordane-3	5.830	4.817	70052392	118.4E6	433.899	429.267
26)	Chlordane-4	5.908	4.878	84686980	122.4E6	431.577	424.237
27)	Chlordane-5	6.765	5.543	14429381	32362224	413.651	423.980


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080522\
Data File : PL076916.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2022 11:41
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 22:24:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:34:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

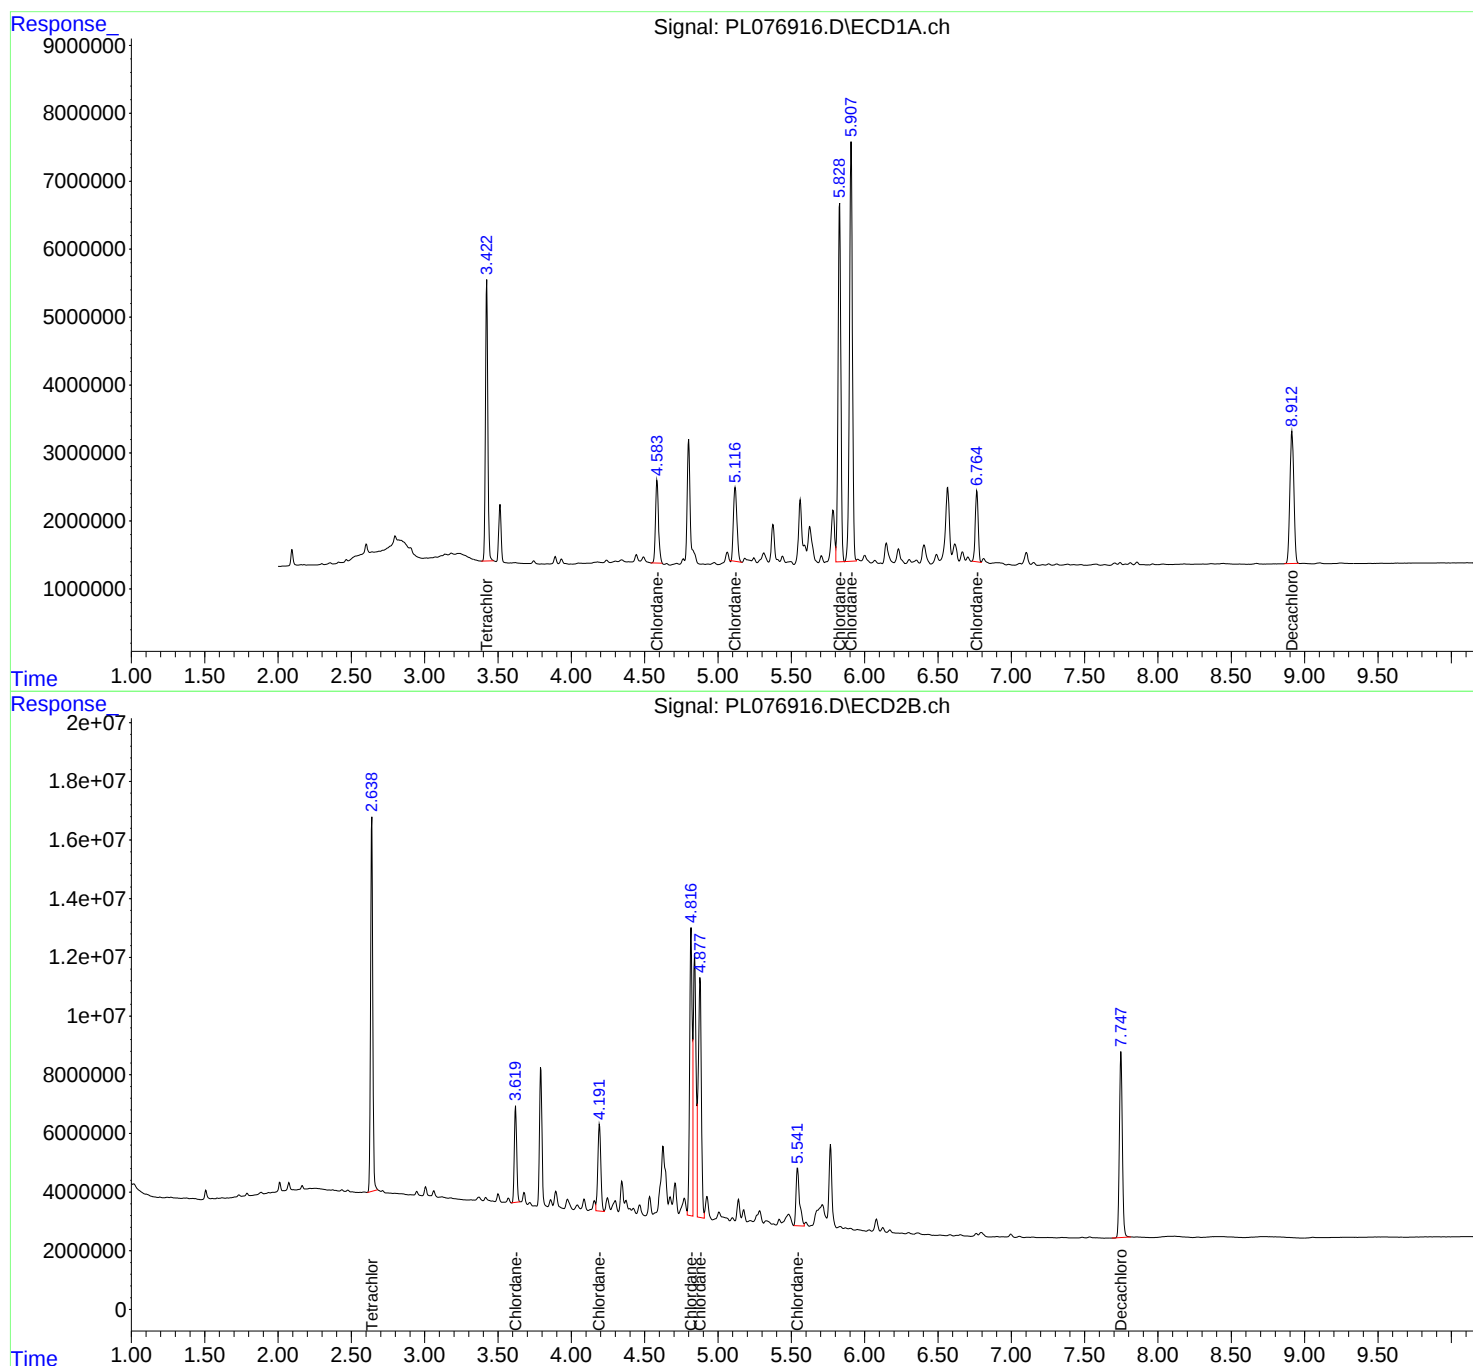


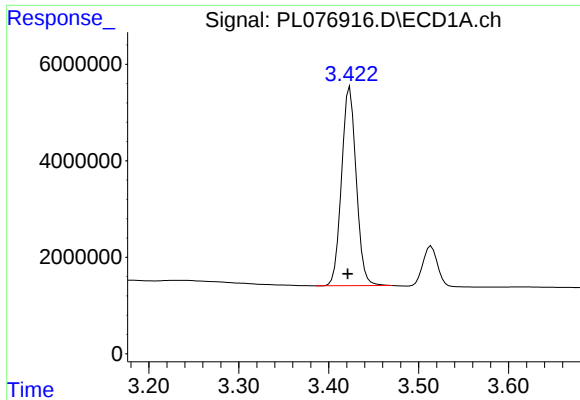

#1 Tetrachloro-m-xylene


R.T.: 3.424 min
Delta R.T.: 0.003 min
Response: 46712225
Conc: 49.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

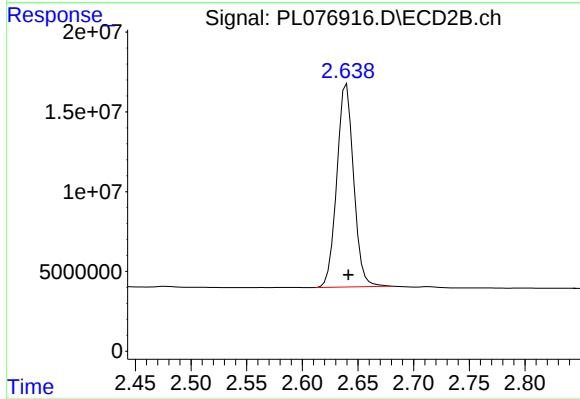


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: -0.002 min
Response: 133731278
Conc: 57.94 ng/ml

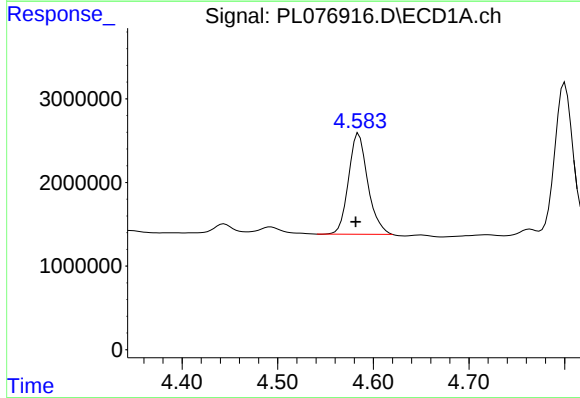


#23 Chlordane-1

R.T.: 4.585 min
Delta R.T.: 0.003 min
Response: 16922002
Conc: 450.63 ng/ml

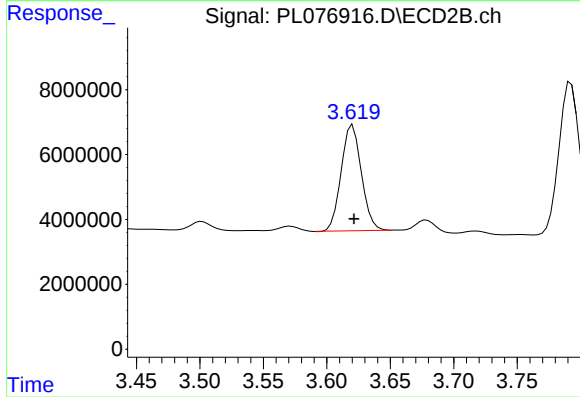

#23 Chlordane-1


R.T.: 3.620 min
Delta R.T.: 0.000 min
Response: 36163868
Conc: 453.26 ng/ml

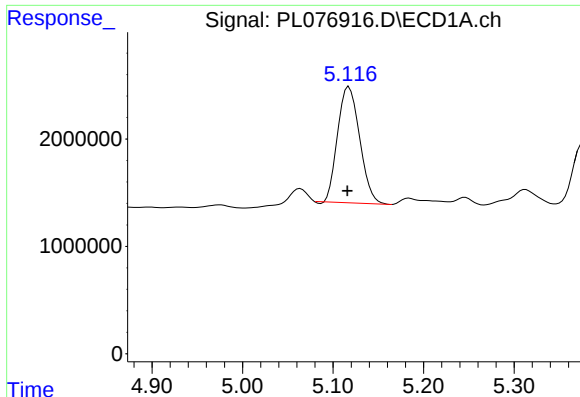

#24 Chlordane-2


R.T.: 5.117 min
Delta R.T.: 0.002 min
Response: 18334056
Conc: 440.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

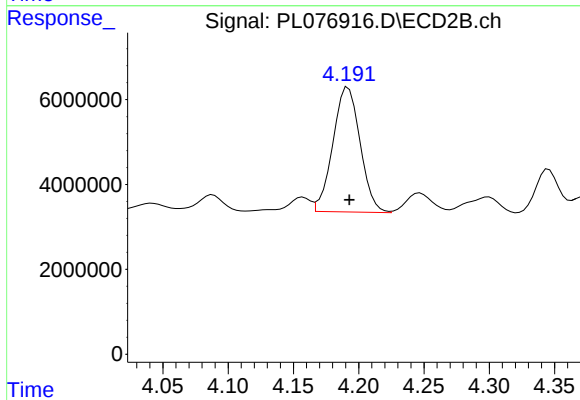


#24 Chlordane-2

R.T.: 4.192 min
Delta R.T.: -0.001 min
Response: 42720542
Conc: 433.75 ng/ml

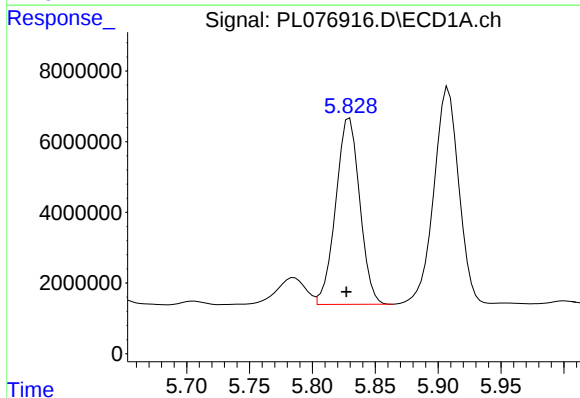


#25 Chlordane-3

R.T.: 5.830 min
Delta R.T.: 0.003 min
Response: 70052392
Conc: 433.90 ng/ml

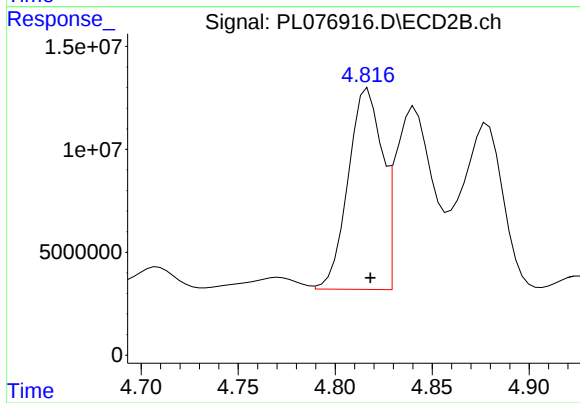

#25 Chlordane-3


R.T.: 4.817 min
Delta R.T.: -0.001 min
Response: 118378426
Conc: 429.27 ng/ml

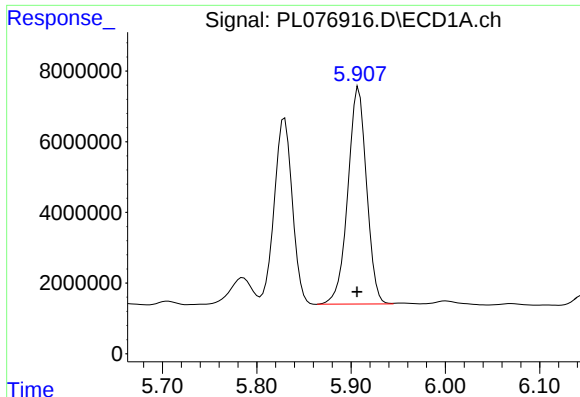

#26 Chlordane-4


R.T.: 5.908 min
Delta R.T.: 0.002 min
Response: 84686980
Conc: 431.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

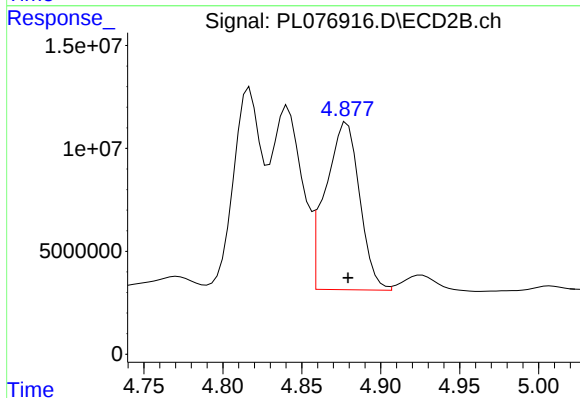


#26 Chlordane-4

R.T.: 4.878 min
Delta R.T.: 0.000 min
Response: 122376348
Conc: 424.24 ng/ml

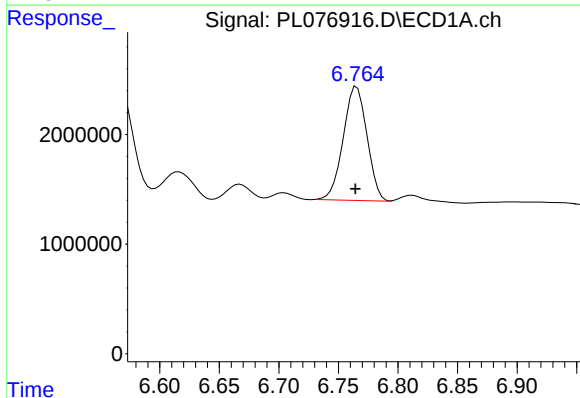


#27 Chlordane-5

R.T.: 6.765 min
Delta R.T.: 0.001 min
Response: 14429381
Conc: 413.65 ng/ml

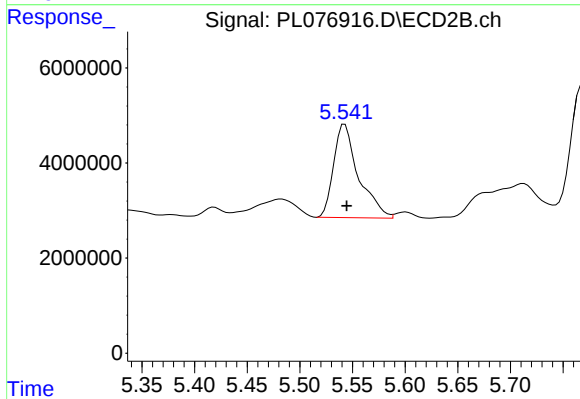

#27 Chlordane-5


R.T.: 5.543 min
Delta R.T.: -0.002 min
Response: 32362224
Conc: 423.98 ng/ml

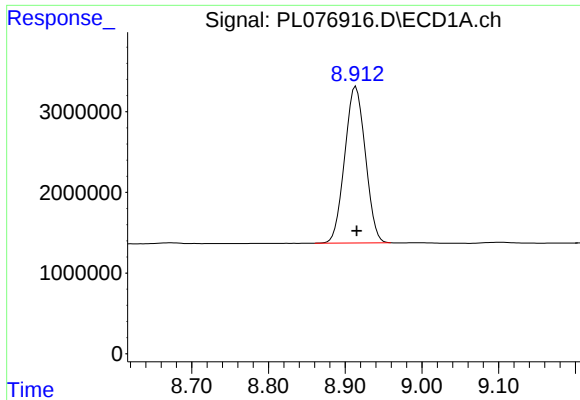

#28 Decachlorobiphenyl

R.T.: 8.914 min
Delta R.T.: -0.001 min
Response: 36478527
Conc: 45.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

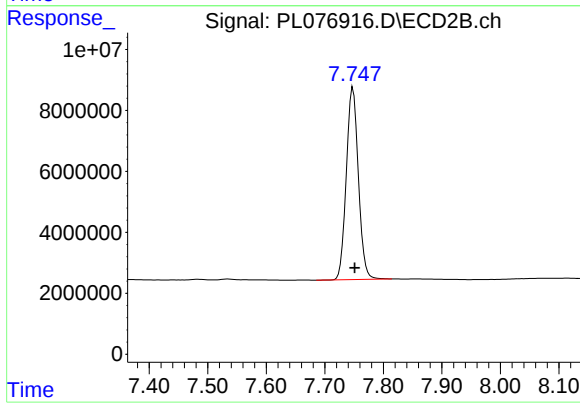

#28 Decachlorobiphenyl

R.T.: 7.748 min
Delta R.T.: -0.003 min
Response: 90333567
Conc: 46.99 ng/ml