

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080522\
 Data File : PL076921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2022 13:19
 Operator : AR\AJ
 Sample : PB146770BS
 Misc : CHLOR BS
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB146770BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 13:33:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:34:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.640	18616536	53925766	19.555	23.363
28)	SA Decachlor...	8.912	7.747	16245216	40102976	20.443	20.859
Target Compounds							
23)	Chlordane-1	4.582	3.620	6841220	14741347	182.183	184.760
24)	Chlordane-2	5.115	4.191	7789540	17919185	187.087	181.937
25)	Chlordane-3	5.826	4.816	27413807	46853110	169.799	169.900
26)	Chlordane-4	5.905	4.878	33870758	49132081	172.610	170.324
27)	Chlordane-5	6.763	5.542	5686991	13996188	163.030	183.365



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080522\
Data File : PL076921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2022 13:19
Operator : AR\AJ
Sample : PB146770BS
Misc : CHLOR BS
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB146770BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 13:33:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:34:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

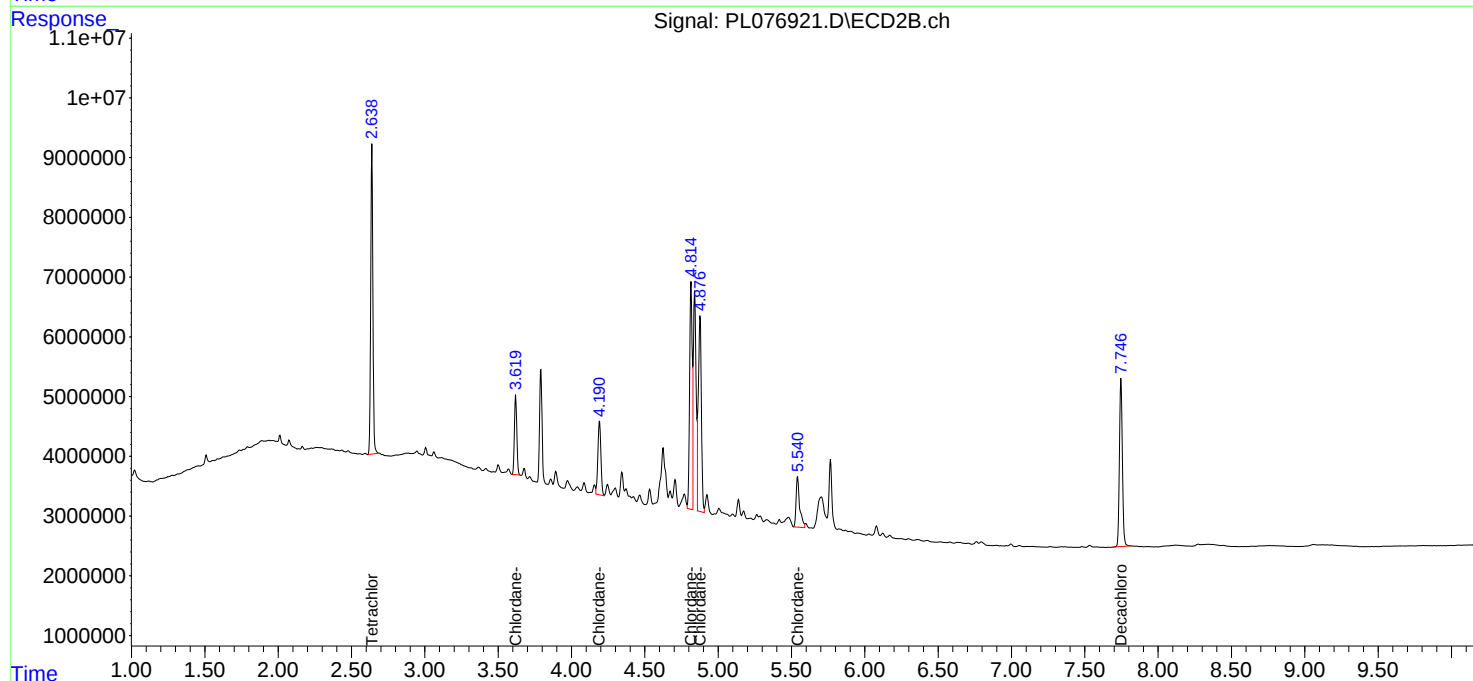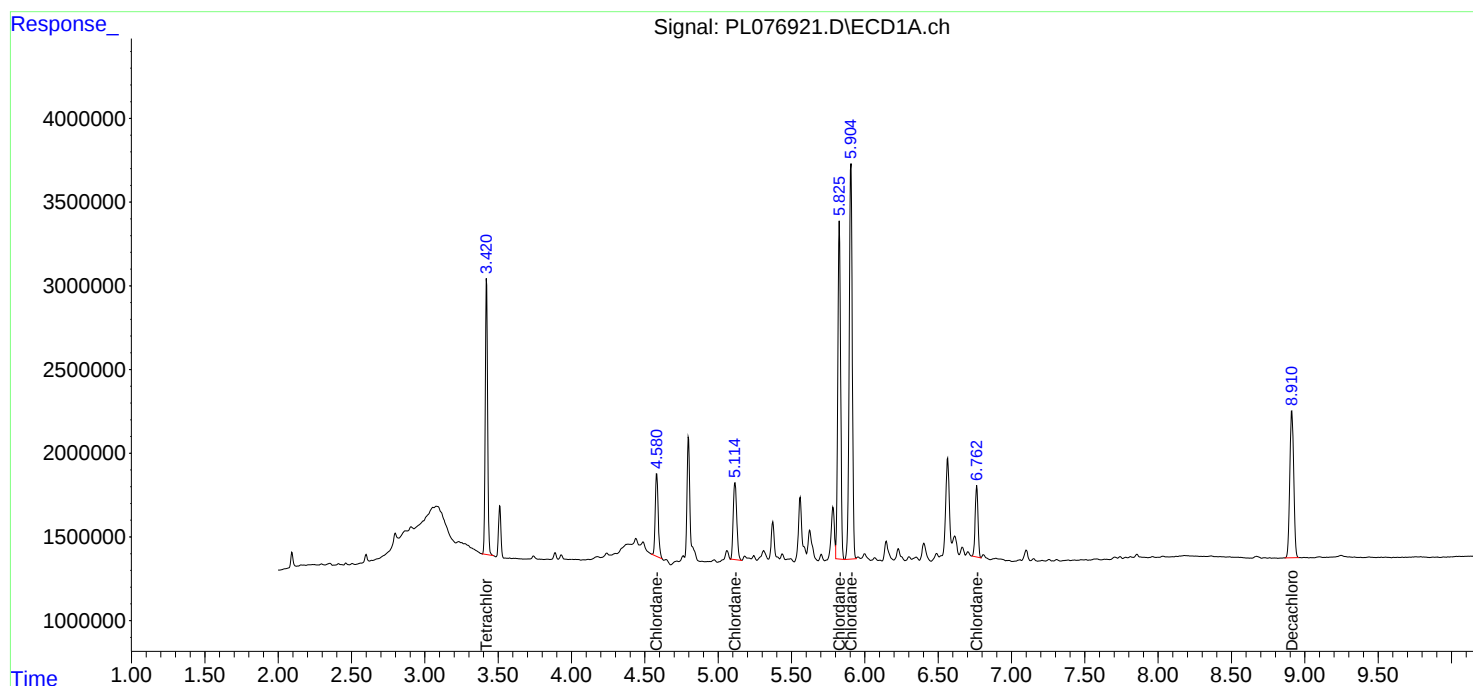


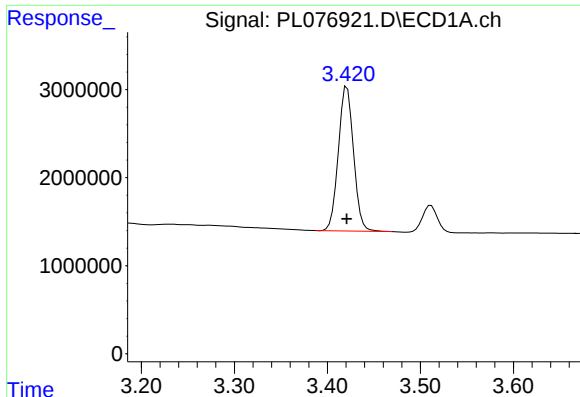

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 18616536
Conc: 19.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB146770BS

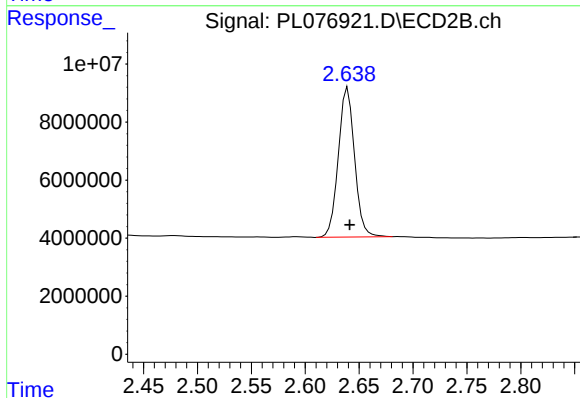


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: -0.002 min
Response: 53925766
Conc: 23.36 ng/ml

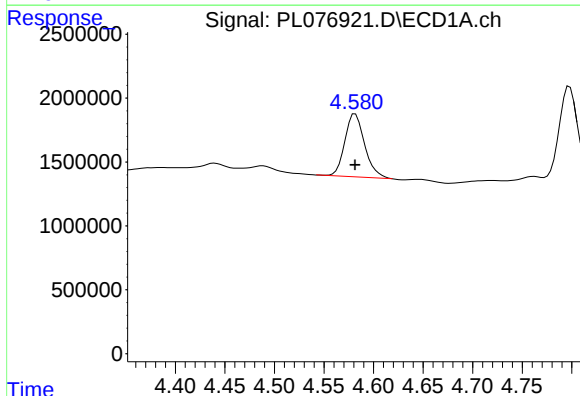


#23 Chlordane-1

R.T.: 4.582 min
Delta R.T.: 0.000 min
Response: 6841220
Conc: 182.18 ng/ml

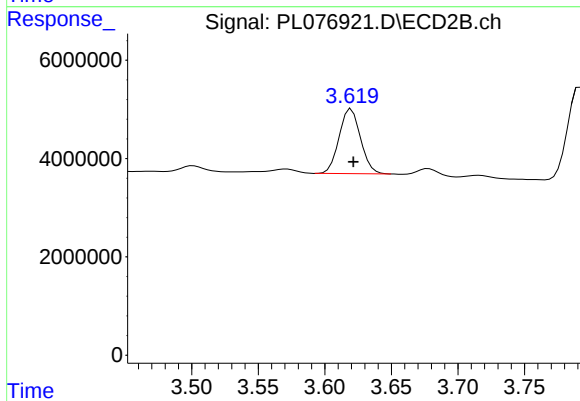

#23 Chlordane-1


R.T.: 3.620 min
Delta R.T.: -0.001 min
Response: 14741347
Conc: 184.76 ng/ml

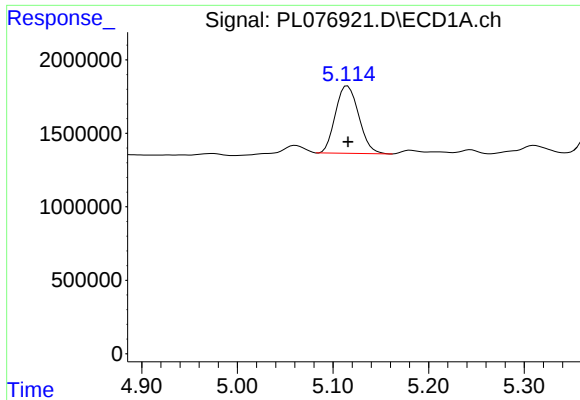

#24 Chlordane-2


R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 7789540
Conc: 187.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB146770BS

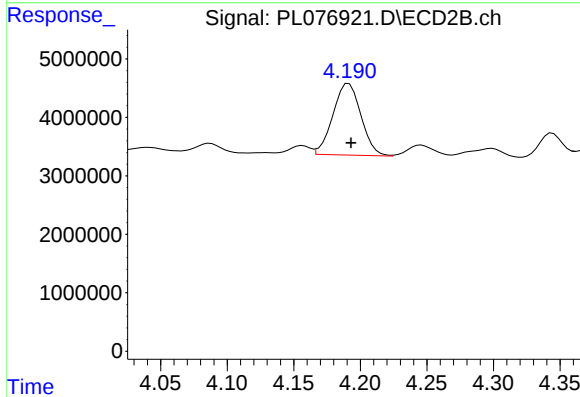


#24 Chlordane-2

R.T.: 4.191 min
Delta R.T.: -0.002 min
Response: 17919185
Conc: 181.94 ng/ml

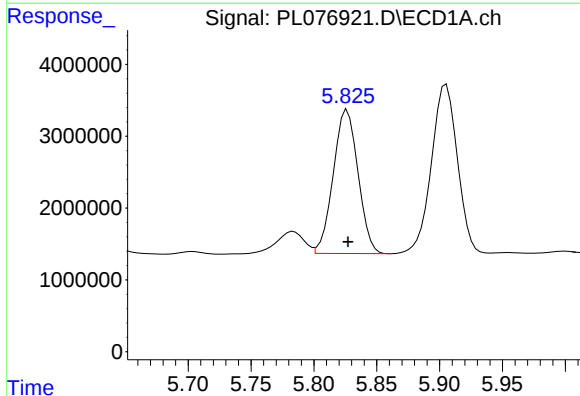


#25 Chlordane-3

R.T.: 5.826 min
Delta R.T.: 0.000 min
Response: 27413807
Conc: 169.80 ng/ml

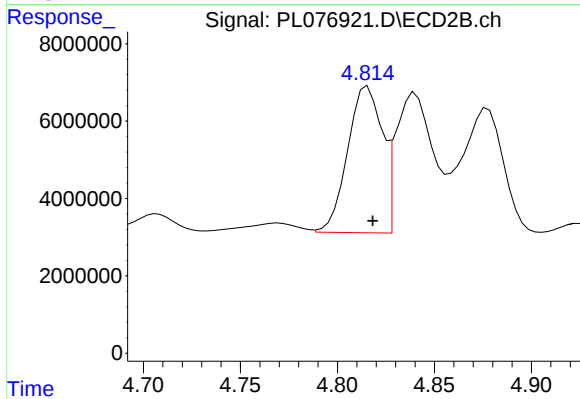

#25 Chlordane-3


R.T.: 4.816 min
Delta R.T.: -0.003 min
Response: 46853110
Conc: 169.90 ng/ml

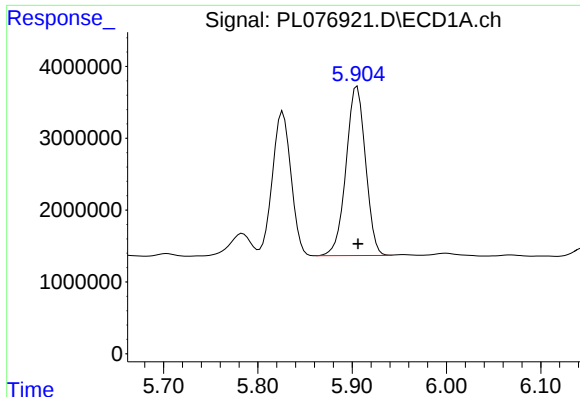

#26 Chlordane-4


R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 33870758
Conc: 172.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB146770BS

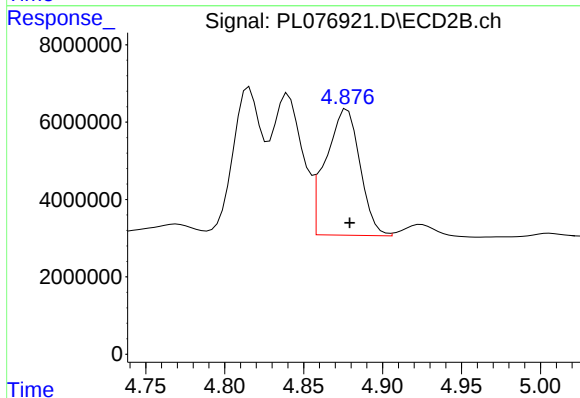


#26 Chlordane-4

R.T.: 4.878 min
Delta R.T.: -0.002 min
Response: 49132081
Conc: 170.32 ng/ml

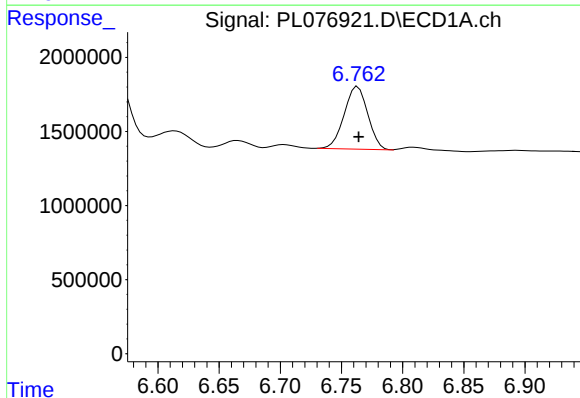


#27 Chlordane-5

R.T.: 6.763 min
Delta R.T.: 0.000 min
Response: 5686991
Conc: 163.03 ng/ml

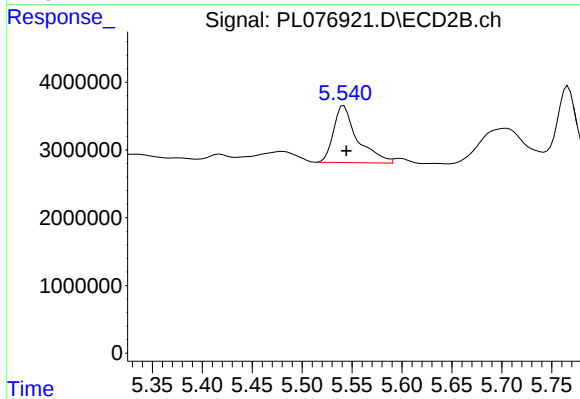

#27 Chlordane-5


R.T.: 5.542 min
Delta R.T.: -0.003 min
Response: 13996188
Conc: 183.37 ng/ml

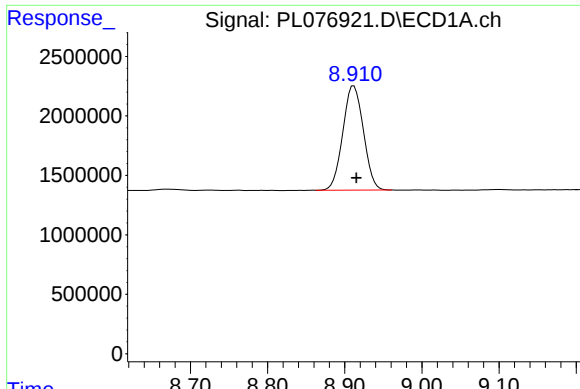

#28 Decachlorobiphenyl

R.T.: 8.912 min
Delta R.T.: -0.003 min
Response: 16245216
Conc: 20.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB146770BS

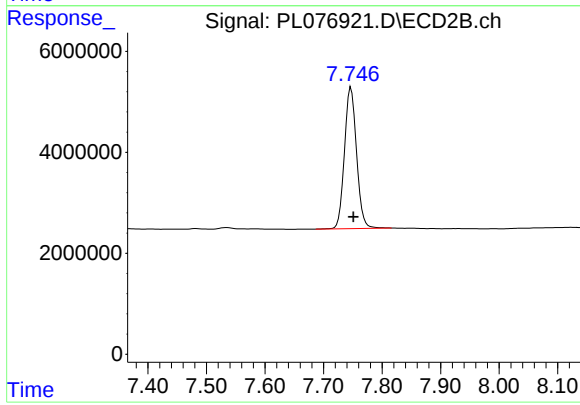

#28 Decachlorobiphenyl

R.T.: 7.747 min
Delta R.T.: -0.004 min
Response: 40102976
Conc: 20.86 ng/ml