

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080522\
 Data File : PL076927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2022 14:43
 Operator : AR\AJ
 Sample : M3980-09
 Misc : CHLOR MDL 25 PPB
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 03:46:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:34:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.640	16754669	41609649	17.600	18.027
28)	SA Decachlor...	8.912	7.747	15819501	37881459	19.907	19.704
Target Compounds							
23)	Chlordane-1	4.580	3.619	622405	1552879	16.575	19.463
24)	Chlordane-2	5.114	4.190	763148	2090914	18.329	21.229
25)	Chlordane-3	5.826	4.815	3012478	5211841	18.659	18.899
26)	Chlordane-4	5.905	4.876	3792028	5384370	19.325	18.666
27)	Chlordane-5	6.764	5.541	537419	1637082	15.406	21.448 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080522\
Data File : PL076927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2022 14:43
Operator : AR\AJ
Sample : M3980-09
Misc : CHLOR MDL 25 PPB
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 03:46:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:34:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

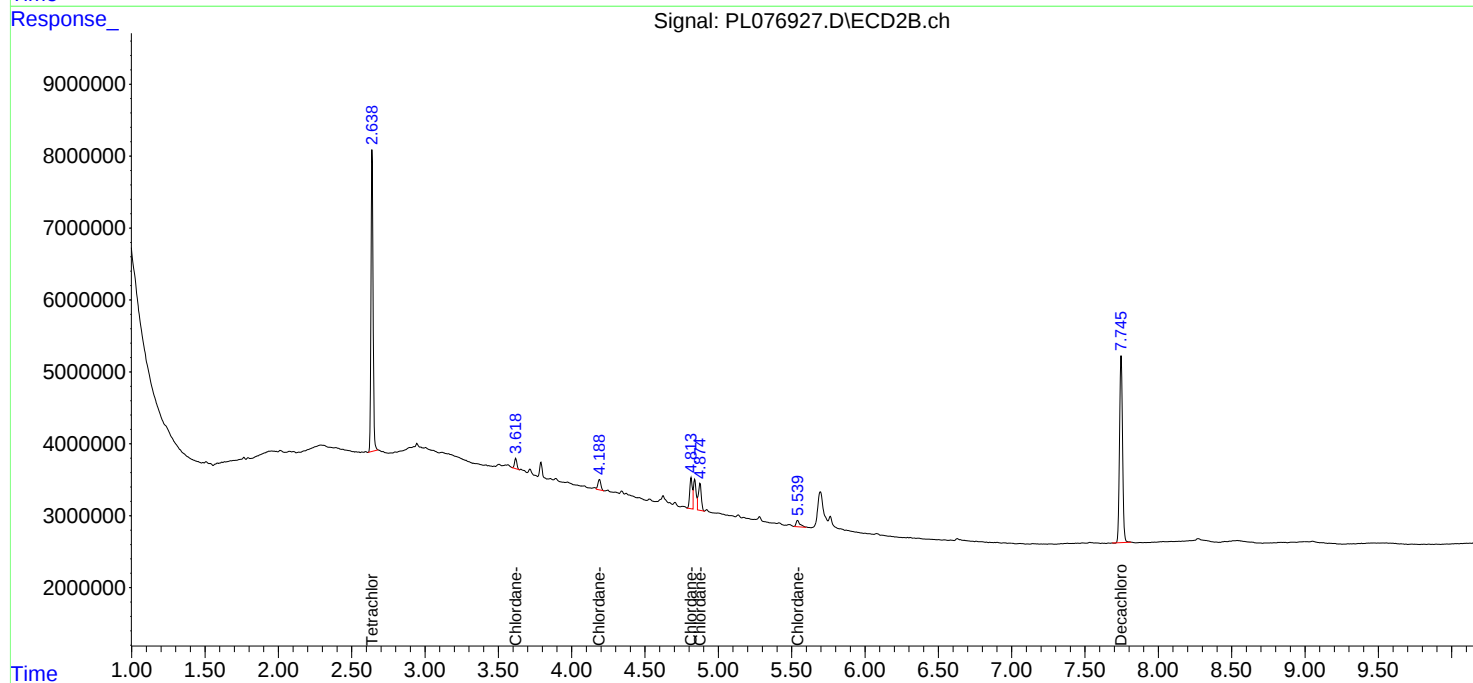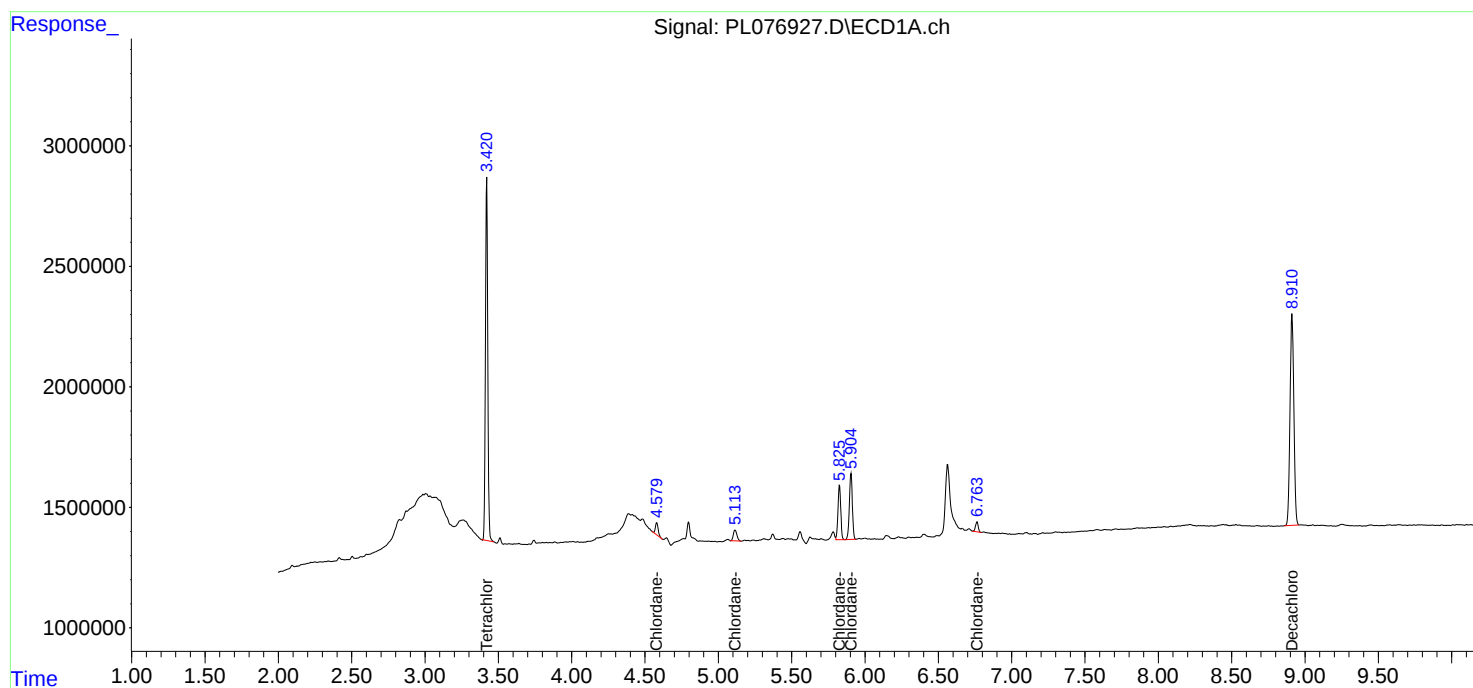


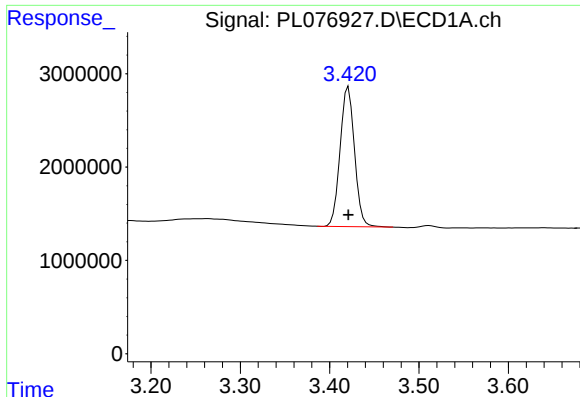

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 16754669
Conc: 17.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-WATER-03-QT3-2022

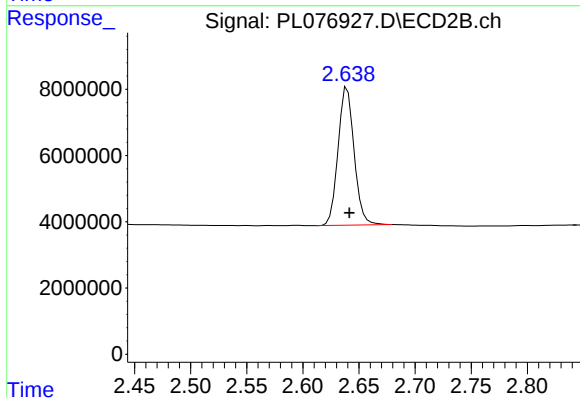


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: -0.002 min
Response: 41609649
Conc: 18.03 ng/ml

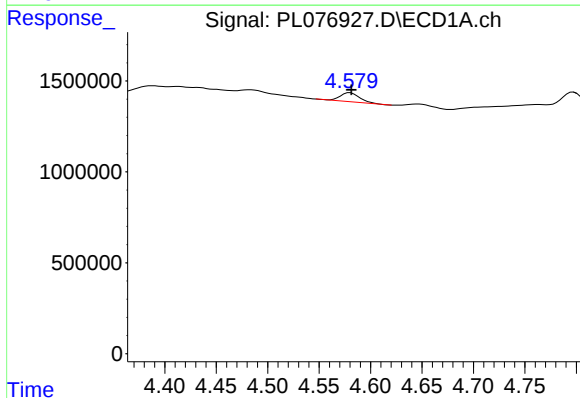


#23 Chlordane-1

R.T.: 4.580 min
Delta R.T.: -0.001 min
Response: 622405
Conc: 16.57 ng/ml

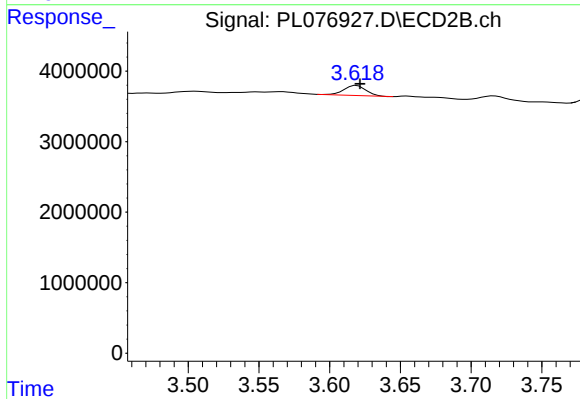

#23 Chlordane-1


R.T.: 3.619 min
Delta R.T.: -0.002 min
Response: 1552879
Conc: 19.46 ng/ml

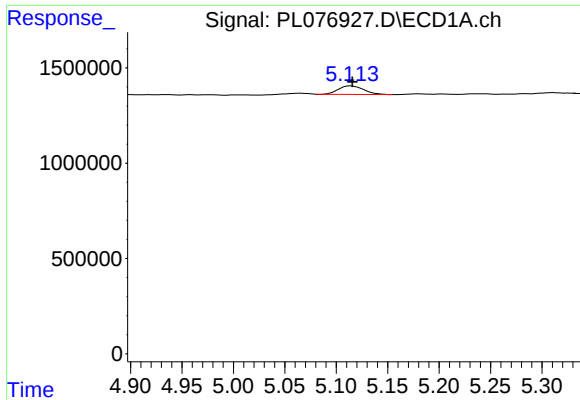

#24 Chlordane-2


R.T.: 5.114 min
Delta R.T.: -0.002 min
Response: 763148
Conc: 18.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-WATER-03-QT3-2022

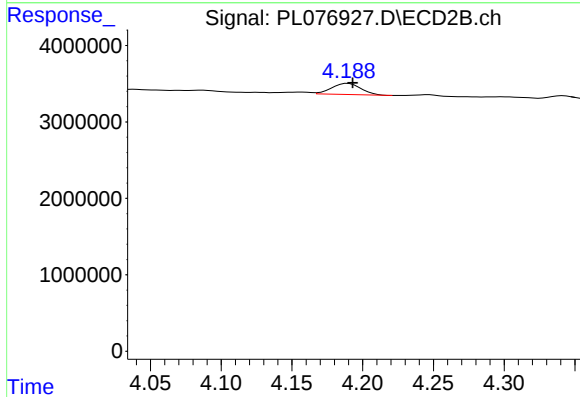


#24 Chlordane-2

R.T.: 4.190 min
Delta R.T.: -0.003 min
Response: 2090914
Conc: 21.23 ng/ml

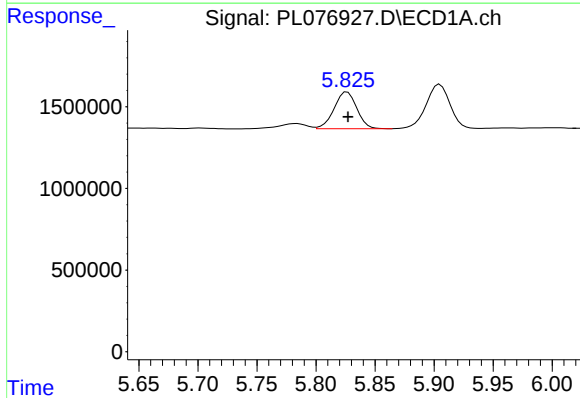


#25 Chlordane-3

R.T.: 5.826 min
Delta R.T.: 0.000 min
Response: 3012478
Conc: 18.66 ng/ml

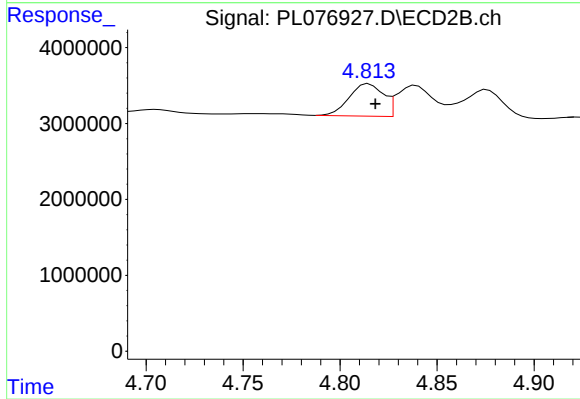

#25 Chlordane-3


R.T.: 4.815 min
Delta R.T.: -0.003 min
Response: 5211841
Conc: 18.90 ng/ml

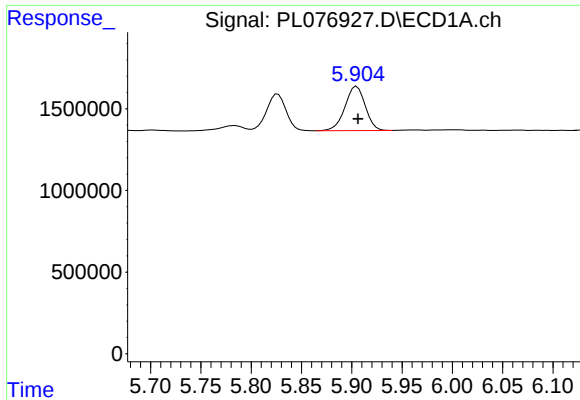

#26 Chlordane-4


R.T.: 5.905 min
Delta R.T.: -0.001 min
Response: 3792028
Conc: 19.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-WATER-03-QT3-2022

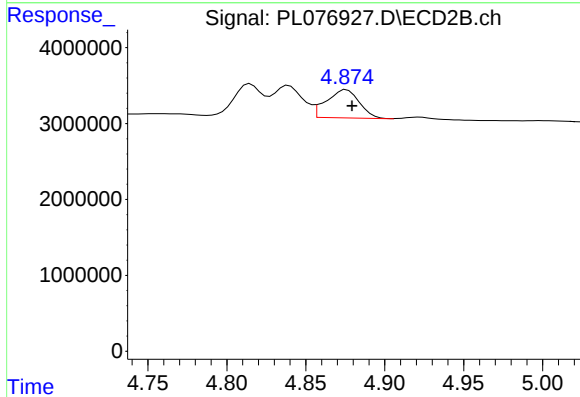


#26 Chlordane-4

R.T.: 4.876 min
Delta R.T.: -0.003 min
Response: 5384370
Conc: 18.67 ng/ml

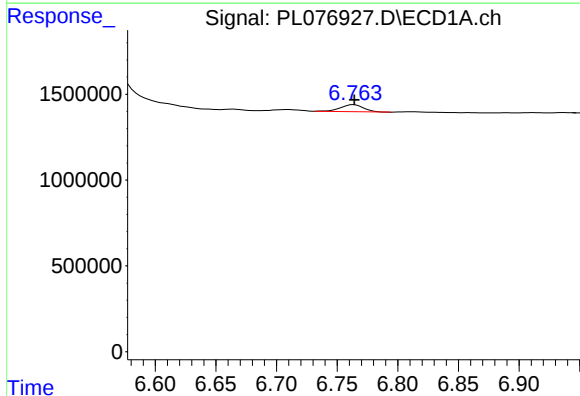


#27 Chlordane-5

R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 537419
Conc: 15.41 ng/ml

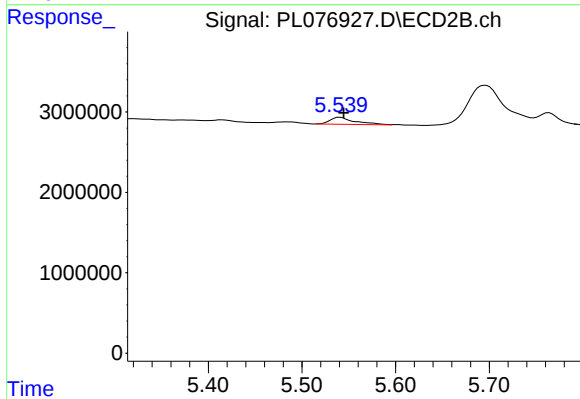

#27 Chlordane-5


R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 1637082
Conc: 21.45 ng/ml

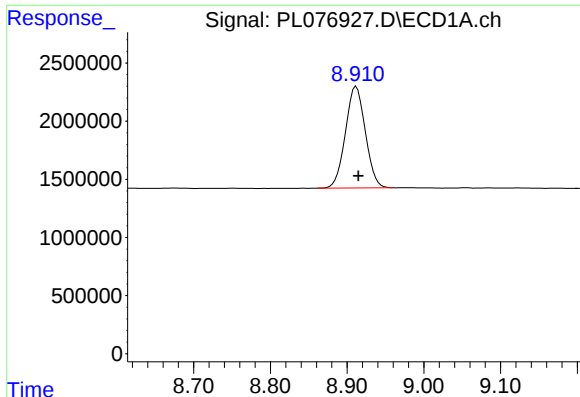

#28 Decachlorobiphenyl

R.T.: 8.912 min
Delta R.T.: -0.003 min
Response: 15819501
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-WATER-03-QT3-2022

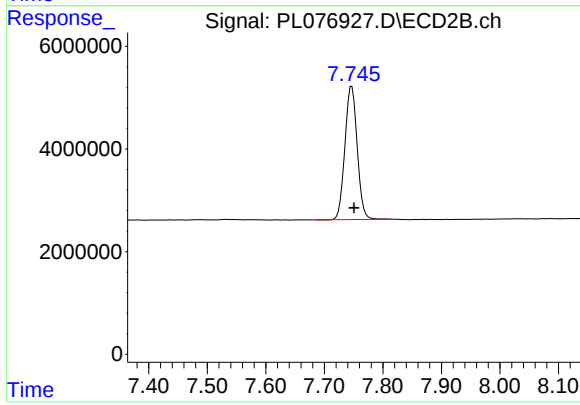

#28 Decachlorobiphenyl

R.T.: 7.747 min
Delta R.T.: -0.004 min
Response: 37881459
Conc: 19.70 ng/ml