

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080522\
 Data File : PL076941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2022 18:54
 Operator : AR\AJ
 Sample : N4044-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-241

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 02:09:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:34:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.638	8959731	23585937	9.412	10.219
28)	SA Decachlor...	8.904	7.740	5088748	14339247	6.404	7.458
Target Compounds							
12)	B 4,4'-DDE	6.079	5.067	409504	1067968	0.434	0.459



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080522\
Data File : PL076941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2022 18:54
Operator : AR\AJ
Sample : N4044-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VNJ-241

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 02:09:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:34:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

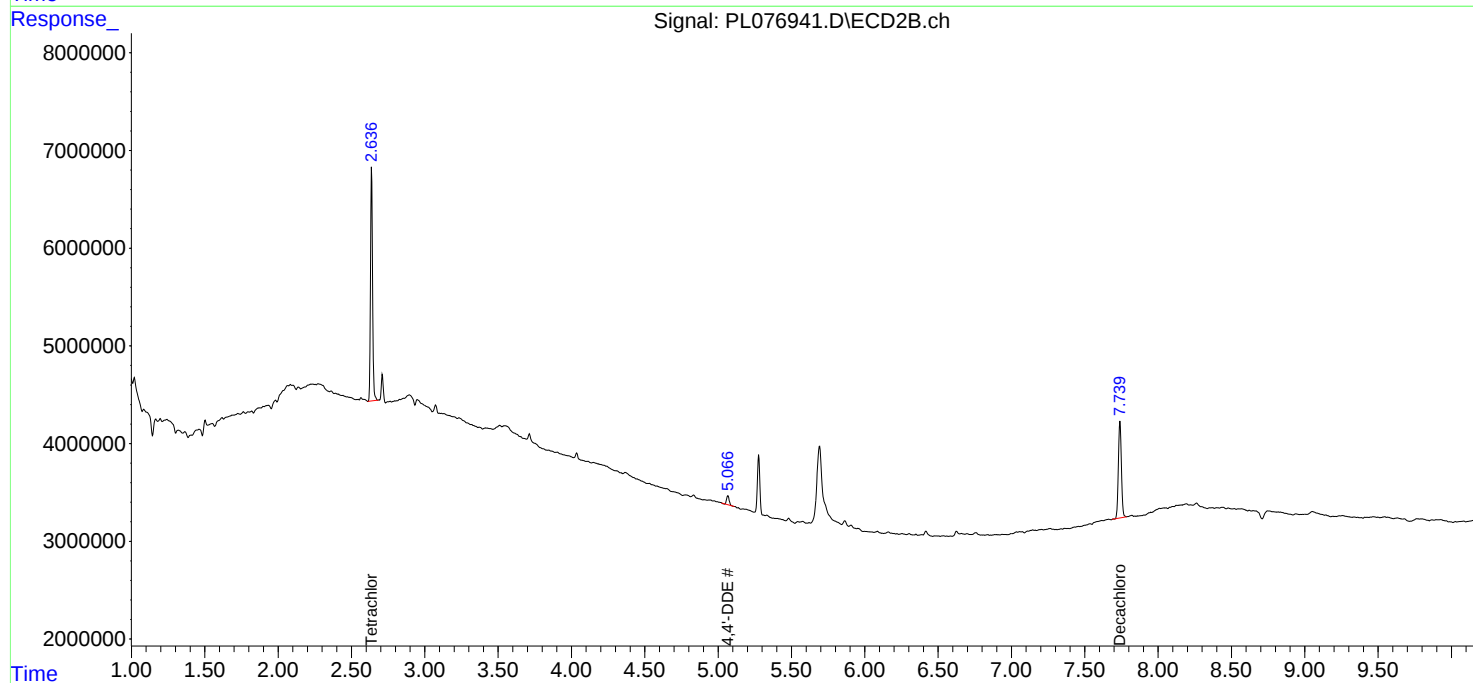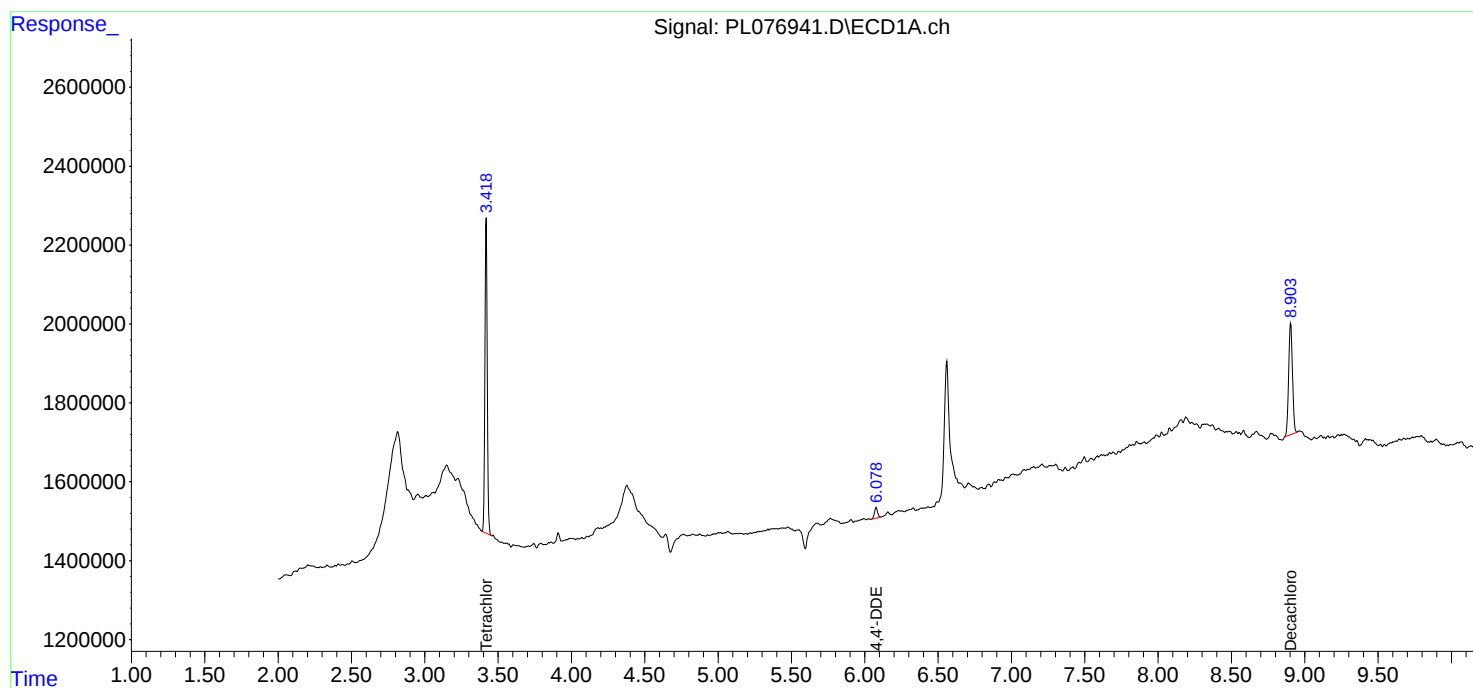


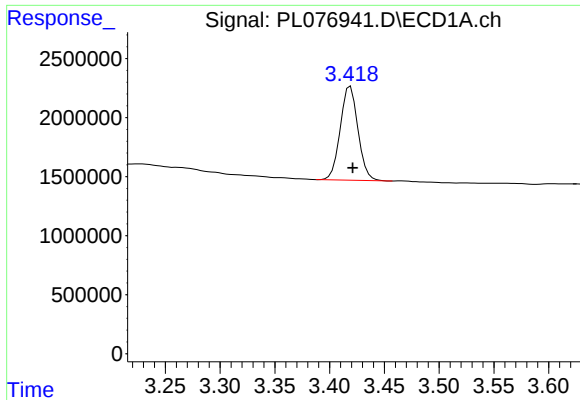

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: -0.002 min
Response: 8959731
Conc: 9.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-241

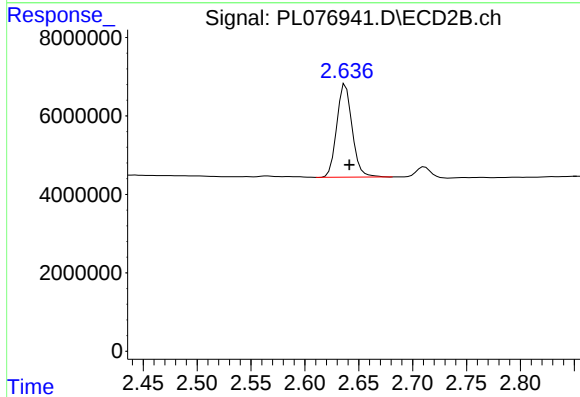


#1 Tetrachloro-m-xylene

R.T.: 2.638 min
Delta R.T.: -0.004 min
Response: 23585937
Conc: 10.22 ng/ml

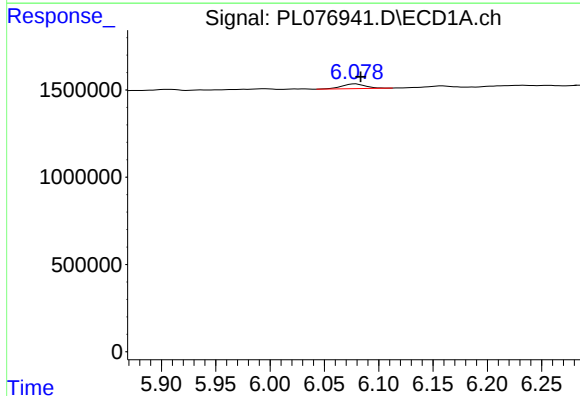


#12 4,4'-DDE

R.T.: 6.079 min
Delta R.T.: -0.005 min
Response: 409504
Conc: 0.43 ng/ml

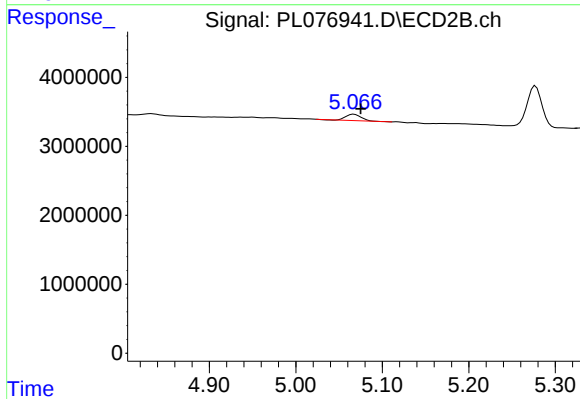

#12 4,4'-DDE


R.T.: 5.067 min
Delta R.T.: -0.008 min
Response: 1067968
Conc: 0.46 ng/ml

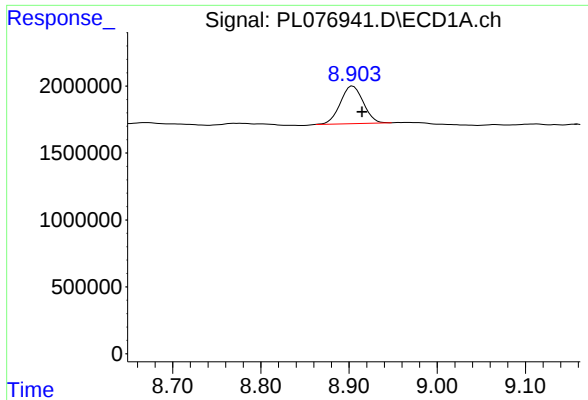

#28 Decachlorobiphenyl

R.T.: 8.904 min
Delta R.T.: -0.011 min
Response: 5088748
Conc: 6.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-241

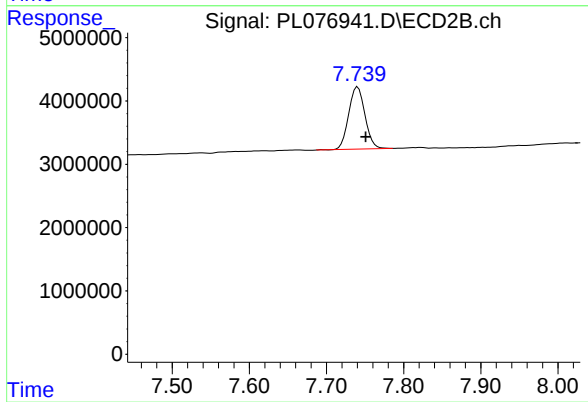

#28 Decachlorobiphenyl

R.T.: 7.740 min
Delta R.T.: -0.011 min
Response: 14339247
Conc: 7.46 ng/ml