

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080524\
 Data File : PL090777.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2024 16:16
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 17:42:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 05 17:39:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.785	185.1E6	214.2E6	100.617	102.264
28)	SA Decachlor...	9.054	7.926	127.7E6	159.8E6	97.083	98.400
Target Compounds							
23)	Chlordane-1	4.705	3.785	86246208	66890412	987.273	1019.334
24)	Chlordane-2	5.234	4.362	91797504	77224324	972.481	990.120
25)	Chlordane-3	5.944	4.992	312.7E6	232.3E6	1000.870	1027.658
26)	Chlordane-4	6.026	5.055	382.9E6	218.0E6	997.168	1018.705
27)	Chlordane-5	6.874	5.720	78566456	62611264	973.168	1002.254



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080524\
Data File : PL090777.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2024 16:16
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 17:42:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
Quant Title : GC Extractables
QLast Update : Mon Aug 05 17:39:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

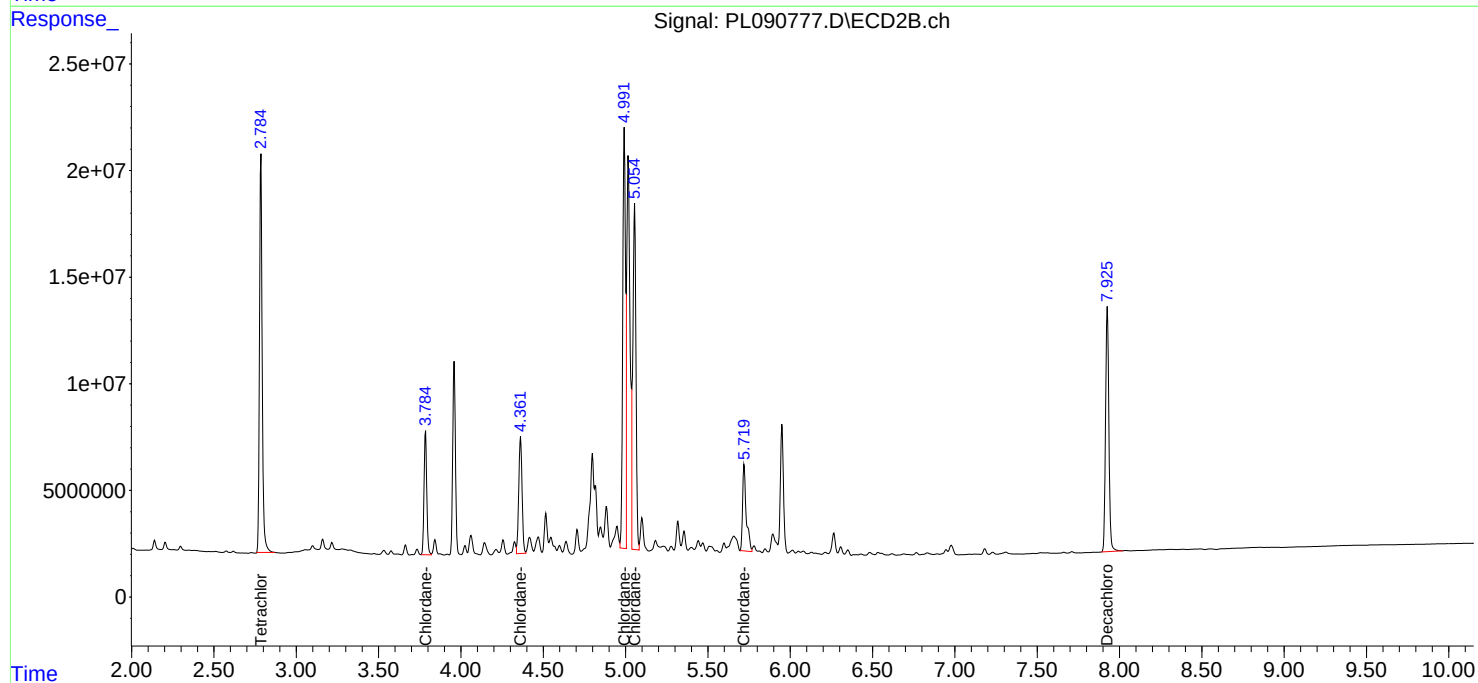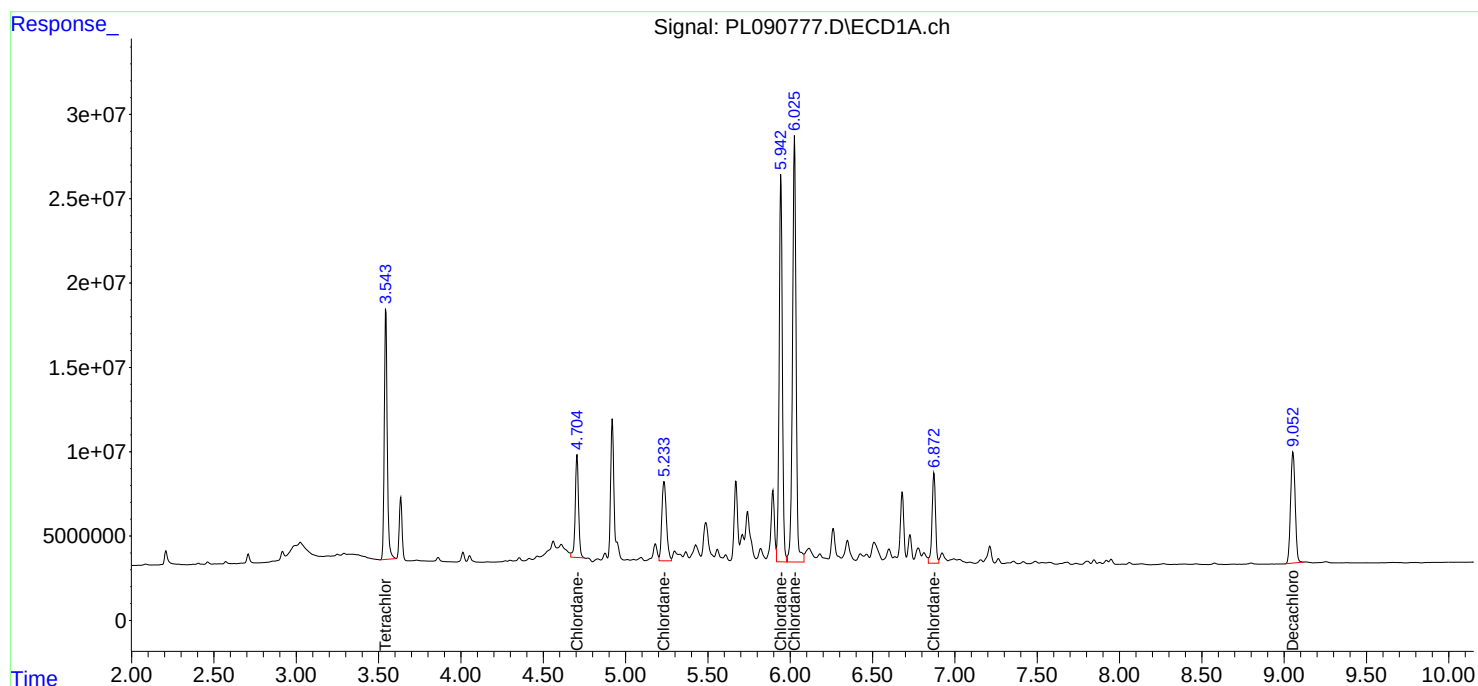


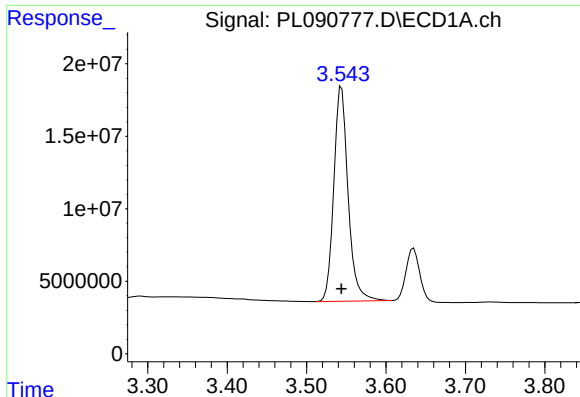

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 185140034
Conc: 100.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

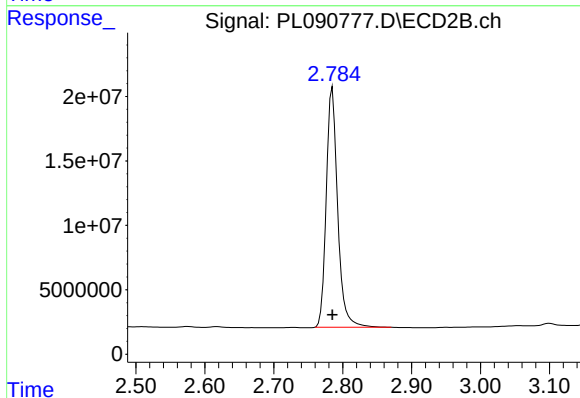


#1 Tetrachloro-m-xylene

R.T.: 2.785 min
Delta R.T.: 0.000 min
Response: 214172720
Conc: 102.26 ng/ml

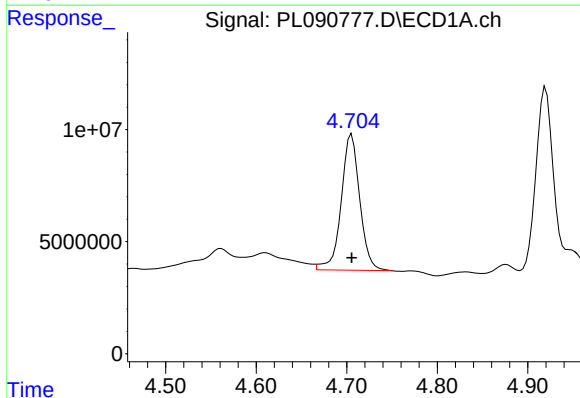


#23 Chlordane-1

R.T.: 4.705 min
Delta R.T.: 0.000 min
Response: 86246208
Conc: 987.27 ng/ml

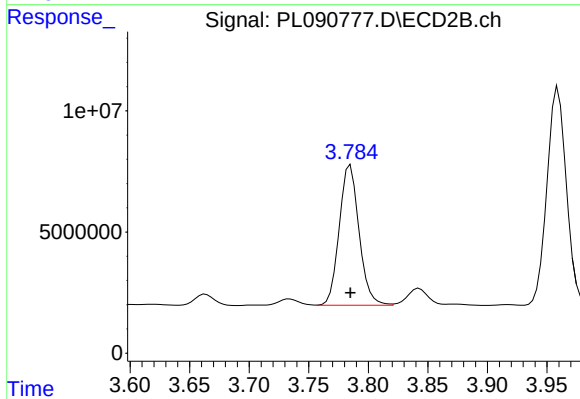

#23 Chlordane-1


R.T.: 3.785 min
Delta R.T.: 0.000 min
Response: 66890412
Conc: 1019.33 ng/ml

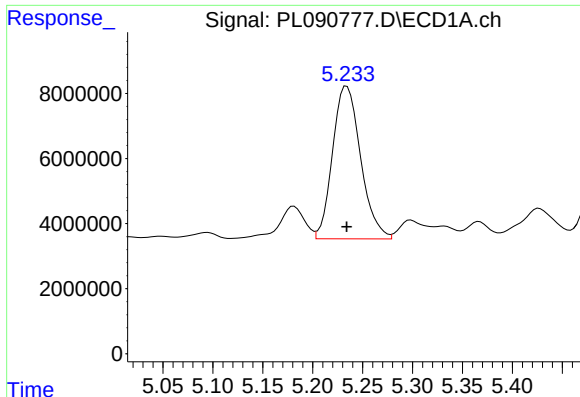

#24 Chlordane-2


R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 91797504
Conc: 972.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

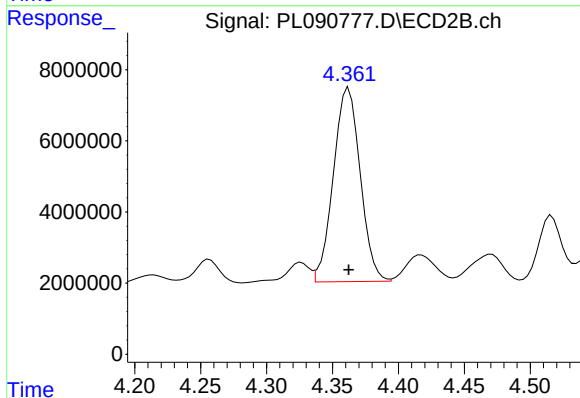


#24 Chlordane-2

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 77224324
Conc: 990.12 ng/ml

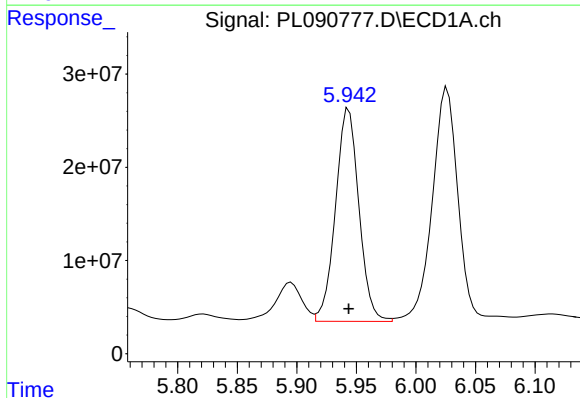


#25 Chlordane-3

R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 312681051
Conc: 1000.87 ng/ml

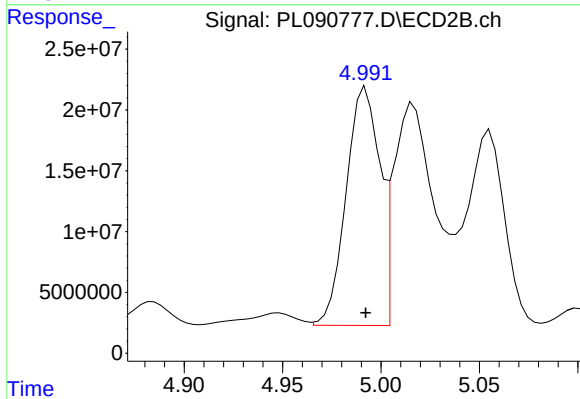

#25 Chlordane-3


R.T.: 4.992 min
Delta R.T.: 0.000 min
Response: 232333853
Conc: 1027.66 ng/ml

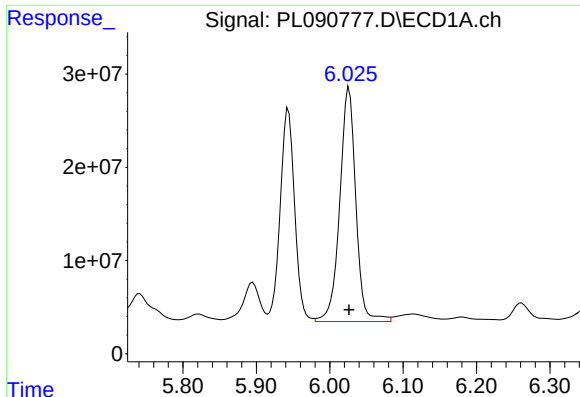

#26 Chlordane-4


R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 382881387
Conc: 997.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

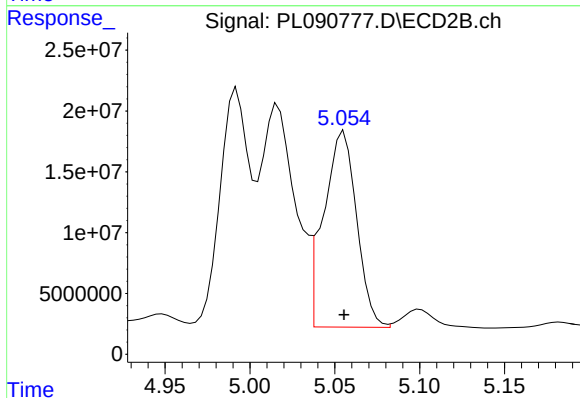


#26 Chlordane-4

R.T.: 5.055 min
Delta R.T.: 0.000 min
Response: 218038238
Conc: 1018.70 ng/ml

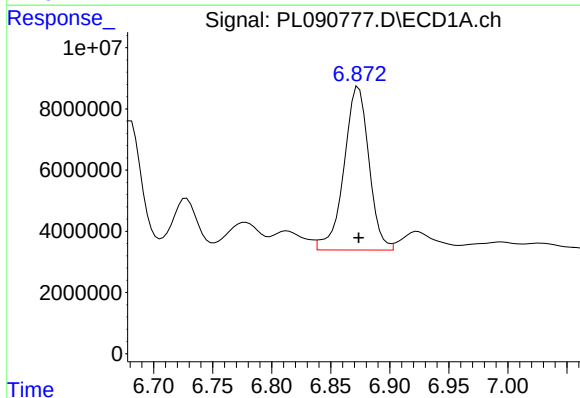


#27 Chlordane-5

R.T.: 6.874 min
Delta R.T.: 0.000 min
Response: 78566456
Conc: 973.17 ng/ml

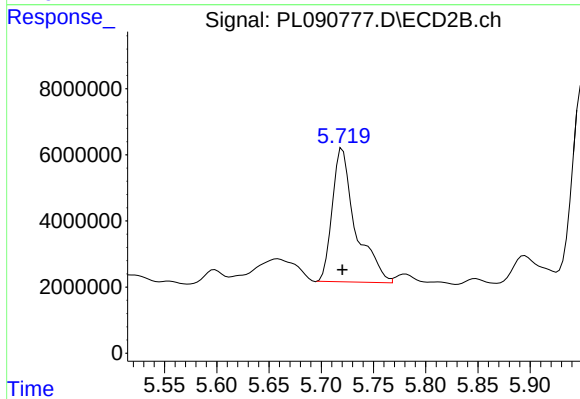

#27 Chlordane-5


R.T.: 5.720 min
Delta R.T.: 0.000 min
Response: 62611264
Conc: 1002.25 ng/ml

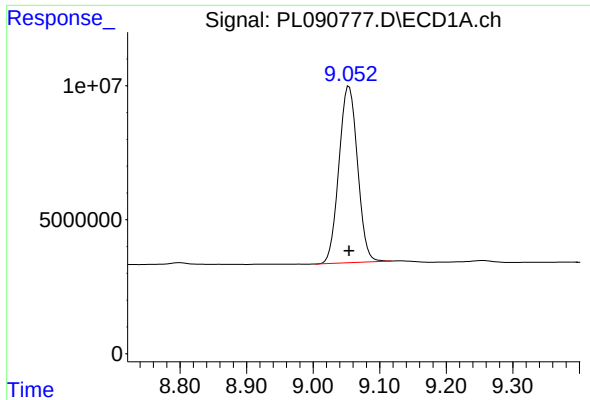

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 127700216
Conc: 97.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

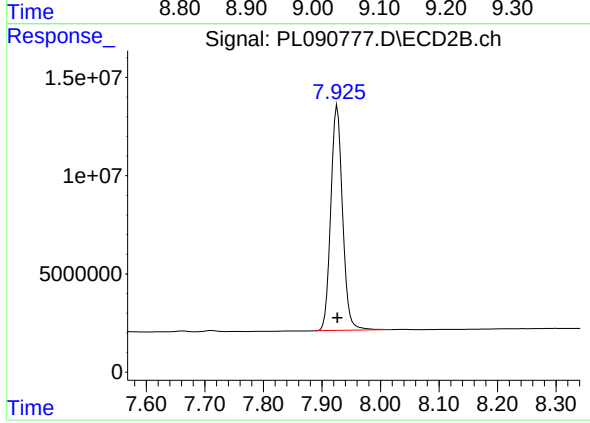

#28 Decachlorobiphenyl

R.T.: 7.926 min
Delta R.T.: 0.000 min
Response: 159832735
Conc: 98.40 ng/ml