

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080524\
 Data File : PL090778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2024 16:30
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 17:44:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 05 17:39:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.785	133.0E6	152.3E6	73.172	73.464
28)	SA Decachlor...	9.055	7.926	96192515	118.8E6	73.742	73.756
Target Compounds							
23)	Chlordane-1	4.705	3.784	62637039	47580584	727.683	733.197
24)	Chlordane-2	5.233	4.362	68220342	56211255	731.584	730.212
25)	Chlordane-3	5.943	4.992	227.0E6	166.3E6	734.300	740.399
26)	Chlordane-4	6.025	5.055	279.3E6	155.6E6	734.731	734.540
27)	Chlordane-5	6.873	5.721	58718290	45781617	734.724	738.480



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080524\
Data File : PL090778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2024 16:30
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 17:44:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
Quant Title : GC Extractables
QLast Update : Mon Aug 05 17:39:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

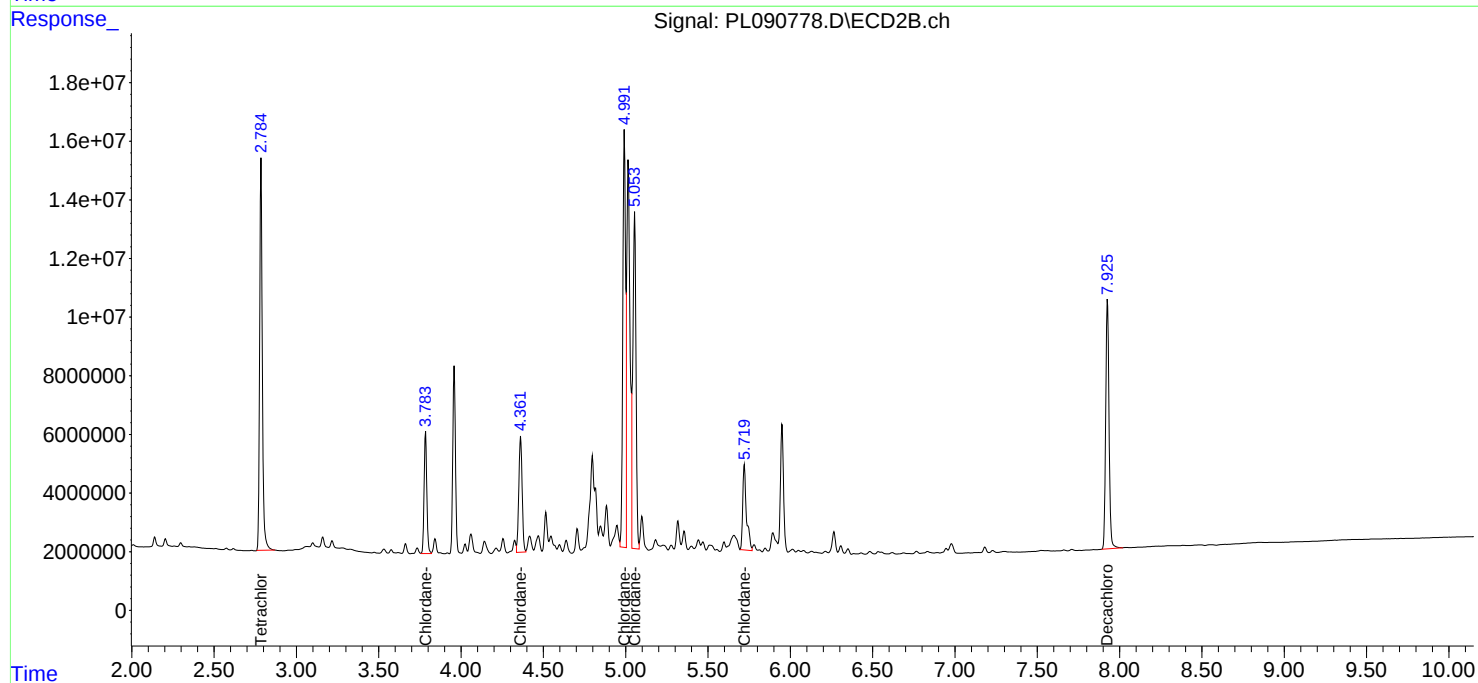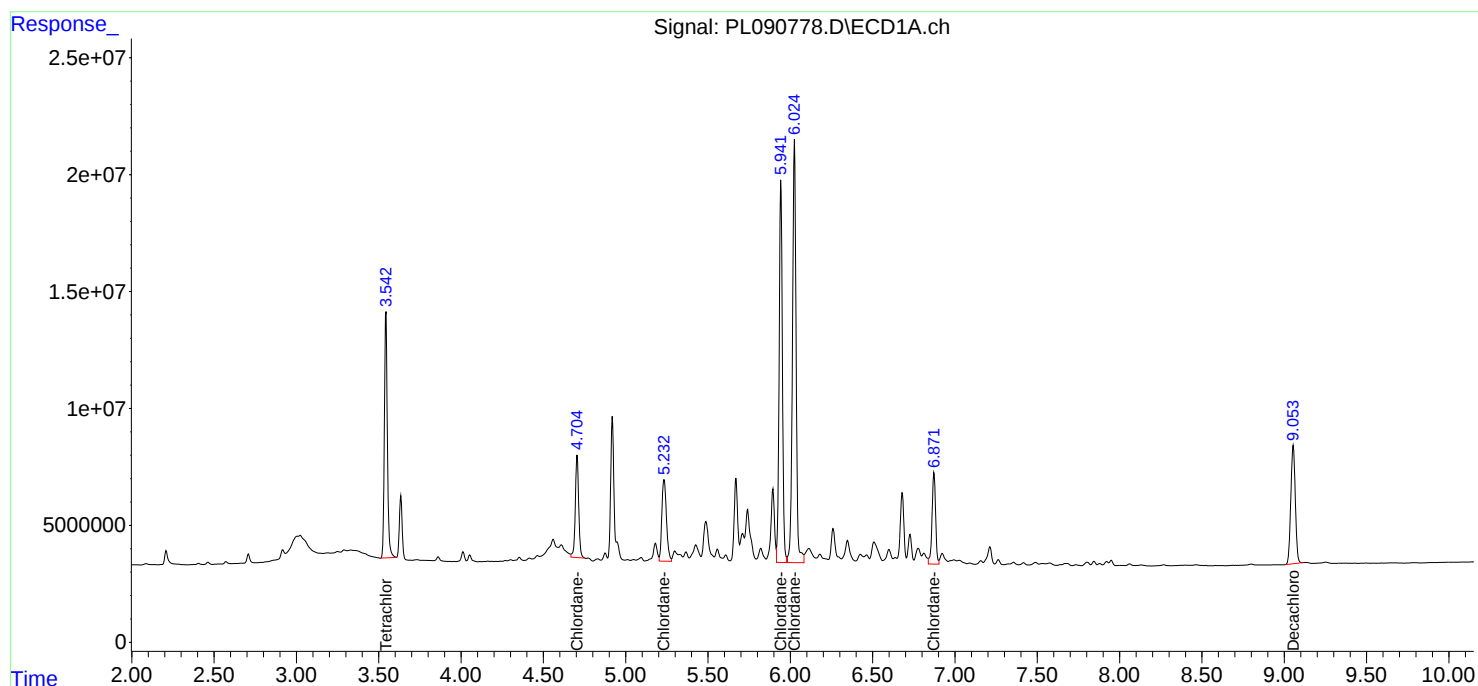


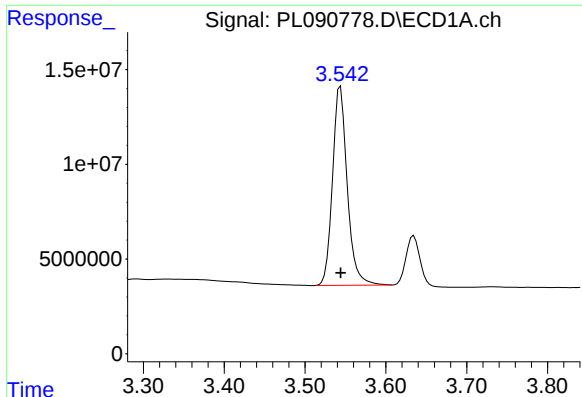

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 133020572
Conc: 73.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

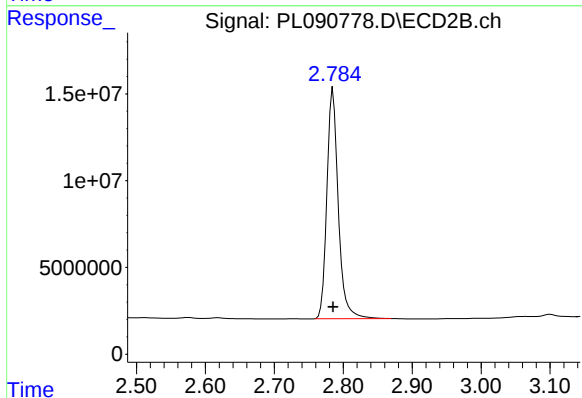


#1 Tetrachloro-m-xylene

R.T.: 2.785 min
Delta R.T.: 0.000 min
Response: 152295266
Conc: 73.46 ng/ml

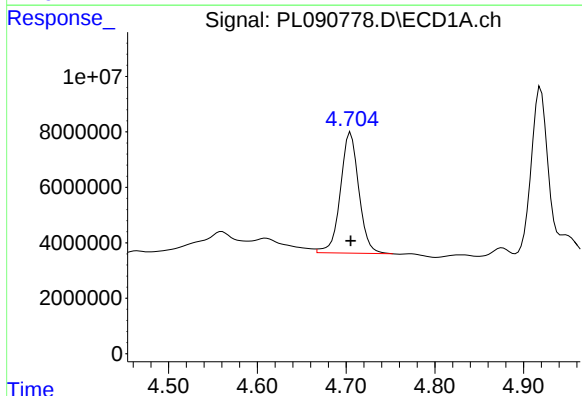


#23 Chlordane-1

R.T.: 4.705 min
Delta R.T.: 0.000 min
Response: 62637039
Conc: 727.68 ng/ml

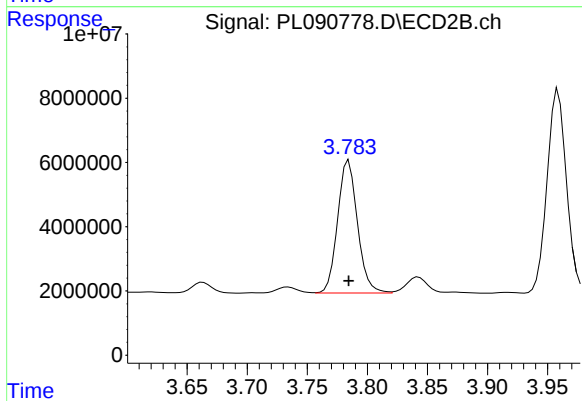

#23 Chlordane-1


R.T.: 3.784 min
Delta R.T.: 0.000 min
Response: 47580584
Conc: 733.20 ng/ml

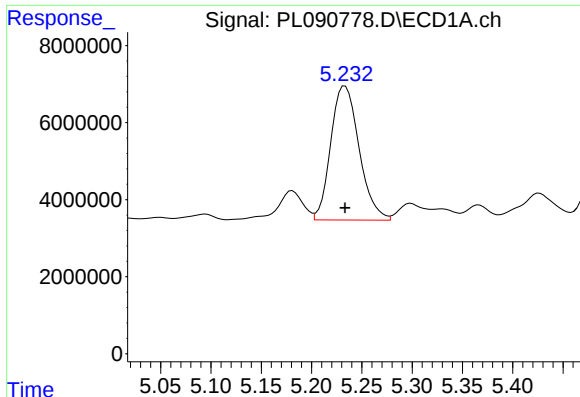

#24 Chlordane-2


R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 68220342
Conc: 731.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

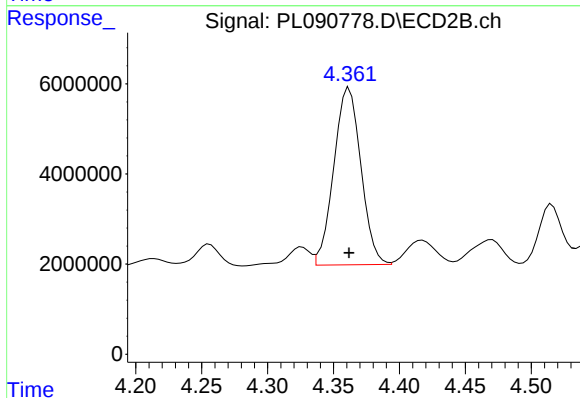


#24 Chlordane-2

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 56211255
Conc: 730.21 ng/ml

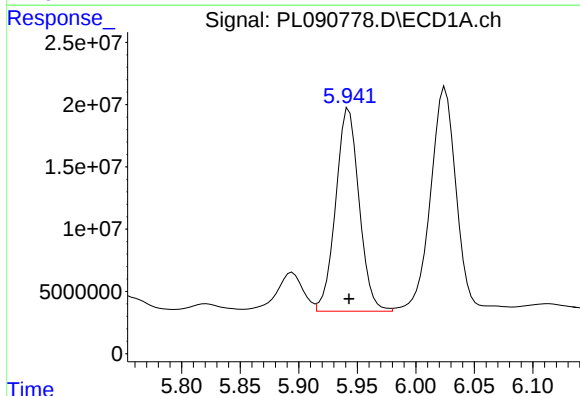


#25 Chlordane-3

R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 227025911
Conc: 734.30 ng/ml

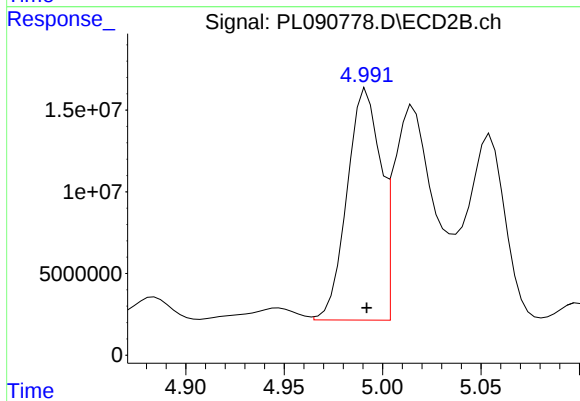

#25 Chlordane-3


R.T.: 4.992 min
Delta R.T.: 0.000 min
Response: 166325578
Conc: 740.40 ng/ml

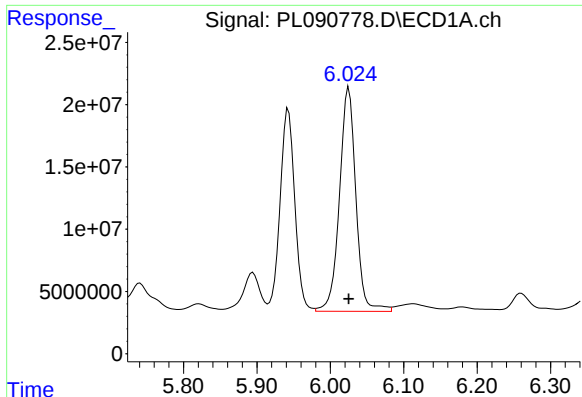

#26 Chlordane-4


R.T.: 6.025 min
Delta R.T.: 0.000 min
Response: 279270716
Conc: 734.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

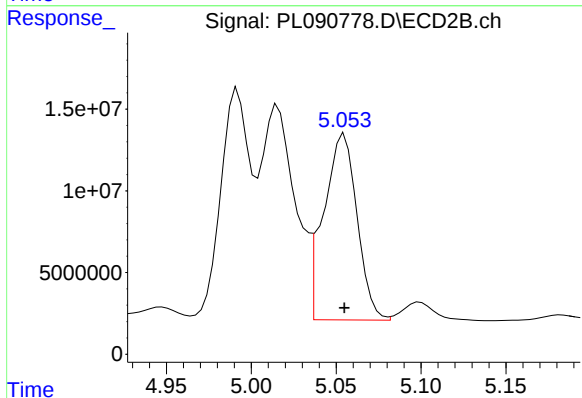


#26 Chlordane-4

R.T.: 5.055 min
Delta R.T.: 0.000 min
Response: 155613350
Conc: 734.54 ng/ml

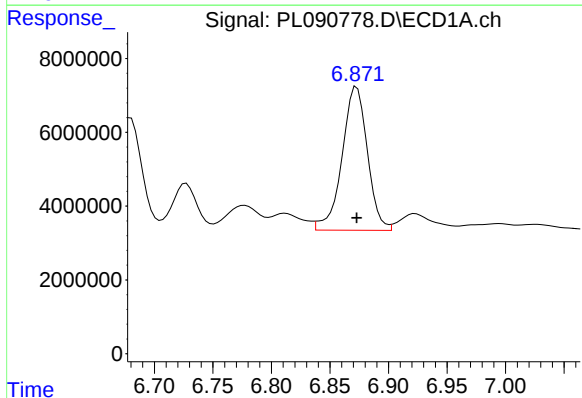


#27 Chlordane-5

R.T.: 6.873 min
Delta R.T.: 0.000 min
Response: 58718290
Conc: 734.72 ng/ml

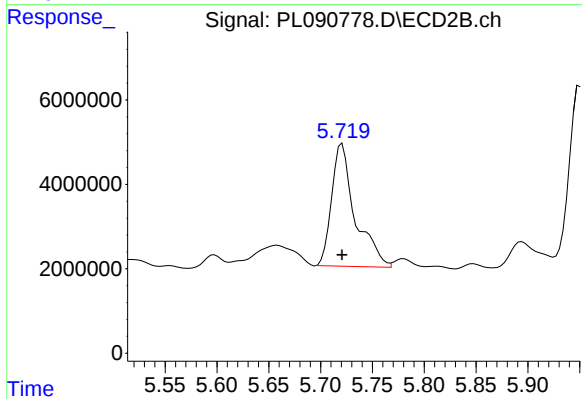

#27 Chlordane-5

R.T.: 5.721 min
Delta R.T.: 0.000 min
Response: 45781617
Conc: 738.48 ng/ml

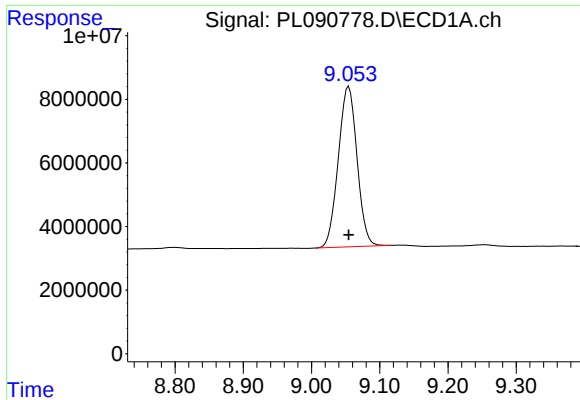

#28 Decachlorobiphenyl


R.T.: 9.055 min

Delta R.T.: 0.000 min

Response: 96192515

Conc: 73.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

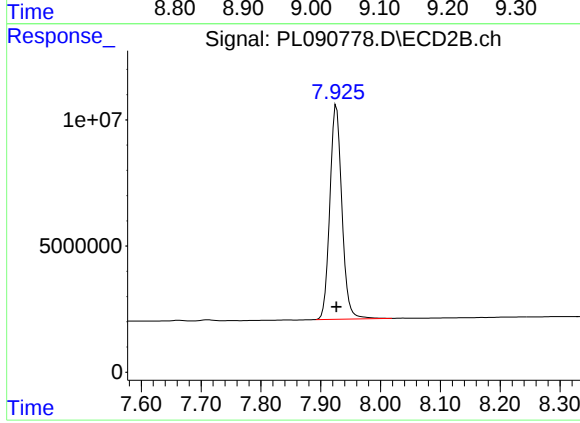

#28 Decachlorobiphenyl

R.T.: 7.926 min

Delta R.T.: 0.000 min

Response: 118818598

Conc: 73.76 ng/ml