

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080524\
 Data File : PL090780.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2024 16:58
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 17:46:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 05 17:39:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.785	48885407	52149743	26.392	25.117
28)	SA Decachlor...	9.053	7.926	36713637	42937677	27.287	26.220
Target Compounds							
23)	Chlordane-1	4.704	3.784	25468746	16557070	282.902	253.833
24)	Chlordane-2	5.234	4.362	26114623	20623712	271.879	263.198
25)	Chlordane-3	5.943	4.992	81596404	53923691	260.295	242.456
26)	Chlordane-4	6.025	5.055	100.6E6	51883566	260.918	246.160
27)	Chlordane-5	6.872	5.720	20360046	16196498	253.552	258.349



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080524\
Data File : PL090780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2024 16:58
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 17:46:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
Quant Title : GC Extractables
QLast Update : Mon Aug 05 17:39:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

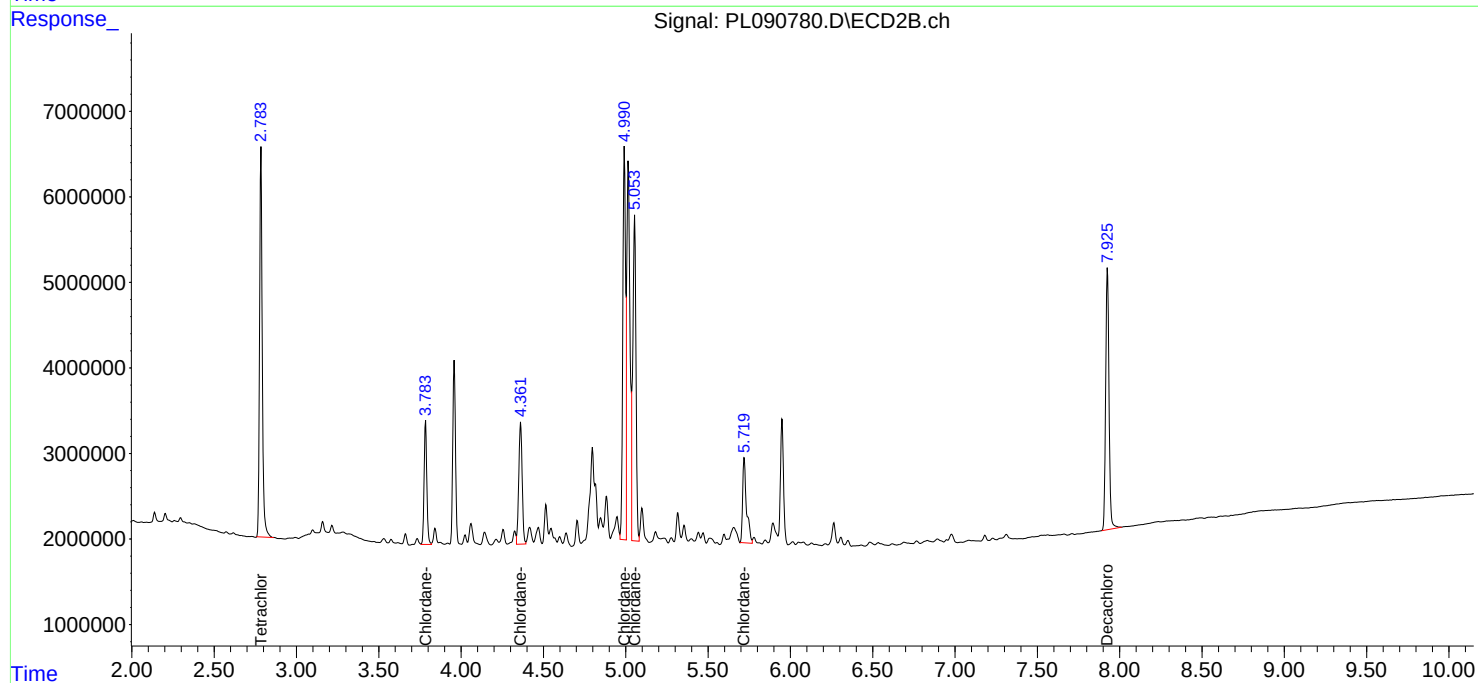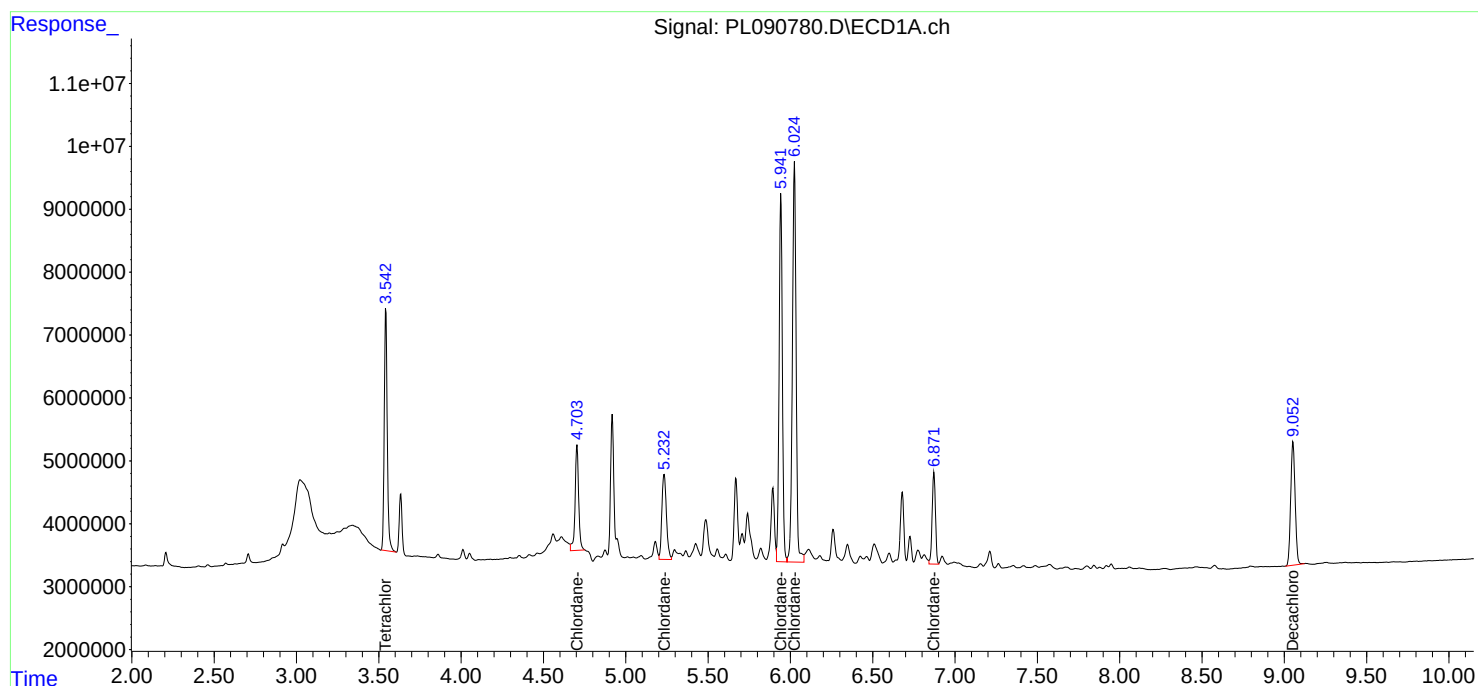


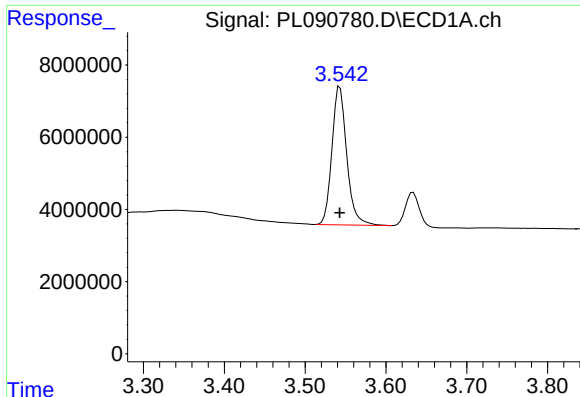

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 48885407
Conc: 26.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

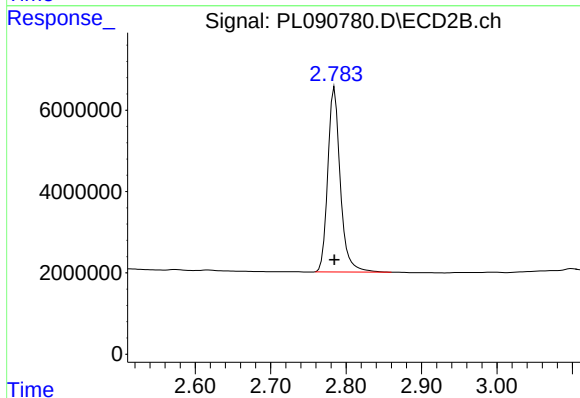


#1 Tetrachloro-m-xylene

R.T.: 2.785 min
Delta R.T.: 0.000 min
Response: 52149743
Conc: 25.12 ng/ml

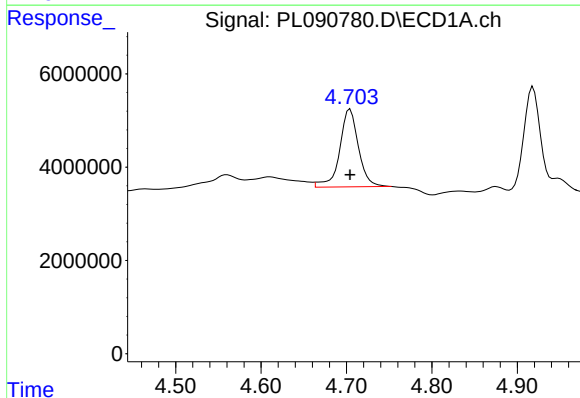


#23 Chlordane-1

R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 25468746
Conc: 282.90 ng/ml

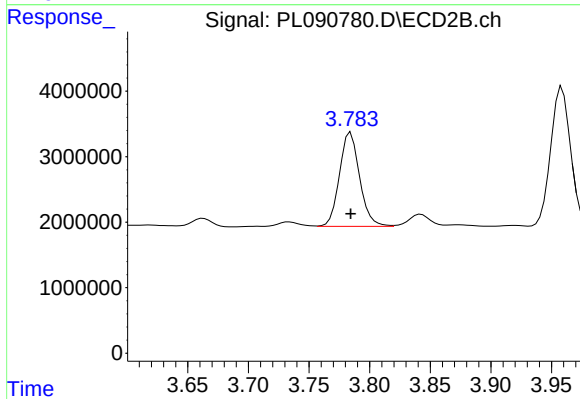

#23 Chlordane-1


R.T.: 3.784 min
Delta R.T.: 0.000 min
Response: 16557070
Conc: 253.83 ng/ml

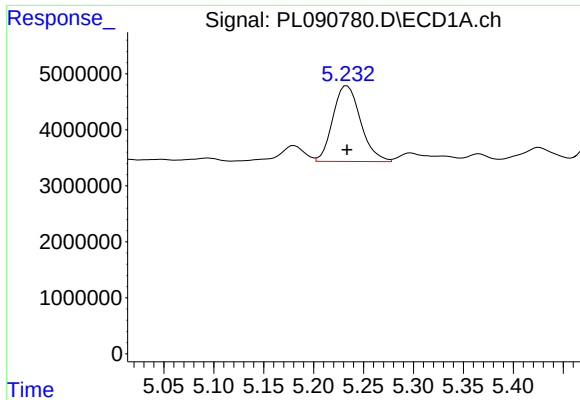

#24 Chlordane-2


R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 26114623
Conc: 271.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

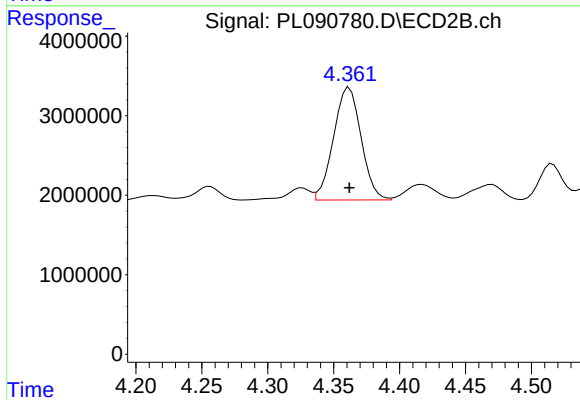


#24 Chlordane-2

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 20623712
Conc: 263.20 ng/ml

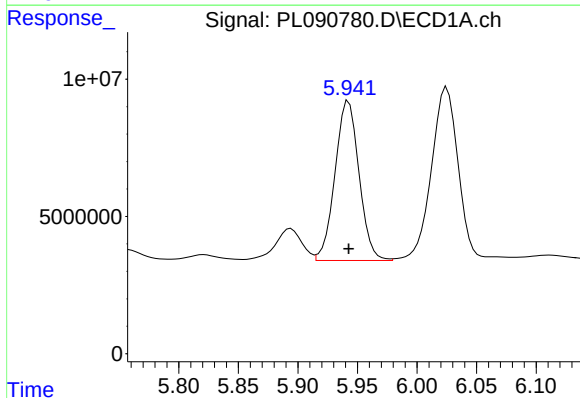


#25 Chlordane-3

R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 81596404
Conc: 260.30 ng/ml

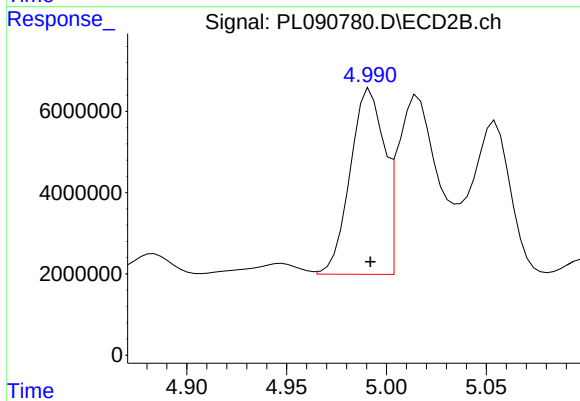

#25 Chlordane-3


R.T.: 4.992 min
Delta R.T.: 0.000 min
Response: 53923691
Conc: 242.46 ng/ml

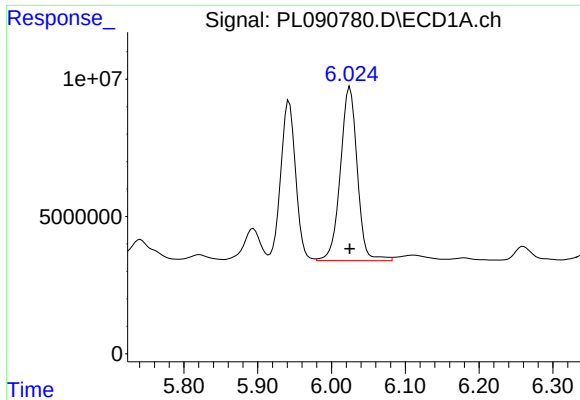

#26 Chlordane-4


R.T.: 6.025 min
Delta R.T.: 0.000 min
Response: 100640007
Conc: 260.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

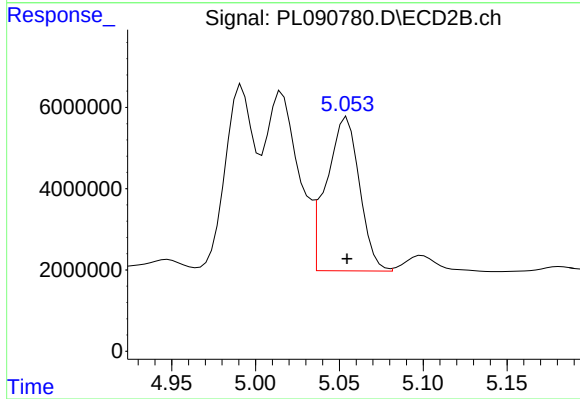


#26 Chlordane-4

R.T.: 5.055 min
Delta R.T.: 0.000 min
Response: 51883566
Conc: 246.16 ng/ml

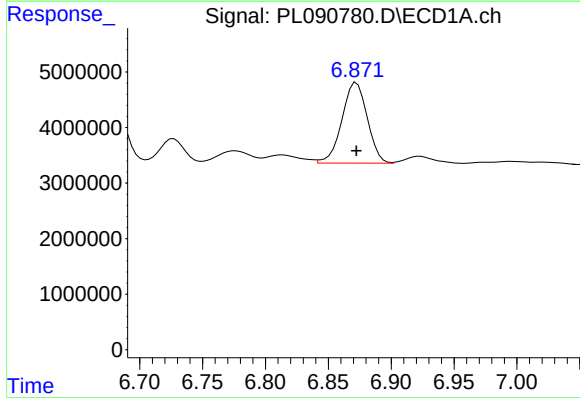


#27 Chlordane-5

R.T.: 6.872 min
Delta R.T.: 0.000 min
Response: 20360046
Conc: 253.55 ng/ml

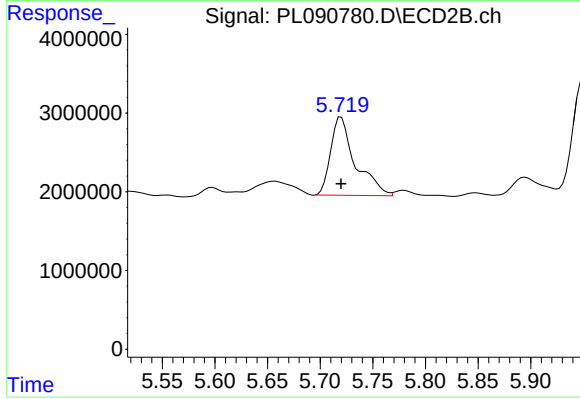

#27 Chlordane-5


R.T.: 5.720 min
Delta R.T.: 0.000 min
Response: 16196498
Conc: 258.35 ng/ml

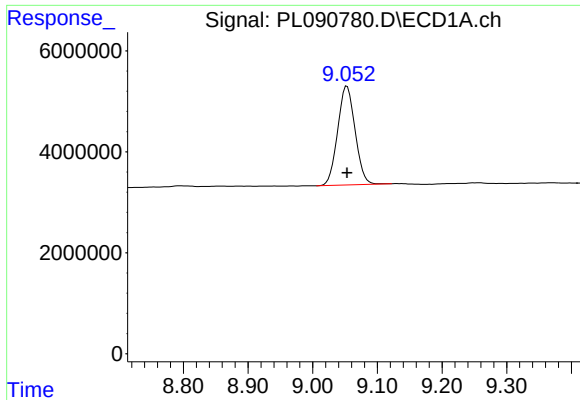

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: 0.000 min
Response: 36713637
Conc: 27.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

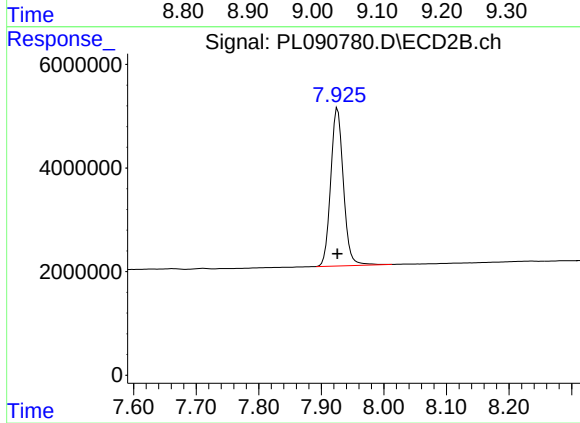

#28 Decachlorobiphenyl

R.T.: 7.926 min
Delta R.T.: 0.000 min
Response: 42937677
Conc: 26.22 ng/ml