

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080525\
 Data File : PL096700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2025 10:14
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 01:51:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	4.885f	0.000	33311322	0	8.016	N.D.	#
7) B	delta-BHC	4.769f	0.000	6161845	0	1.544	N.D.	#
8) B	Heptachlo...	5.648	0.000	27485271	0	7.127	N.D.	#
9) A	Endosulfan I	6.031	0.000	7282318	0	2.025	N.D.	#
11) B	alpha-Chl...	5.971f	0.000	13079848	0	3.393	N.D.	#
13) MA	Dieldrin	0.000	5.421	0	39816294	N.D.	6.741	#
14) MA	Endrin	0.000	5.716	0	23709767	N.D.	4.386	#
24)	Chlordane-2	5.190f	4.405	12743471	18591056	72.817	76.635	
26)	Chlordane-4	5.971f	0.000	13079848	0	15.803	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080525\
Data File : PL096700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2025 10:14
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 01:51:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:58:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

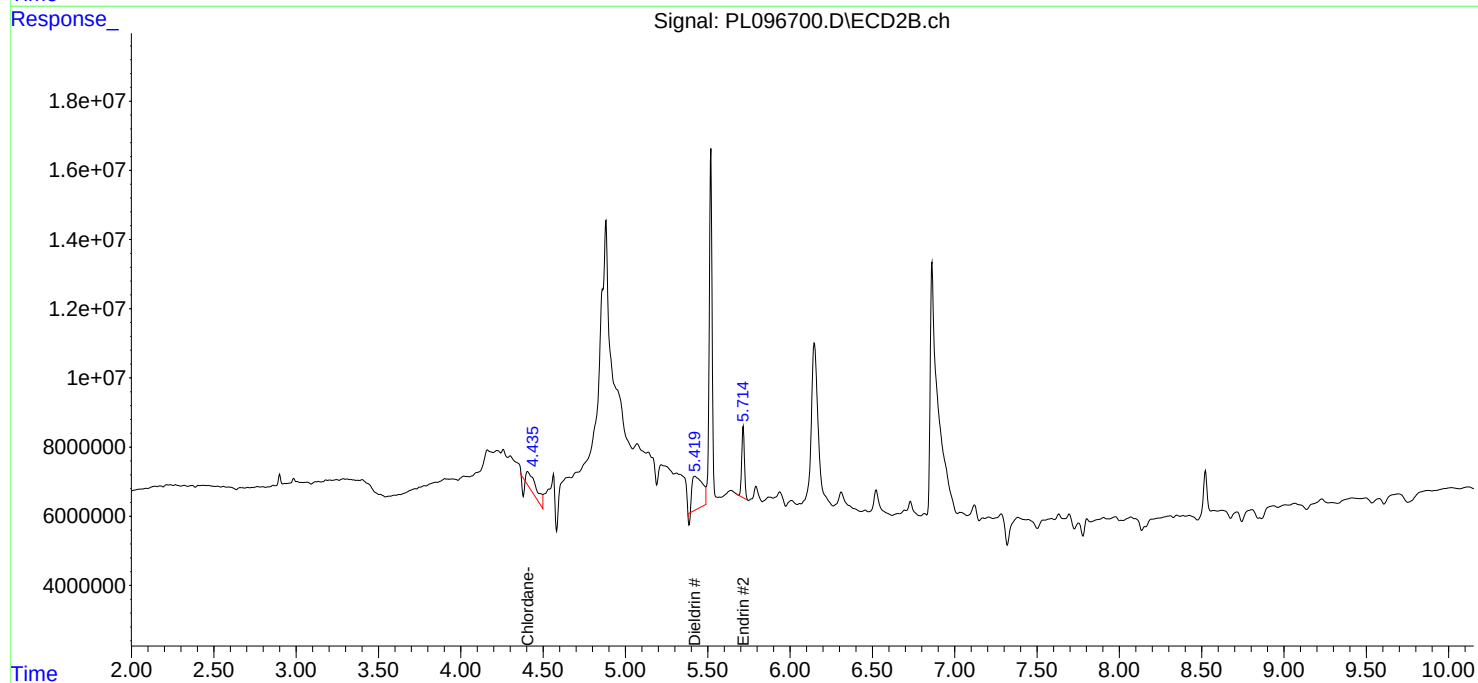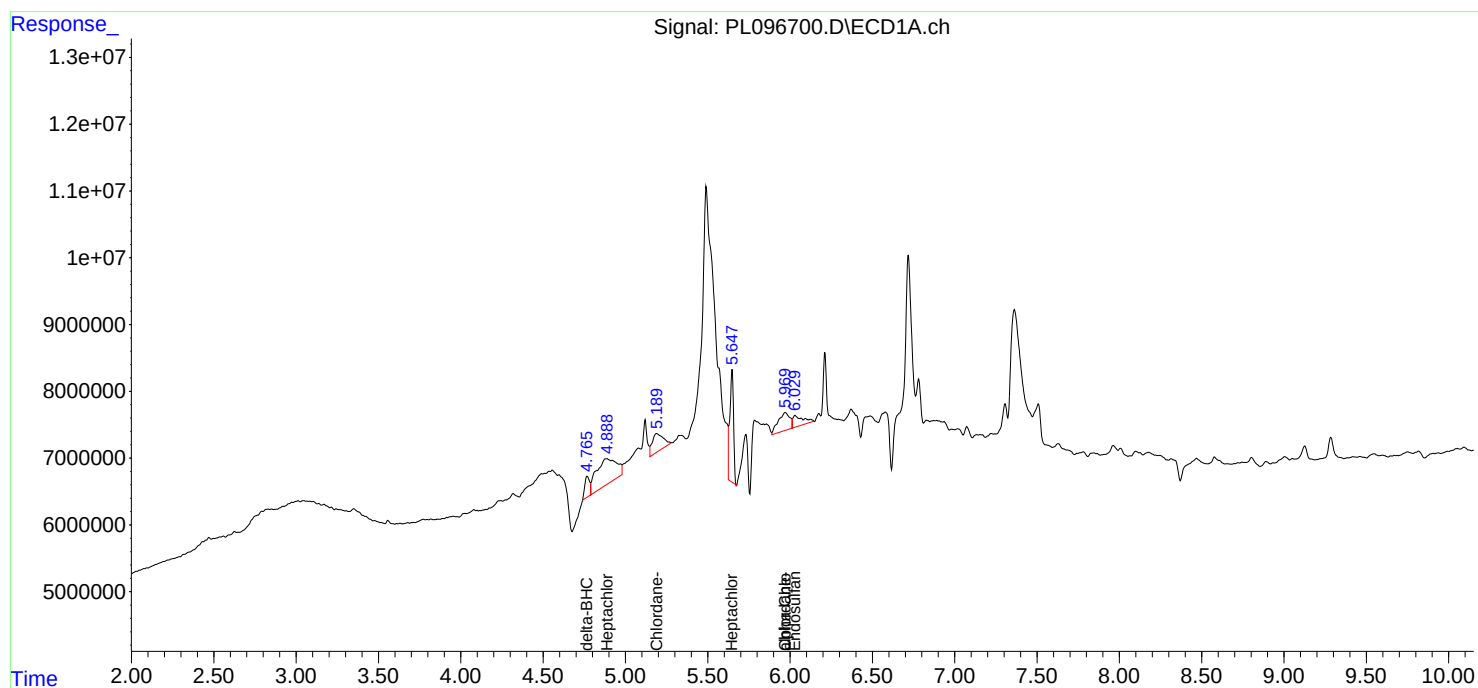


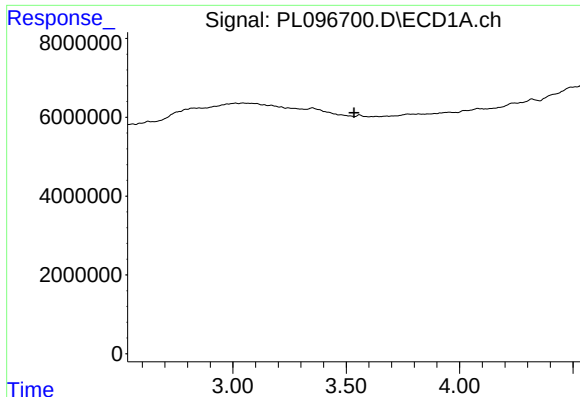

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.535 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

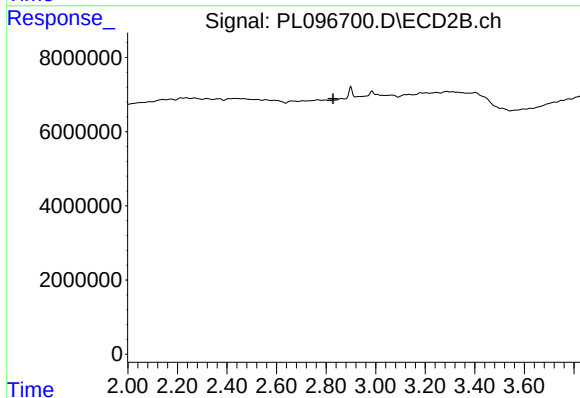


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.828 min
Response: 0
Conc: N.D.

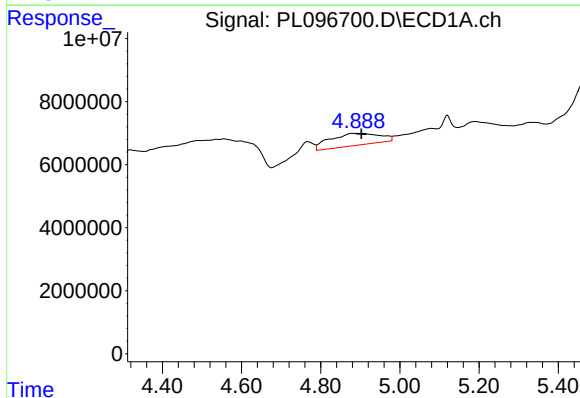


#4 Heptachlor

R.T.: 4.885 min
Delta R.T.: -0.017 min
Response: 33311322
Conc: 8.02 ng/ml

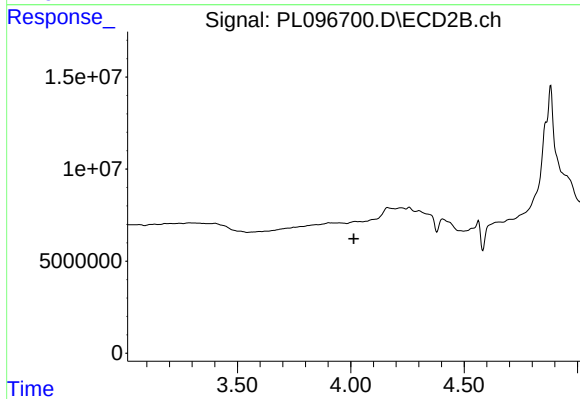

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.014 min
Response: 0
Conc: N.D.

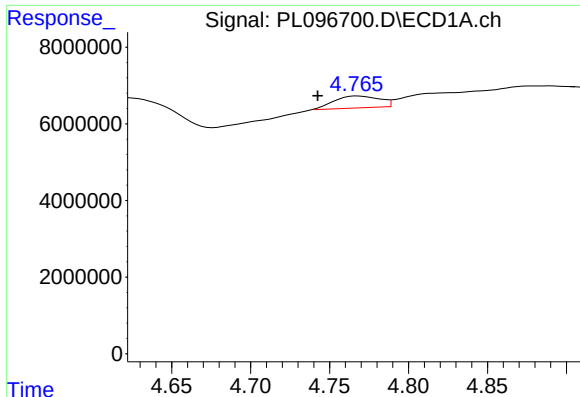

#7 delta-BHC


R.T.: 4.769 min
Delta R.T.: 0.026 min
Response: 6161845
Conc: 1.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

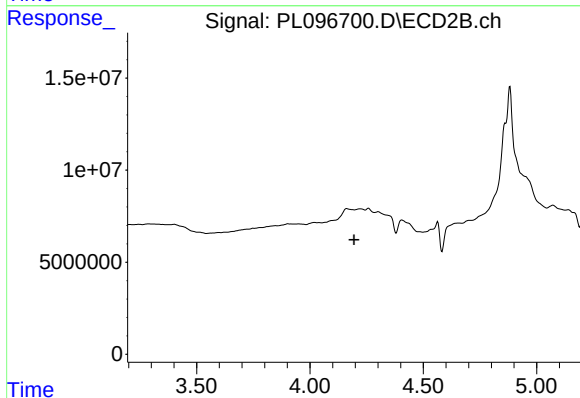


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.195 min
Response: 0
Conc: N.D.

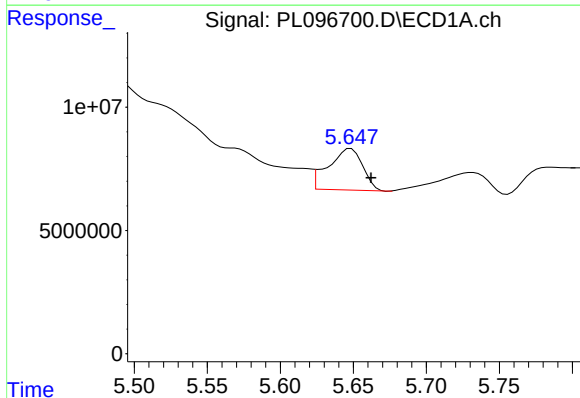


#8 Heptachlor epoxide

R.T.: 5.648 min
Delta R.T.: -0.015 min
Response: 27485271
Conc: 7.13 ng/ml

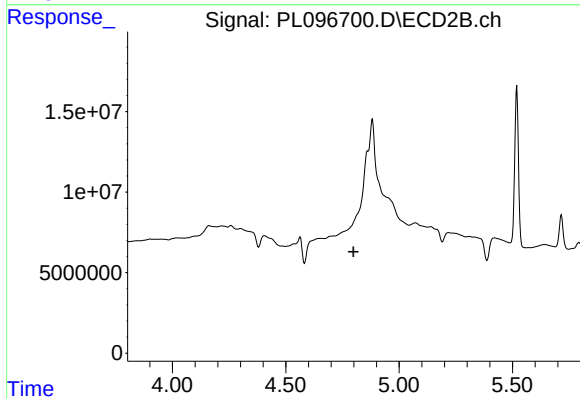

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.799 min
Response: 0
Conc: N.D.

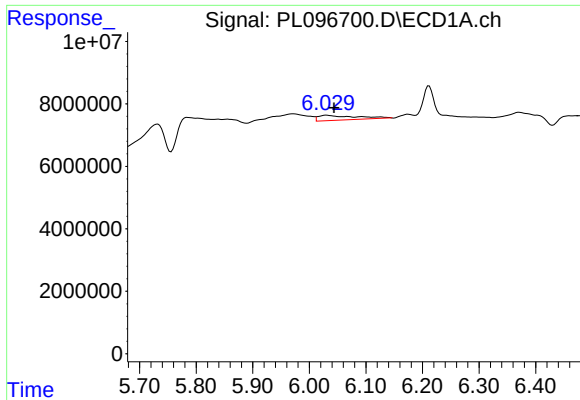

#9 Endosulfan I


R.T.: 6.031 min
Delta R.T.: -0.013 min
Response: 7282318
Conc: 2.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

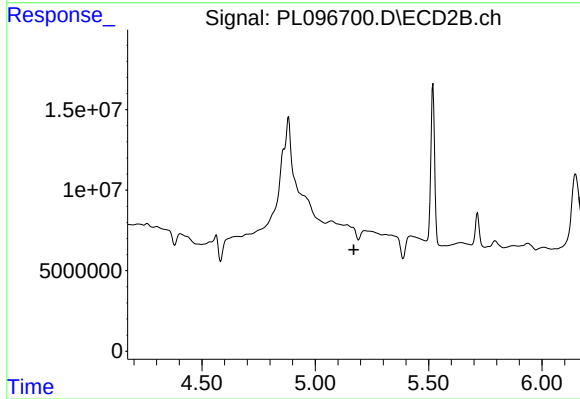


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

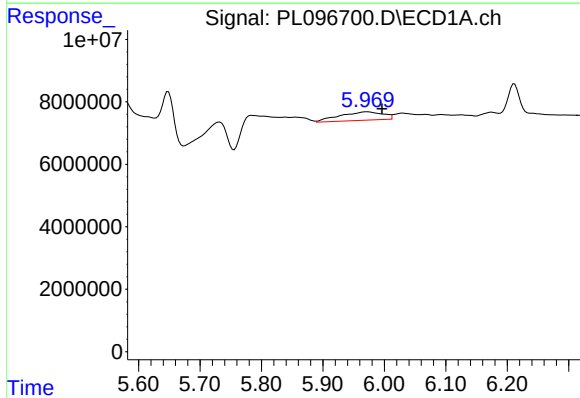


#11 alpha-Chlordane

R.T.: 5.971 min
Delta R.T.: -0.025 min
Response: 13079848
Conc: 3.39 ng/ml

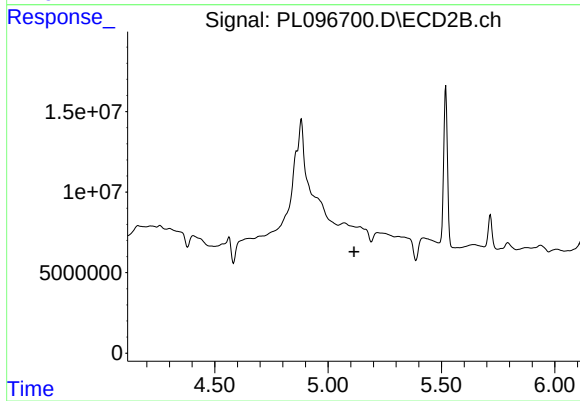

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

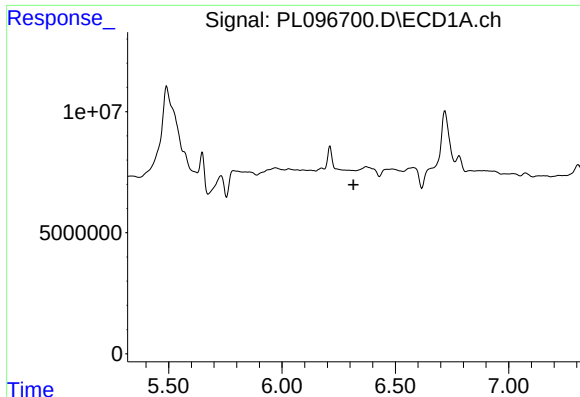

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

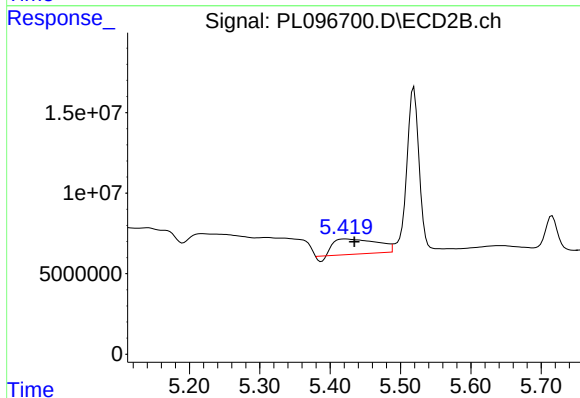


#13 Dieldrin

R.T.: 5.421 min
Delta R.T.: -0.014 min
Response: 39816294
Conc: 6.74 ng/ml

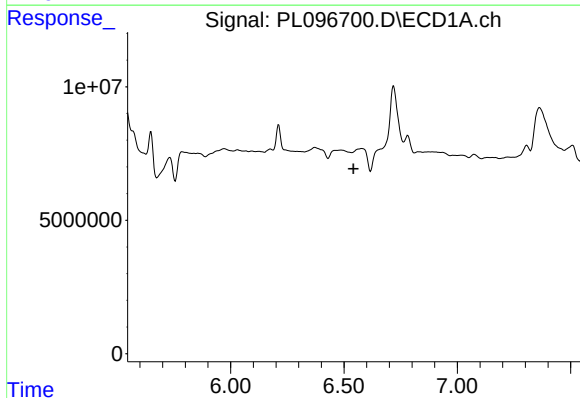


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.542 min
Response: 0
Conc: N.D.

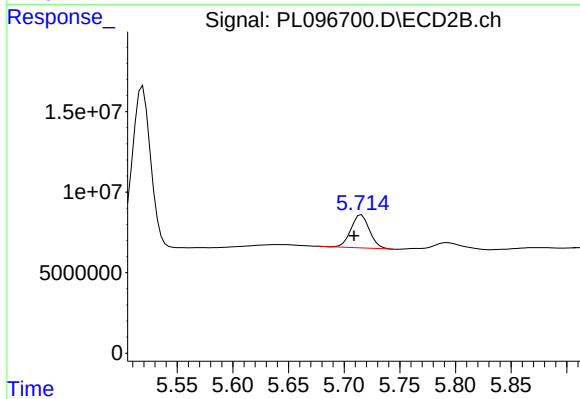

#14 Endrin


R.T.: 5.716 min
Delta R.T.: 0.007 min
Response: 23709767
Conc: 4.39 ng/ml

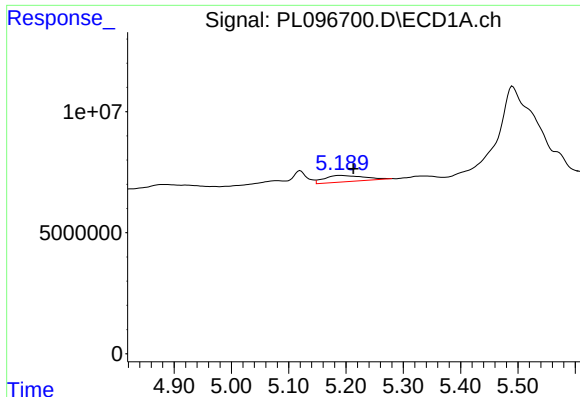

#24 Chlordane-2


R.T.: 5.190 min
Delta R.T.: -0.023 min
Response: 12743471
Conc: 72.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

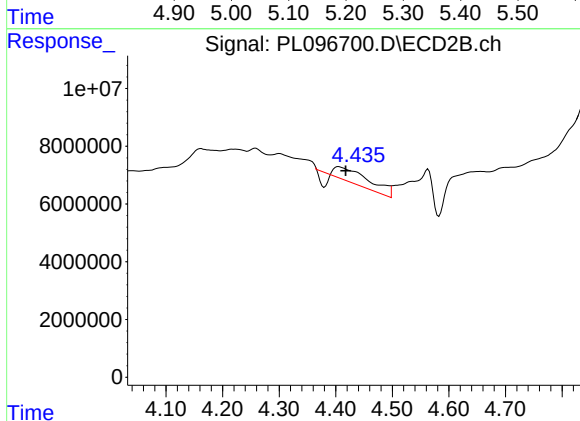


#24 Chlordane-2

R.T.: 4.405 min
Delta R.T.: -0.013 min
Response: 18591056
Conc: 76.64 ng/ml

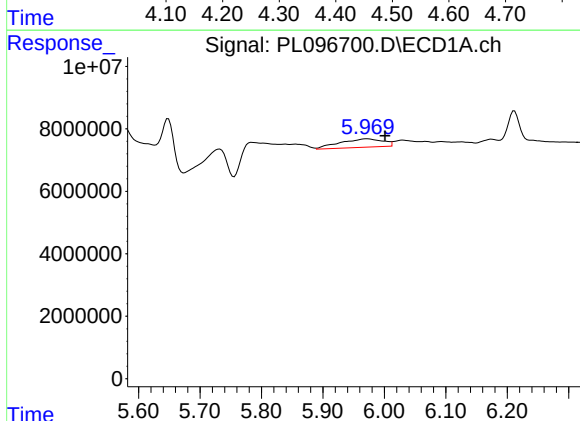


#26 Chlordane-4

R.T.: 5.971 min
Delta R.T.: -0.030 min
Response: 13079848
Conc: 15.80 ng/ml

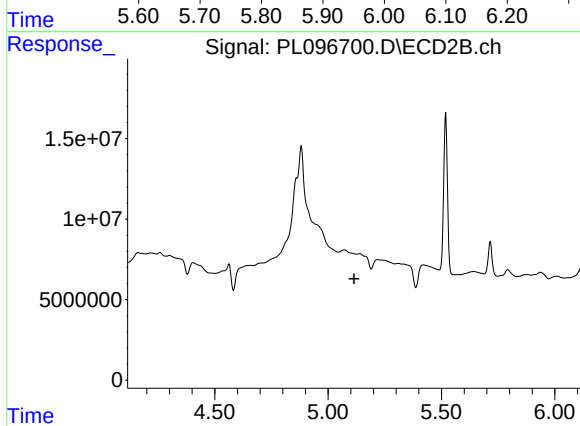

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

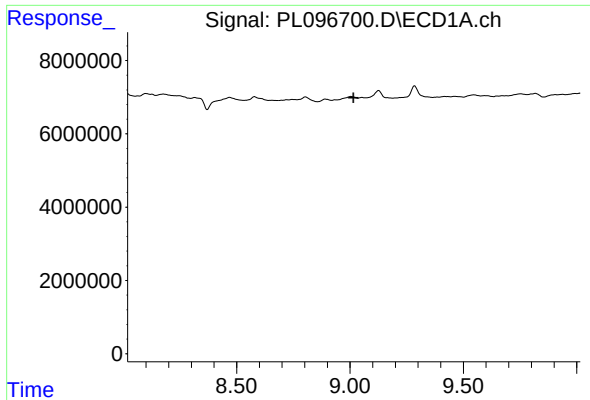

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.016 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

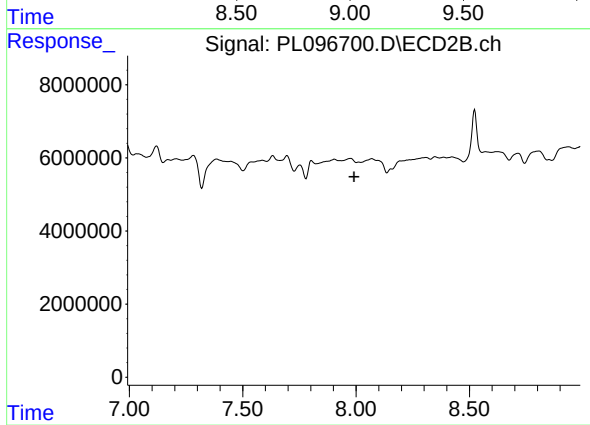

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.