

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080525\
 Data File : PL096706.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2025 15:21
 Operator : AR\AJ
 Sample : Q2759-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 01:52:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.532	2.826	32983990	54874191	10.370	11.485
28)	SA Decachlor...	9.009	7.988	29620690	57328326	12.421	13.214
Target Compounds							
8)	B Heptachlo...	5.651	0.000	2474650	0	0.642	N.D. #
12)	B 4,4'-DDE	6.161	5.301	6379746	6443588	1.987	1.169 #
13)	MA Dieldrin	0.000	5.433	0	4656705	N.D.	0.788 #
14)	MA Endrin	0.000	5.716	0	1629743	N.D.	0.301 #
15)	B Endosulfa...	0.000	5.990	0	5517830	N.D.	1.074 #
16)	A 4,4'-DDD	6.687	0.000	6004821	0	2.375	N.D. #
17)	MA 4,4'-DDT	6.984	6.103	6378348	27198976	2.224	5.377 #
19)	B Endosulfa...	0.000	6.402	0	2085965	N.D.	0.410 #
21)	B Endrin ke...	7.579f	0.000	6168743	0	2.052	N.D. #
27)	Chlordane-5	0.000	5.990f	0	5517830	N.D.	21.629 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080525\
Data File : PL096706.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2025 15:21
Operator : AR\AJ
Sample : Q2759-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 01:52:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:58:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

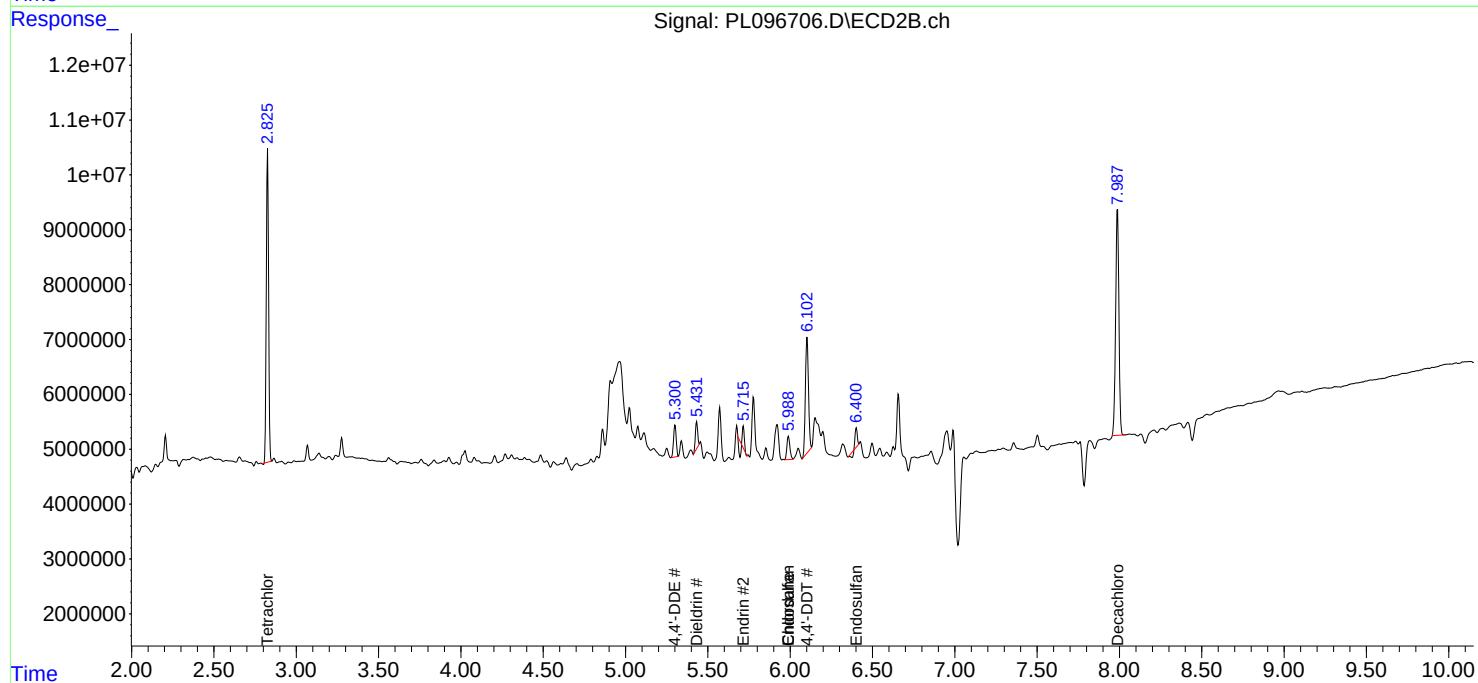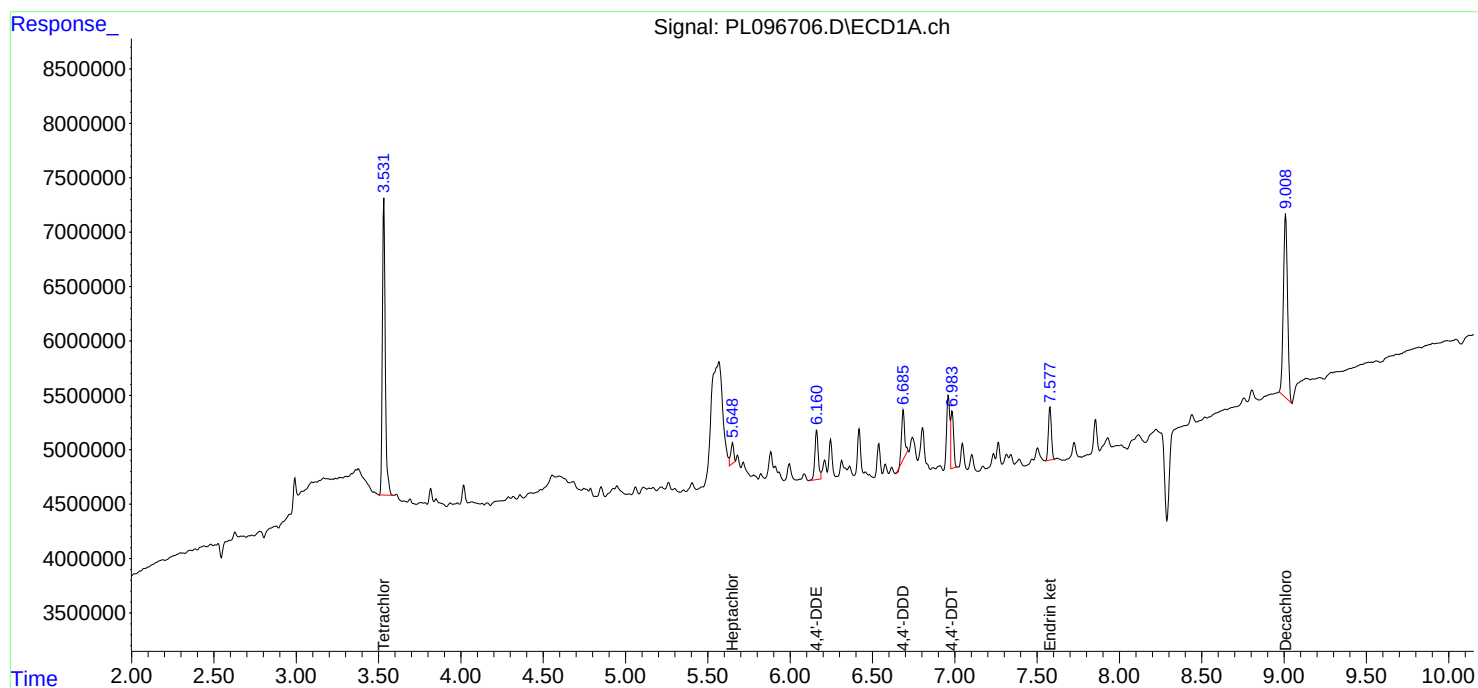


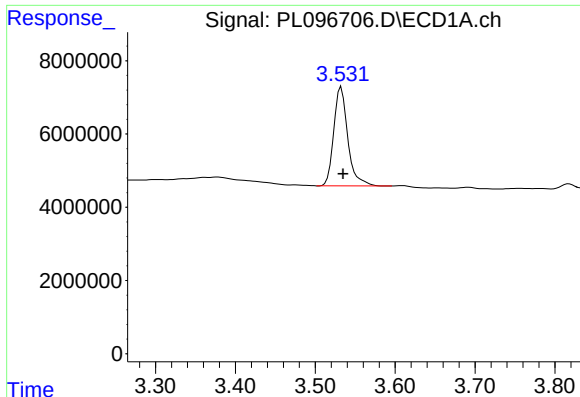

#1 Tetrachloro-m-xylene


R.T.: 3.532 min
Delta R.T.: -0.003 min
Response: 32983990
Conc: 10.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

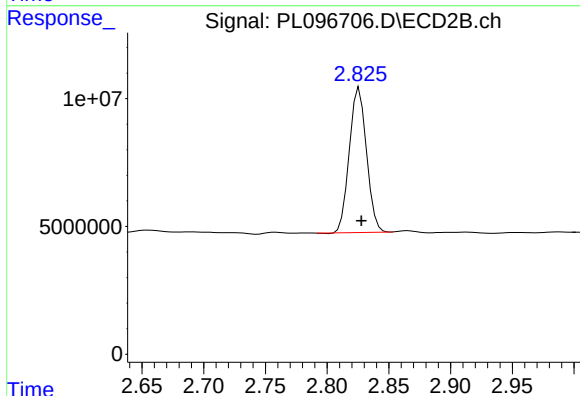


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: -0.002 min
Response: 54874191
Conc: 11.49 ng/ml

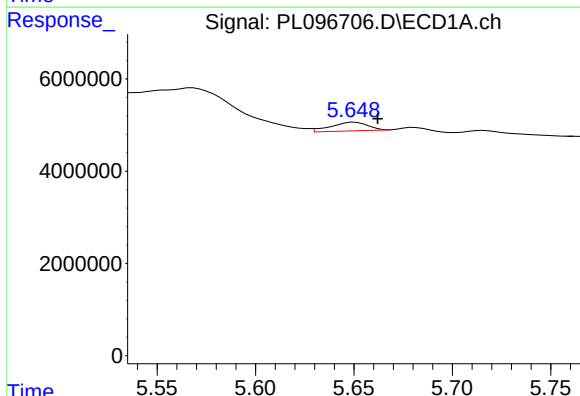


#8 Heptachlor epoxide

R.T.: 5.651 min
Delta R.T.: -0.012 min
Response: 2474650
Conc: 0.64 ng/ml

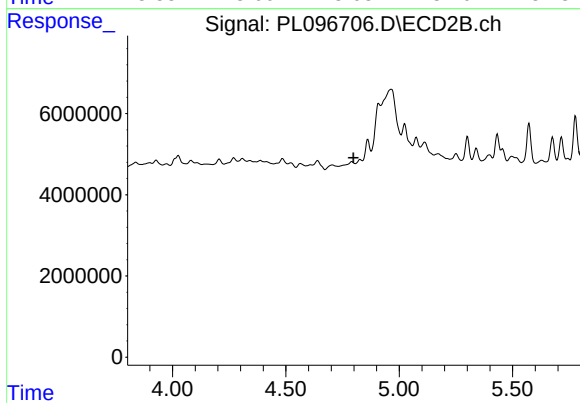

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.799 min
Response: 0
Conc: N.D.

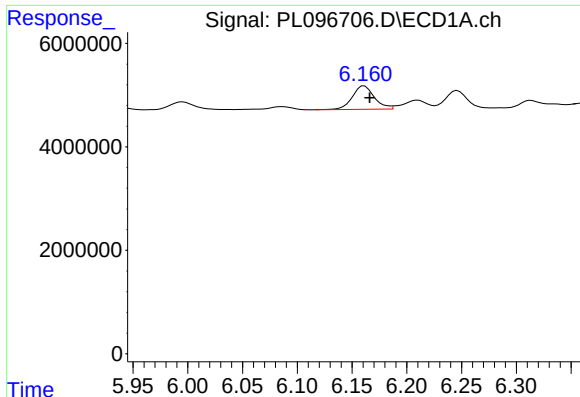

#12 4,4'-DDE


R.T.: 6.161 min
Delta R.T.: -0.005 min
Response: 6379746
Conc: 1.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

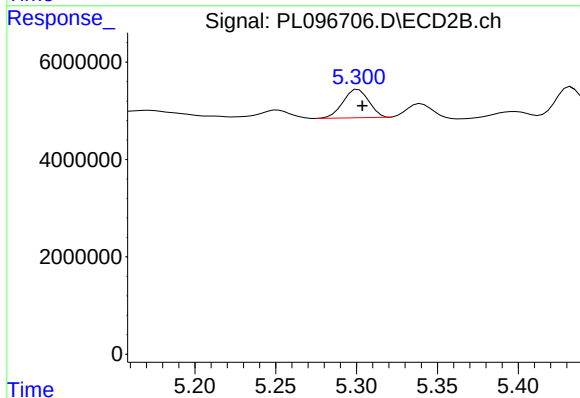


#12 4,4'-DDE

R.T.: 5.301 min
Delta R.T.: -0.003 min
Response: 6443588
Conc: 1.17 ng/ml

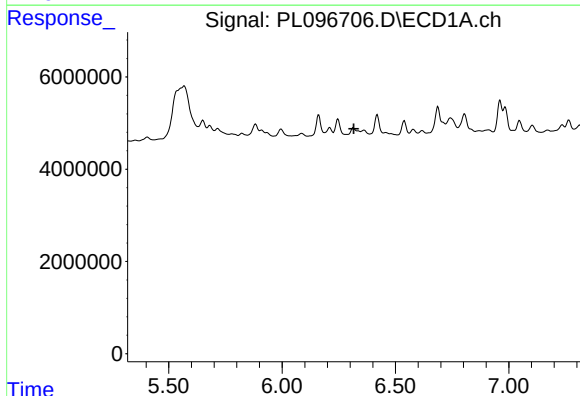


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.316 min
Response: 0
Conc: N.D.

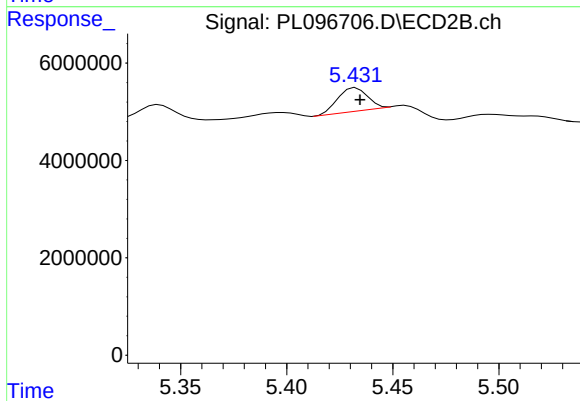

#13 Dieldrin


R.T.: 5.433 min
Delta R.T.: -0.002 min
Response: 4656705
Conc: 0.79 ng/ml

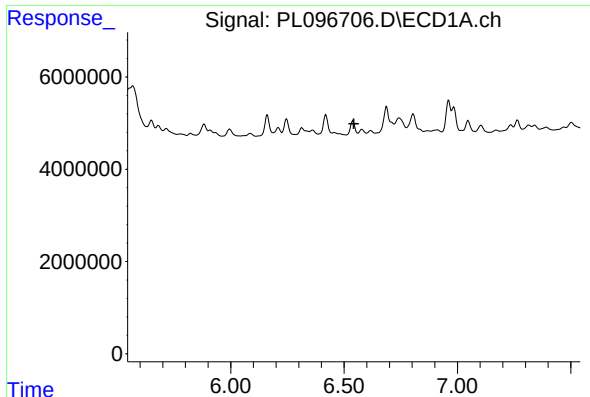

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

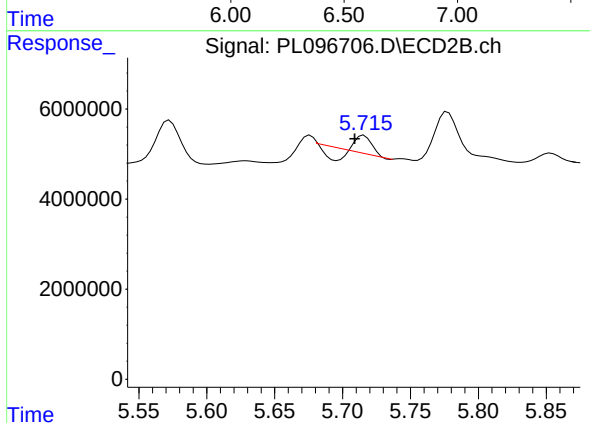


#14 Endrin

R.T.: 5.716 min
Delta R.T.: 0.007 min
Response: 1629743
Conc: 0.30 ng/ml

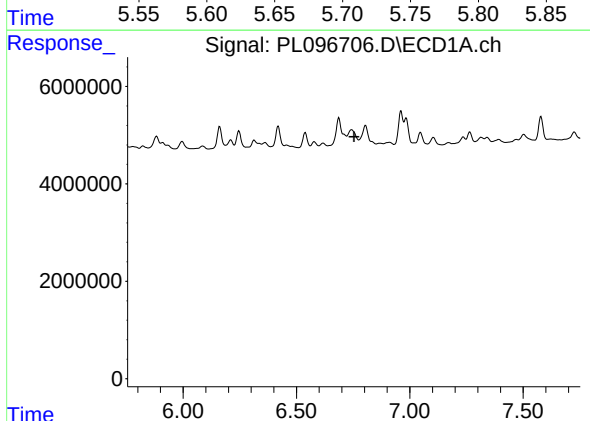


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.755 min
Response: 0
Conc: N.D.

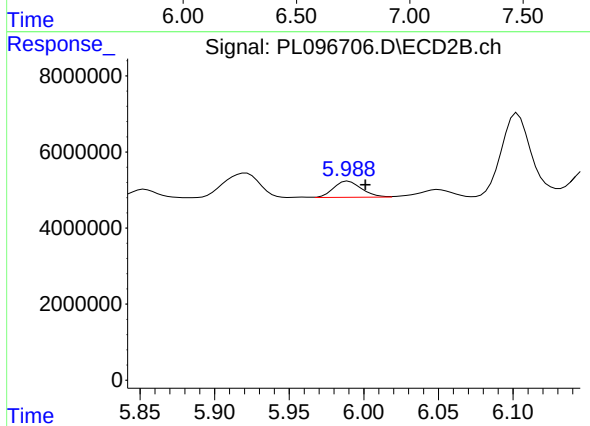

#15 Endosulfan II


R.T.: 5.990 min
Delta R.T.: -0.012 min
Response: 5517830
Conc: 1.07 ng/ml

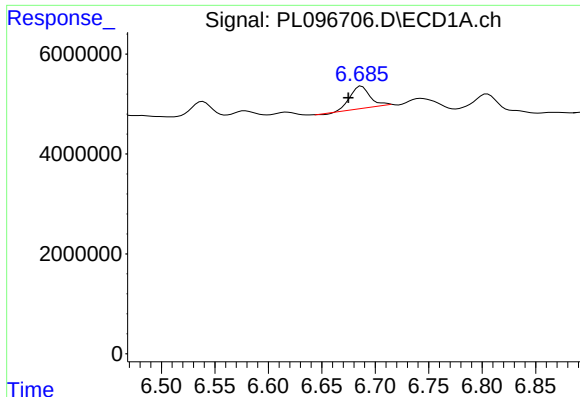

#16 4,4'-DDD


R.T.: 6.687 min
Delta R.T.: 0.012 min
Response: 6004821
Conc: 2.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

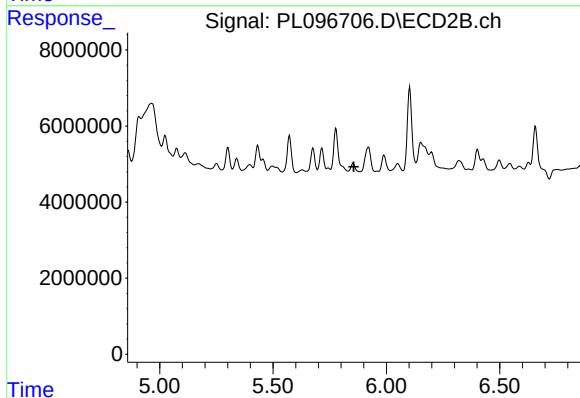


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.856 min
Response: 0
Conc: N.D.

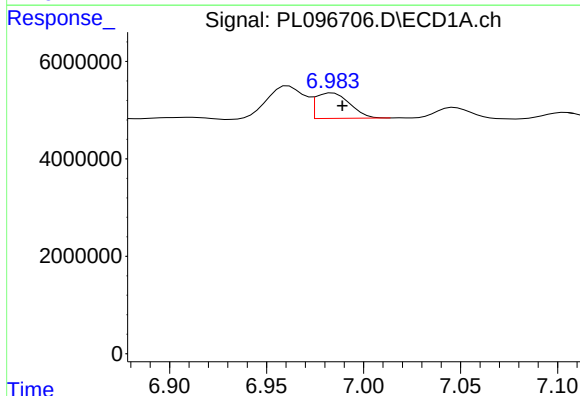


#17 4,4'-DDT

R.T.: 6.984 min
Delta R.T.: -0.005 min
Response: 6378348
Conc: 2.22 ng/ml

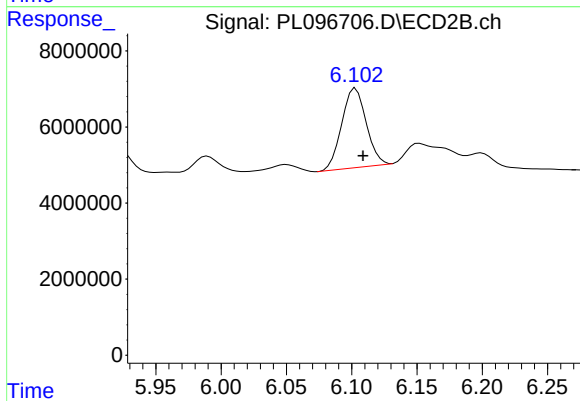

#17 4,4'-DDT


R.T.: 6.103 min
Delta R.T.: -0.006 min
Response: 27198976
Conc: 5.38 ng/ml

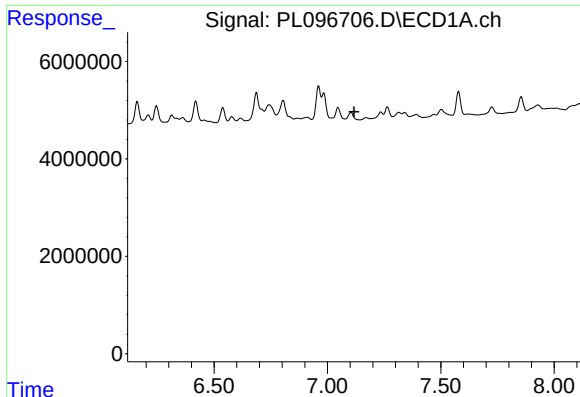

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

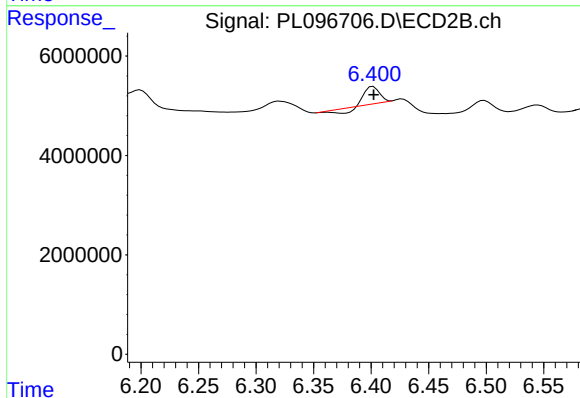


#19 Endosulfan Sulfate

R.T.: 6.402 min
Delta R.T.: 0.000 min
Response: 2085965
Conc: 0.41 ng/ml

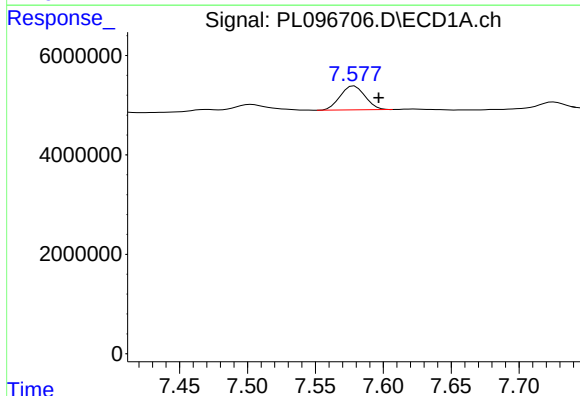


#21 Endrin ketone

R.T.: 7.579 min
Delta R.T.: -0.018 min
Response: 6168743
Conc: 2.05 ng/ml

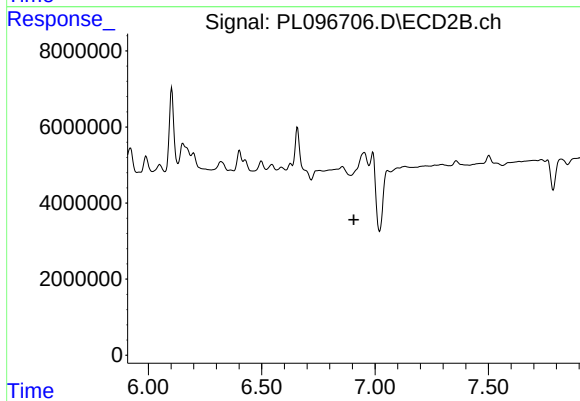

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.907 min
Response: 0
Conc: N.D.

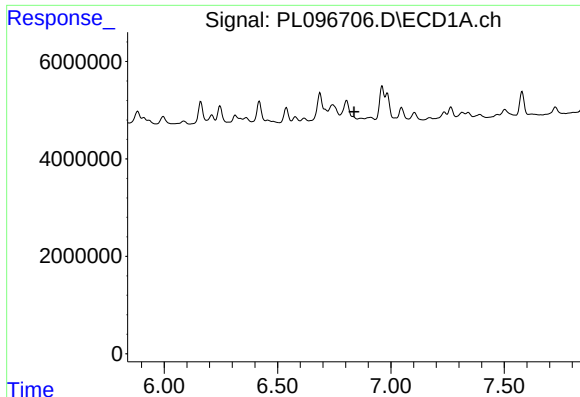

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.838 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

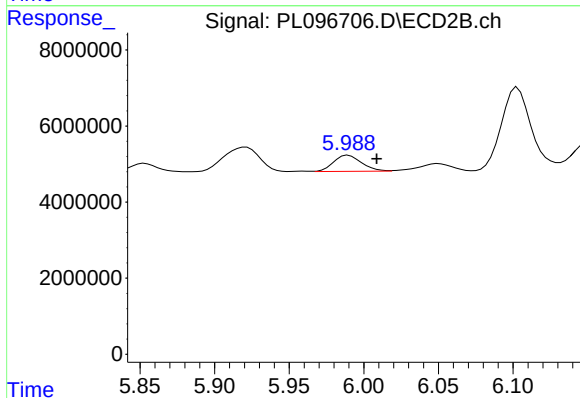


#27 Chlordane-5

R.T.: 5.990 min
Delta R.T.: -0.019 min
Response: 5517830
Conc: 21.63 ng/ml

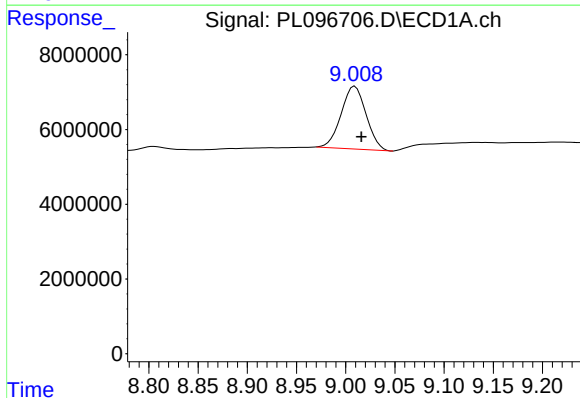

#28 Decachlorobiphenyl

R.T.: 9.009 min
Delta R.T.: -0.006 min
Response: 29620690
Conc: 12.42 ng/ml

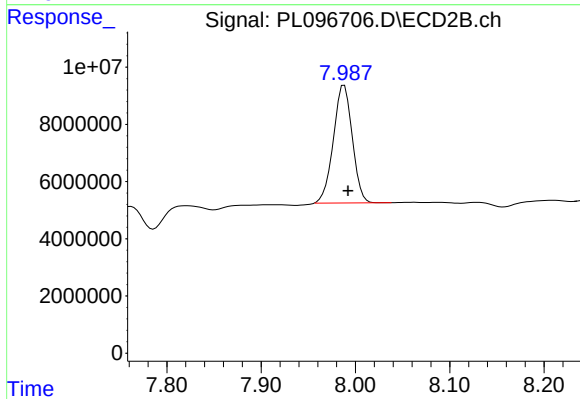

#28 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: -0.004 min
Response: 57328326
Conc: 13.21 ng/ml