

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080525\
 Data File : PL096708.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2025 15:48
 Operator : AR\AJ
 Sample : Q2763-01 101X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 01:53:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.532	2.826	10283355	10029198	3.233	2.099 #
28)	SA Decachlor...	0.000	7.988	0	9274421	N.D.	2.138 #
Target Compounds							
8)	B Heptachlo...	5.651	0.000	3462306	0	0.898	N.D. #
10)	B gamma-Chl...	0.000	5.052	0	8090933	N.D.	1.376 #
12)	B 4,4'-DDE	6.162	5.301	8174917	11356822	2.546	2.059
13)	MA Dieldrin	0.000	5.432	0	9489300	N.D.	1.607 #
14)	MA Endrin	0.000	5.715	0	6372157	N.D.	1.179 #
16)	A 4,4'-DDD	6.671	5.854	84442366	156.3E6	33.398	33.218
17)	MA 4,4'-DDT	0.000	6.101	0	8039734	N.D.	1.589 #
25)	Chlordane-3	0.000	5.052	0	8090933	N.D.	11.637 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080525\
Data File : PL096708.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2025 15:48
Operator : AR\AJ
Sample : Q2763-01 101X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 01:53:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:58:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

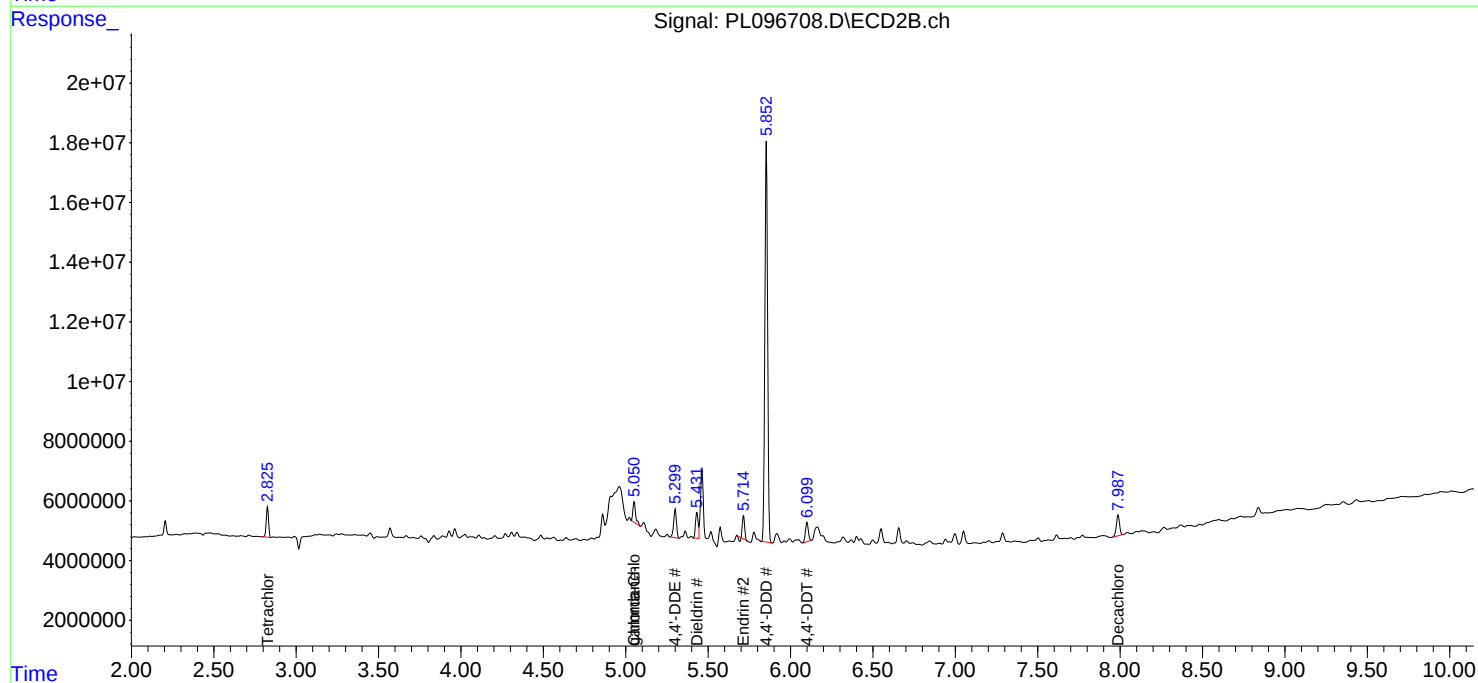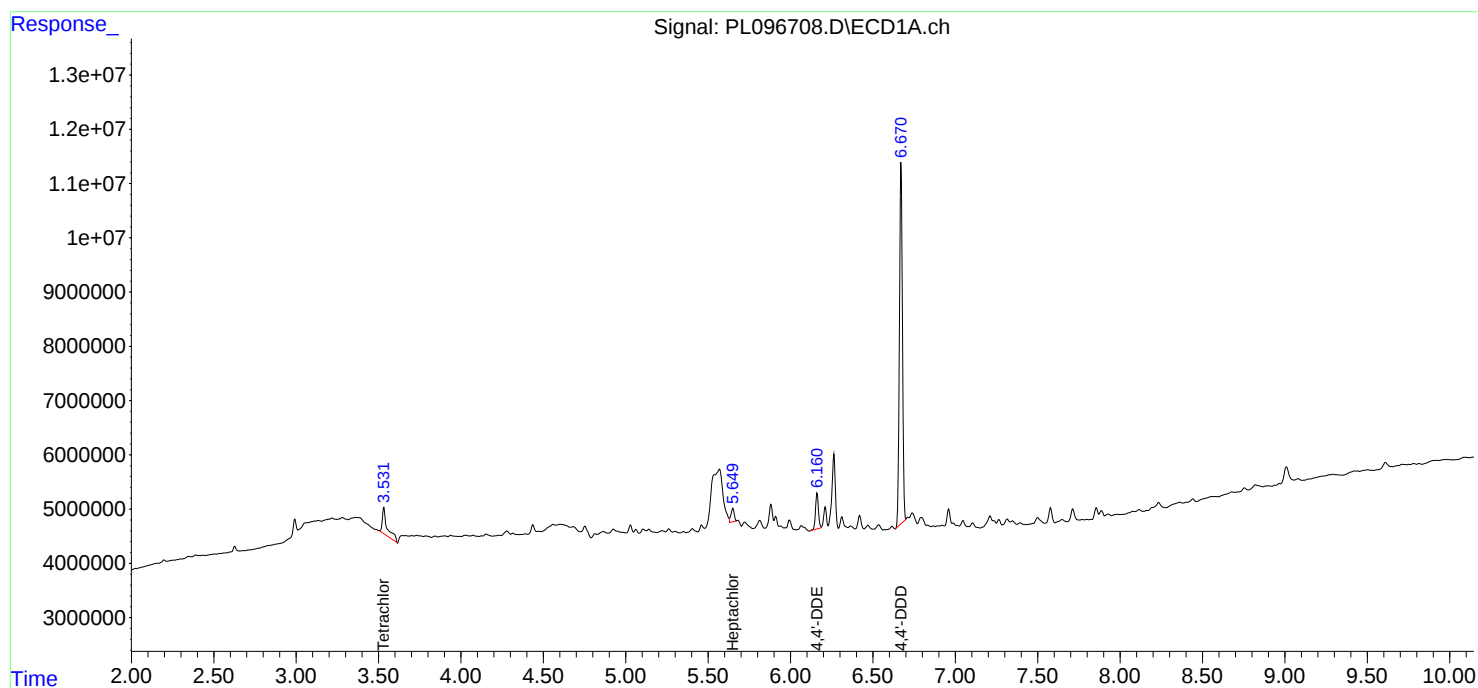


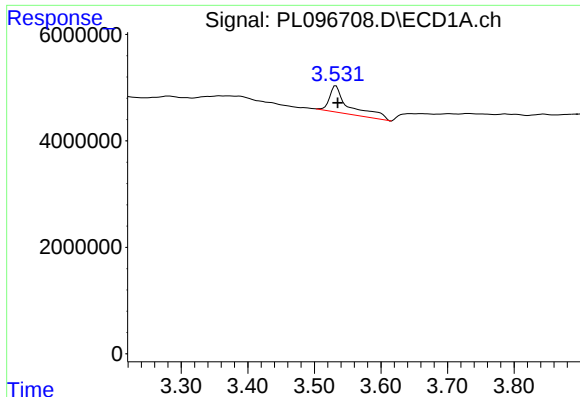

#1 Tetrachloro-m-xylene


R.T.: 3.532 min
Delta R.T.: -0.003 min
Response: 10283355
Conc: 3.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

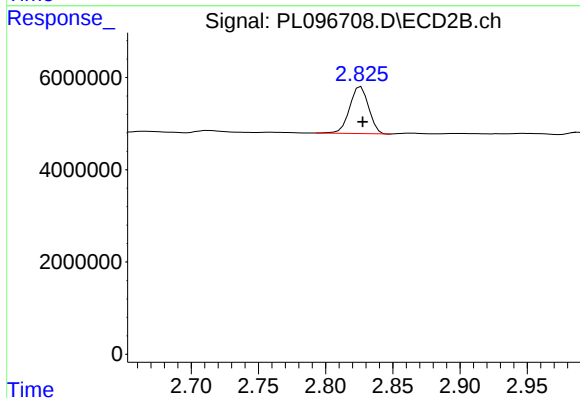


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: -0.001 min
Response: 10029198
Conc: 2.10 ng/ml

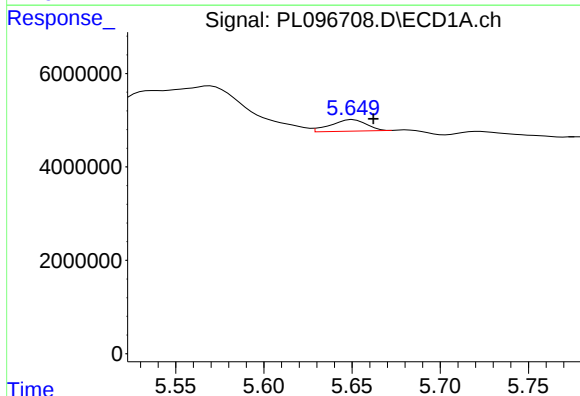


#8 Heptachlor epoxide

R.T.: 5.651 min
Delta R.T.: -0.012 min
Response: 3462306
Conc: 0.90 ng/ml

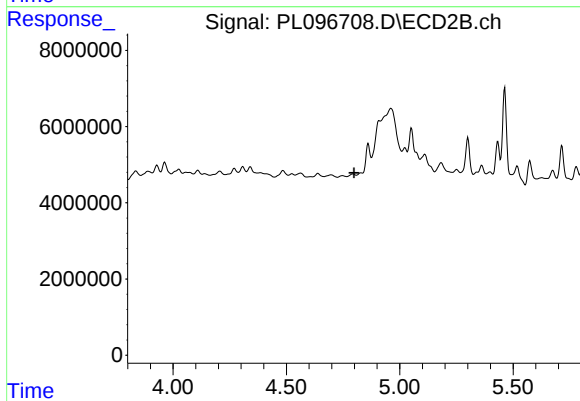

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.799 min
Response: 0
Conc: N.D.

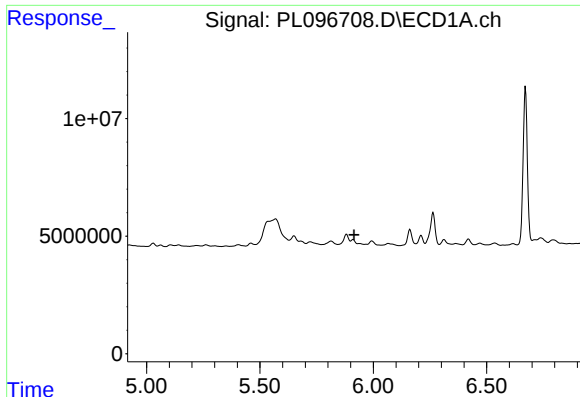

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.916 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

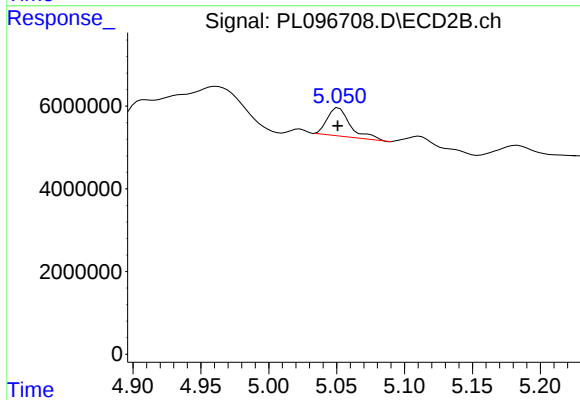


#10 gamma-Chlordane

R.T.: 5.052 min
Delta R.T.: 0.000 min
Response: 8090933
Conc: 1.38 ng/ml

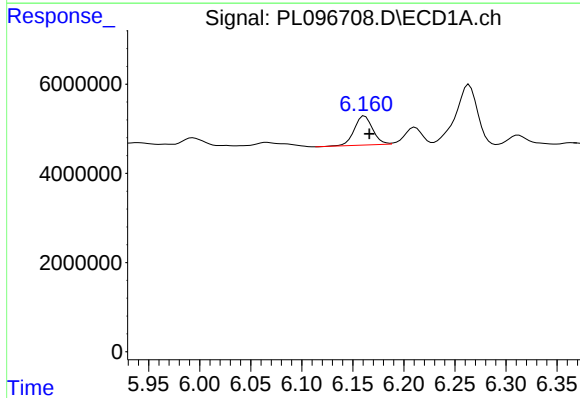


#12 4,4'-DDE

R.T.: 6.162 min
Delta R.T.: -0.005 min
Response: 8174917
Conc: 2.55 ng/ml

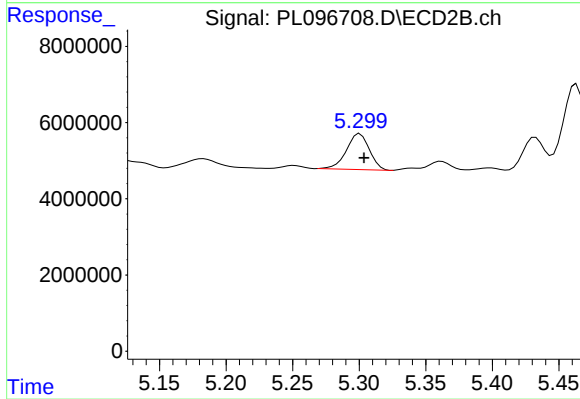

#12 4,4'-DDE


R.T.: 5.301 min
Delta R.T.: -0.003 min
Response: 11356822
Conc: 2.06 ng/ml

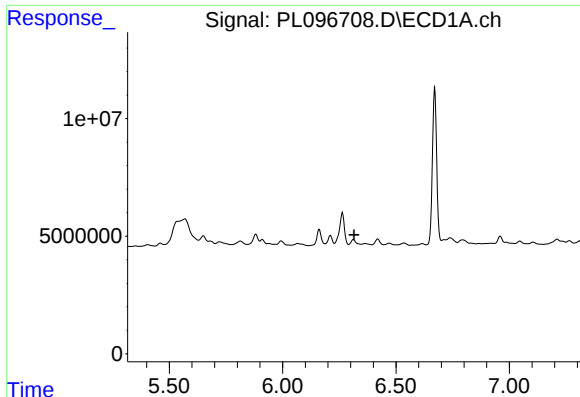

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

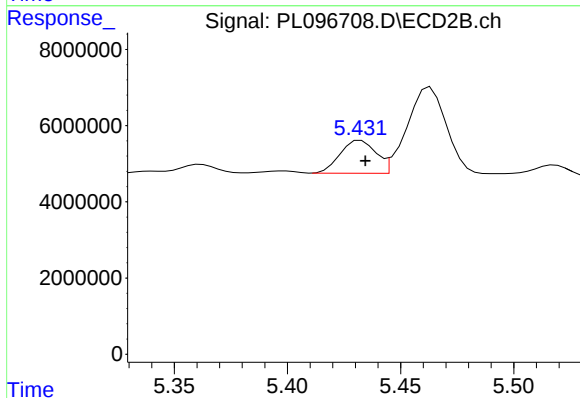


#13 Dieldrin

R.T.: 5.432 min
Delta R.T.: -0.002 min
Response: 9489300
Conc: 1.61 ng/ml

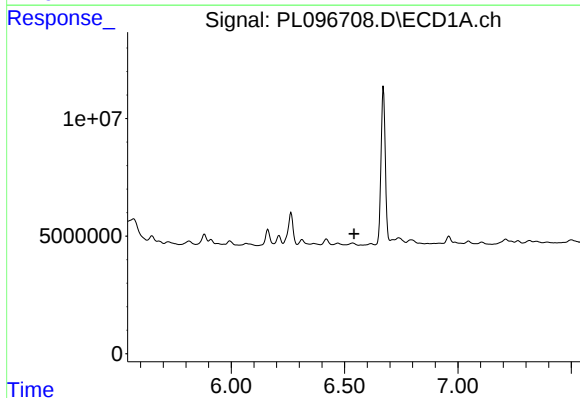


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.542 min
Response: 0
Conc: N.D.

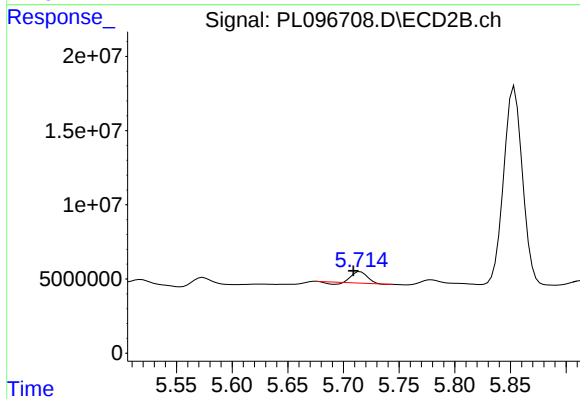

#14 Endrin


R.T.: 5.715 min
Delta R.T.: 0.006 min
Response: 6372157
Conc: 1.18 ng/ml

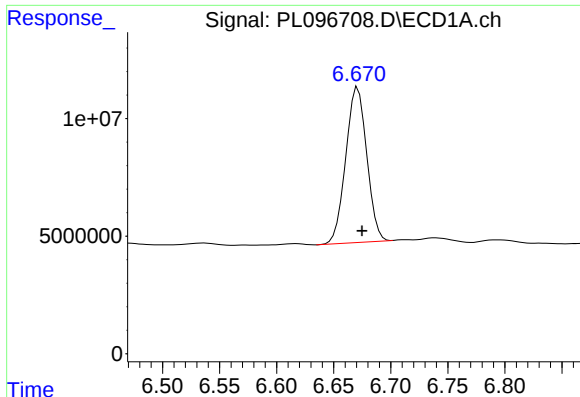

#16 4,4'-DDD


R.T.: 6.671 min
Delta R.T.: -0.004 min
Response: 84442366
Conc: 33.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

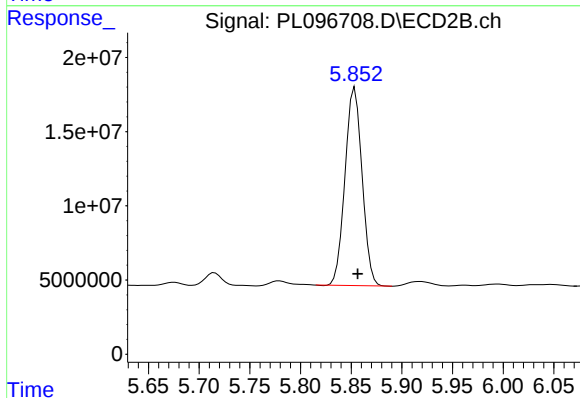


#16 4,4'-DDD

R.T.: 5.854 min
Delta R.T.: -0.003 min
Response: 156300756
Conc: 33.22 ng/ml

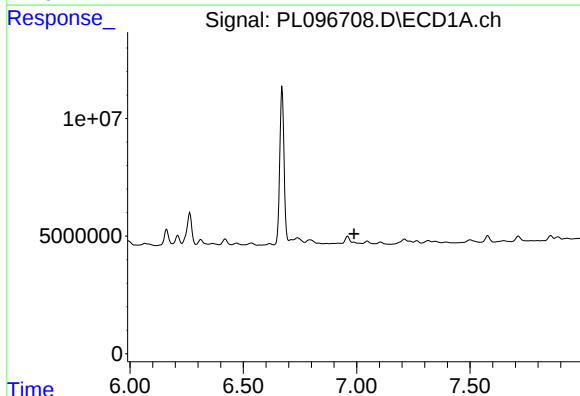


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.

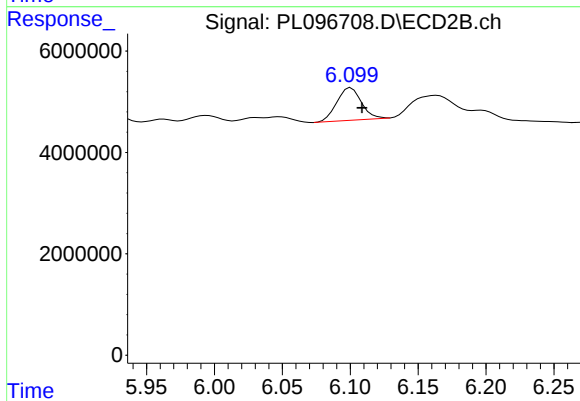

#17 4,4'-DDT


R.T.: 6.101 min
Delta R.T.: -0.008 min
Response: 8039734
Conc: 1.59 ng/ml

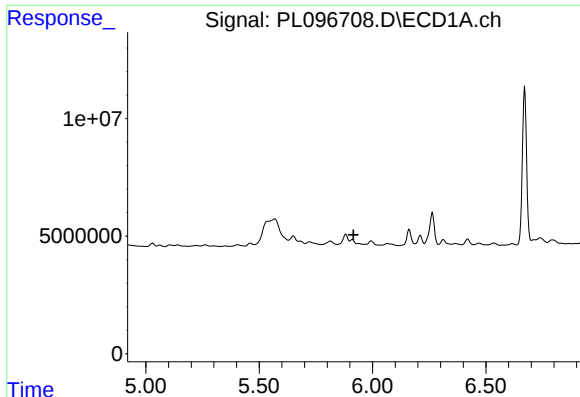

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.917 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

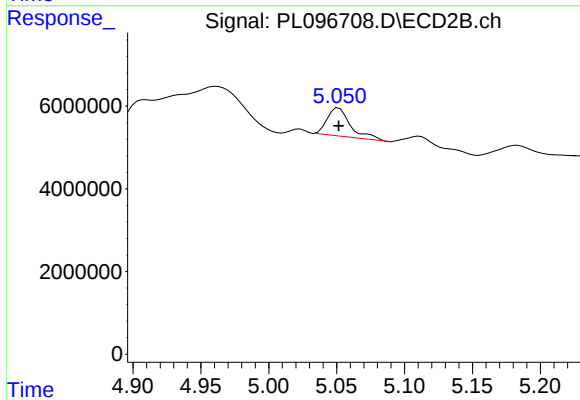


#25 Chlordane-3

R.T.: 5.052 min
Delta R.T.: 0.000 min
Response: 8090933
Conc: 11.64 ng/ml

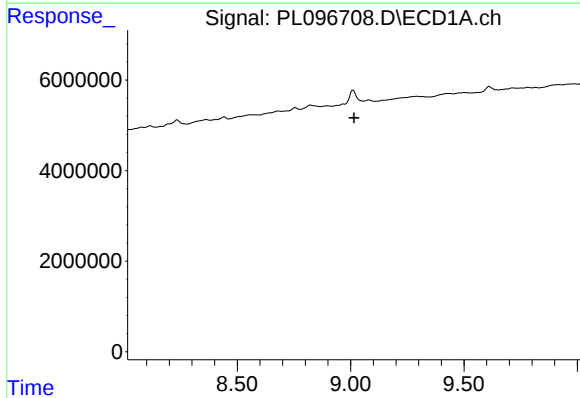

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.016 min
Response: 0
Conc: N.D.

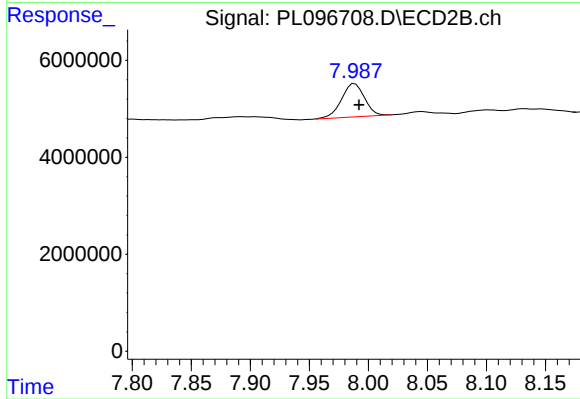

#28 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: -0.004 min
Response: 9274421
Conc: 2.14 ng/ml