

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
 Data File : PL038966.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2018 17:22
 Operator : AJ\SJ
 Sample : PB111791BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 04:20:58 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.927	147.0E6	57915085	19.739	22.063
28)	SA Decachlor...	7.989	8.932	145.2E6	55878896	19.147	22.860
Target Compounds							
2)	A alpha-BHC	0.000	4.323	0	510611	N.D.	0.132 #
3)	MA gamma-BHC...	0.000	4.585	0	197327	N.D.	0.055 #
4)	MA Heptachlor	0.000	5.100	0	294141	N.D.	0.092 #
7)	B delta-BHC	0.000	4.956	0	1327288	N.D.	0.400 #
8)	B Heptachlo...	0.000	5.800	0	667812	N.D.	0.235 #
15)	B Endosulfa...	0.000	6.826	0	369008	N.D.	0.154 #
16)	A 4,4'-DDD	0.000	6.753	0	48483	N.D.	0.023 #
23)	Chlordane-1	4.236	4.956	15388749	1327288	44.444	11.454 #
27)	Chlordane-5	0.000	6.826	0	369008	N.D.	4.119 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
Data File : PL038966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2018 17:22
Operator : AJ\SJ
Sample : PB111791BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 04:20:58 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

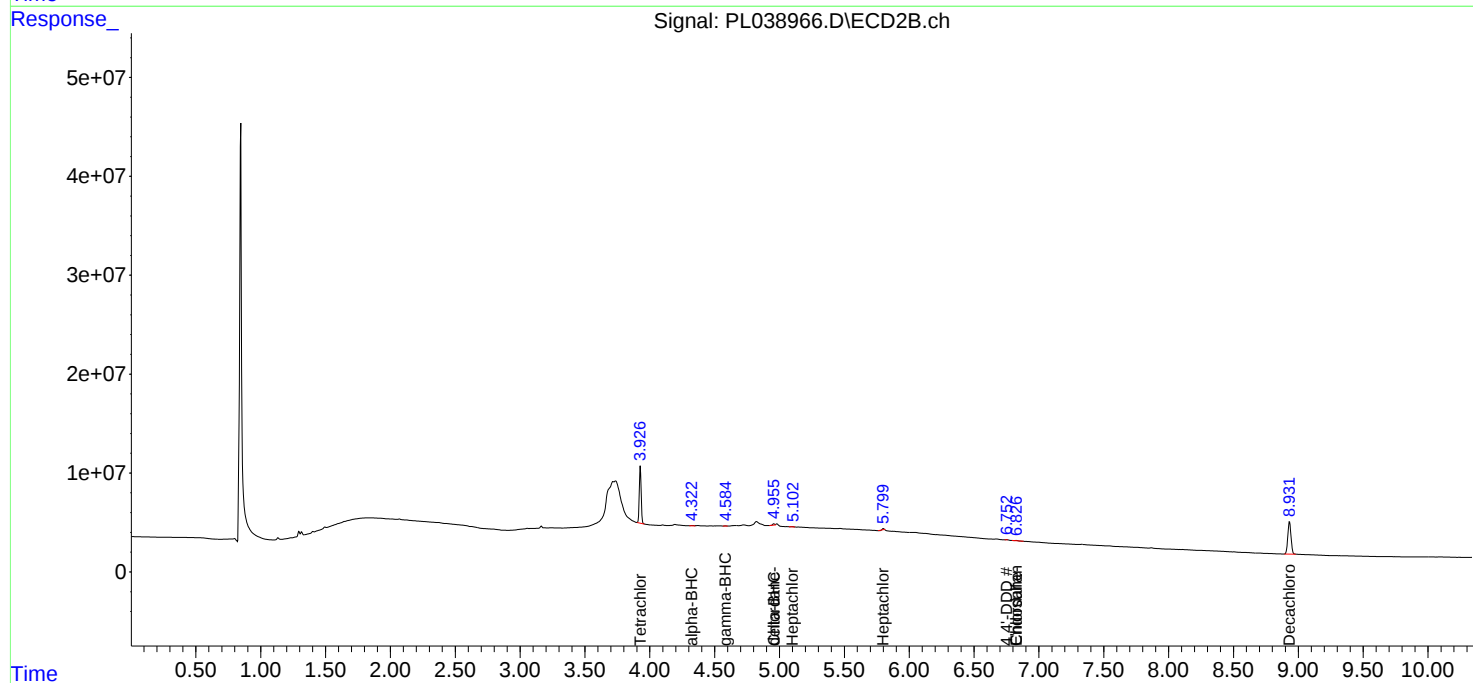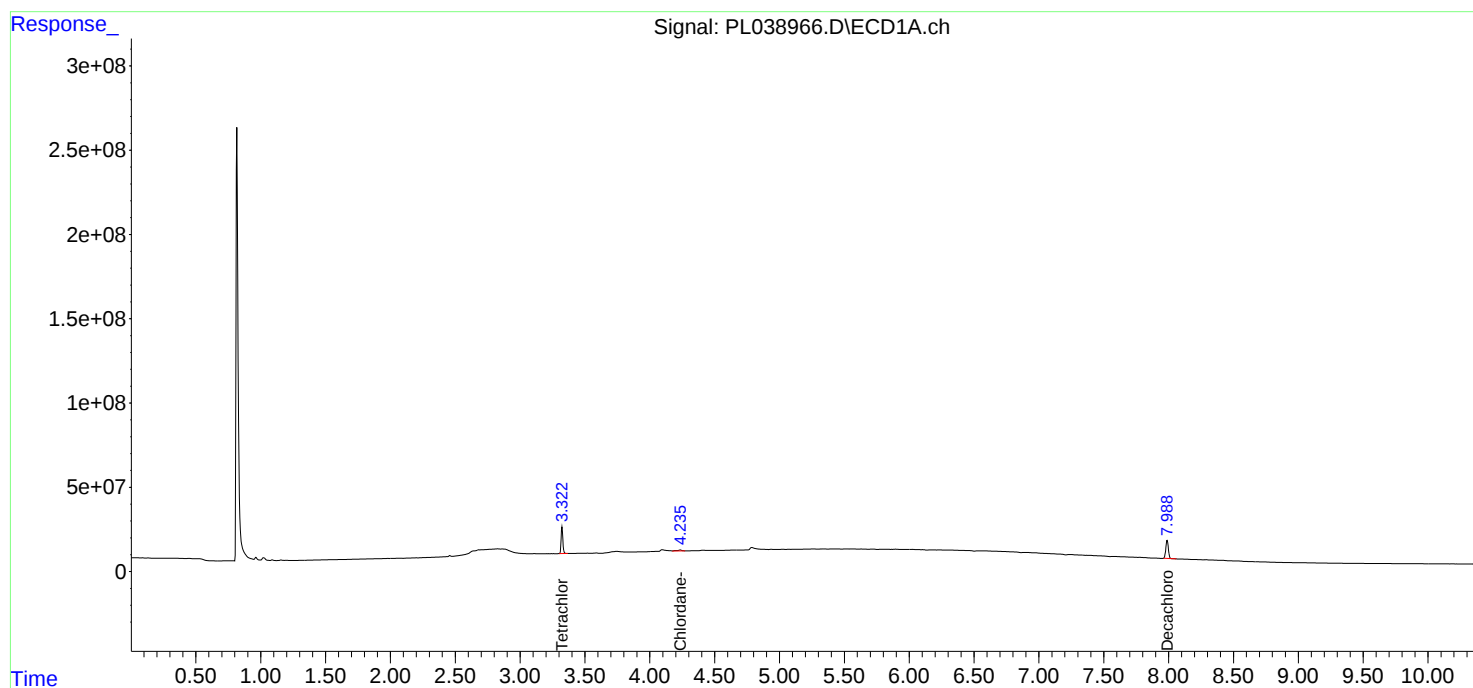


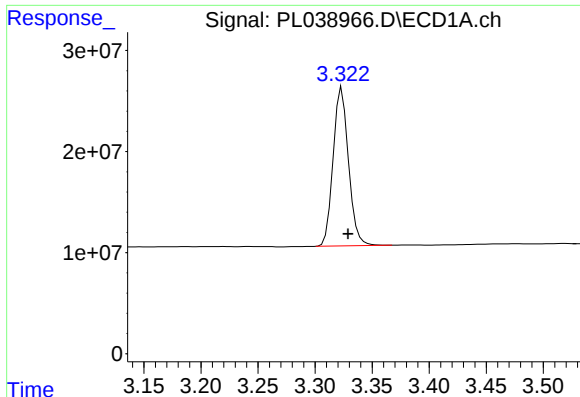

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: -0.006 min
Response: 146982934
Conc: 19.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

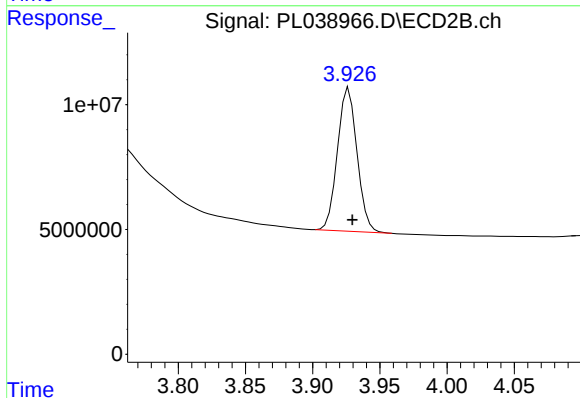


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 57915085
Conc: 22.06 ng/ml

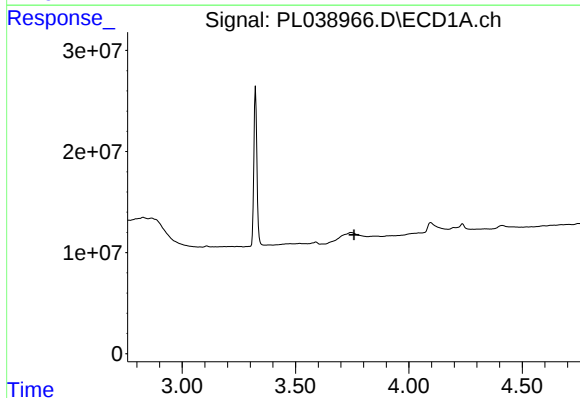


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

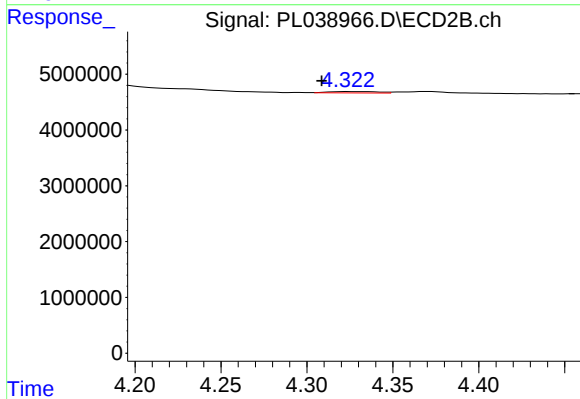

#2 alpha-BHC


R.T.: 4.323 min
Delta R.T.: 0.015 min
Response: 510611
Conc: 0.13 ng/ml

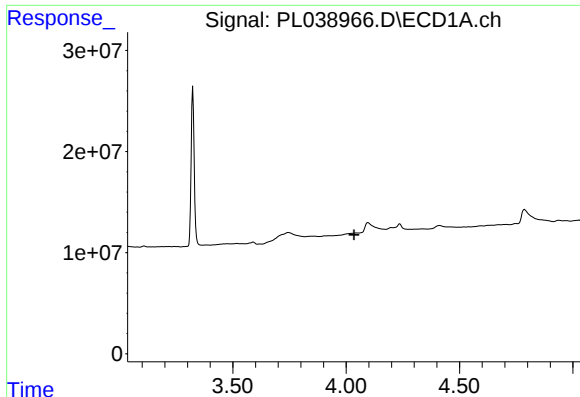

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

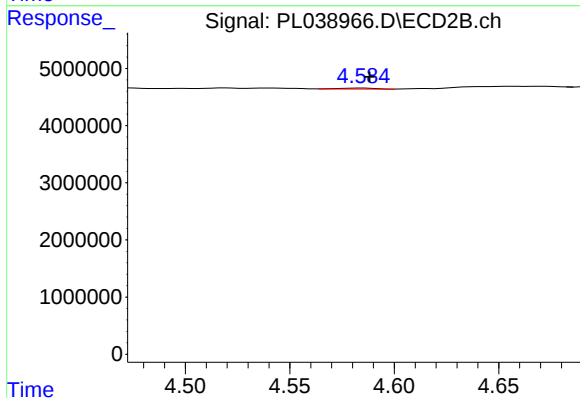


#3 gamma-BHC (Lindane)

R.T.: 4.585 min
Delta R.T.: -0.003 min
Response: 197327
Conc: 0.05 ng/ml

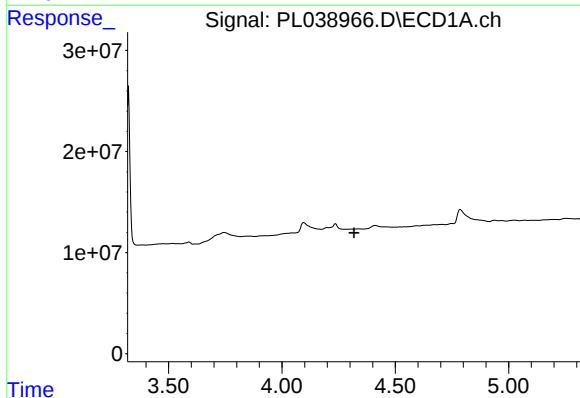


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

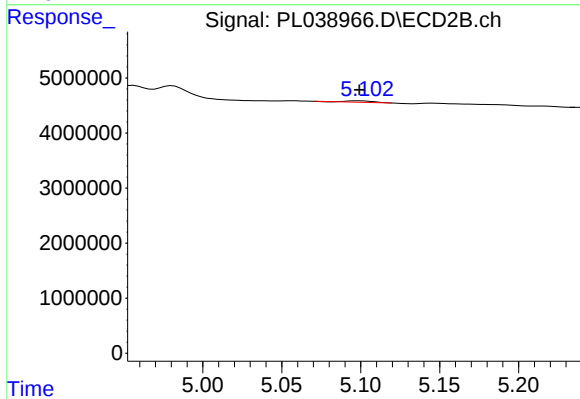

#4 Heptachlor


R.T.: 5.100 min
Delta R.T.: 0.000 min
Response: 294141
Conc: 0.09 ng/ml

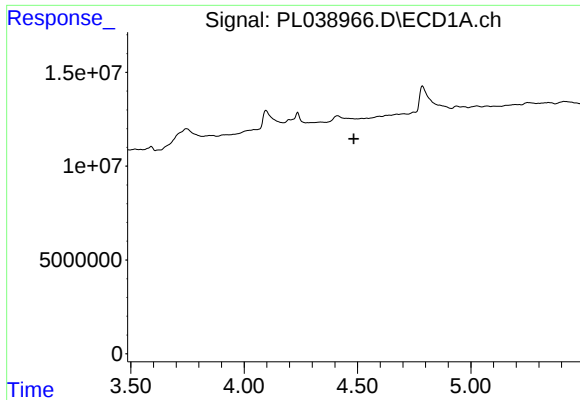

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

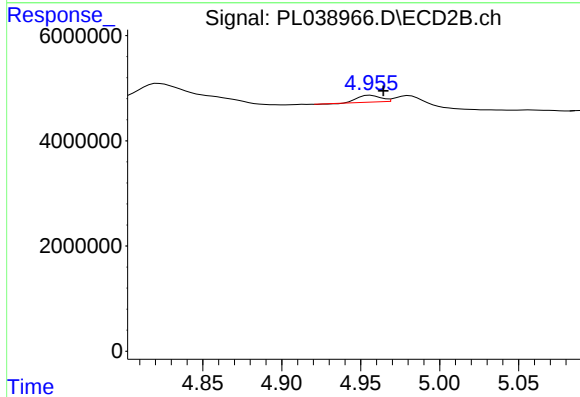


#7 delta-BHC

R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 1327288
Conc: 0.40 ng/ml

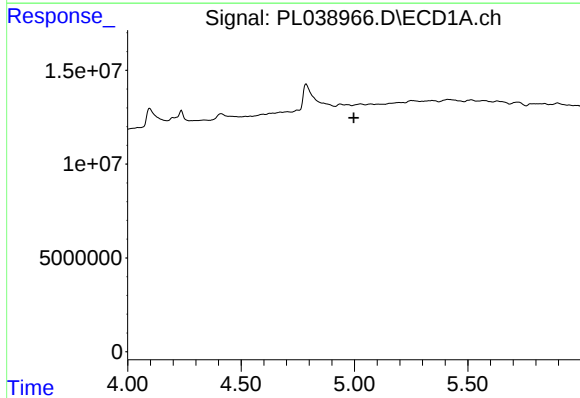


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

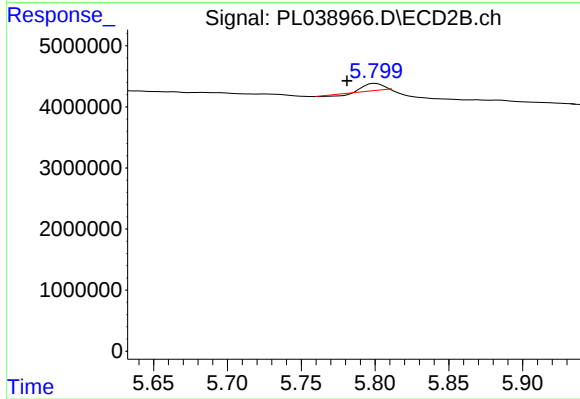

#8 Heptachlor epoxide


R.T.: 5.800 min
Delta R.T.: 0.019 min
Response: 667812
Conc: 0.23 ng/ml

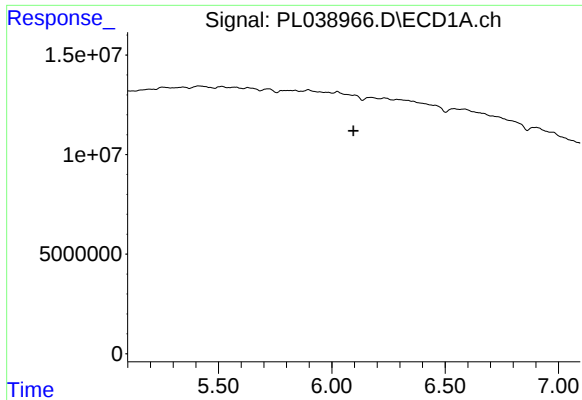

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

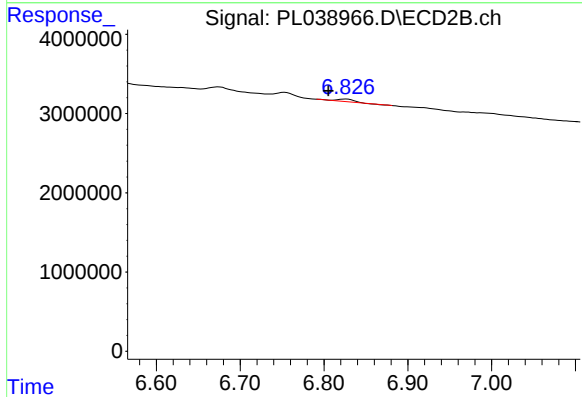


#15 Endosulfan II

R.T.: 6.826 min
Delta R.T.: 0.021 min
Response: 369008
Conc: 0.15 ng/ml

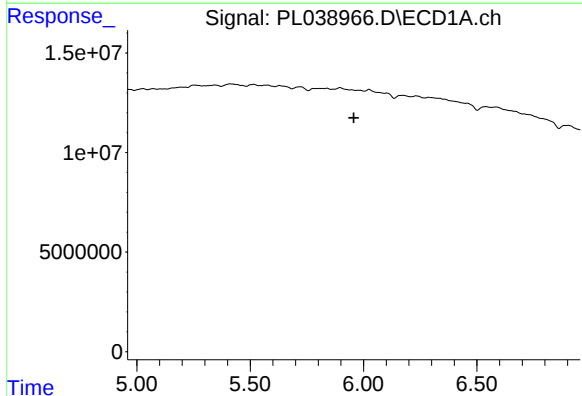


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

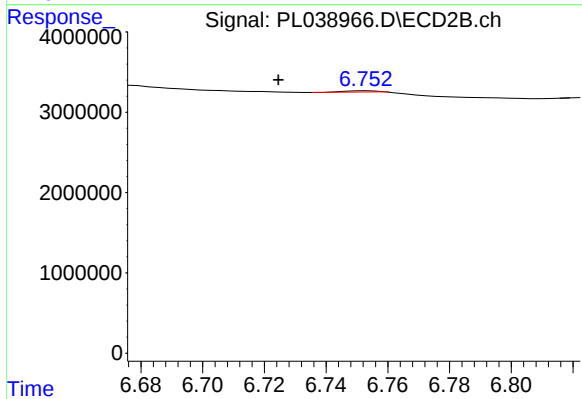

#16 4,4'-DDD


R.T.: 6.753 min
Delta R.T.: 0.029 min
Response: 48483
Conc: 0.02 ng/ml

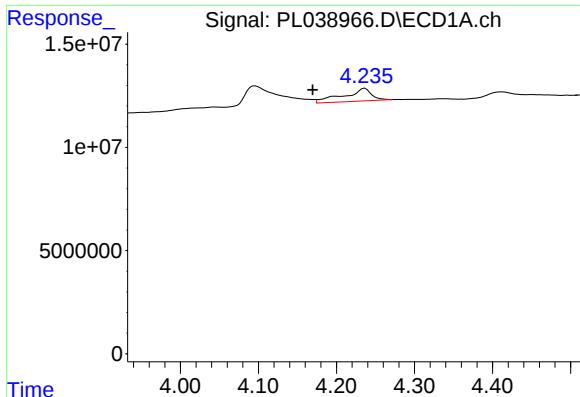

#23 Chlordane-1


R.T.: 4.236 min
Delta R.T.: 0.067 min
Response: 15388749
Conc: 44.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

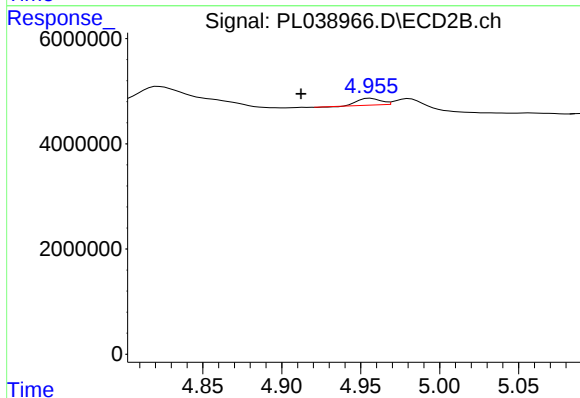


#23 Chlordane-1

R.T.: 4.956 min
Delta R.T.: 0.044 min
Response: 1327288
Conc: 11.45 ng/ml

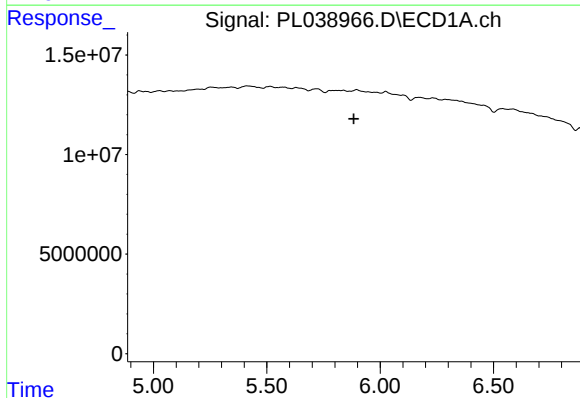


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.883 min
Response: 0
Conc: N.D.

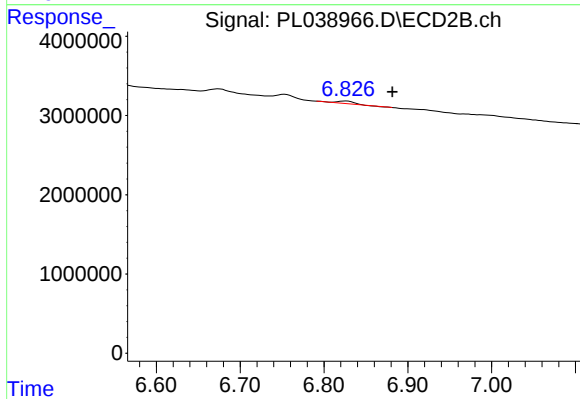

#27 Chlordane-5


R.T.: 6.826 min
Delta R.T.: -0.055 min
Response: 369008
Conc: 4.12 ng/ml

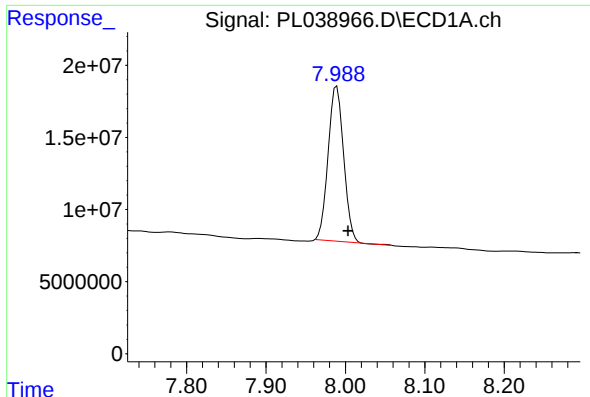

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.014 min
Response: 145246714
Conc: 19.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

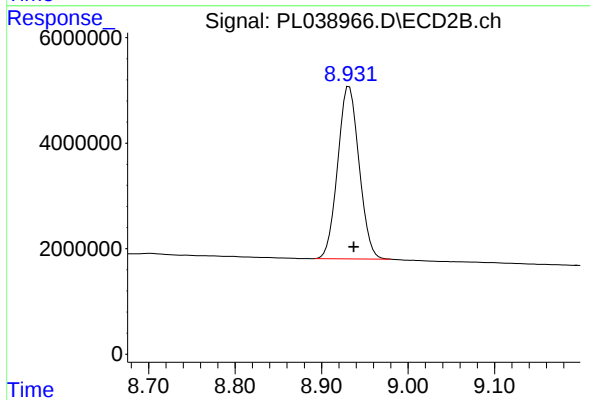

#28 Decachlorobiphenyl

R.T.: 8.932 min
Delta R.T.: -0.005 min
Response: 55878896
Conc: 22.86 ng/ml