

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
 Data File : PL038974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2018 01:57
 Operator : AJ\SJ
 Sample : J4283-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 04:24:17 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.927	130.8E6	52032691	17.563	19.822
28)	SA Decachlor...	7.990	8.933	143.3E6	54981039	18.888	22.492
Target Compounds							
2)	A alpha-BHC	0.000	4.275f	0	2166593	N.D.	0.560 #
3)	MA gamma-BHC...	0.000	4.554f	0	198210	N.D.	0.055 #
4)	MA Heptachlor	0.000	5.149f	0	1158273	N.D.	0.362 #
7)	B delta-BHC	0.000	4.956	0	5274411	N.D.	1.590 #
8)	B Heptachlo...	0.000	5.800	0	1247984	N.D.	0.439 #
15)	B Endosulfa...	0.000	6.825	0	648098	N.D.	0.270 #
16)	A 4,4'-DDD	0.000	6.673f	0	330639	N.D.	0.154 #
23)	Chlordane-1	4.238	4.956	23573908	5274411	68.083	45.514 #
27)	Chlordane-5	0.000	6.825	0	648098	N.D.	7.235 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
Data File : PL038974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2018 01:57
Operator : AJ\SJ
Sample : J4283-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 04:24:17 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

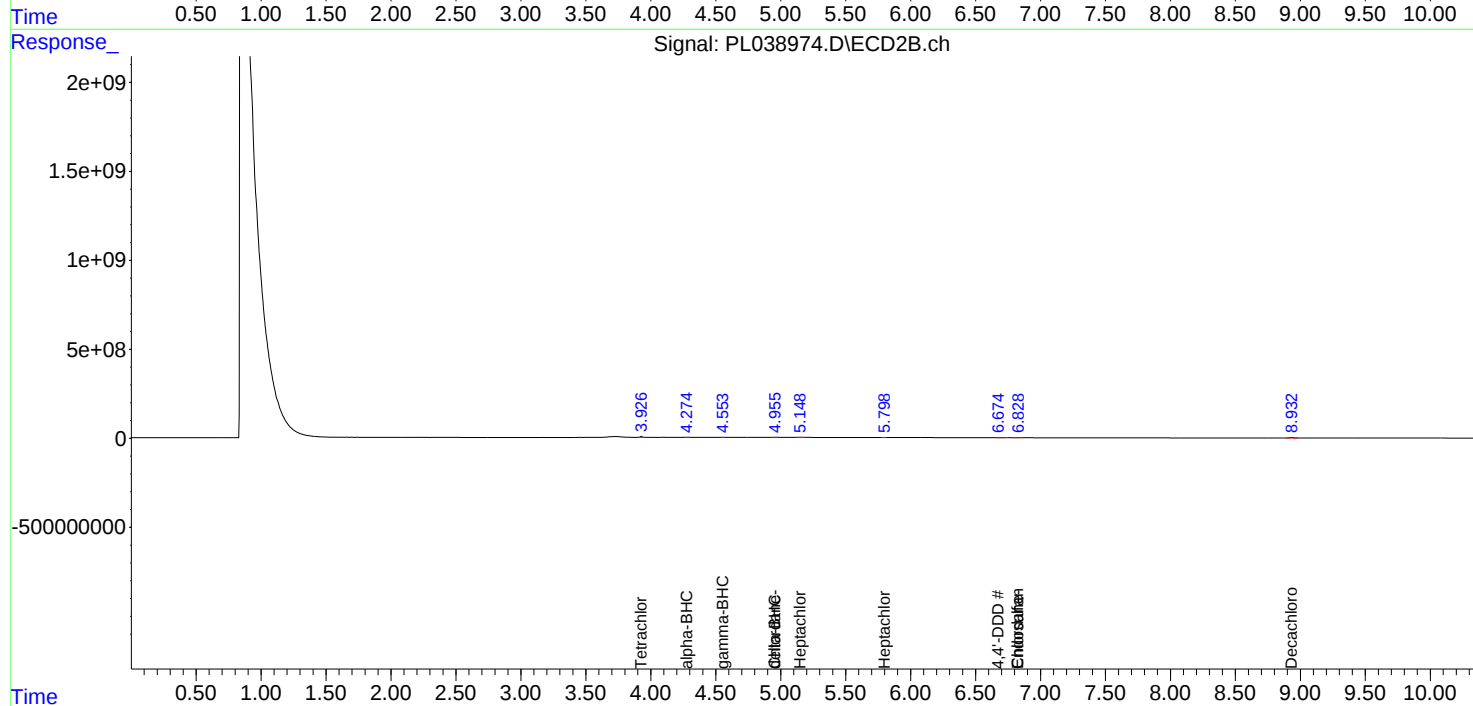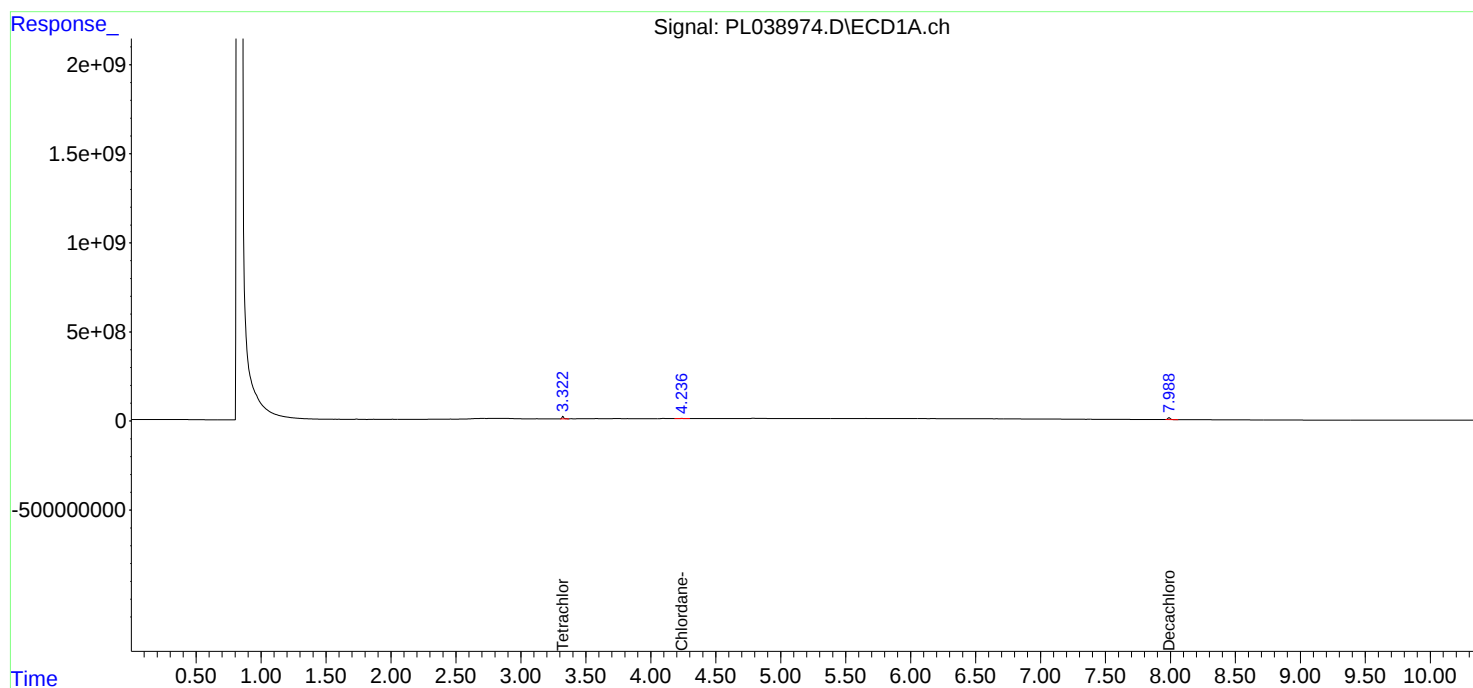


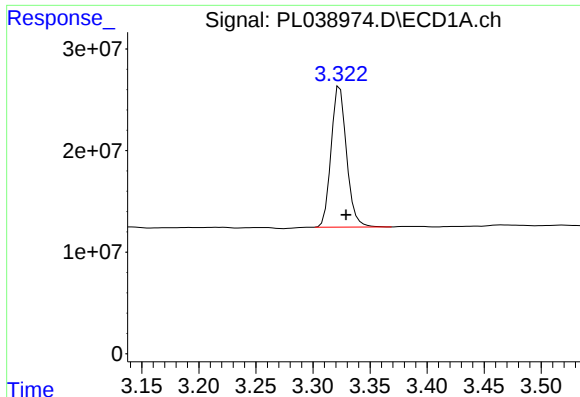

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.005 min
Response: 130782835
Conc: 17.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

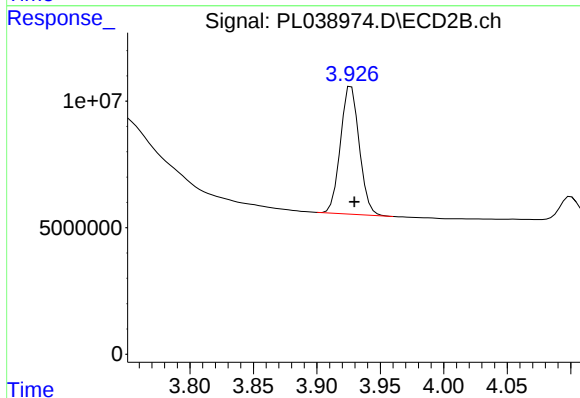


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.002 min
Response: 52032691
Conc: 19.82 ng/ml

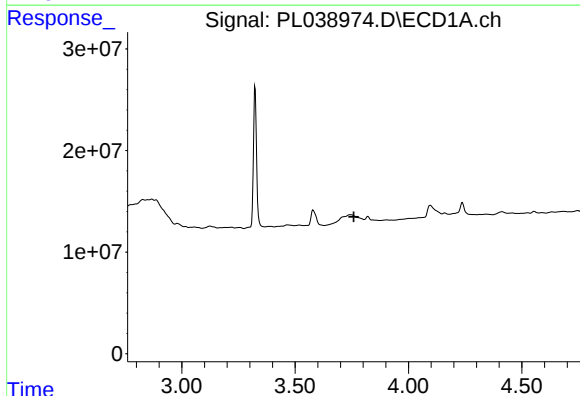


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

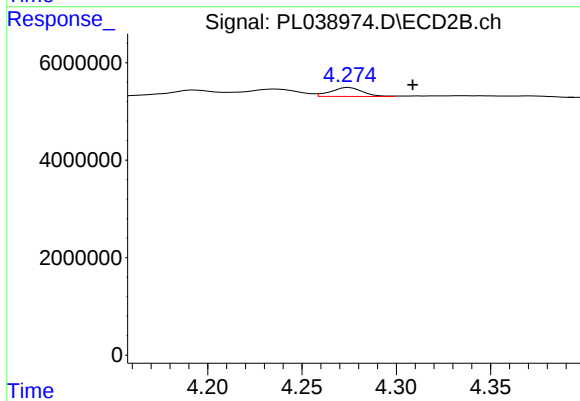

#2 alpha-BHC


R.T.: 4.275 min
Delta R.T.: -0.033 min
Response: 2166593
Conc: 0.56 ng/ml

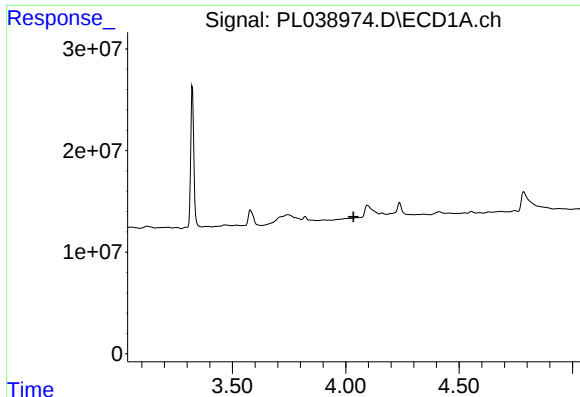

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

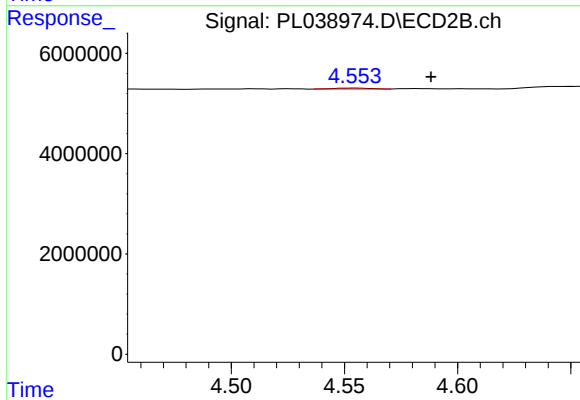


#3 gamma-BHC (Lindane)

R.T.: 4.554 min
Delta R.T.: -0.034 min
Response: 198210
Conc: 0.05 ng/ml

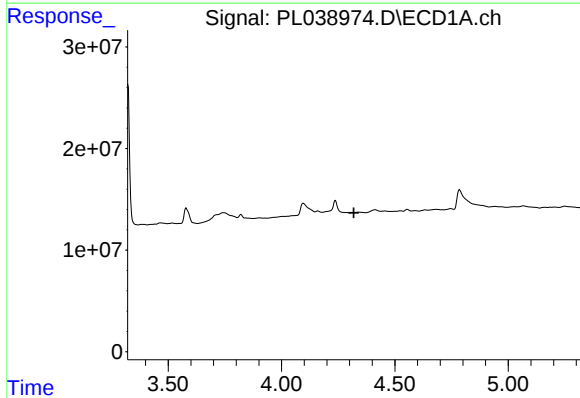


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

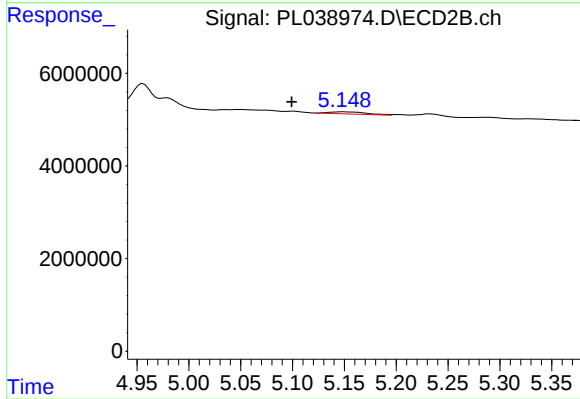

#4 Heptachlor


R.T.: 5.149 min
Delta R.T.: 0.050 min
Response: 1158273
Conc: 0.36 ng/ml

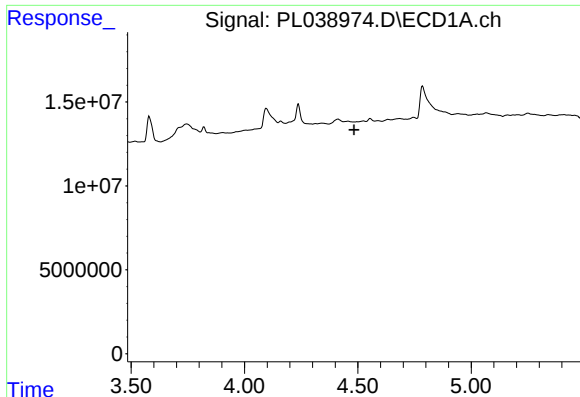

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

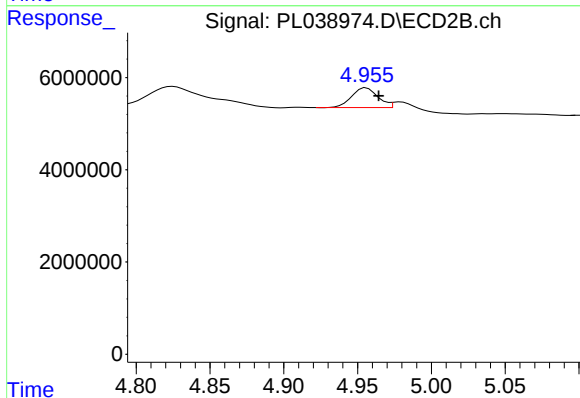


#7 delta-BHC

R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 5274411
Conc: 1.59 ng/ml

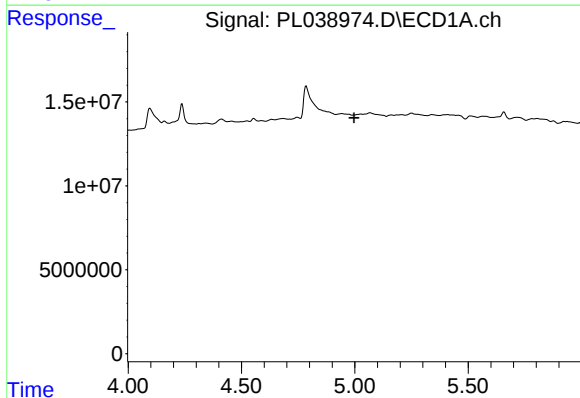


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

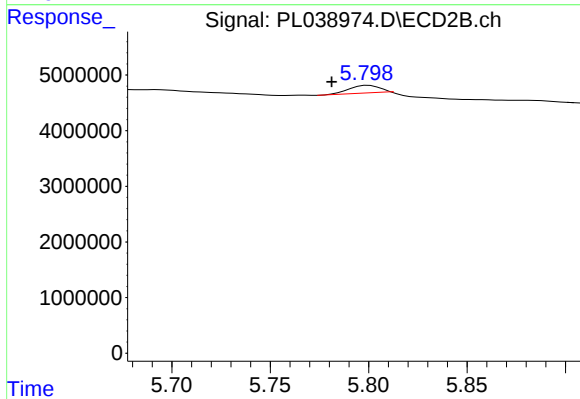

#8 Heptachlor epoxide


R.T.: 5.800 min
Delta R.T.: 0.019 min
Response: 1247984
Conc: 0.44 ng/ml

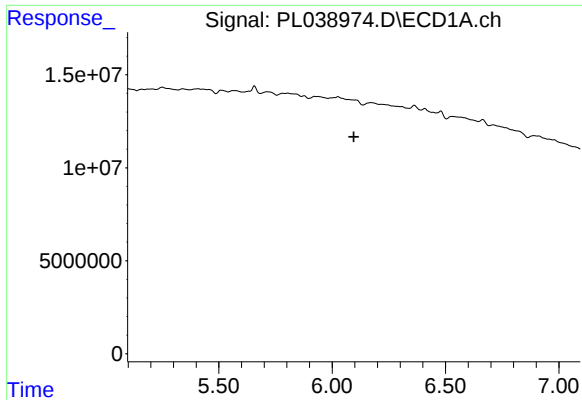

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

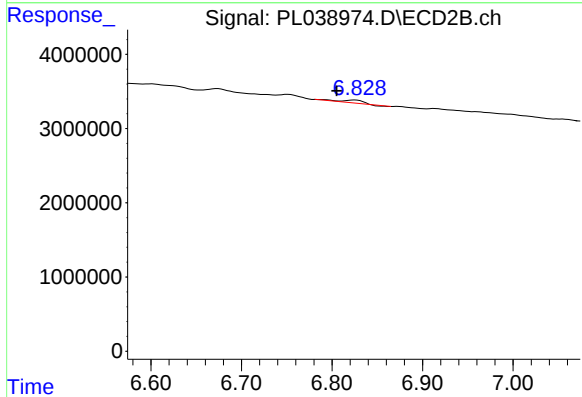


#15 Endosulfan II

R.T.: 6.825 min
Delta R.T.: 0.020 min
Response: 648098
Conc: 0.27 ng/ml

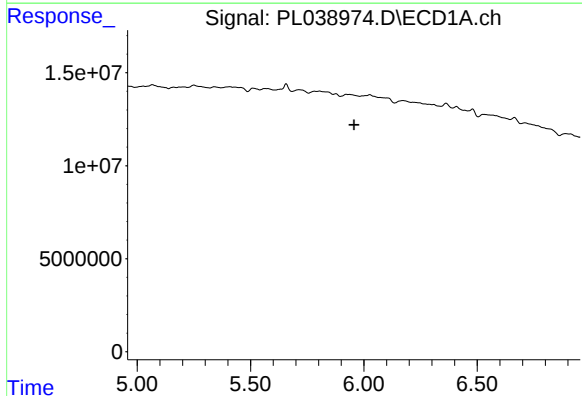


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

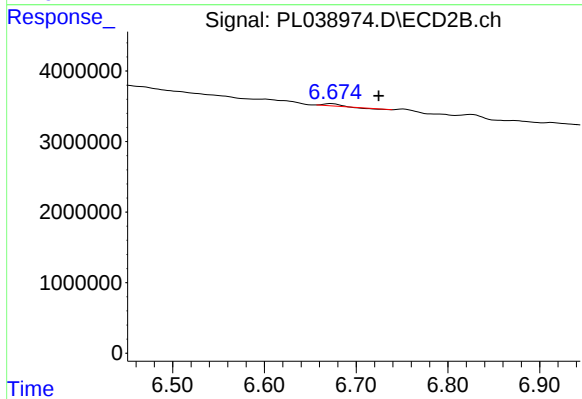

#16 4,4'-DDD


R.T.: 6.673 min
Delta R.T.: -0.051 min
Response: 330639
Conc: 0.15 ng/ml

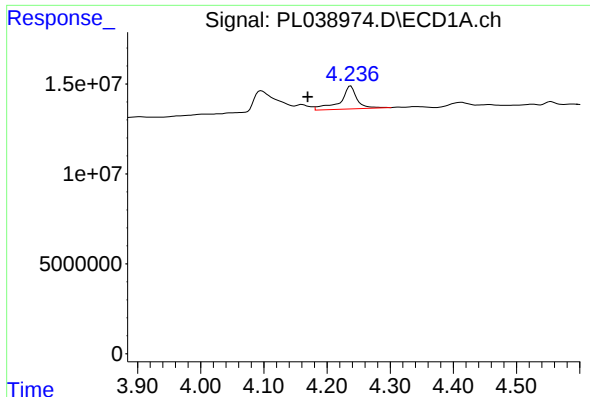

#23 Chlordane-1


R.T.: 4.238 min
Delta R.T.: 0.068 min
Response: 23573908
Conc: 68.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

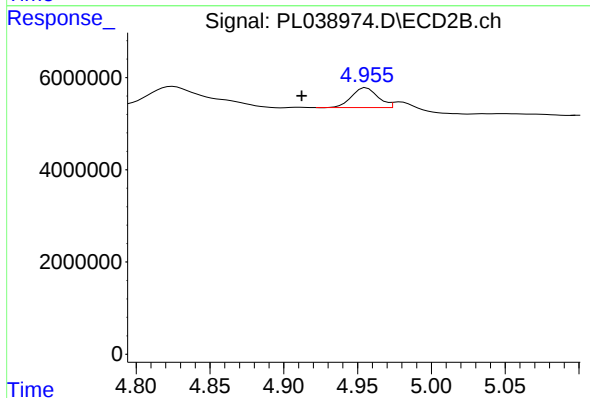


#23 Chlordane-1

R.T.: 4.956 min
Delta R.T.: 0.044 min
Response: 5274411
Conc: 45.51 ng/ml

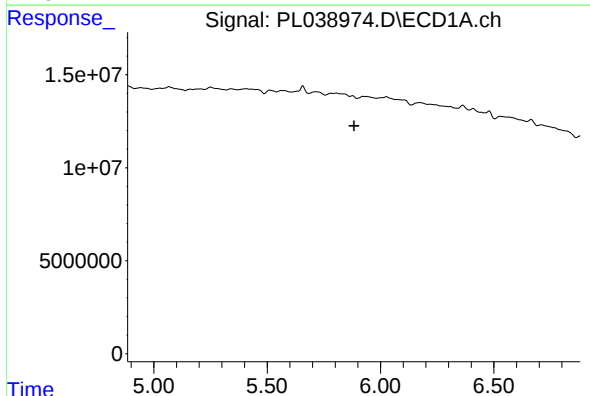


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.883 min
Response: 0
Conc: N.D.

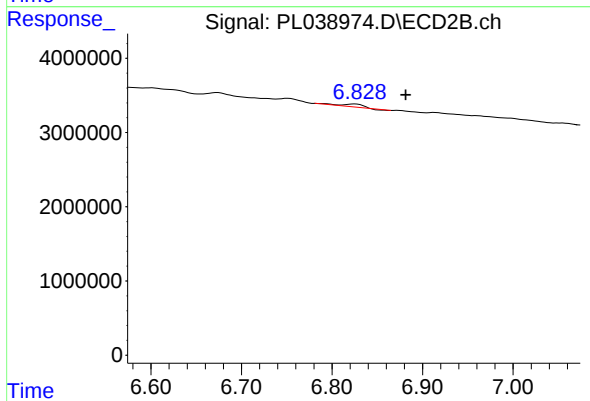

#27 Chlordane-5


R.T.: 6.825 min
Delta R.T.: -0.056 min
Response: 648098
Conc: 7.23 ng/ml

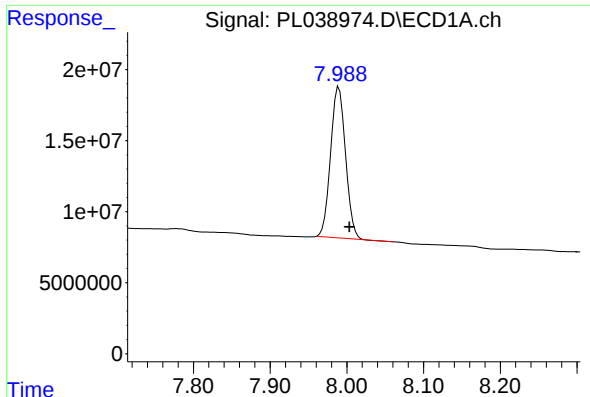

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.014 min
Response: 143282894
Conc: 18.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

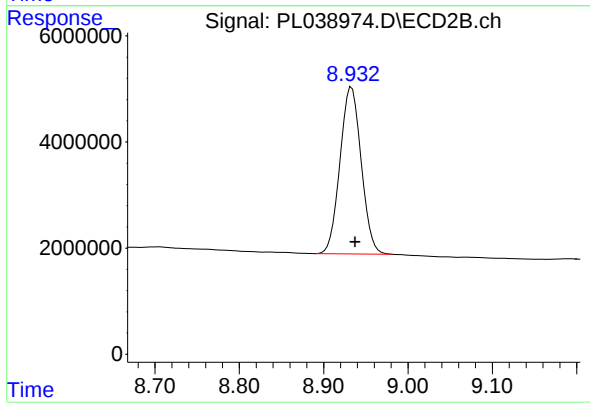

#28 Decachlorobiphenyl

R.T.: 8.933 min
Delta R.T.: -0.004 min
Response: 54981039
Conc: 22.49 ng/ml