

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
 Data File : PL038975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2018 02:11
 Operator : AJ\SJ
 Sample : J4333-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 04:24:35 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.927	127.9E6	51541735	17.177	19.635
28)	SA Decachlor...	7.990	8.935	145.0E6	55128446	19.114	22.553
Target Compounds							
2)	A alpha-BHC	0.000	4.276f	0	1528824	N.D.	0.395 #
3)	MA gamma-BHC...	0.000	4.547f	0	307921	N.D.	0.085 #
6)	B beta-BHC	0.000	4.730	0	441386	N.D.	0.291 #
7)	B delta-BHC	0.000	4.955	0	2067775	N.D.	0.623 #
8)	B Heptachlo...	0.000	5.801	0	2452107	N.D.	0.863 #
15)	B Endosulfa...	0.000	6.827	0	242614	N.D.	0.101 #
16)	A 4,4'-DDD	0.000	6.674f	0	155550	N.D.	0.073 #
23)	Chlordane-1	4.238	4.955	18003086	2067775	51.994	17.843 #
27)	Chlordane-5	0.000	6.827	0	242614	N.D.	2.708 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
Data File : PL038975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2018 02:11
Operator : AJ\SJ
Sample : J4333-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 04:24:35 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

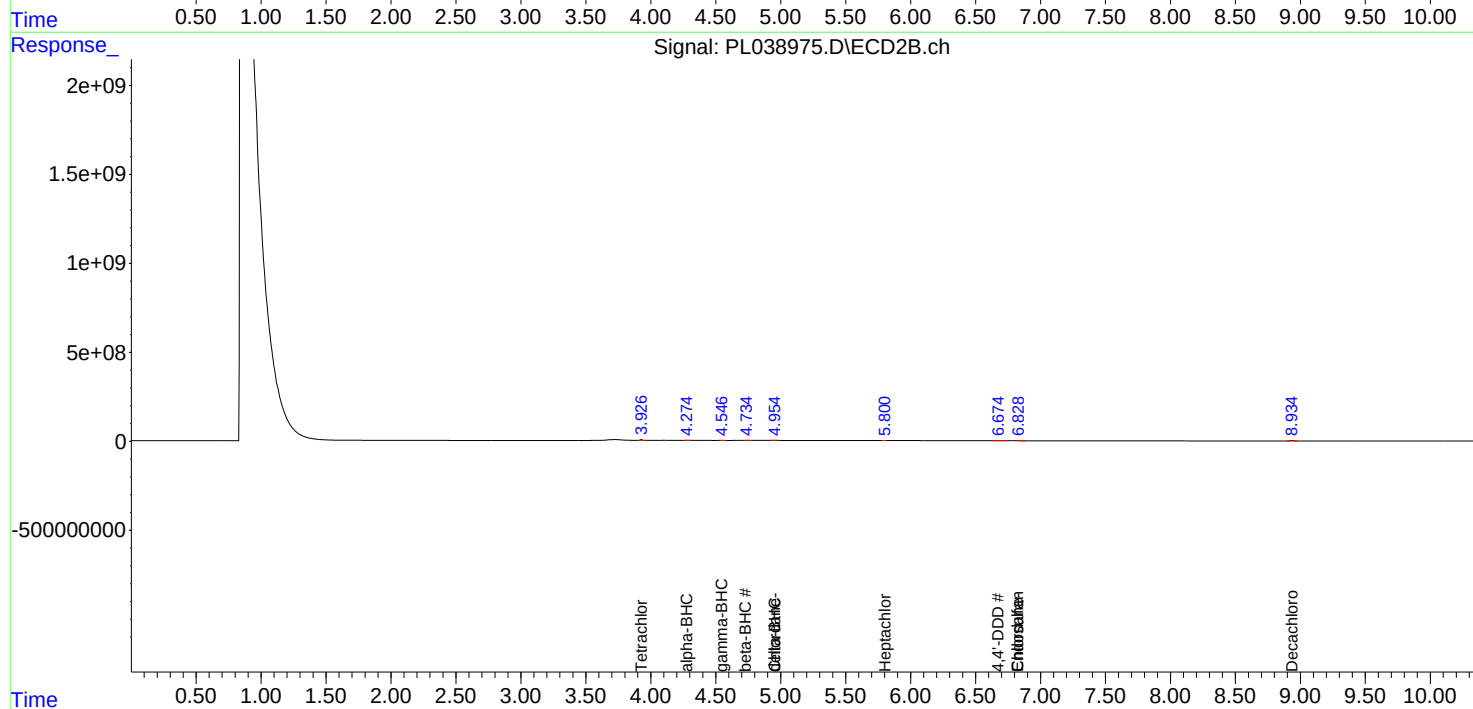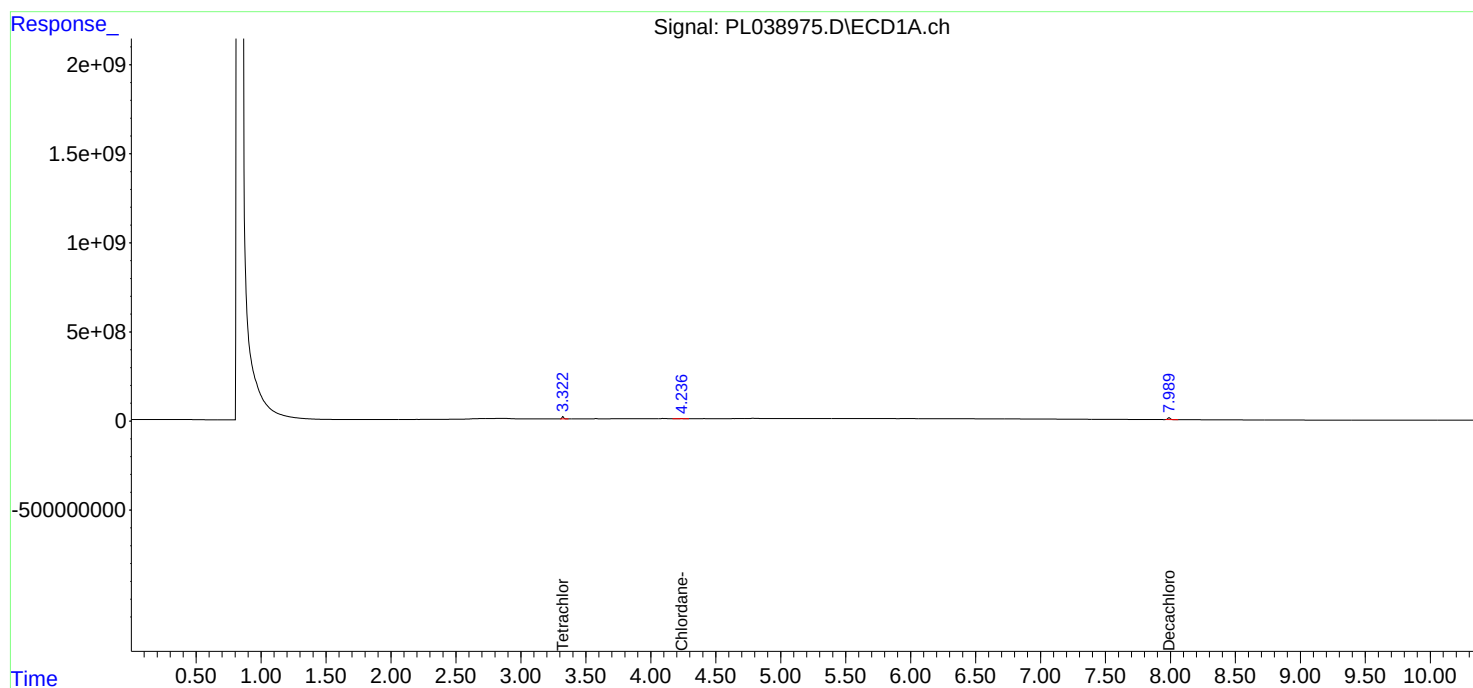


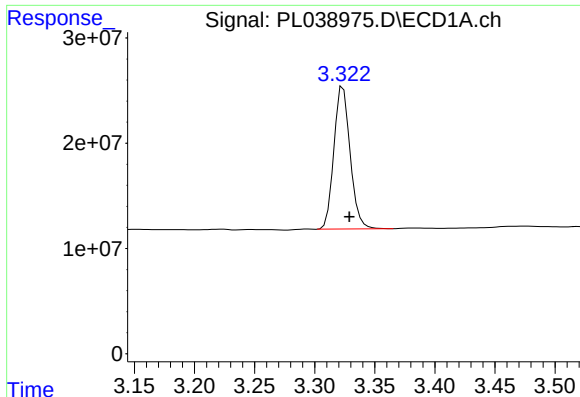

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.005 min
Response: 127909307
Conc: 17.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

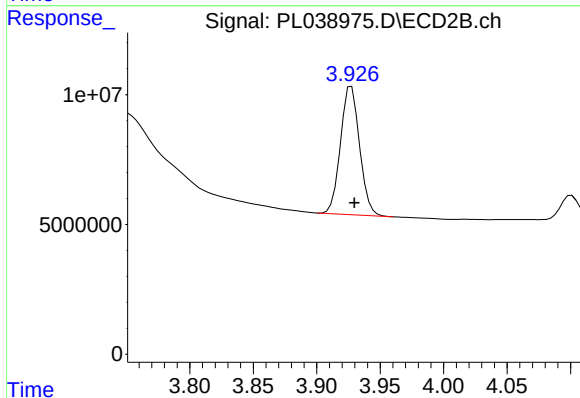


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.002 min
Response: 51541735
Conc: 19.64 ng/ml

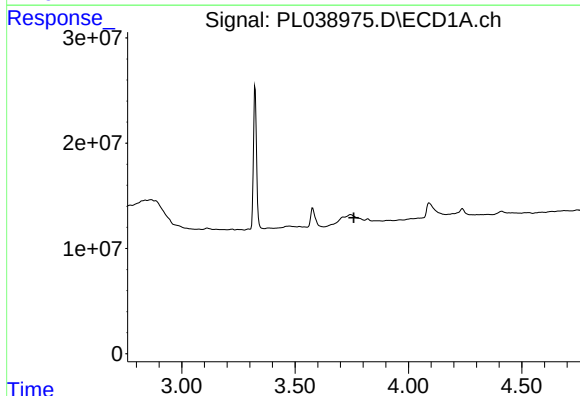


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

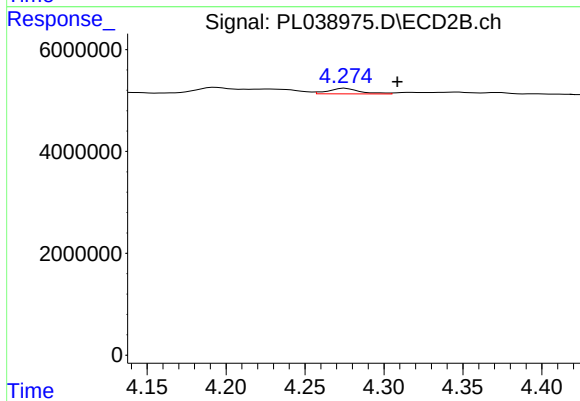

#2 alpha-BHC


R.T.: 4.276 min
Delta R.T.: -0.033 min
Response: 1528824
Conc: 0.40 ng/ml

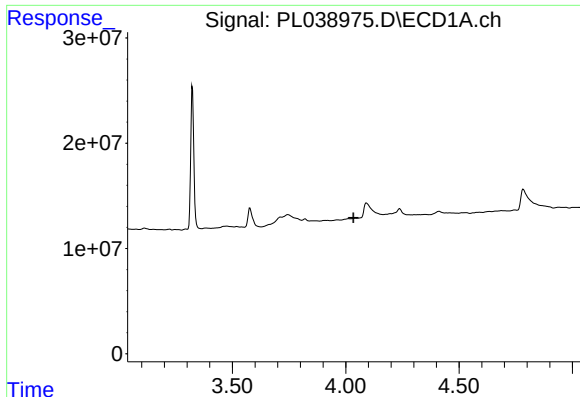

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

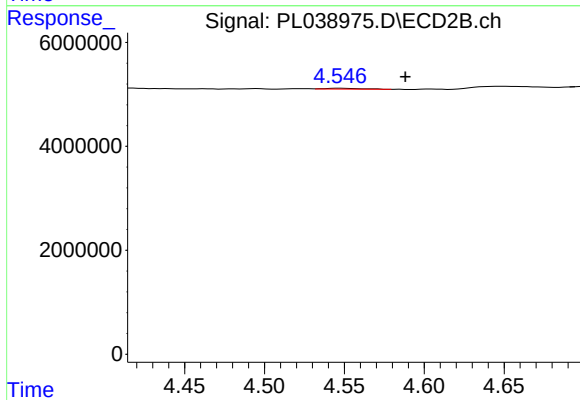


#3 gamma-BHC (Lindane)

R.T.: 4.547 min
Delta R.T.: -0.041 min
Response: 307921
Conc: 0.09 ng/ml

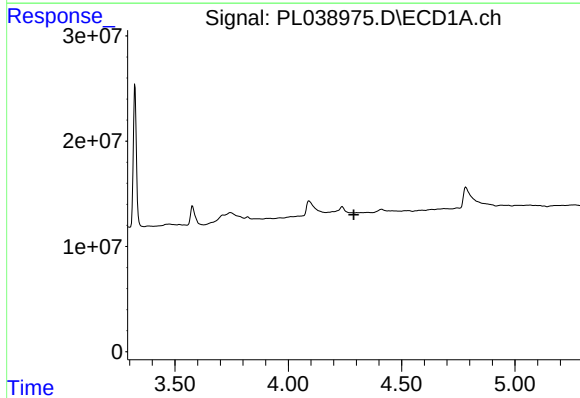


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.289 min
Response: 0
Conc: N.D.

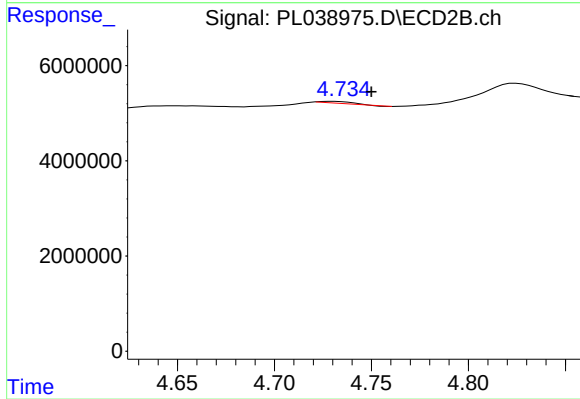

#6 beta-BHC


R.T.: 4.730 min
Delta R.T.: -0.020 min
Response: 441386
Conc: 0.29 ng/ml

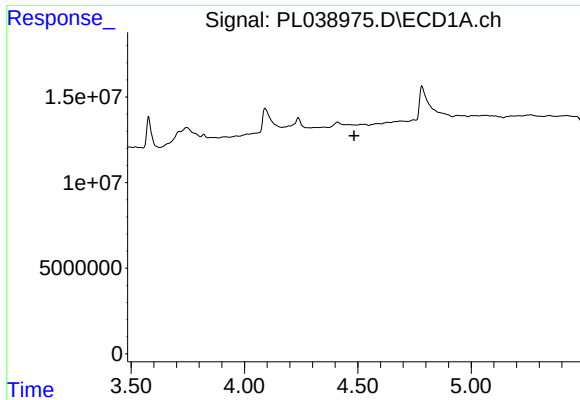

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

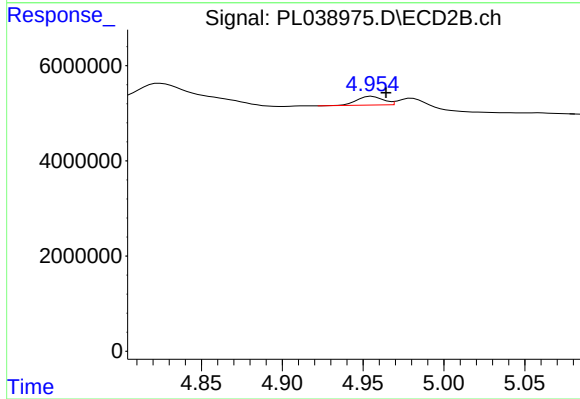


#7 delta-BHC

R.T.: 4.955 min
Delta R.T.: -0.009 min
Response: 2067775
Conc: 0.62 ng/ml

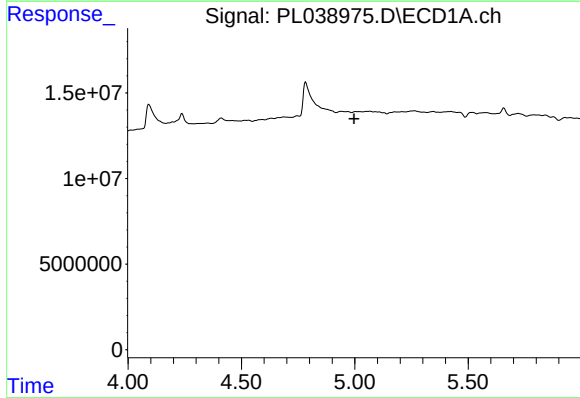


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

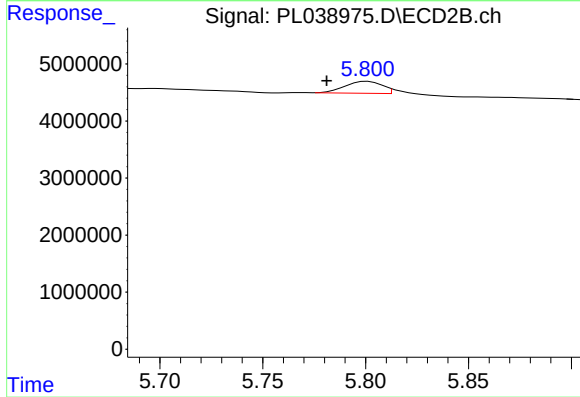

#8 Heptachlor epoxide


R.T.: 5.801 min
Delta R.T.: 0.020 min
Response: 2452107
Conc: 0.86 ng/ml

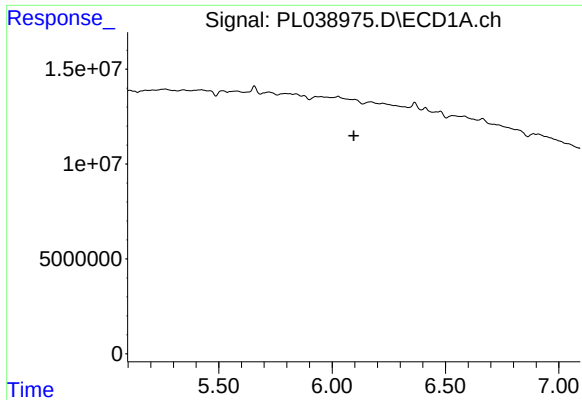

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

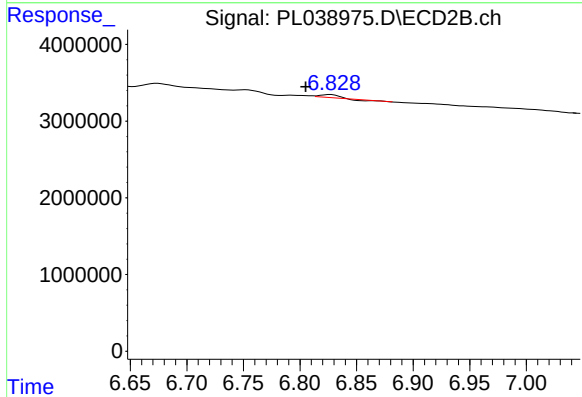


#15 Endosulfan II

R.T.: 6.827 min
Delta R.T.: 0.022 min
Response: 242614
Conc: 0.10 ng/ml

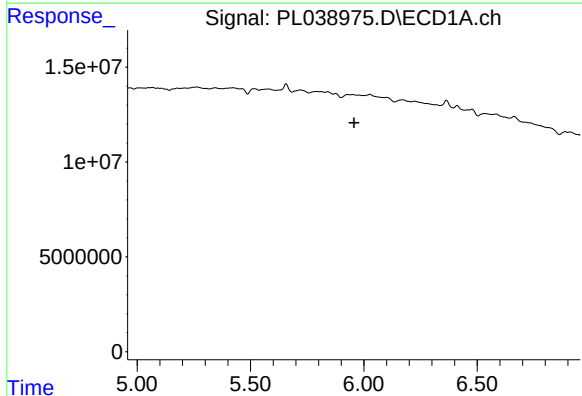


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.956 min
Response: 0
Conc: N.D.

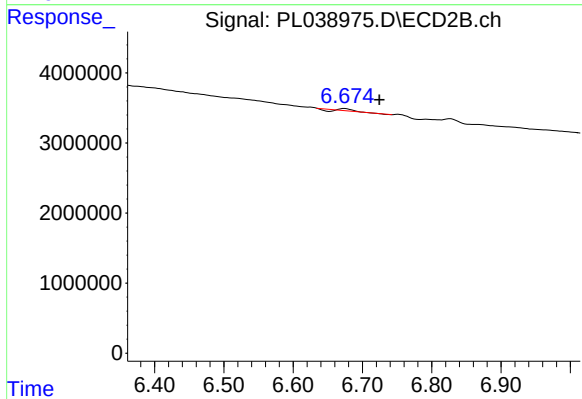

#16 4,4'-DDD


R.T.: 6.674 min
Delta R.T.: -0.051 min
Response: 155550
Conc: 0.07 ng/ml

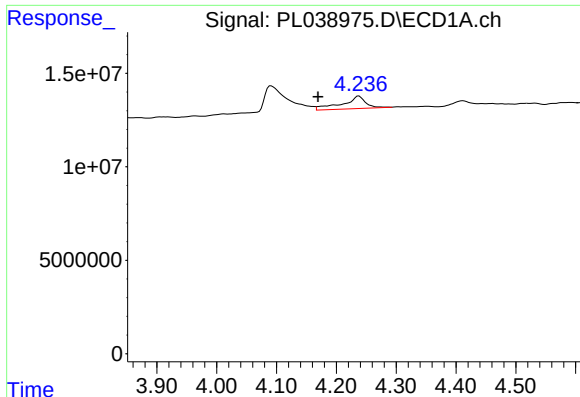

#23 Chlordane-1


R.T.: 4.238 min
Delta R.T.: 0.068 min
Response: 18003086
Conc: 51.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

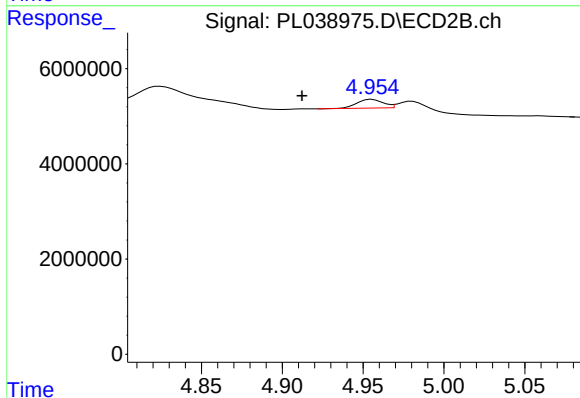


#23 Chlordane-1

R.T.: 4.955 min
Delta R.T.: 0.043 min
Response: 2067775
Conc: 17.84 ng/ml

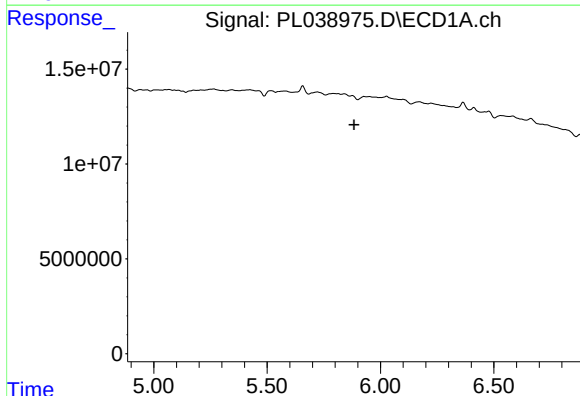


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.883 min
Response: 0
Conc: N.D.

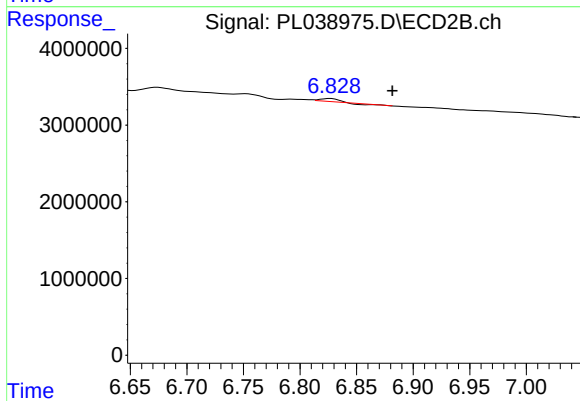

#27 Chlordane-5


R.T.: 6.827 min
Delta R.T.: -0.055 min
Response: 242614
Conc: 2.71 ng/ml

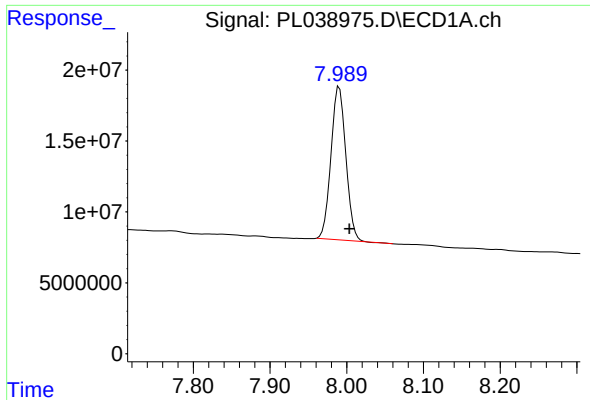

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.013 min
Response: 14500332
Conc: 19.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

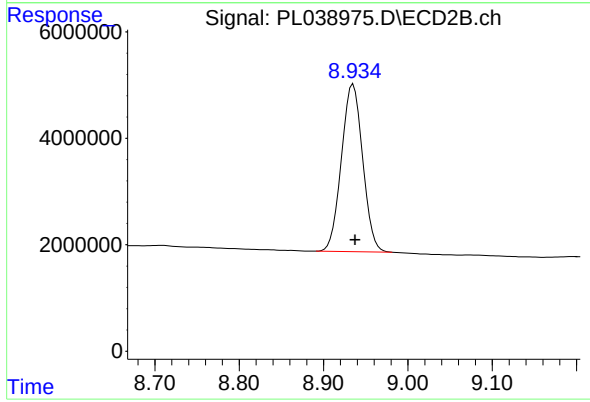

#28 Decachlorobiphenyl

R.T.: 8.935 min
Delta R.T.: -0.002 min
Response: 55128446
Conc: 22.55 ng/ml