

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
 Data File : PL038976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2018 02:25
 Operator : AJ\SJ
 Sample : J4333-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 04:24:54 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.927	141.3E6	59247939	18.980	22.571
28)	SA Decachlor...	7.990	8.933	140.3E6	54035454	18.501	22.105
Target Compounds							
2)	A alpha-BHC	3.752	4.306	13699180	4082677	1.159	1.055
3)	MA gamma-BHC...	0.000	4.551f	0	604023	N.D.	0.167 #
4)	MA Heptachlor	0.000	5.163f	0	1305810	N.D.	0.409 #
7)	B delta-BHC	0.000	4.956	0	8921196	N.D.	2.690 #
8)	B Heptachlo...	0.000	5.801	0	1129537	N.D.	0.397 #
15)	B Endosulfa...	0.000	6.826	0	685405	N.D.	0.285 #
16)	A 4,4'-DDD	0.000	6.675f	0	712478	N.D.	0.333 #
23)	Chlordane-1	4.238	4.956	23999223	8921196	69.312	76.983
27)	Chlordane-5	0.000	6.826	0	685405	N.D.	7.651 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
Data File : PL038976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2018 02:25
Operator : AJ\SJ
Sample : J4333-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 04:24:54 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

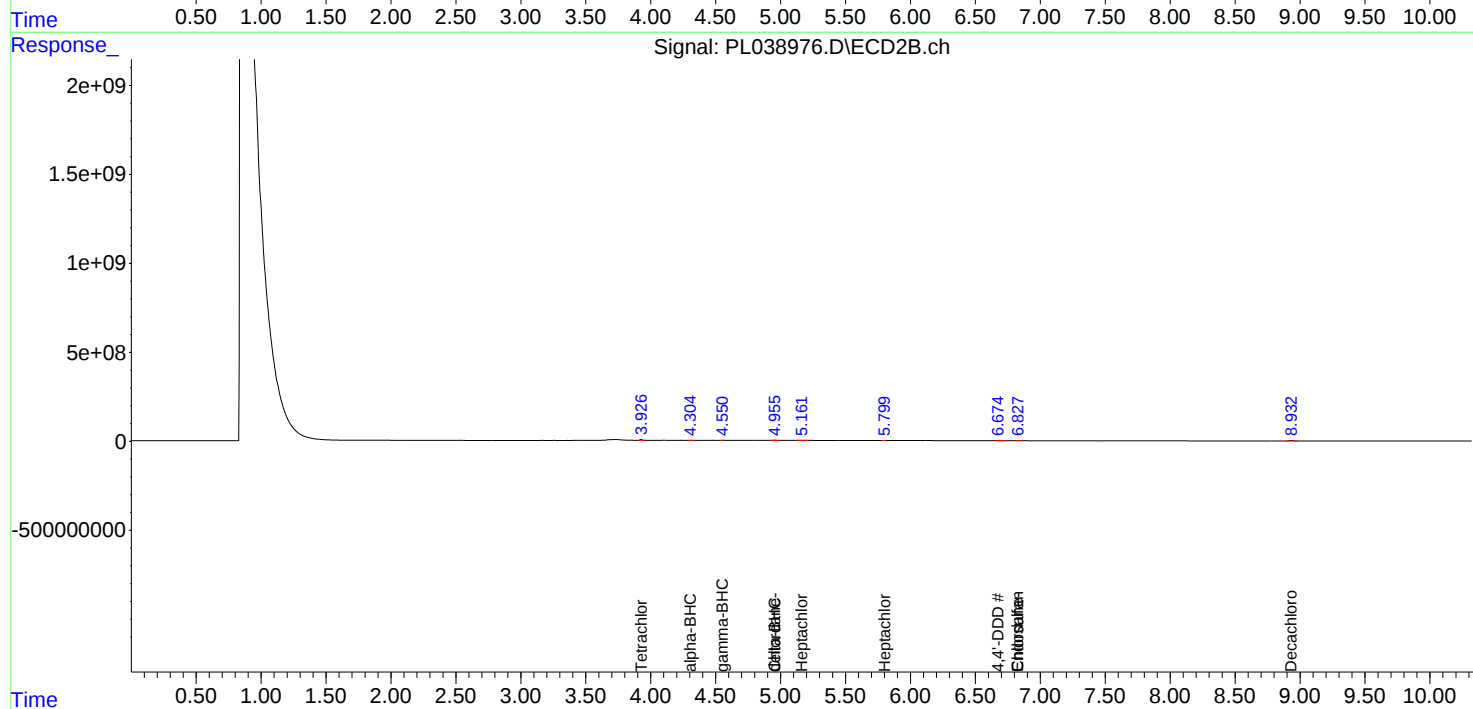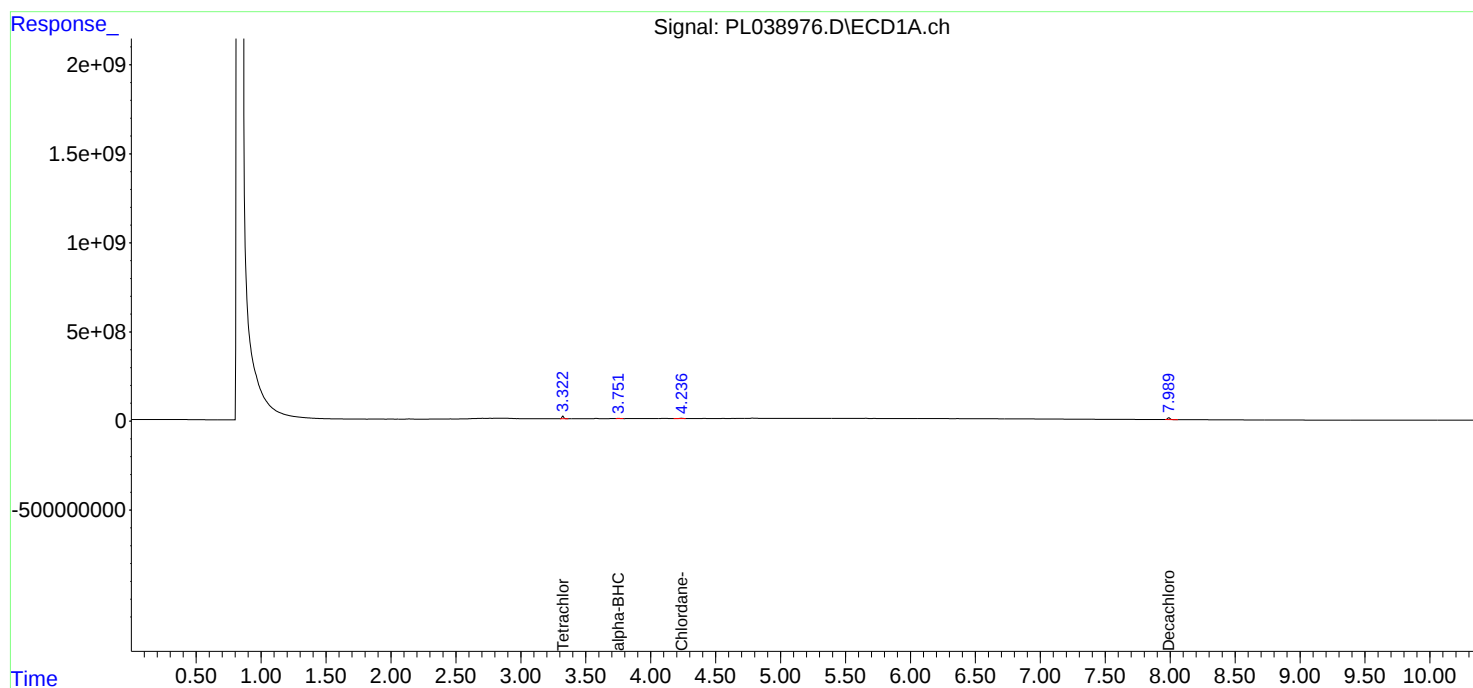


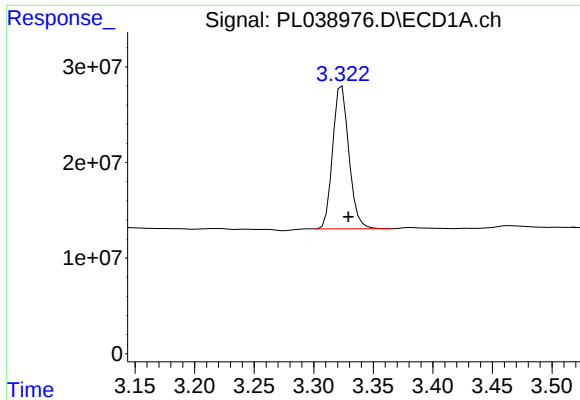

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.005 min
Response: 141334423
Conc: 18.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

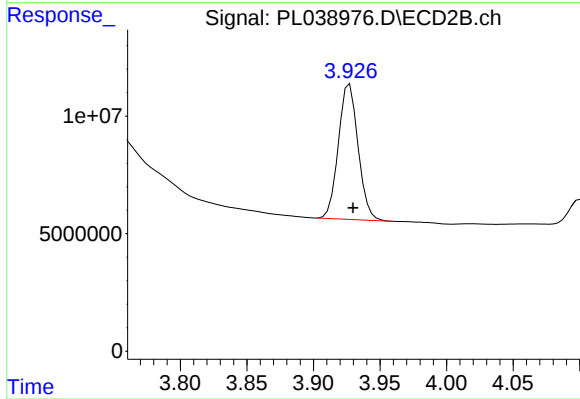


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.002 min
Response: 59247939
Conc: 22.57 ng/ml

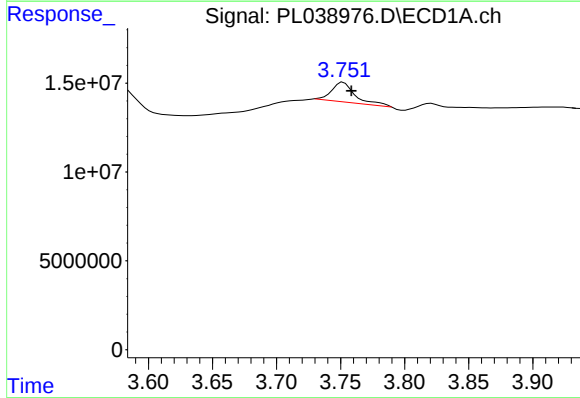


#2 alpha-BHC

R.T.: 3.752 min
Delta R.T.: -0.006 min
Response: 13699180
Conc: 1.16 ng/ml

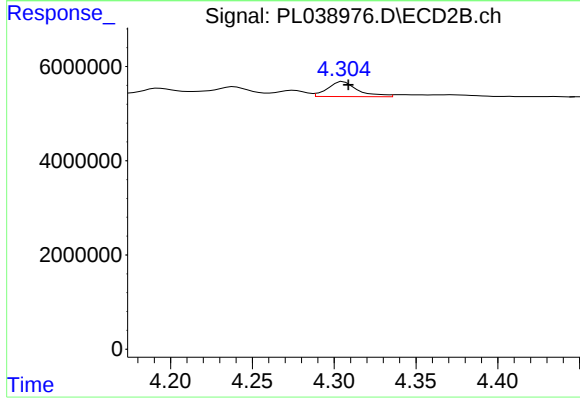

#2 alpha-BHC


R.T.: 4.306 min
Delta R.T.: -0.003 min
Response: 4082677
Conc: 1.05 ng/ml

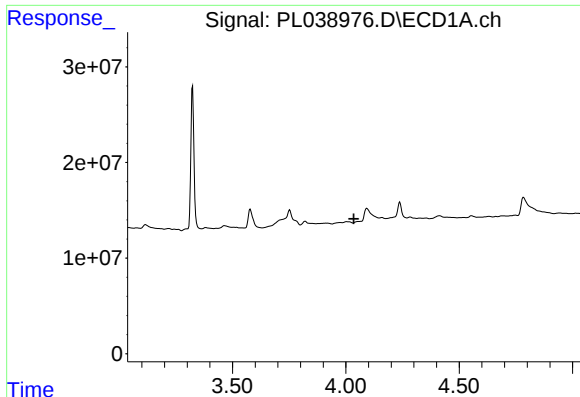

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

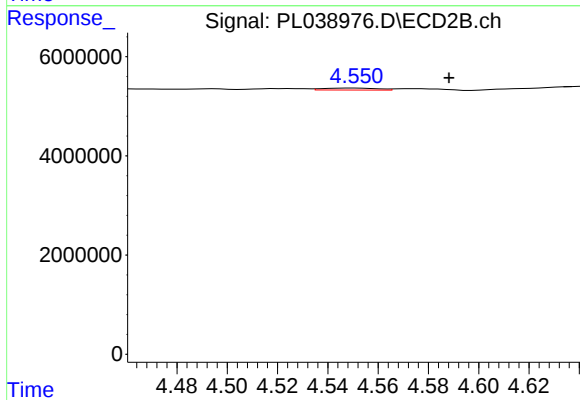


#3 gamma-BHC (Lindane)

R.T.: 4.551 min
Delta R.T.: -0.038 min
Response: 604023
Conc: 0.17 ng/ml

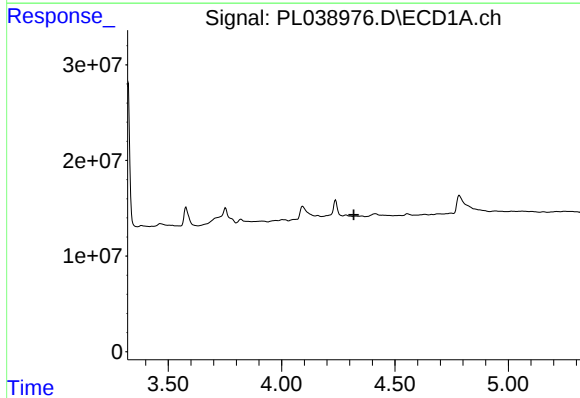


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

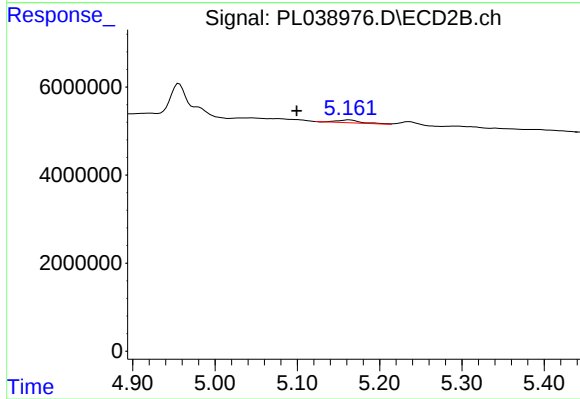

#4 Heptachlor


R.T.: 5.163 min
Delta R.T.: 0.064 min
Response: 1305810
Conc: 0.41 ng/ml

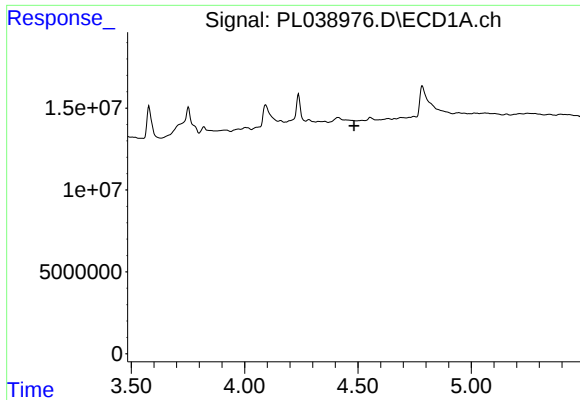

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

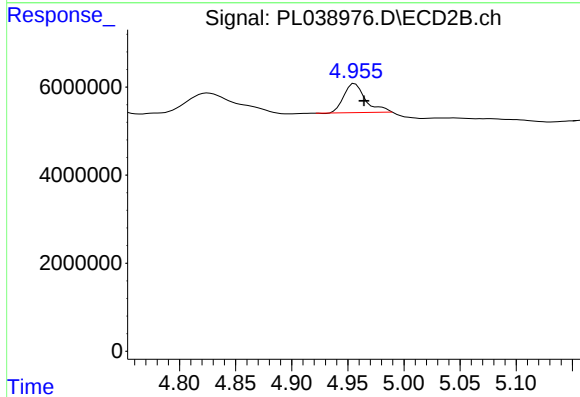


#7 delta-BHC

R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 8921196
Conc: 2.69 ng/ml

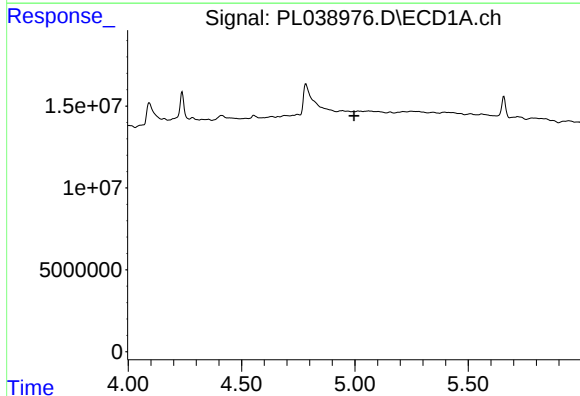


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

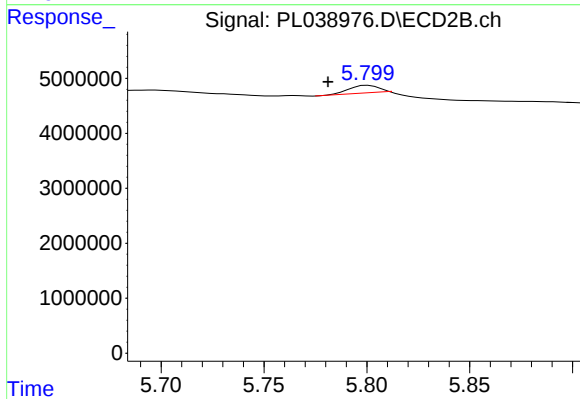

#8 Heptachlor epoxide


R.T.: 5.801 min
Delta R.T.: 0.019 min
Response: 1129537
Conc: 0.40 ng/ml

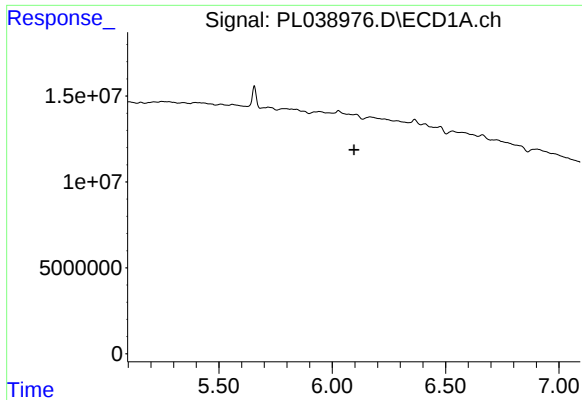

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

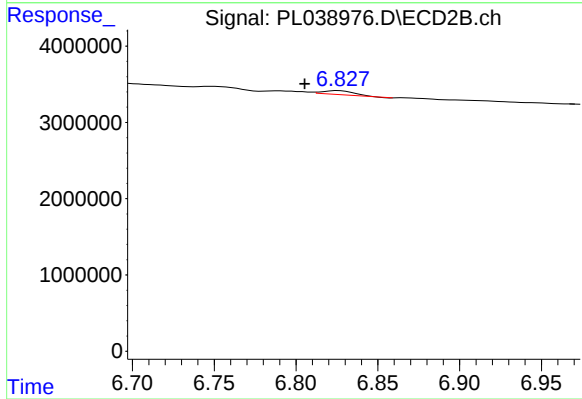


#15 Endosulfan II

R.T.: 6.826 min
Delta R.T.: 0.021 min
Response: 685405
Conc: 0.29 ng/ml

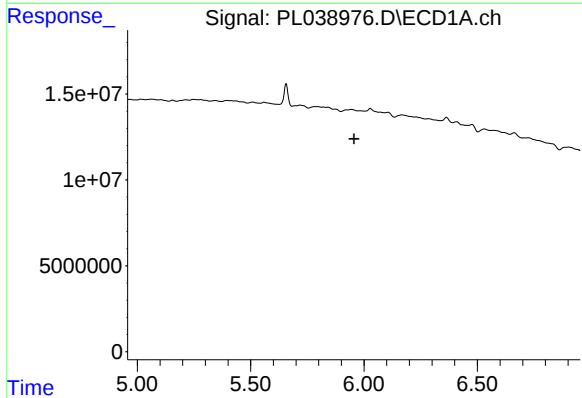


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

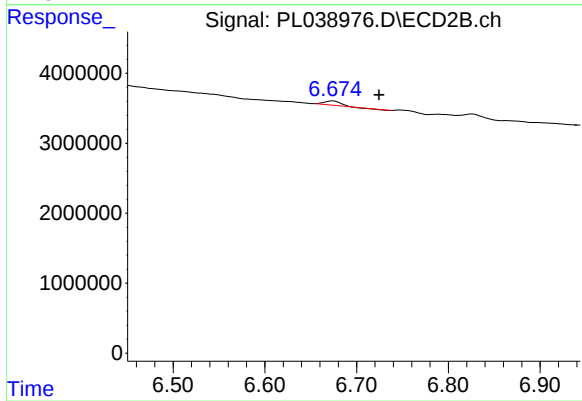

#16 4,4'-DDD


R.T.: 6.675 min
Delta R.T.: -0.050 min
Response: 712478
Conc: 0.33 ng/ml

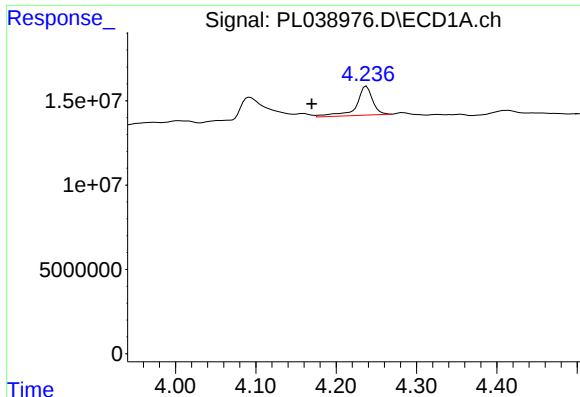

#23 Chlordane-1


R.T.: 4.238 min
Delta R.T.: 0.068 min
Response: 23999223
Conc: 69.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

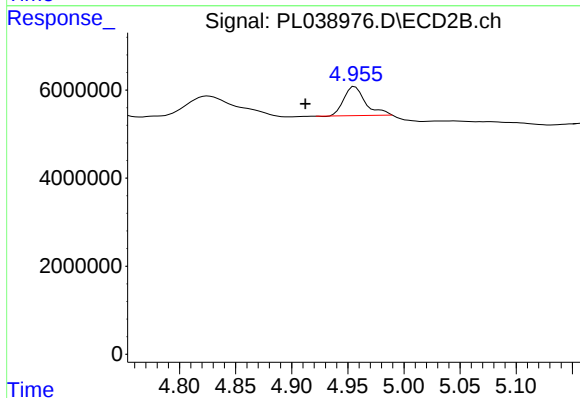


#23 Chlordane-1

R.T.: 4.956 min
Delta R.T.: 0.044 min
Response: 8921196
Conc: 76.98 ng/ml

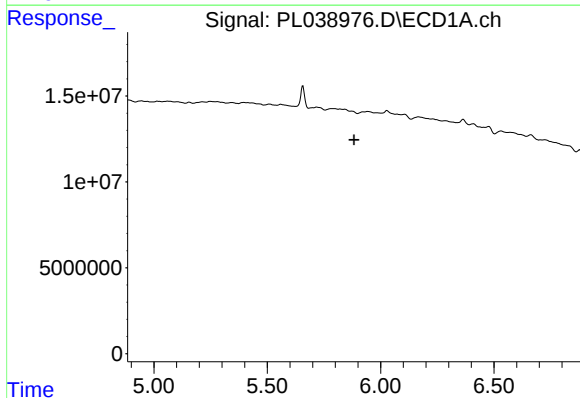


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.883 min
Response: 0
Conc: N.D.

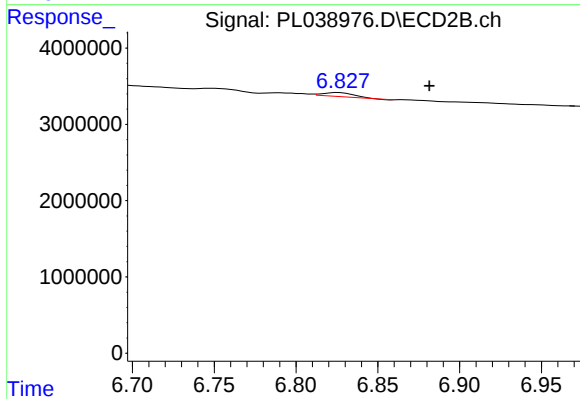

#27 Chlordane-5


R.T.: 6.826 min
Delta R.T.: -0.056 min
Response: 685405
Conc: 7.65 ng/ml

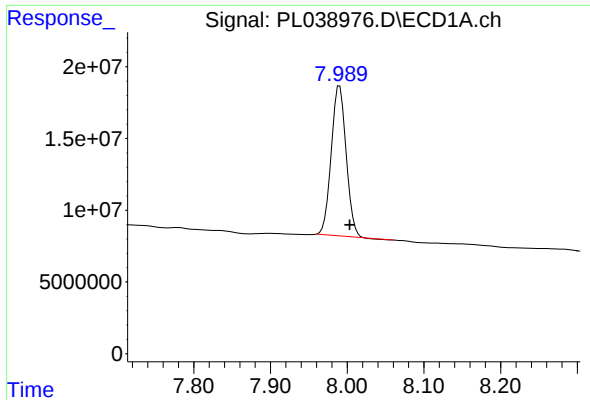

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.013 min
Response: 140348590
Conc: 18.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

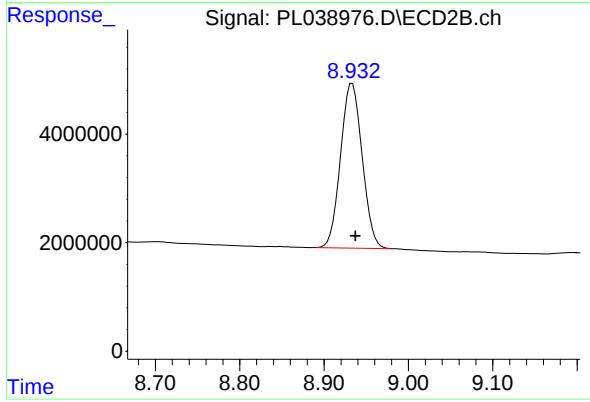

#28 Decachlorobiphenyl

R.T.: 8.933 min
Delta R.T.: -0.004 min
Response: 54035454
Conc: 22.11 ng/ml