

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
 Data File : PL038989.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2018 05:30
 Operator : AJ\SJ
 Sample : J4333-20
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 06:06:07 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.927	144.1E6	57463671	19.349	21.891
28)	SA Decachlor...	7.990	8.934	139.7E6	56021240	18.411	22.918
Target Compounds							
2)	A alpha-BHC	0.000	4.275f	0	1223731	N.D.	0.316 #
3)	MA gamma-BHC...	0.000	4.609	0	122929	N.D.	0.034 #
4)	MA Heptachlor	0.000	5.165f	0	526622	N.D.	0.165 #
7)	B delta-BHC	0.000	4.956	0	7350555	N.D.	2.216 #
8)	B Heptachlo...	0.000	5.801	0	3558013	N.D.	1.252 #
15)	B Endosulfa...	0.000	6.828	0	239731	N.D.	0.100 #
23)	Chlordane-1	4.238	4.956	32050156	7350555	92.564	63.430 #
27)	Chlordane-5	0.000	6.828	0	239731	N.D.	2.676 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
Data File : PL038989.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2018 05:30
Operator : AJ\SJ
Sample : J4333-20
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 06:06:07 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

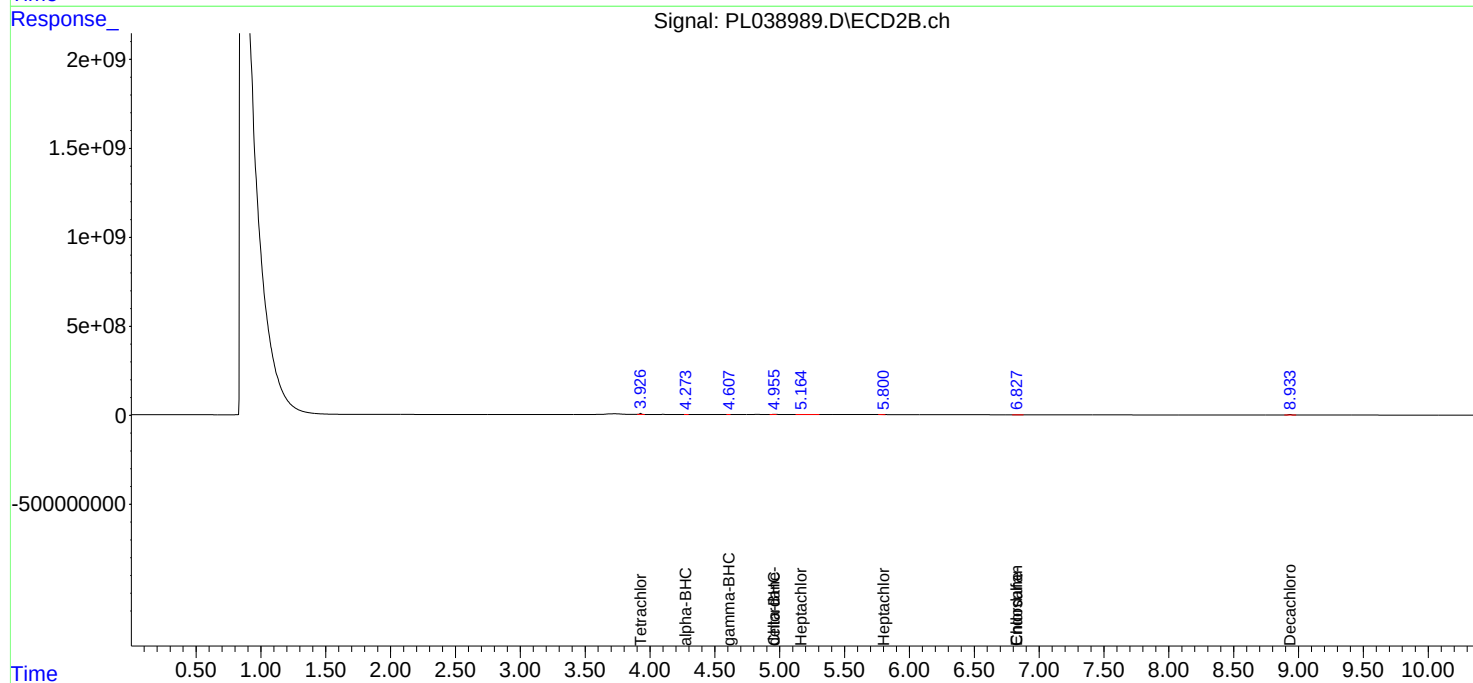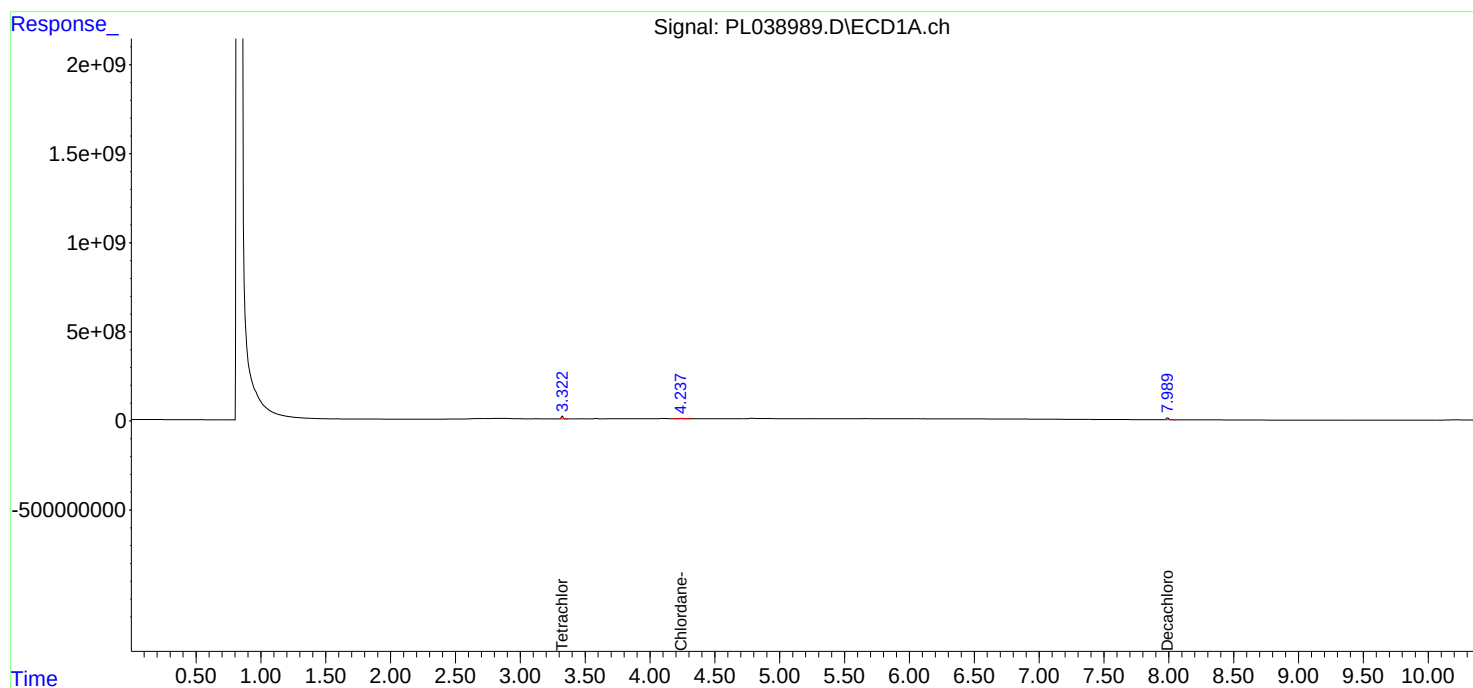


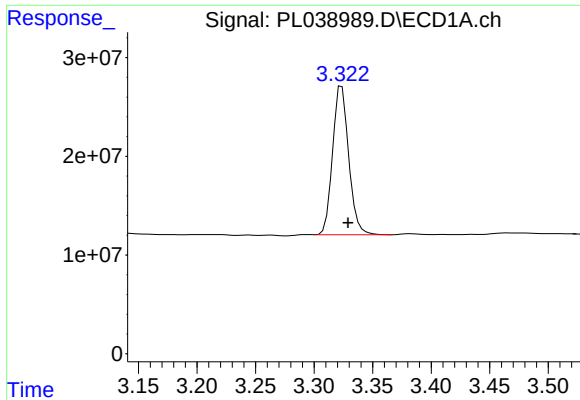

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.005 min
Response: 144079771
Conc: 19.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

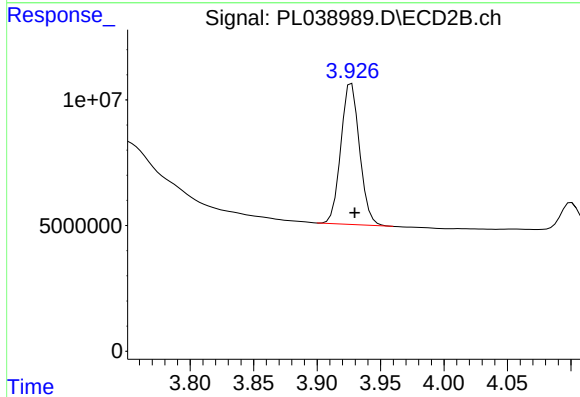


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.002 min
Response: 57463671
Conc: 21.89 ng/ml

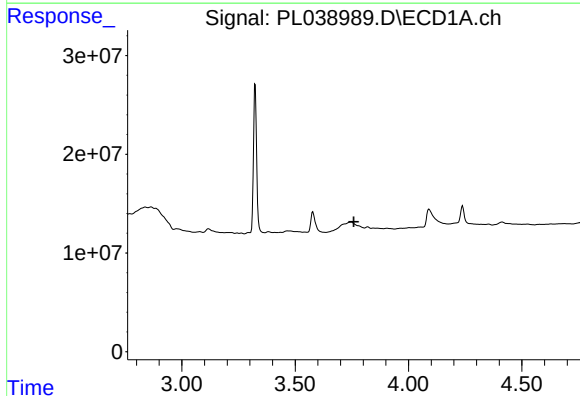


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

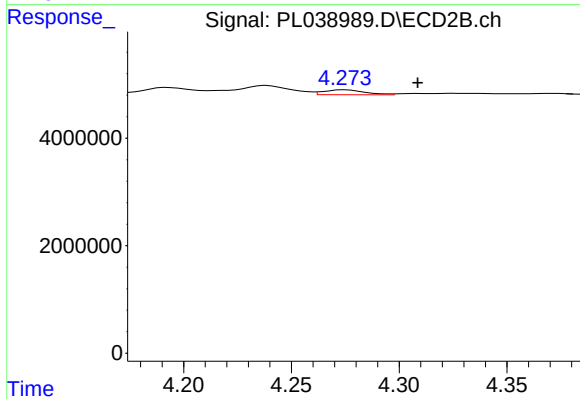

#2 alpha-BHC


R.T.: 4.275 min
Delta R.T.: -0.034 min
Response: 1223731
Conc: 0.32 ng/ml

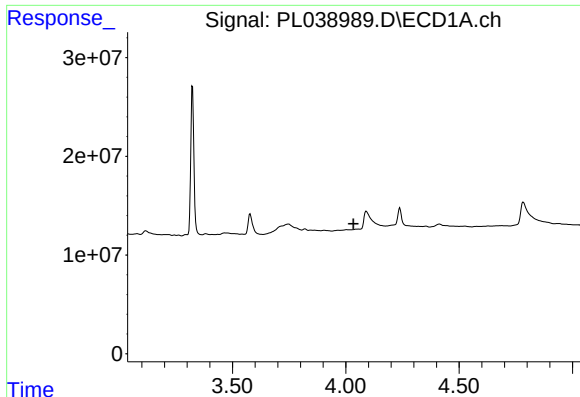

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

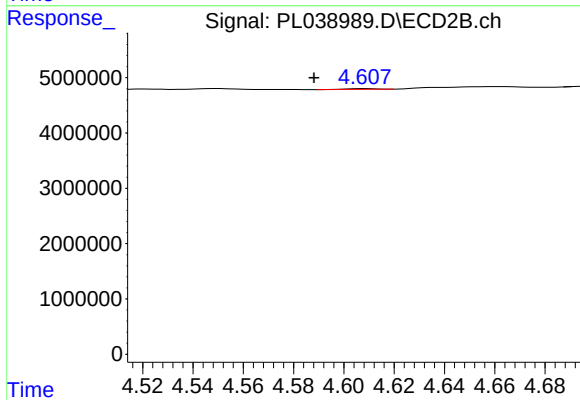


#3 gamma-BHC (Lindane)

R.T.: 4.609 min
Delta R.T.: 0.020 min
Response: 122929
Conc: 0.03 ng/ml

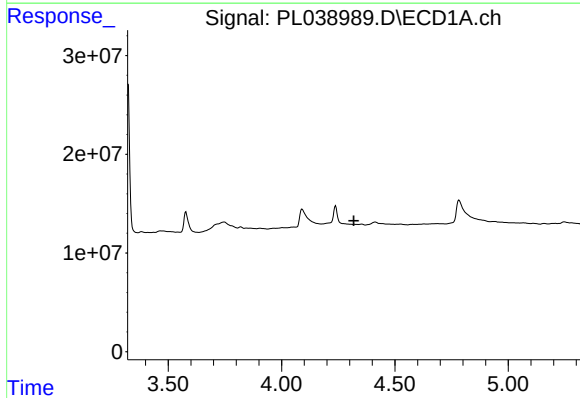


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

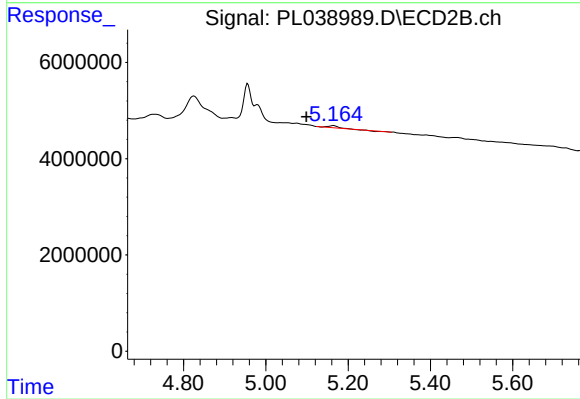

#4 Heptachlor


R.T.: 5.165 min
Delta R.T.: 0.066 min
Response: 526622
Conc: 0.16 ng/ml

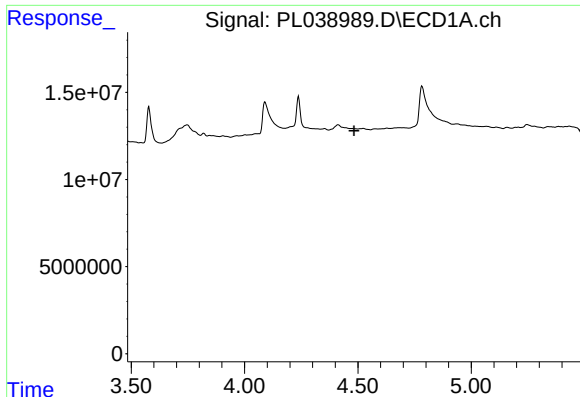

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

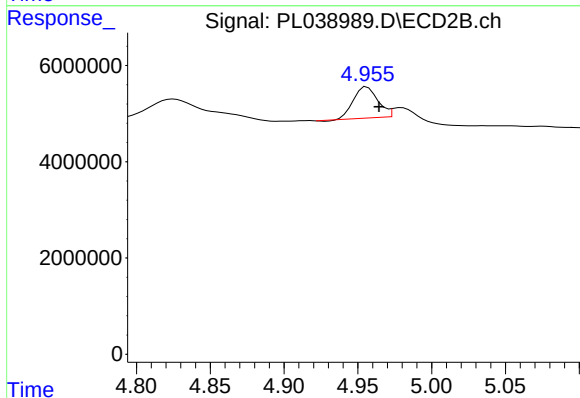


#7 delta-BHC

R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 7350555
Conc: 2.22 ng/ml

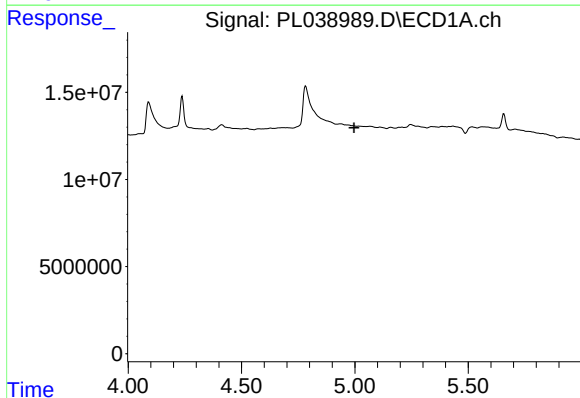


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

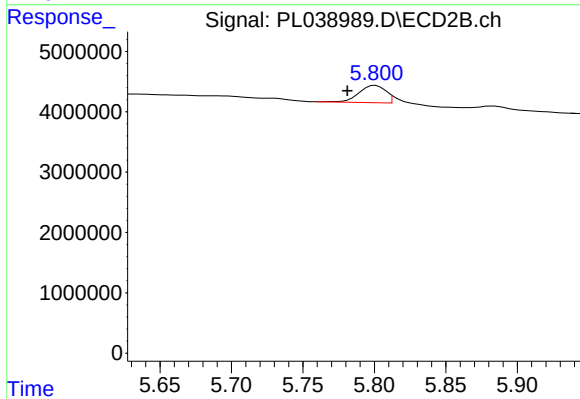

#8 Heptachlor epoxide


R.T.: 5.801 min
Delta R.T.: 0.020 min
Response: 3558013
Conc: 1.25 ng/ml

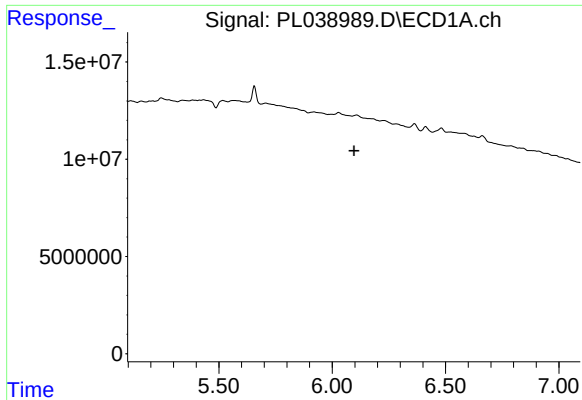

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

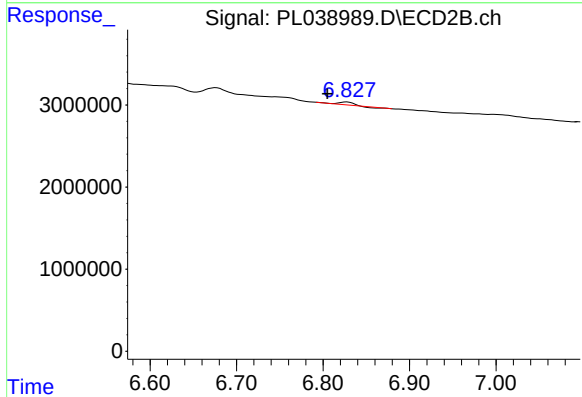


#15 Endosulfan II

R.T.: 6.828 min
Delta R.T.: 0.023 min
Response: 239731
Conc: 0.10 ng/ml

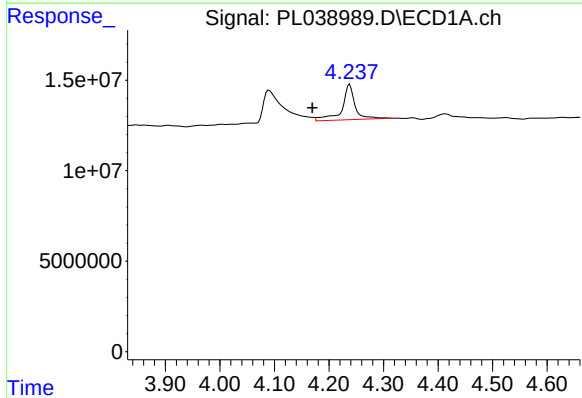


#23 Chlordane-1

R.T.: 4.238 min
Delta R.T.: 0.069 min
Response: 32050156
Conc: 92.56 ng/ml

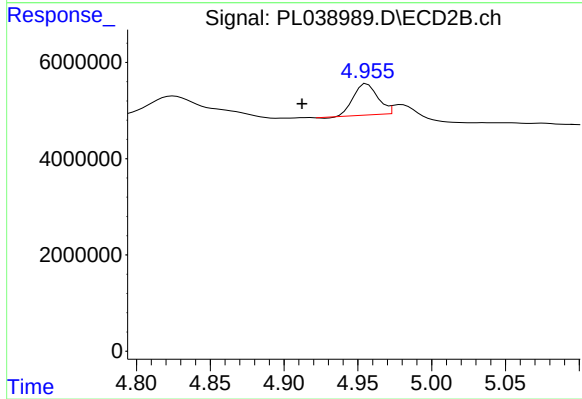

#23 Chlordane-1


R.T.: 4.956 min
Delta R.T.: 0.044 min
Response: 7350555
Conc: 63.43 ng/ml

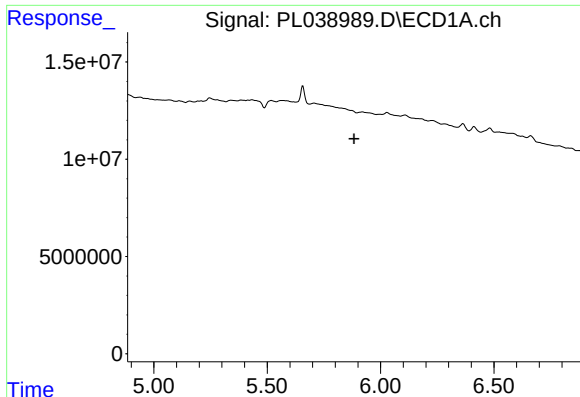

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

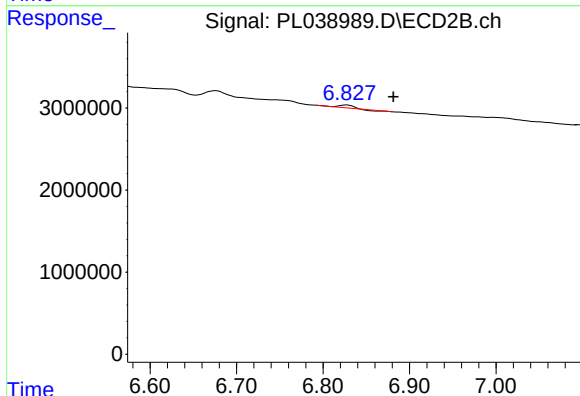


#27 Chlordane-5

R.T.: 6.828 min
Delta R.T.: -0.054 min
Response: 239731
Conc: 2.68 ng/ml

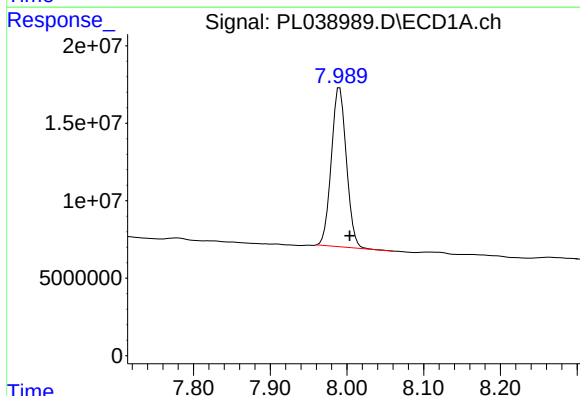

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.013 min
Response: 139663854
Conc: 18.41 ng/ml

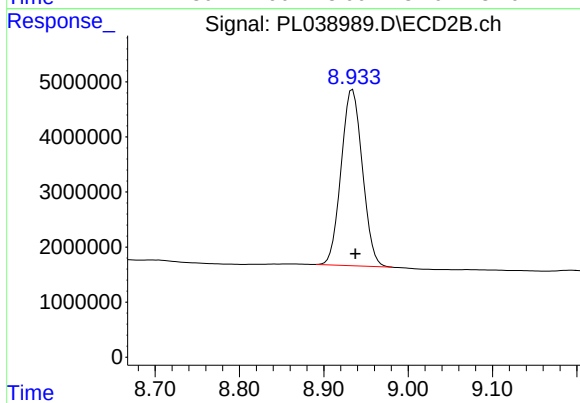

#28 Decachlorobiphenyl

R.T.: 8.934 min
Delta R.T.: -0.003 min
Response: 56021240
Conc: 22.92 ng/ml