

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
 Data File : PL038993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2018 06:26
 Operator : AJ\SJ
 Sample : J4348-05
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 07:03:25 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.927	145.5E6	58189227	19.536	22.168
28)	SA Decachlor...	7.990	8.934	147.2E6	57121099	19.398	23.368
Target Compounds							
2)	A alpha-BHC	3.709f	4.275f	18810580	1604444	1.592	0.415 #
3)	MA gamma-BHC...	0.000	4.548f	0	5662546	N.D.	1.568 #
4)	MA Heptachlor	0.000	5.146f	0	498084	N.D.	0.156 #
7)	B delta-BHC	0.000	4.957	0	5494642	N.D.	1.657 #
8)	B Heptachlo...	0.000	5.801	0	2048425	N.D.	0.721 #
16)	A 4,4'-DDD	0.000	6.674f	0	508196	N.D.	0.237 #
23)	Chlordane-1	4.238	4.957	17293800	5494642	49.946	47.415
27)	Chlordane-5	0.000	6.828	0	1276091	N.D.	14.245 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
Data File : PL038993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2018 06:26
Operator : AJ\SJ
Sample : J4348-05
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 07:03:25 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

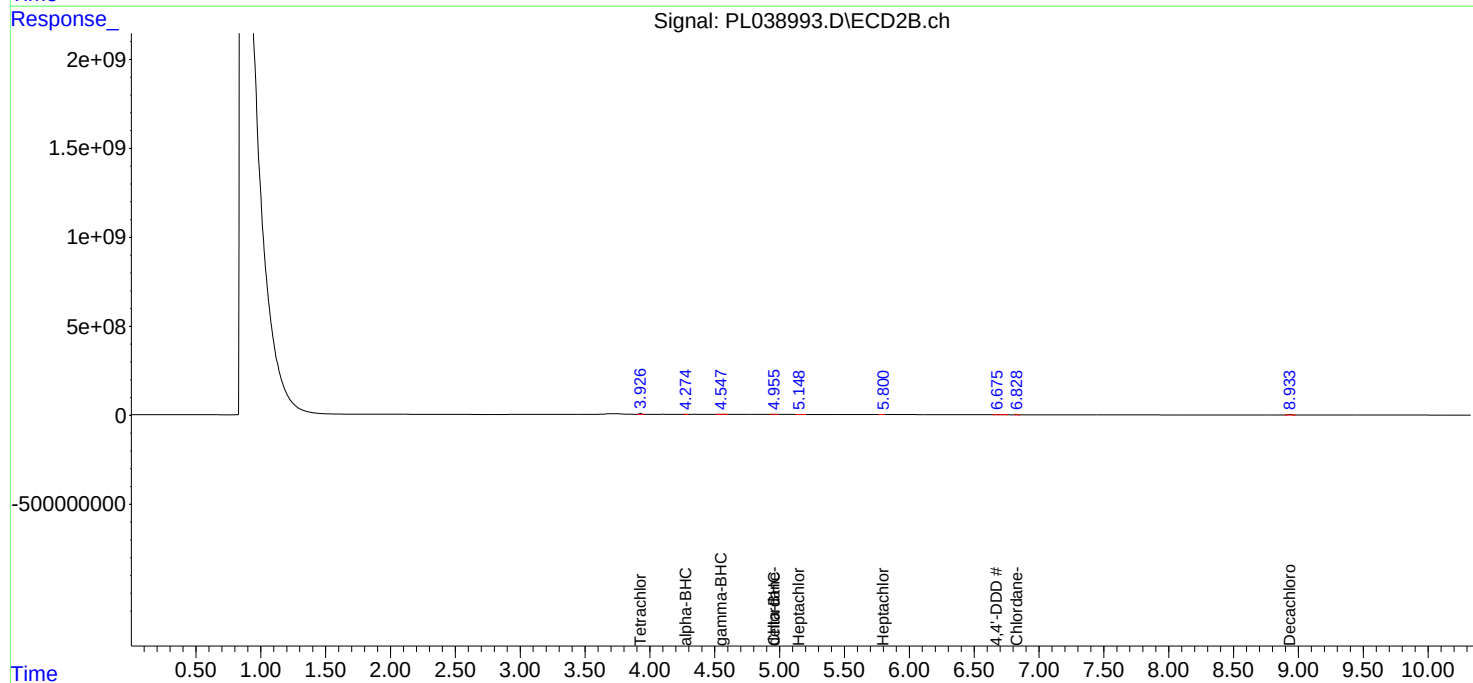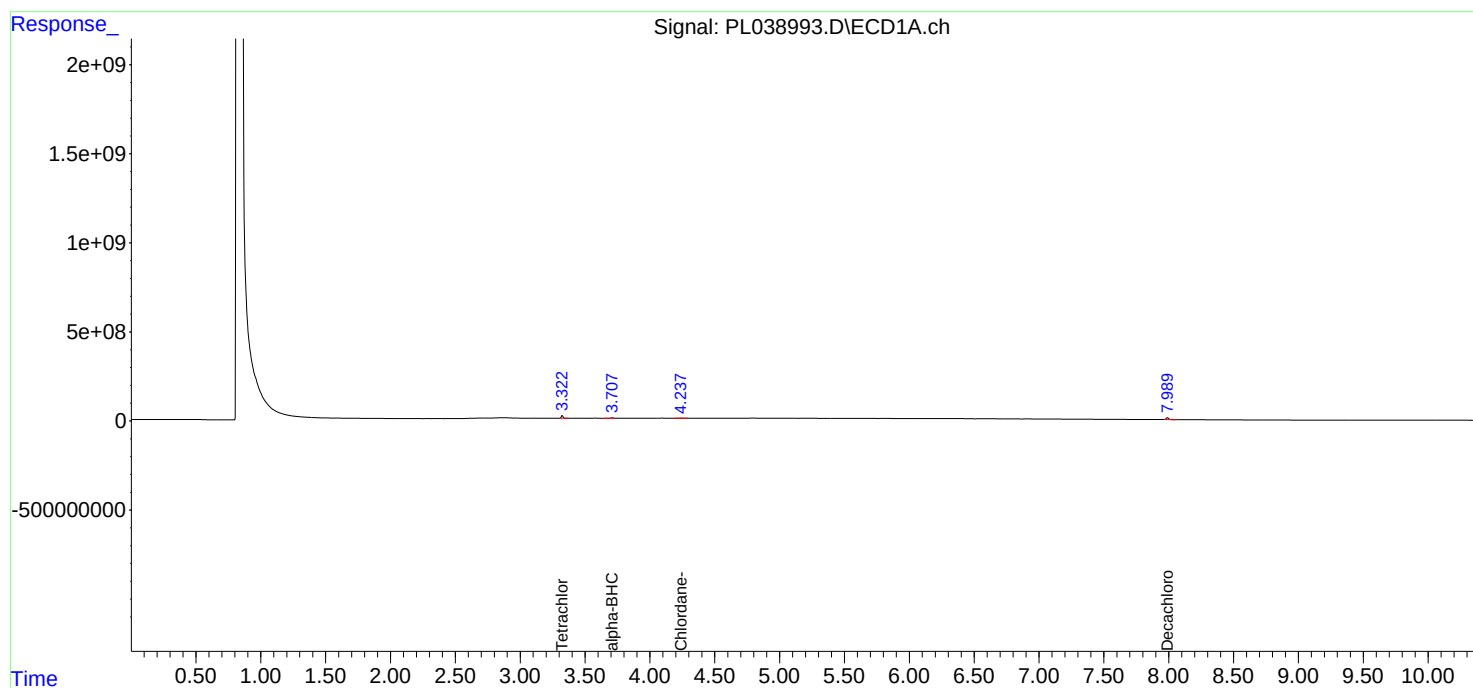


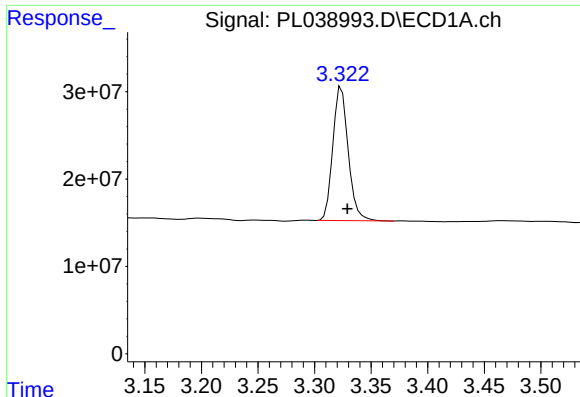

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.005 min
Response: 145475916
Conc: 19.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

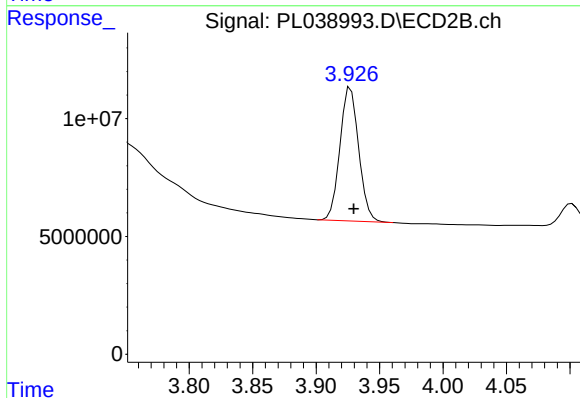


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.002 min
Response: 58189227
Conc: 22.17 ng/ml

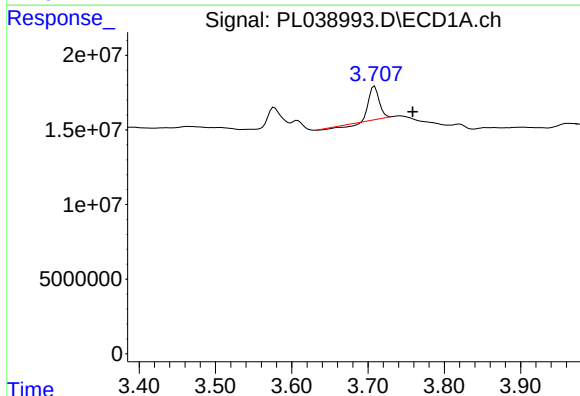


#2 alpha-BHC

R.T.: 3.709 min
Delta R.T.: -0.050 min
Response: 18810580
Conc: 1.59 ng/ml

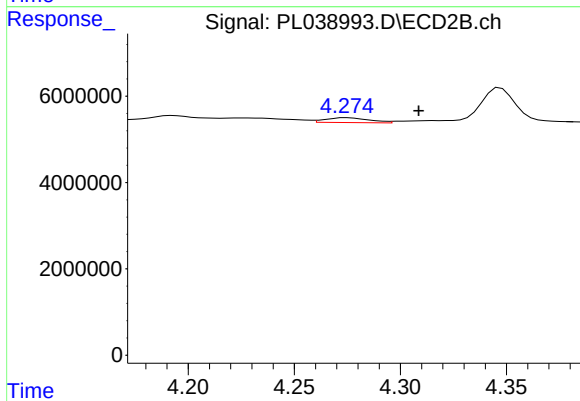

#2 alpha-BHC


R.T.: 4.275 min
Delta R.T.: -0.034 min
Response: 1604444
Conc: 0.41 ng/ml

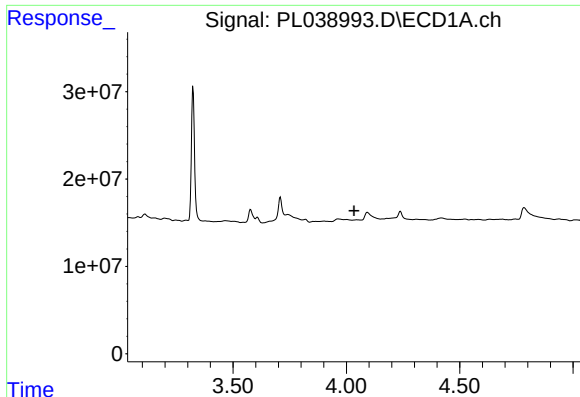

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

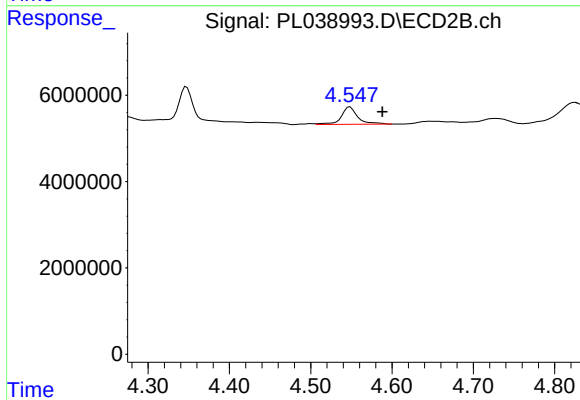


#3 gamma-BHC (Lindane)

R.T.: 4.548 min
Delta R.T.: -0.040 min
Response: 5662546
Conc: 1.57 ng/ml

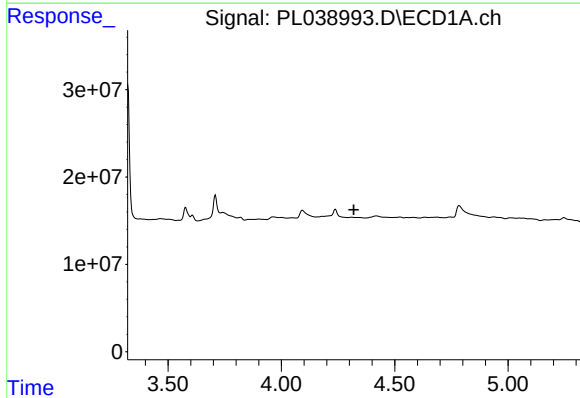


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

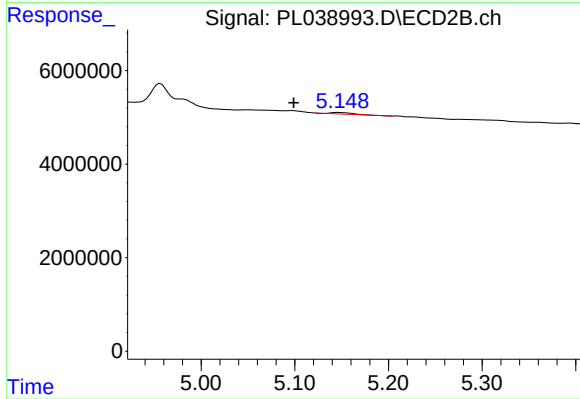

#4 Heptachlor


R.T.: 5.146 min
Delta R.T.: 0.047 min
Response: 498084
Conc: 0.16 ng/ml

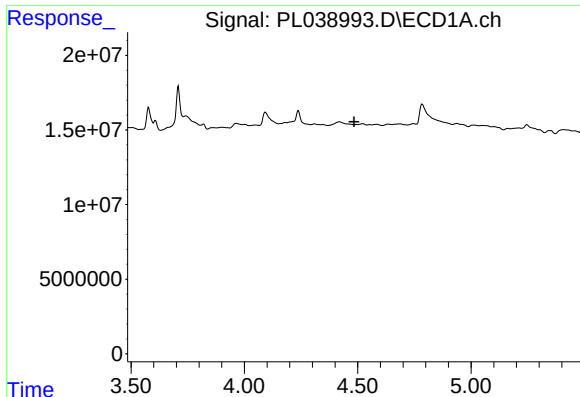

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

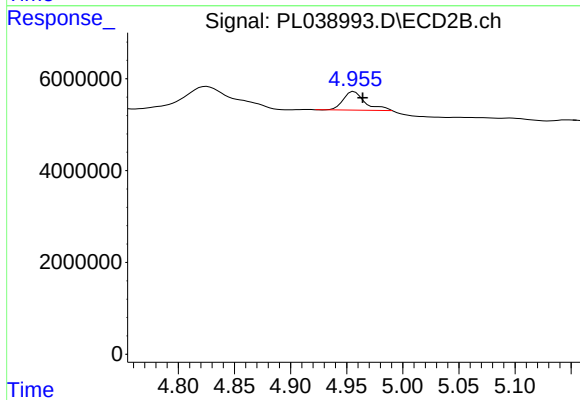


#7 delta-BHC

R.T.: 4.957 min
Delta R.T.: -0.008 min
Response: 5494642
Conc: 1.66 ng/ml

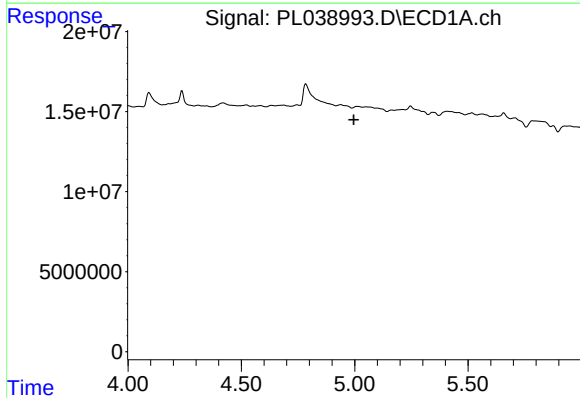


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

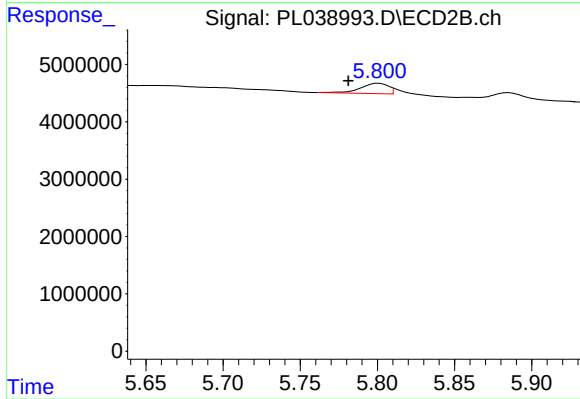

#8 Heptachlor epoxide


R.T.: 5.801 min
Delta R.T.: 0.020 min
Response: 2048425
Conc: 0.72 ng/ml

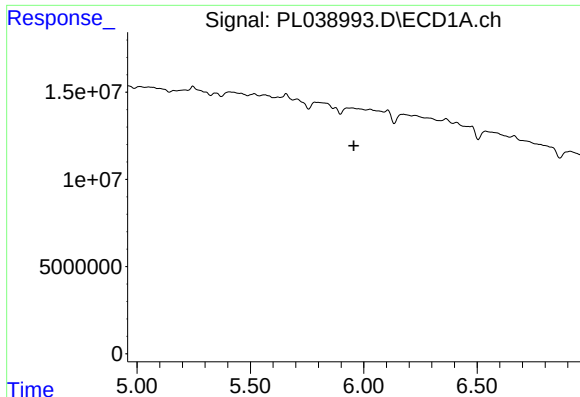

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

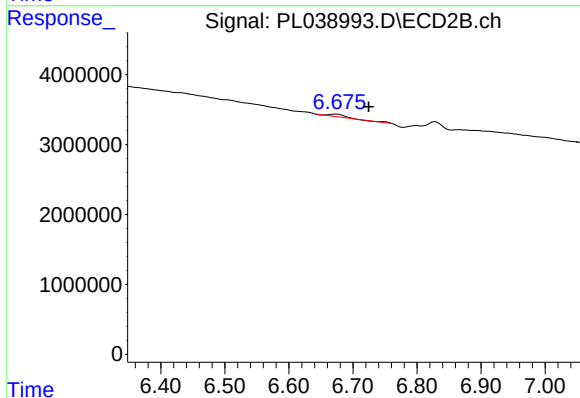


#16 4,4'-DDD

R.T.: 6.674 min
Delta R.T.: -0.050 min
Response: 508196
Conc: 0.24 ng/ml

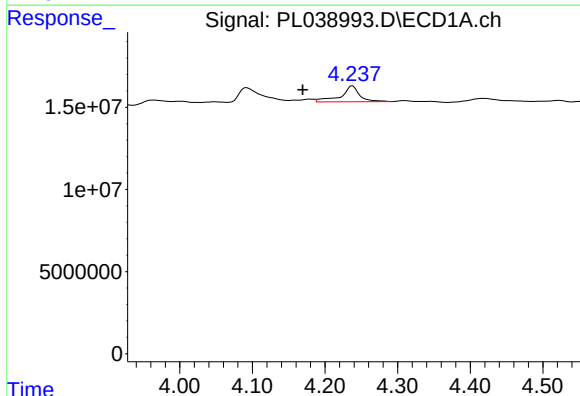


#23 Chlordane-1

R.T.: 4.238 min
Delta R.T.: 0.069 min
Response: 17293800
Conc: 49.95 ng/ml

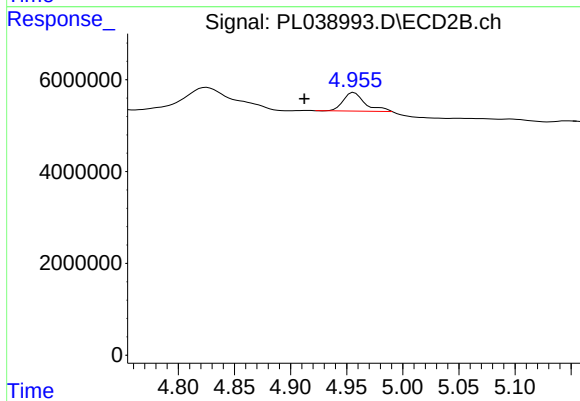

#23 Chlordane-1


R.T.: 4.957 min
Delta R.T.: 0.044 min
Response: 5494642
Conc: 47.41 ng/ml

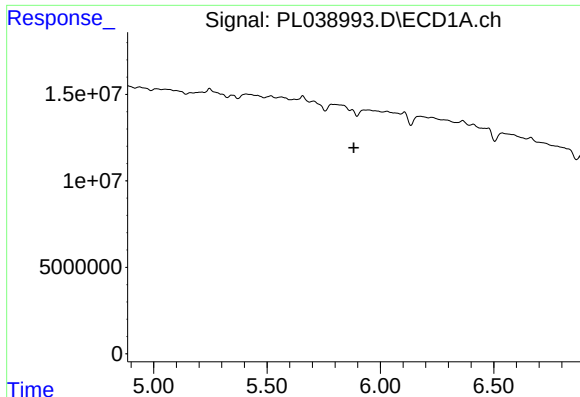

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

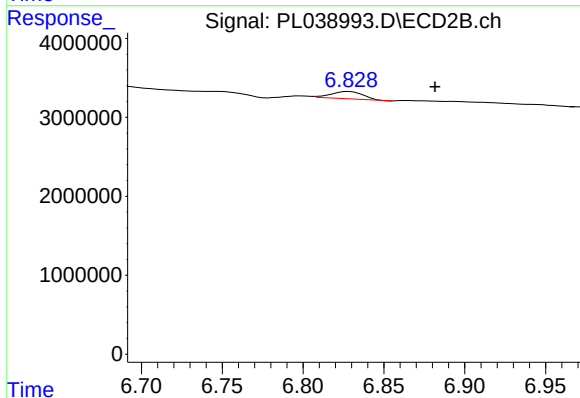


#27 Chlordane-5

R.T.: 6.828 min
Delta R.T.: -0.053 min
Response: 1276091
Conc: 14.25 ng/ml

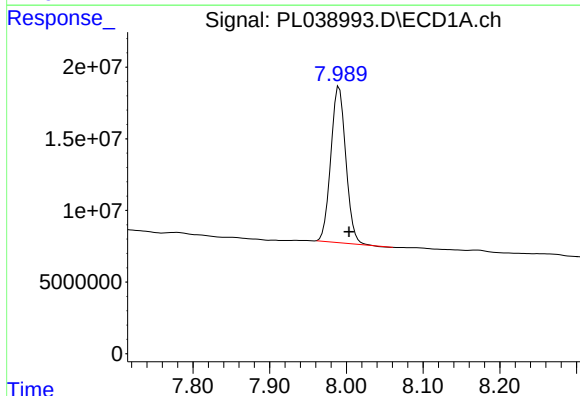

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.013 min
Response: 147150424
Conc: 19.40 ng/ml

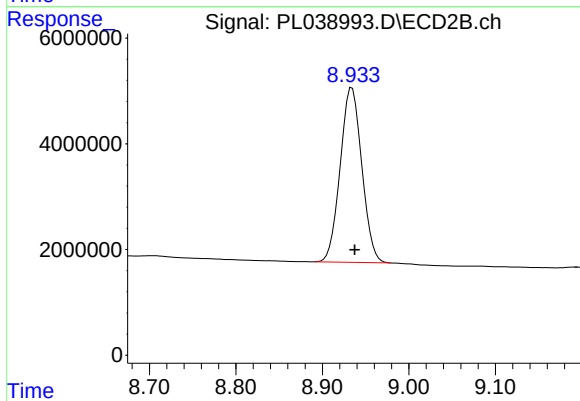

#28 Decachlorobiphenyl

R.T.: 8.934 min
Delta R.T.: -0.003 min
Response: 57121099
Conc: 23.37 ng/ml