

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
 Data File : PL038998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2018 07:37
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 09:48:21 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.927	165.4E6	64894563	22.208	24.722
28)	SA Decachlor...	7.990	8.934	155.3E6	60141927	20.477	24.603
Target Compounds							
2)	A alpha-BHC	0.000	4.327	0	410969	N.D.	0.106 #
3)	MA gamma-BHC...	0.000	4.599	0	102552	N.D.	0.028 #
7)	B delta-BHC	0.000	4.956	0	1721649	N.D.	0.519 #
8)	B Heptachlo...	0.000	5.770	0	1207119	N.D.	0.425 #
10)	B gamma-Chl...	0.000	5.952f	0	64827	N.D.	0.022 #
13)	MA Dieldrin	5.519f	0.000	4386369	0	0.456	N.D. #
20)	A Methoxychlor	0.000	7.546f	0	466887	N.D.	0.410 #
21)	B Endrin ke...	6.914f	7.546f	1791259	466887	0.228	0.196
23)	Chlordane-1	4.236	4.956	8016434	1721649	23.152	14.857 #
25)	Chlordane-3	0.000	5.952	0	64827	N.D.	0.159 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
Data File : PL038998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2018 07:37
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 09:48:21 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

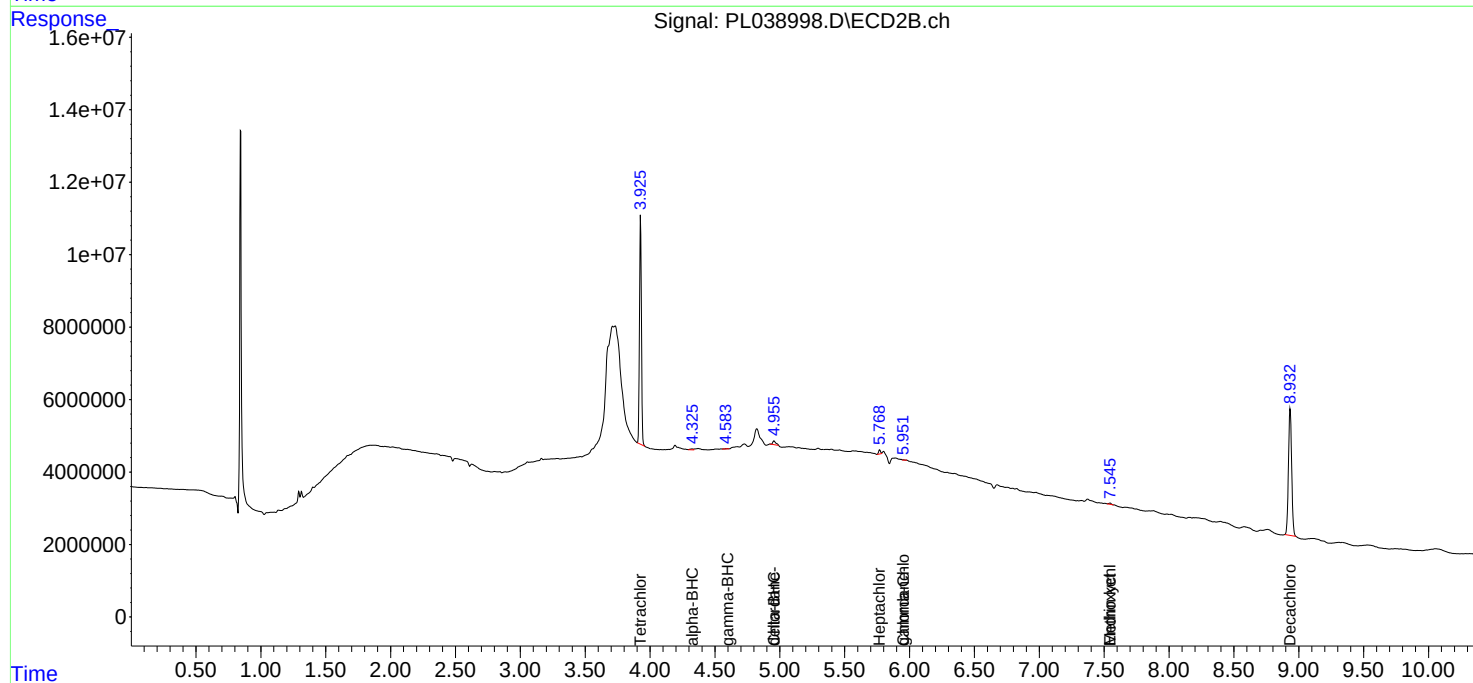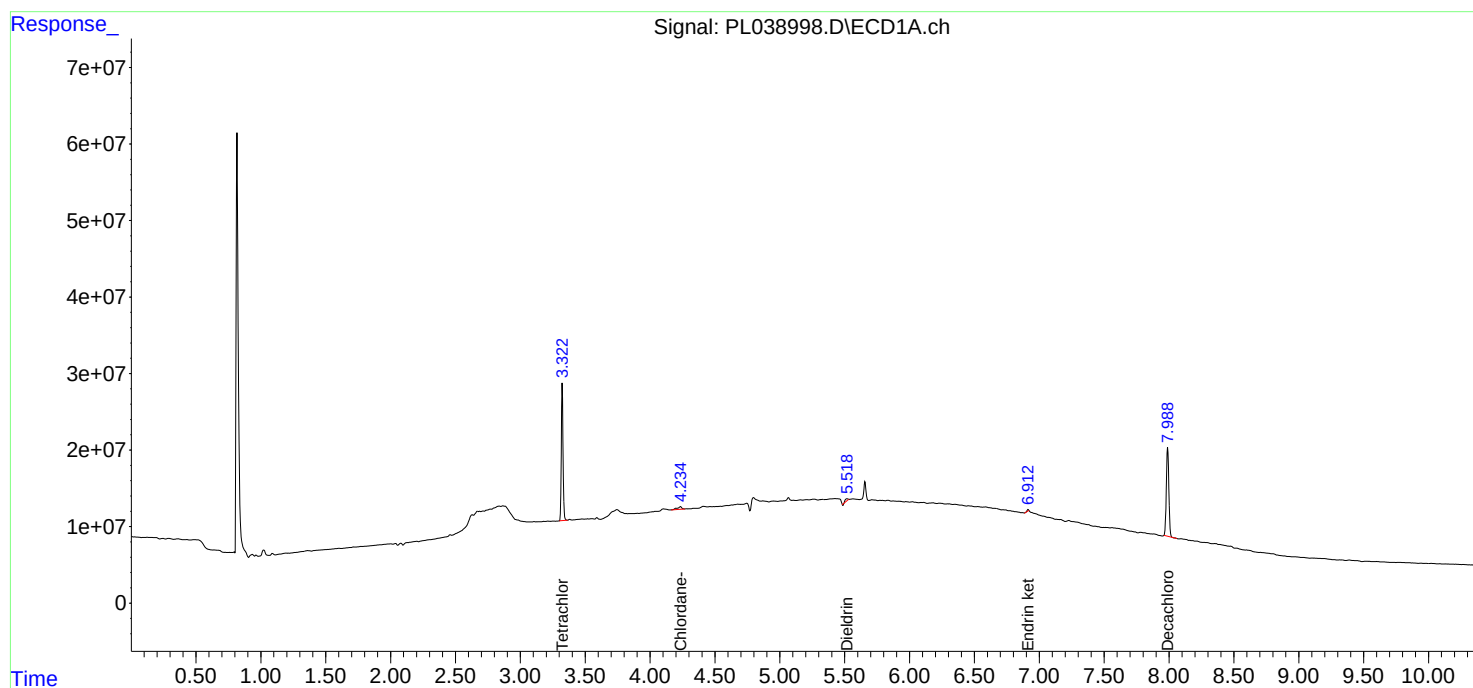


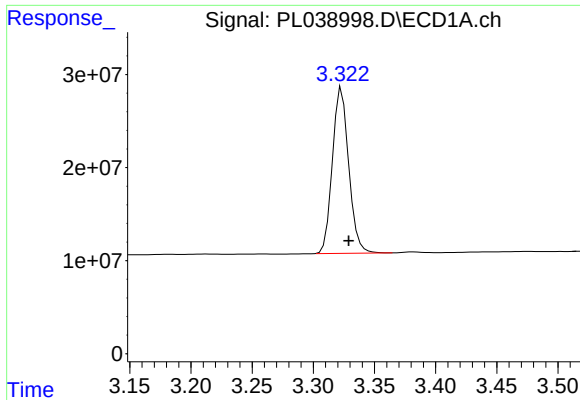

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: -0.006 min
Response: 165367133
Conc: 22.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

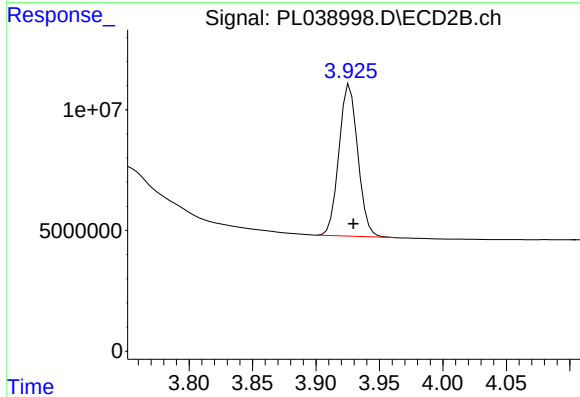


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 64894563
Conc: 24.72 ng/ml

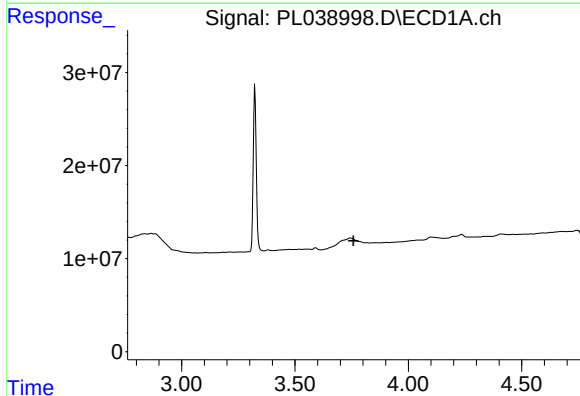


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

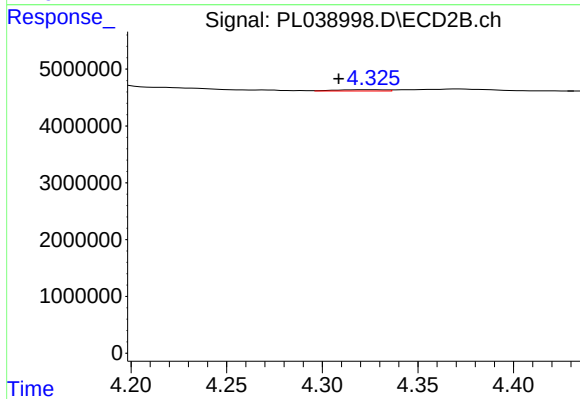

#2 alpha-BHC


R.T.: 4.327 min
Delta R.T.: 0.018 min
Response: 410969
Conc: 0.11 ng/ml

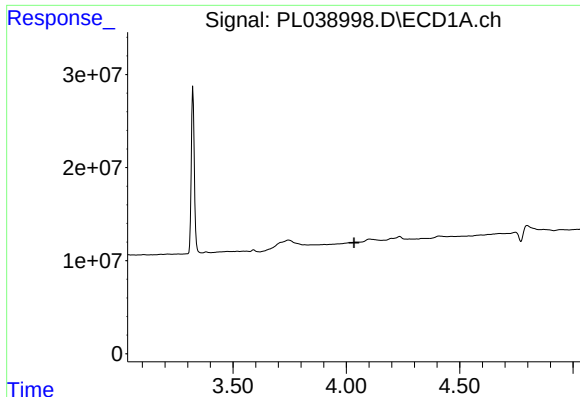

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

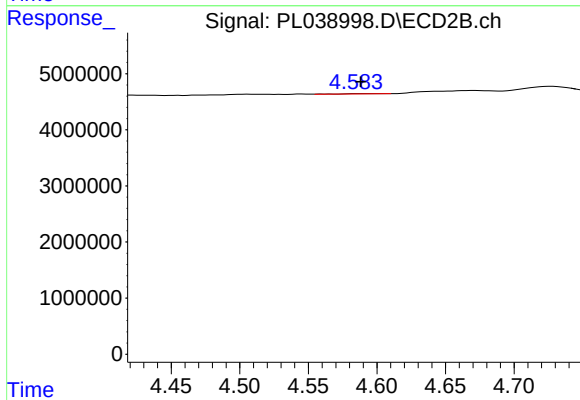


#3 gamma-BHC (Lindane)

R.T.: 4.599 min
Delta R.T.: 0.011 min
Response: 102552
Conc: 0.03 ng/ml

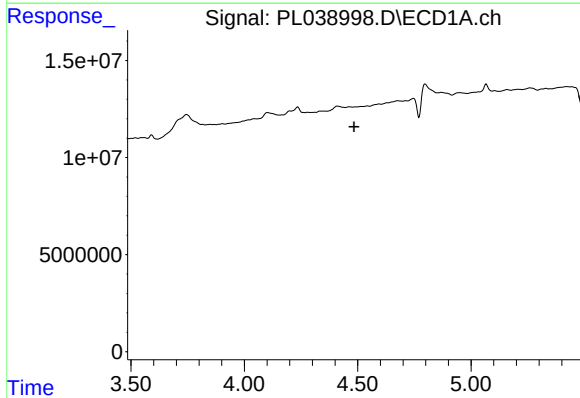


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

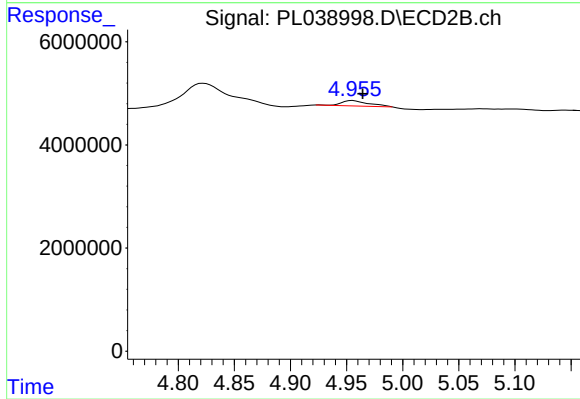

#7 delta-BHC


R.T.: 4.956 min
Delta R.T.: -0.009 min
Response: 1721649
Conc: 0.52 ng/ml

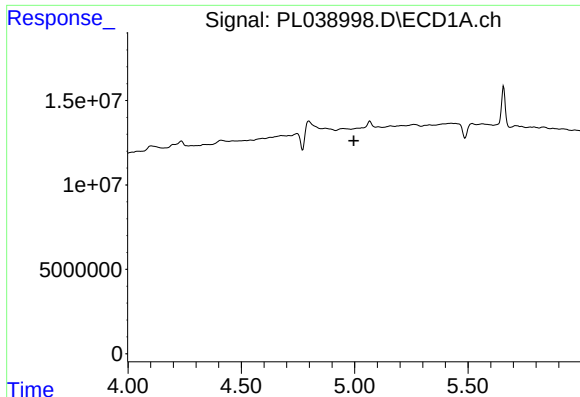

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

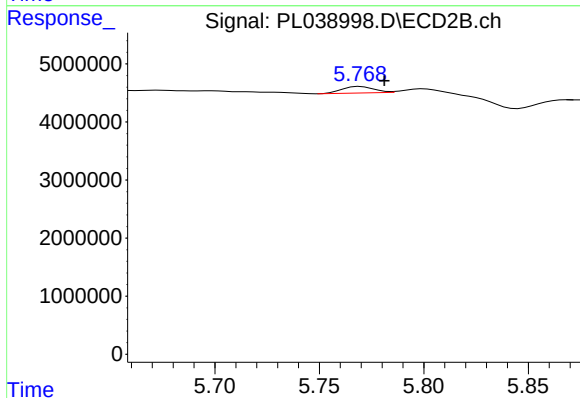


#8 Heptachlor epoxide

R.T.: 5.770 min
Delta R.T.: -0.012 min
Response: 1207119
Conc: 0.42 ng/ml

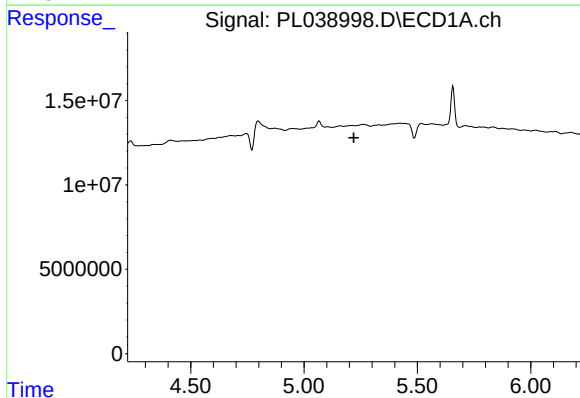


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.219 min
Response: 0
Conc: N.D.

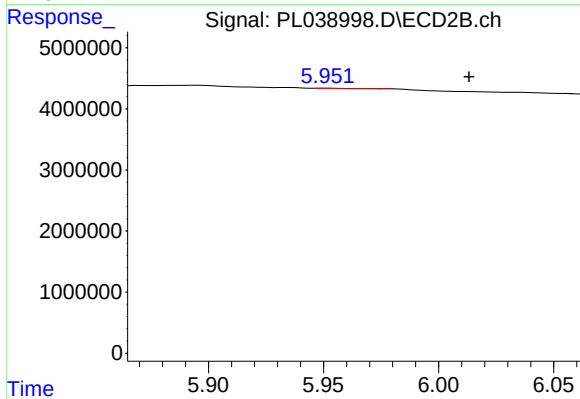

#10 gamma-Chlordane


R.T.: 5.952 min
Delta R.T.: -0.061 min
Response: 64827
Conc: 0.02 ng/ml

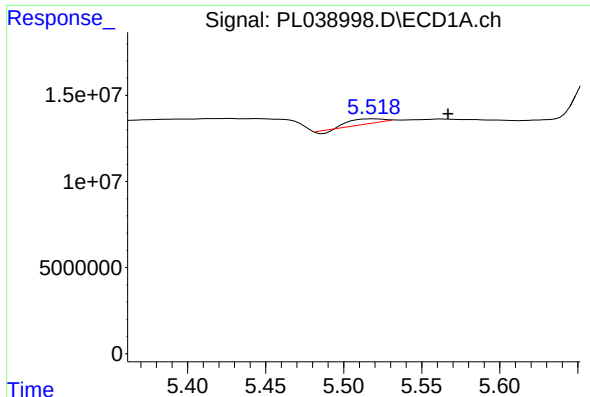

#13 Dieldrin


R.T.: 5.519 min
Delta R.T.: -0.048 min
Response: 4386369
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

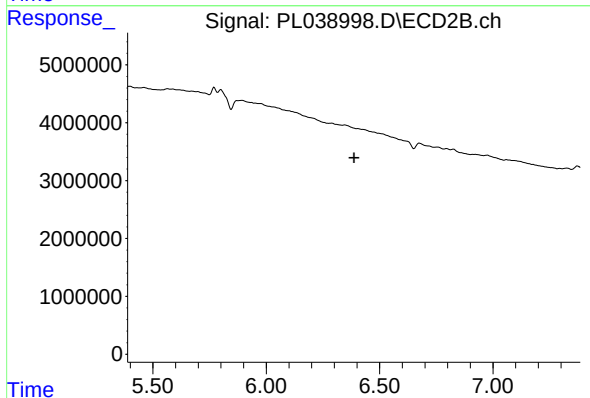


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.387 min
Response: 0
Conc: N.D.

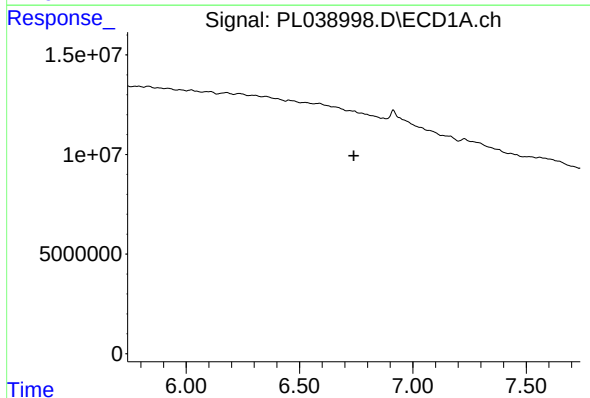


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.739 min
Response: 0
Conc: N.D.

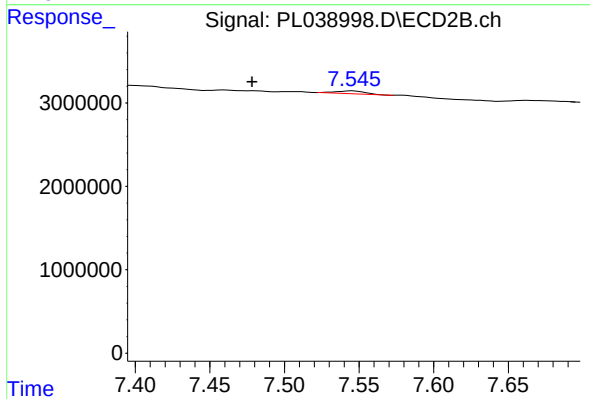

#20 Methoxychlor


R.T.: 7.546 min
Delta R.T.: 0.068 min
Response: 466887
Conc: 0.41 ng/ml

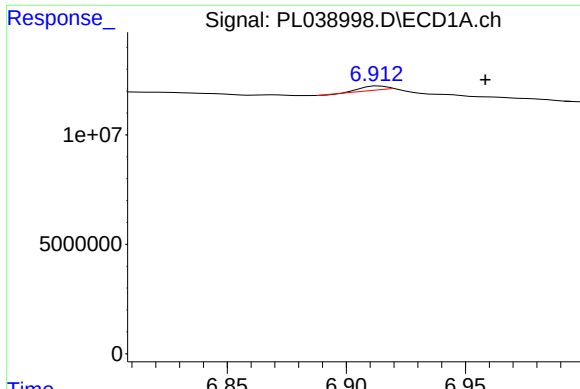

#21 Endrin ketone


R.T.: 6.914 min
Delta R.T.: -0.044 min
Response: 1791259
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

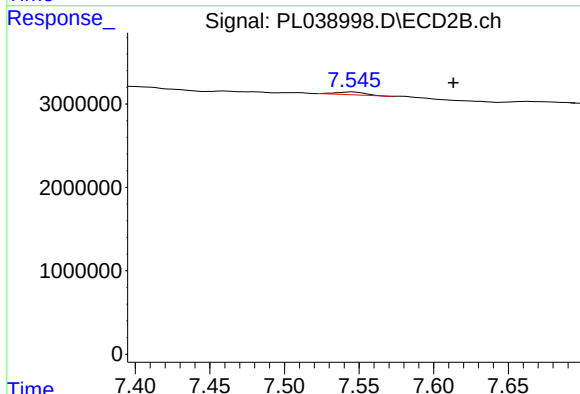


#21 Endrin ketone

R.T.: 7.546 min
Delta R.T.: -0.067 min
Response: 466887
Conc: 0.20 ng/ml

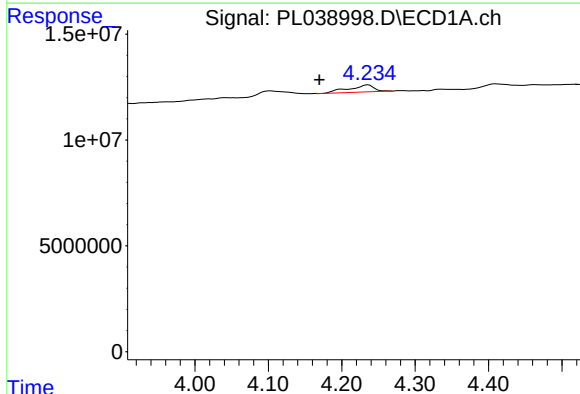


#23 Chlordane-1

R.T.: 4.236 min
Delta R.T.: 0.066 min
Response: 8016434
Conc: 23.15 ng/ml

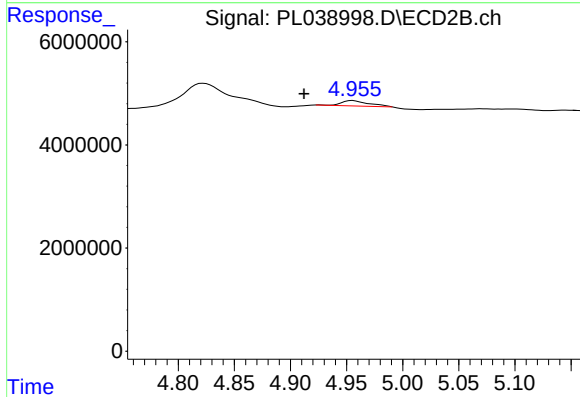

#23 Chlordane-1


R.T.: 4.956 min
Delta R.T.: 0.043 min
Response: 1721649
Conc: 14.86 ng/ml

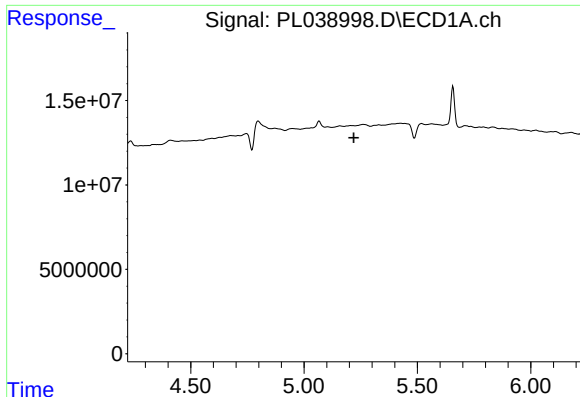

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

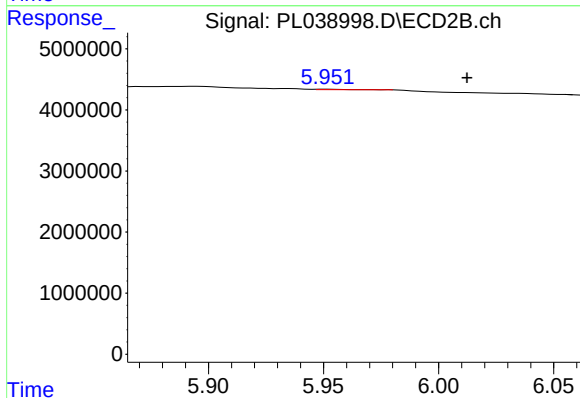


#25 Chlordane-3

R.T.: 5.952 min
Delta R.T.: -0.061 min
Response: 64827
Conc: 0.16 ng/ml

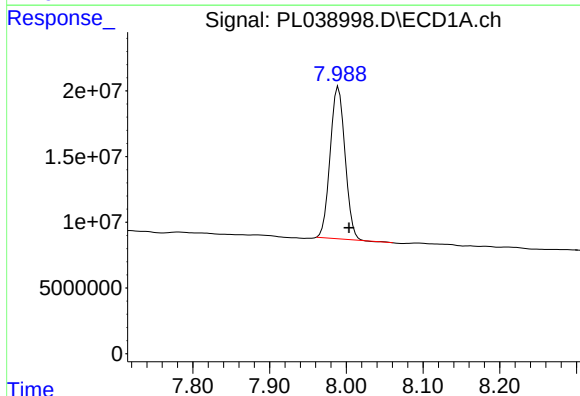

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.014 min
Response: 155336156
Conc: 20.48 ng/ml

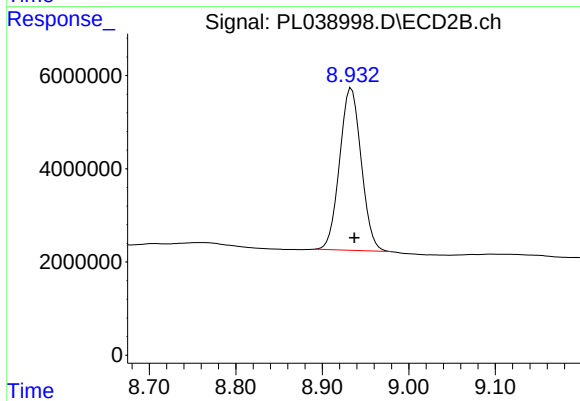

#28 Decachlorobiphenyl

R.T.: 8.934 min
Delta R.T.: -0.004 min
Response: 60141927
Conc: 24.60 ng/ml