

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
 Data File : PL039002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2018 09:03
 Operator : AJ\SJ
 Sample : PB111791BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 09:49:29 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.927	153.9E6	59626850	20.664	22.716
28)	SA Decachlor...	7.989	8.933	149.9E6	56850132	19.754	23.257
Target Compounds							
2)	A alpha-BHC	0.000	4.339f	0	654034	N.D.	0.169 #
7)	B delta-BHC	0.000	4.957	0	2310998	N.D.	0.697 #
8)	B Heptachlo...	0.000	5.771	0	270060	N.D.	0.095 #
13)	MA Dieldrin	5.519f	0.000	3082693	0	0.321	N.D. #
16)	A 4,4'-DDD	0.000	6.674f	0	285045	N.D.	0.133 #
20)	A Methoxychlor	0.000	7.515f	0	628429	N.D.	0.552 #
21)	B Endrin ke...	6.913f	0.000	5072138	0	0.646	N.D. #
23)	Chlordane-1	4.236	4.957	8912881	2310998	25.741	19.942



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
Data File : PL039002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2018 09:03
Operator : AJ\SJ
Sample : PB111791BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 09:49:29 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

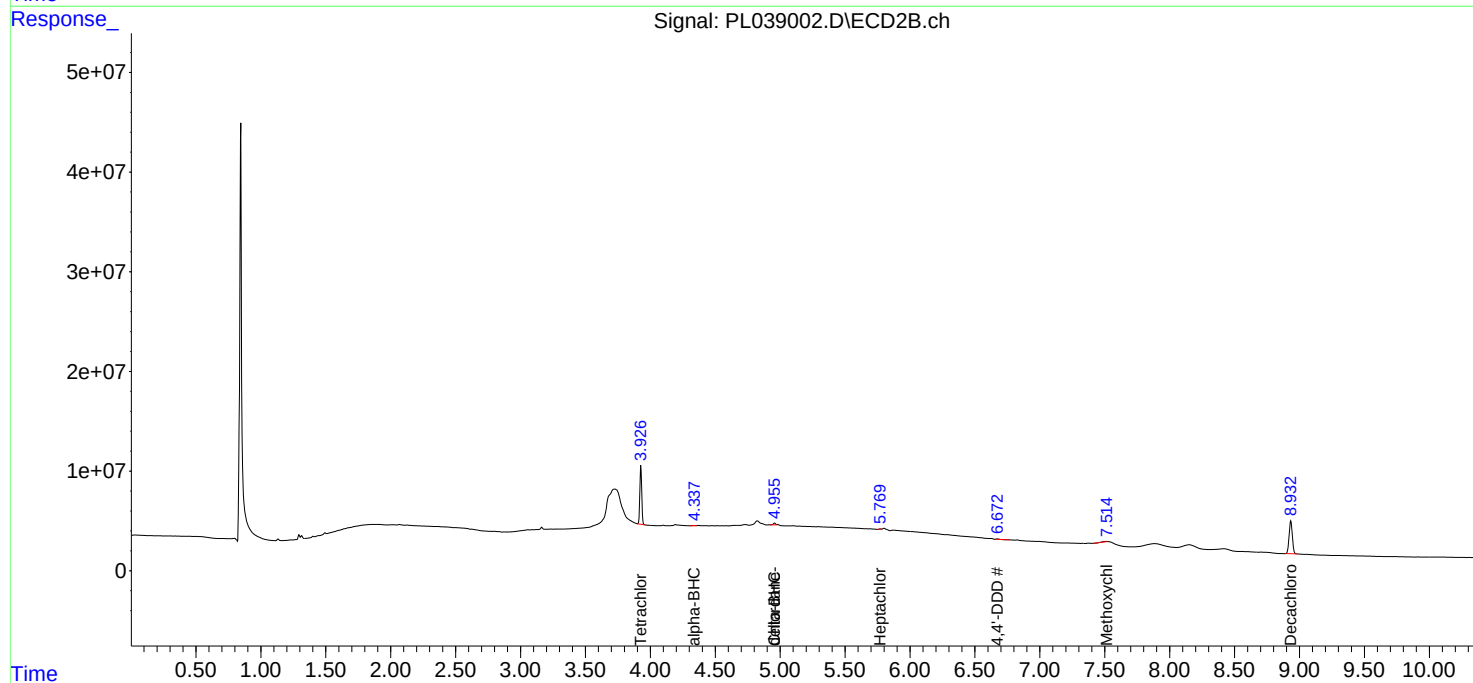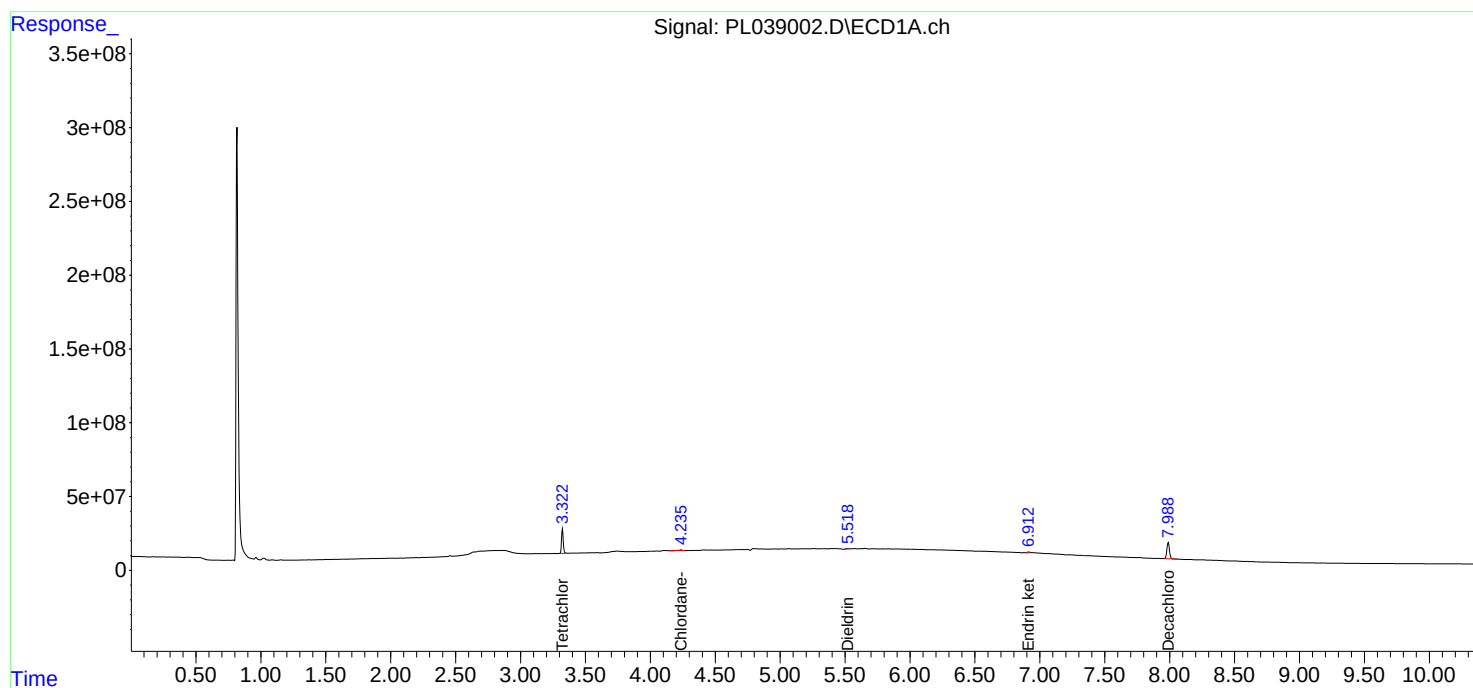


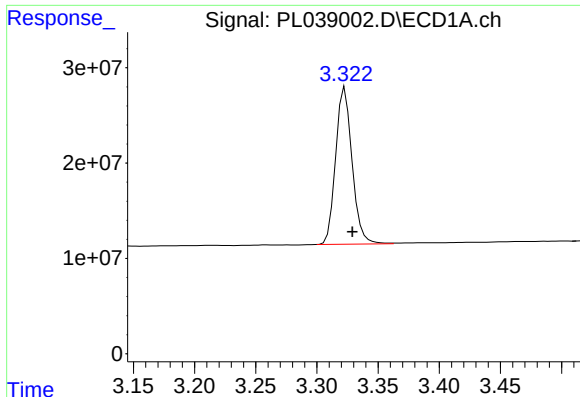

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: -0.006 min
Response: 153873131
Conc: 20.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

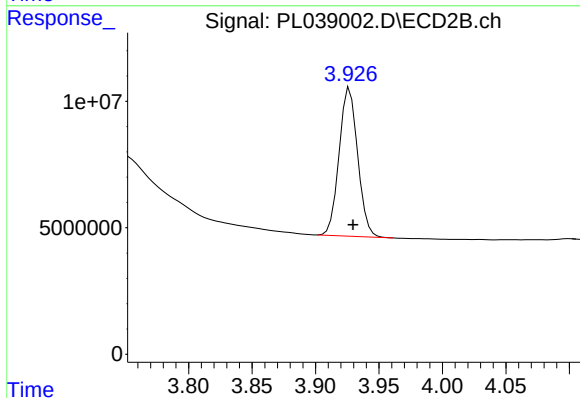


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 59626850
Conc: 22.72 ng/ml

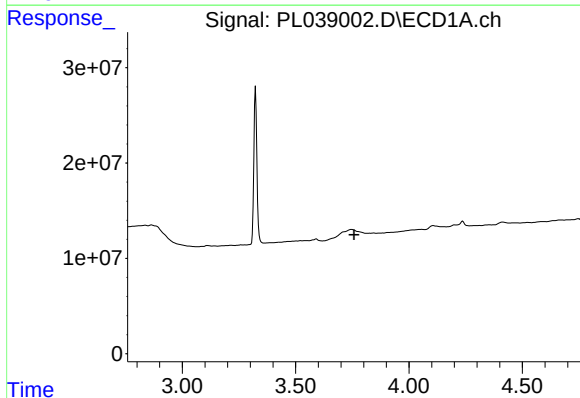


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

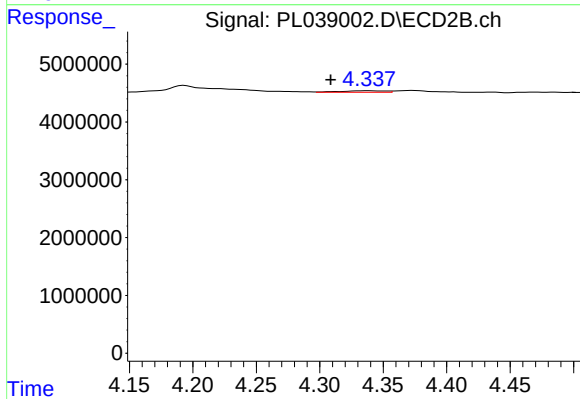

#2 alpha-BHC


R.T.: 4.339 min
Delta R.T.: 0.030 min
Response: 654034
Conc: 0.17 ng/ml

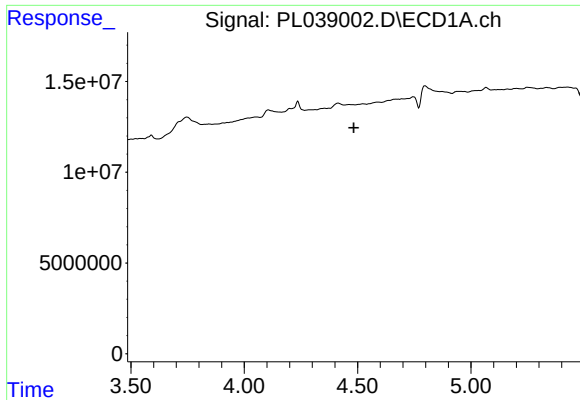

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

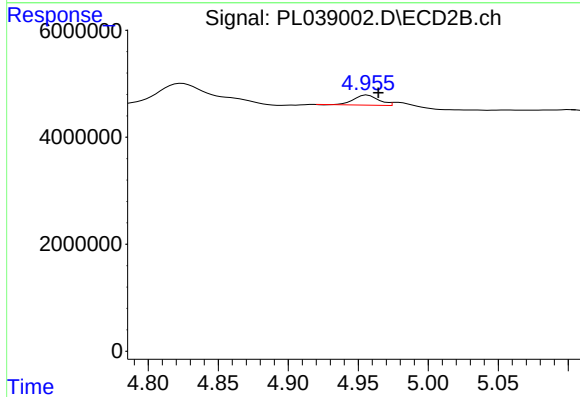


#7 delta-BHC

R.T.: 4.957 min
Delta R.T.: -0.008 min
Response: 2310998
Conc: 0.70 ng/ml

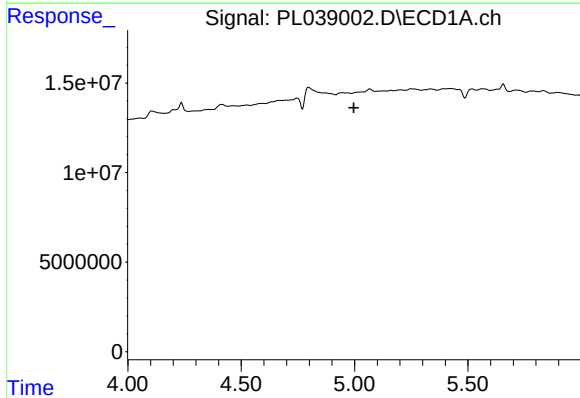


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

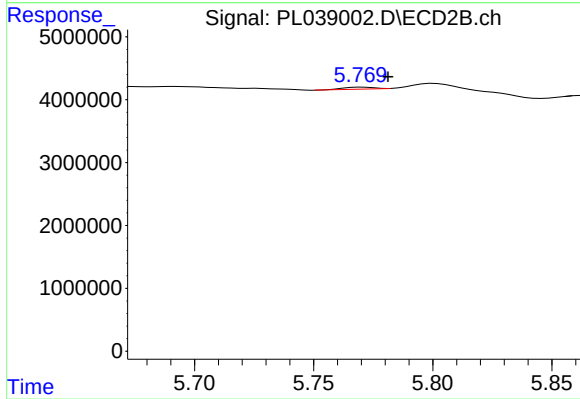

#8 Heptachlor epoxide


R.T.: 5.771 min
Delta R.T.: -0.011 min
Response: 270060
Conc: 0.10 ng/ml

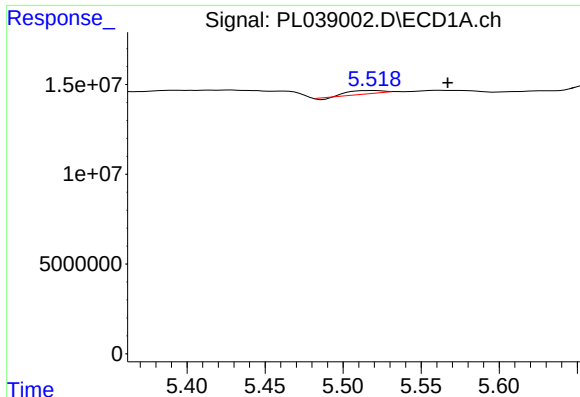

#13 Dieldrin


R.T.: 5.519 min
Delta R.T.: -0.047 min
Response: 3082693
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

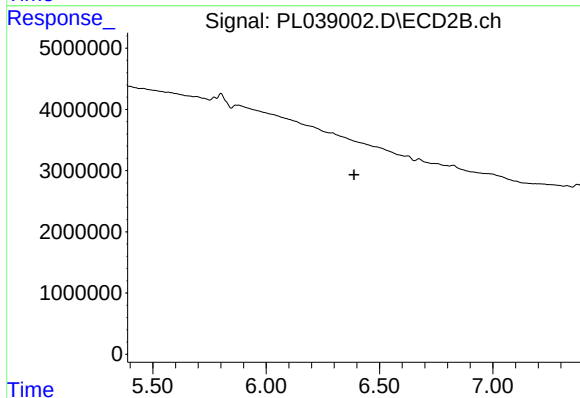


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.387 min
Response: 0
Conc: N.D.

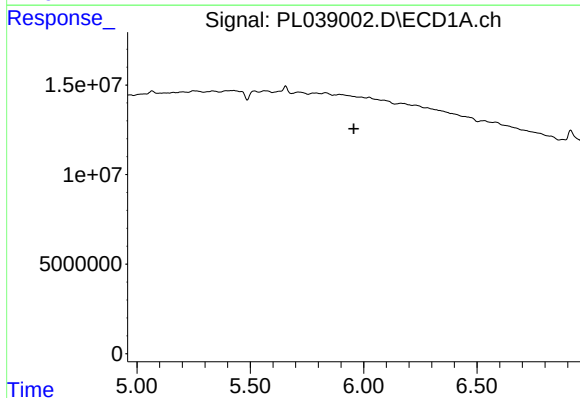


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.956 min
Response: 0
Conc: N.D.

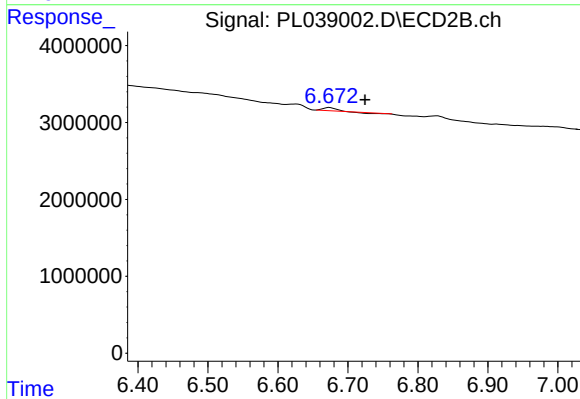

#16 4,4'-DDD


R.T.: 6.674 min
Delta R.T.: -0.051 min
Response: 285045
Conc: 0.13 ng/ml

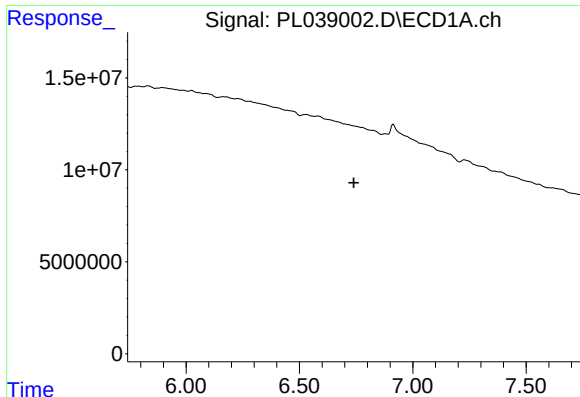

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.739 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

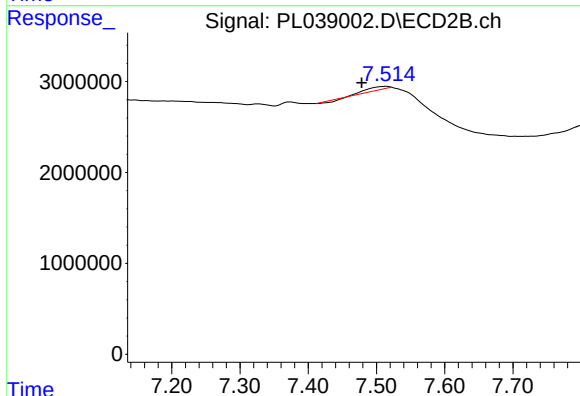


#20 Methoxychlor

R.T.: 7.515 min
Delta R.T.: 0.036 min
Response: 628429
Conc: 0.55 ng/ml

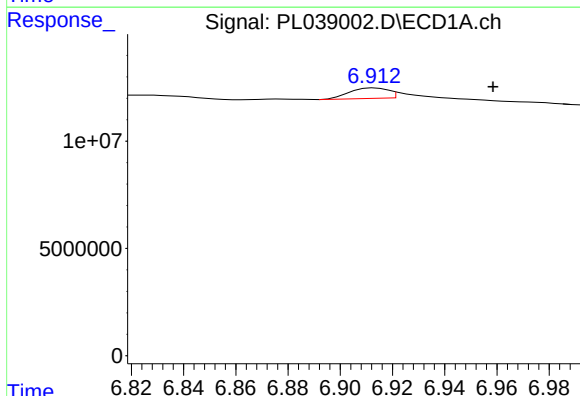


#21 Endrin ketone

R.T.: 6.913 min
Delta R.T.: -0.045 min
Response: 5072138
Conc: 0.65 ng/ml

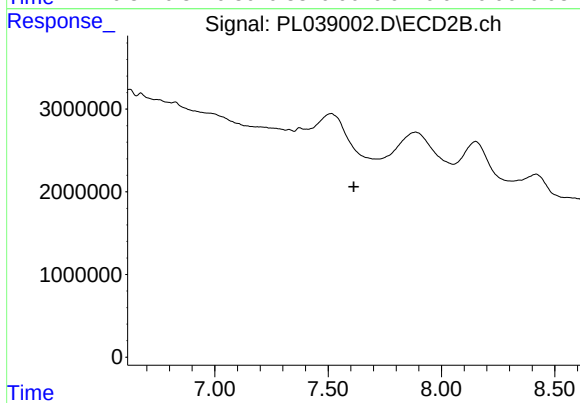

#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.613 min
Response: 0
Conc: N.D.

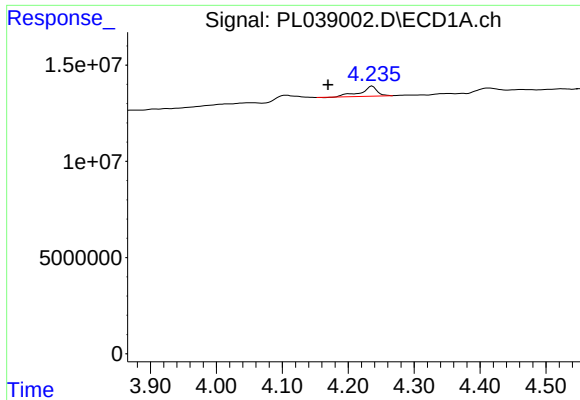

#23 Chlordane-1

R.T.: 4.236 min
Delta R.T.: 0.067 min
Response: 8912881
Conc: 25.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

#23 Chlordane-1

R.T.: 4.957 min
Delta R.T.: 0.044 min
Response: 2310998
Conc: 19.94 ng/ml

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.014 min
Response: 149852810
Conc: 19.75 ng/ml

#28 Decachlorobiphenyl

R.T.: 8.933 min
Delta R.T.: -0.004 min
Response: 56850132
Conc: 23.26 ng/ml