

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
 Data File : PL039010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2018 10:56
 Operator : AJ\SJ
 Sample : J4283-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 11:32:31 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.926	130.6E6	52626869	17.538	20.049
28)	SA Decachlor...	7.989	8.933	141.0E6	55556520	18.592	22.728
Target Compounds							
2)	A alpha-BHC	0.000	4.317	0	592463	N.D.	0.153 #
3)	MA gamma-BHC...	0.000	4.553f	0	233193	N.D.	0.065 #
4)	MA Heptachlor	0.000	5.150f	0	788125	N.D.	0.247 #
7)	B delta-BHC	0.000	4.955	0	5212414	N.D.	1.572 #
8)	B Heptachlo...	4.943f	5.770	2128041	128302	0.226	0.045 #
13)	MA Dieldrin	5.518f	0.000	3911884	0	0.407	N.D. #
15)	B Endosulfa...	0.000	6.826	0	321377	N.D.	0.134 #
23)	Chlordane-1	4.237	4.955	20057491	5212414	57.928	44.979
27)	Chlordane-5	0.000	6.826	0	321377	N.D.	3.588 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080618\
Data File : PL039010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2018 10:56
Operator : AJ\SJ
Sample : J4283-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 11:32:31 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

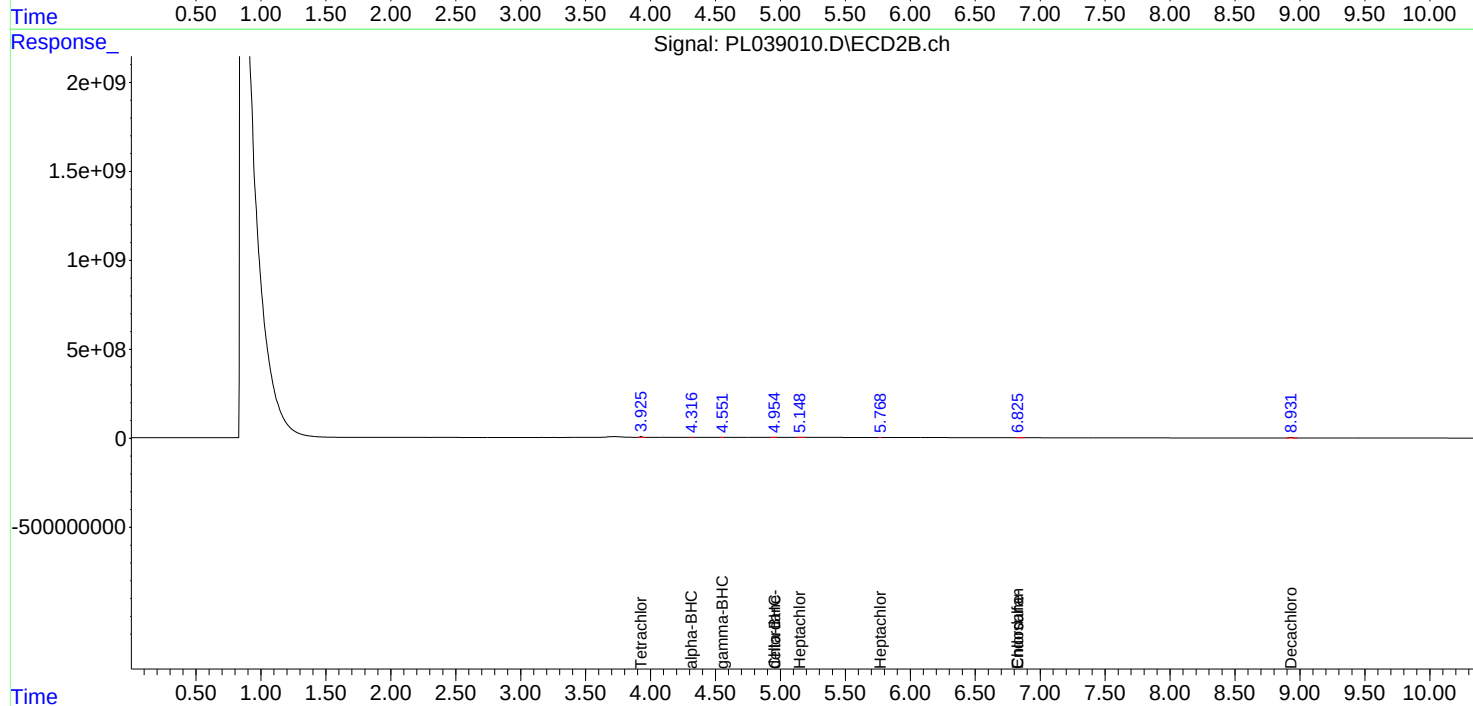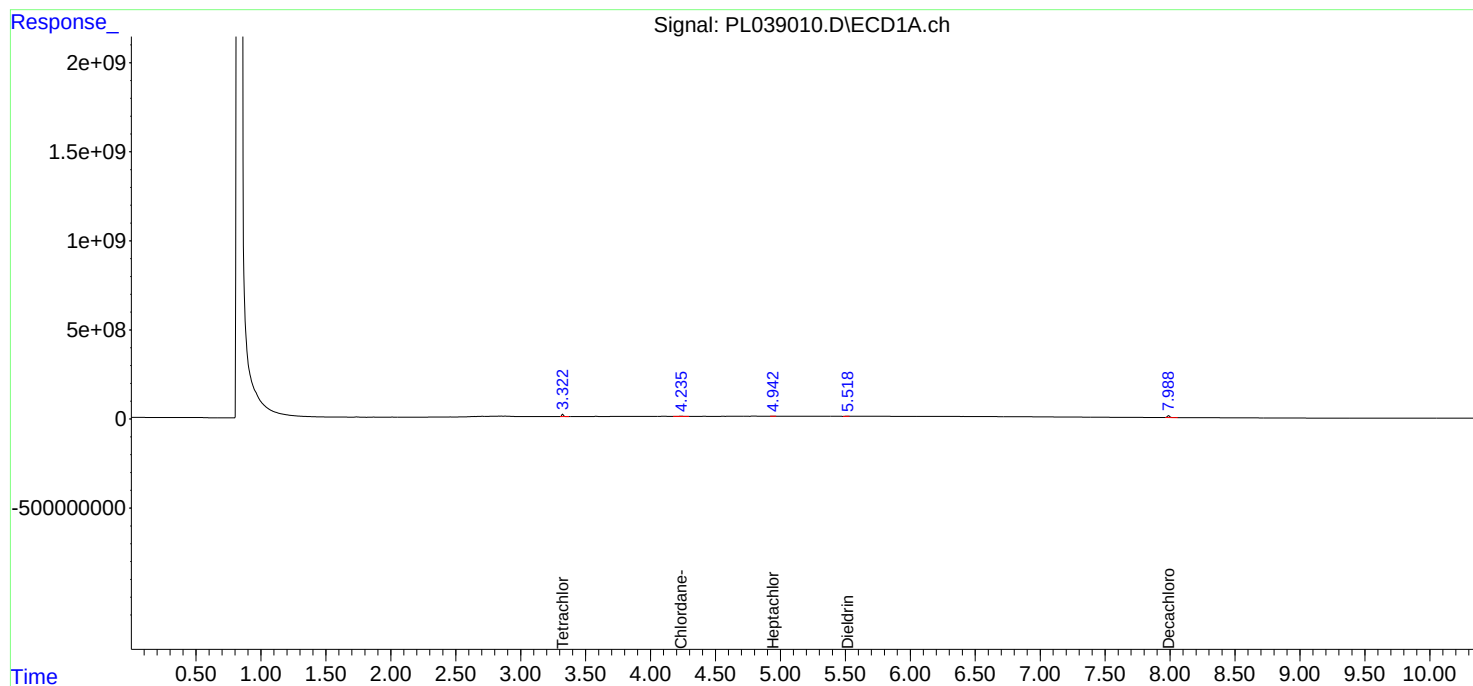


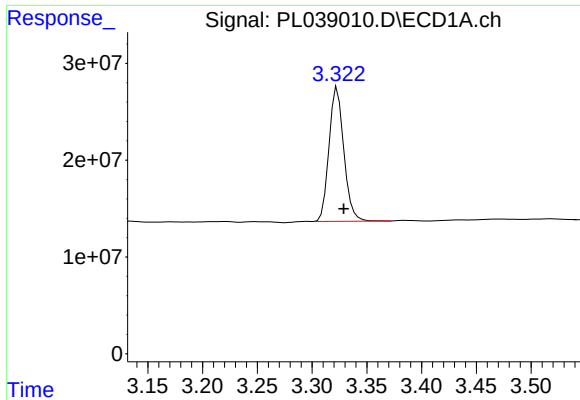

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: -0.006 min
Response: 130592000
Conc: 17.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

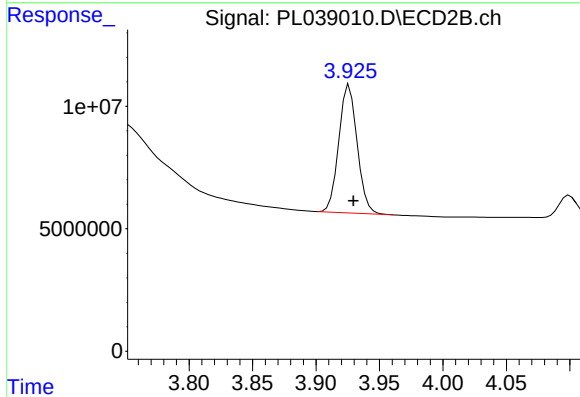


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.003 min
Response: 52626869
Conc: 20.05 ng/ml

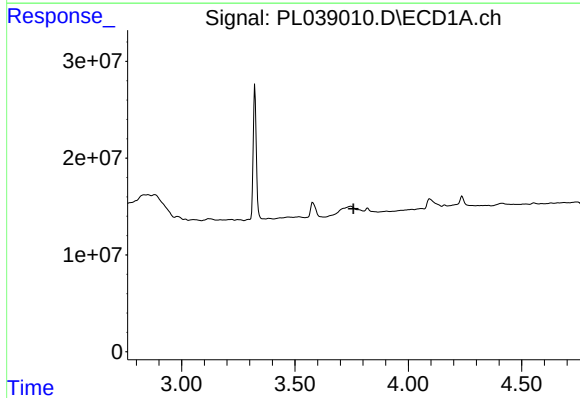


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

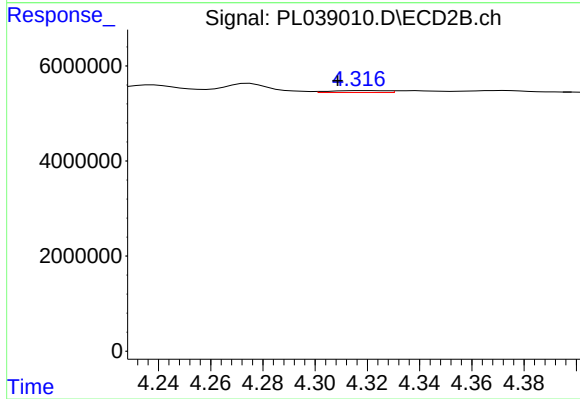

#2 alpha-BHC


R.T.: 4.317 min
Delta R.T.: 0.008 min
Response: 592463
Conc: 0.15 ng/ml

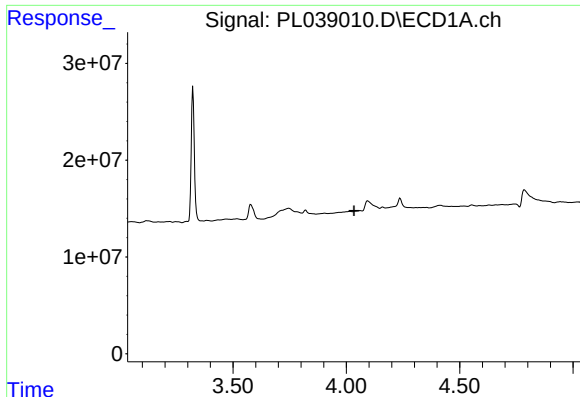

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

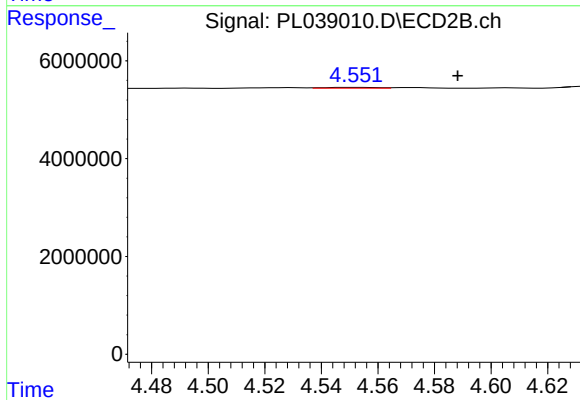


#3 gamma-BHC (Lindane)

R.T.: 4.553 min
Delta R.T.: -0.036 min
Response: 233193
Conc: 0.06 ng/ml

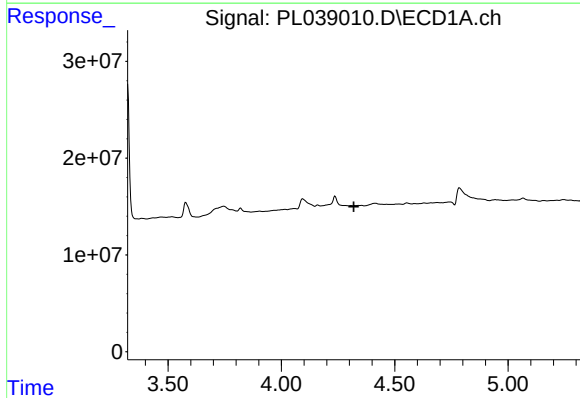


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

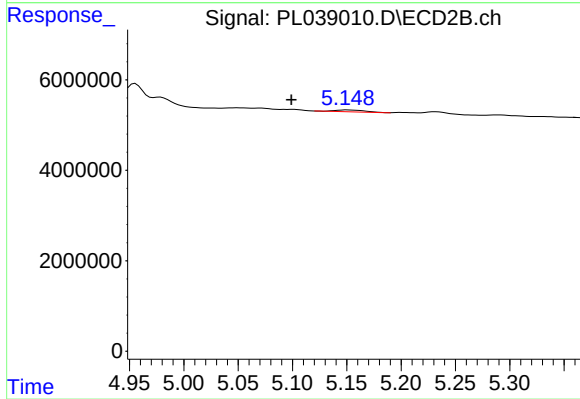

#4 Heptachlor


R.T.: 5.150 min
Delta R.T.: 0.051 min
Response: 788125
Conc: 0.25 ng/ml

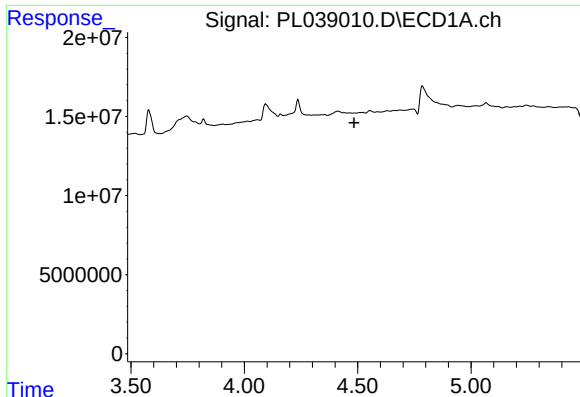

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

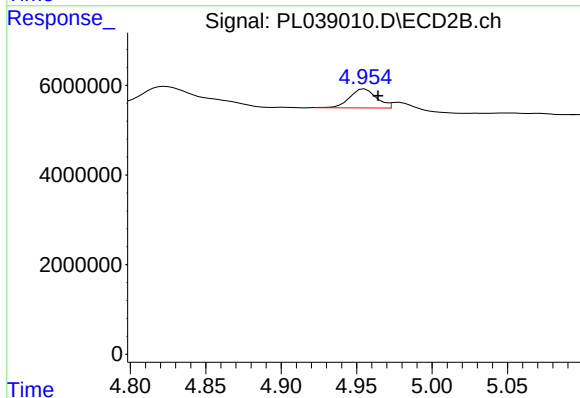


#7 delta-BHC

R.T.: 4.955 min
Delta R.T.: -0.009 min
Response: 5212414
Conc: 1.57 ng/ml

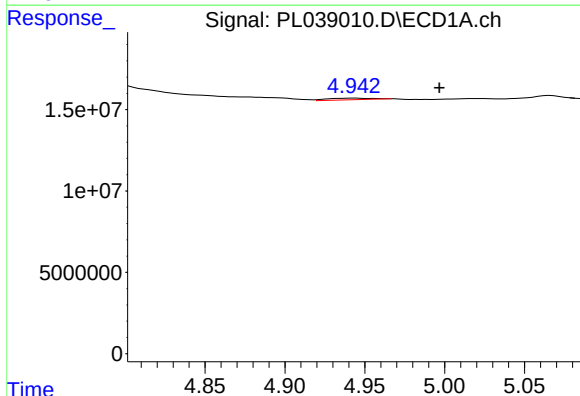


#8 Heptachlor epoxide

R.T.: 4.943 min
Delta R.T.: -0.053 min
Response: 2128041
Conc: 0.23 ng/ml

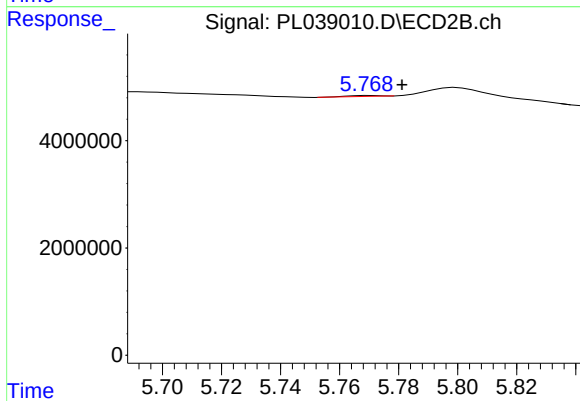

#8 Heptachlor epoxide


R.T.: 5.770 min
Delta R.T.: -0.011 min
Response: 128302
Conc: 0.05 ng/ml

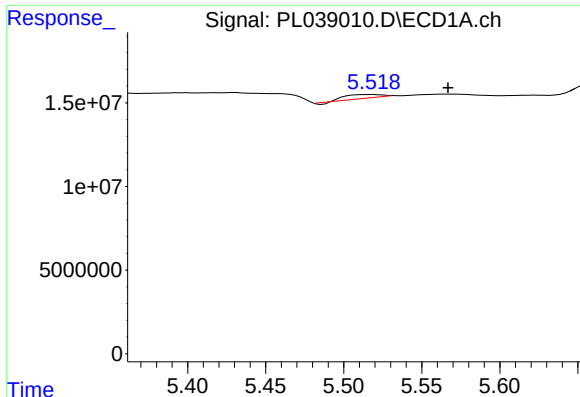

#13 Dieldrin


R.T.: 5.518 min
Delta R.T.: -0.049 min
Response: 3911884
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

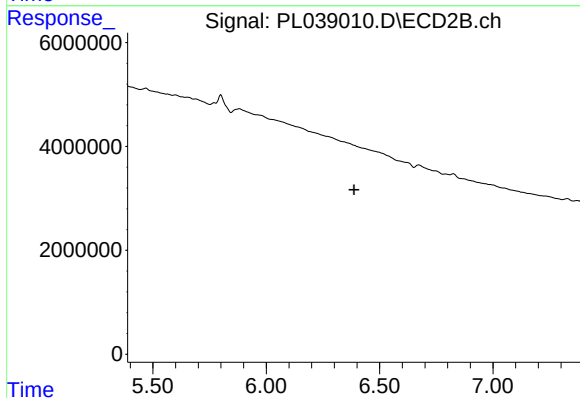


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.387 min
Response: 0
Conc: N.D.

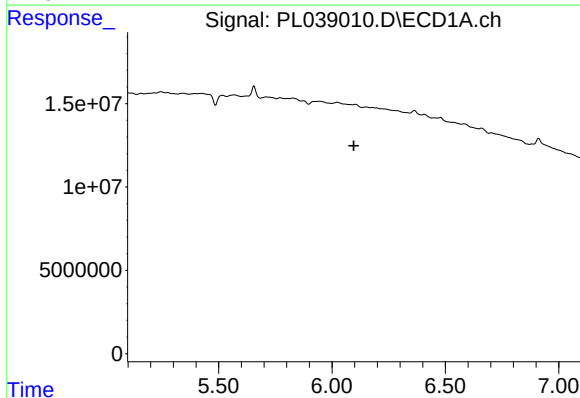


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.096 min
Response: 0
Conc: N.D.

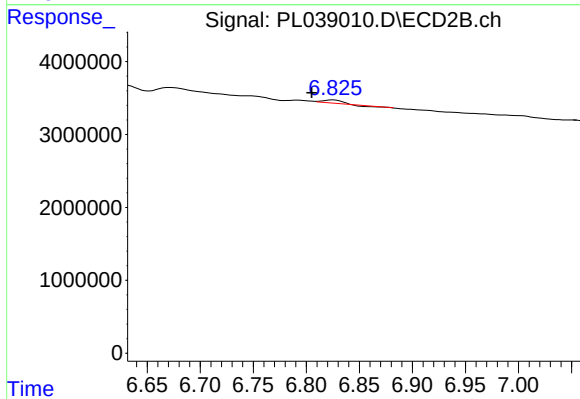

#15 Endosulfan II


R.T.: 6.826 min
Delta R.T.: 0.020 min
Response: 321377
Conc: 0.13 ng/ml

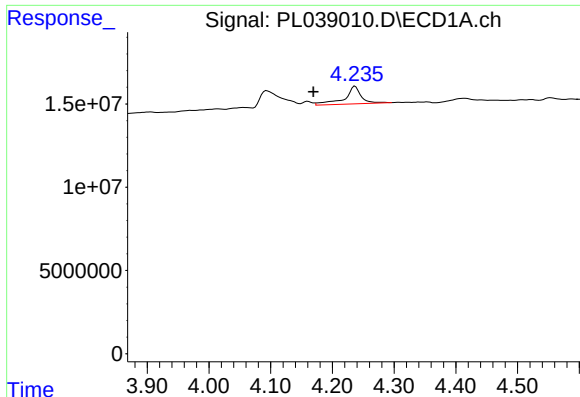

#23 Chlordane-1


R.T.: 4.237 min
Delta R.T.: 0.067 min
Response: 20057491
Conc: 57.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

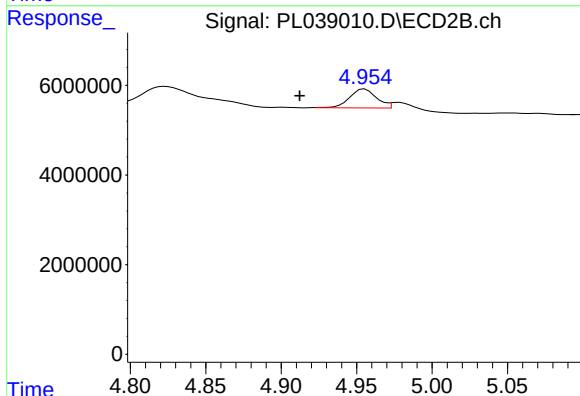


#23 Chlordane-1

R.T.: 4.955 min
Delta R.T.: 0.043 min
Response: 5212414
Conc: 44.98 ng/ml

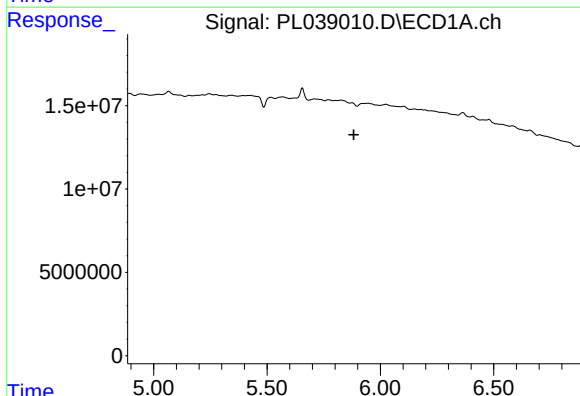


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.883 min
Response: 0
Conc: N.D.

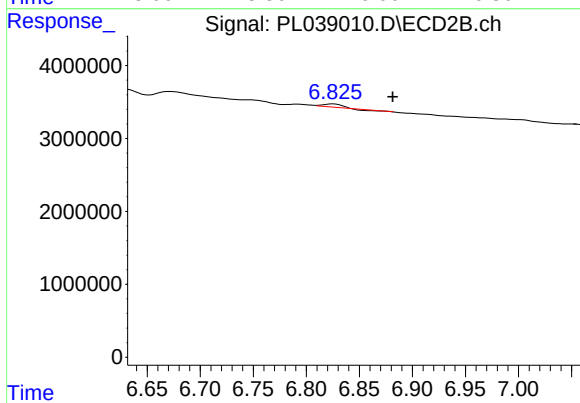

#27 Chlordane-5


R.T.: 6.826 min
Delta R.T.: -0.056 min
Response: 321377
Conc: 3.59 ng/ml

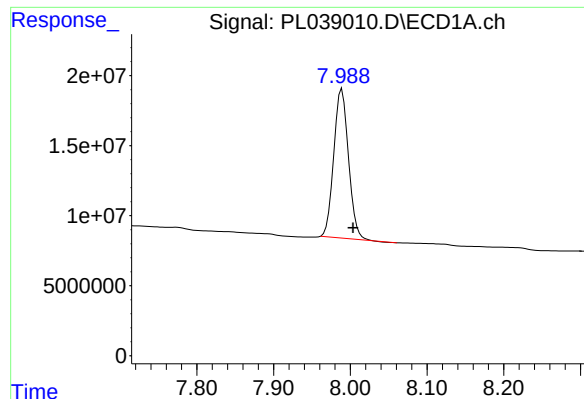

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.015 min
Response: 141037852
Conc: 18.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

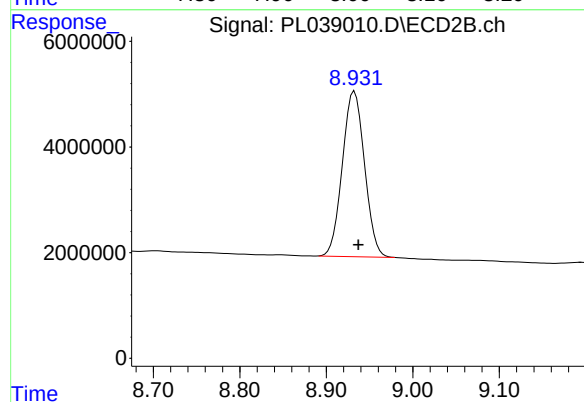

#28 Decachlorobiphenyl

R.T.: 8.933 min
Delta R.T.: -0.005 min
Response: 55556520
Conc: 22.73 ng/ml