

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080619\
 Data File : PL051101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 14:54
 Operator : SM\AJ
 Sample : K4154-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PS-1

Manual Integrations
 APPROVED

Ankita
 8/7/2019 5:44:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 00:39:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.318	3.928	71173591	19037564	7.083	6.672
28) SA Decachlor...	7.978	8.957	44008935	10311204	4.346	3.646
Target Compounds						
10) B gamma-Chl...	5.205	6.023	11949462	5075737	0.757m	1.374 #
11) B alpha-Chl...	5.255	6.096	32778221	15384330	2.149	4.197 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080619\
Data File : PL051101.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 14:54
Operator : SM\AJ
Sample : K4154-01
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampled :
PS-1


Manual Integrations
APPROVED

Ankita
8/7/2019 5:44:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 00:39:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

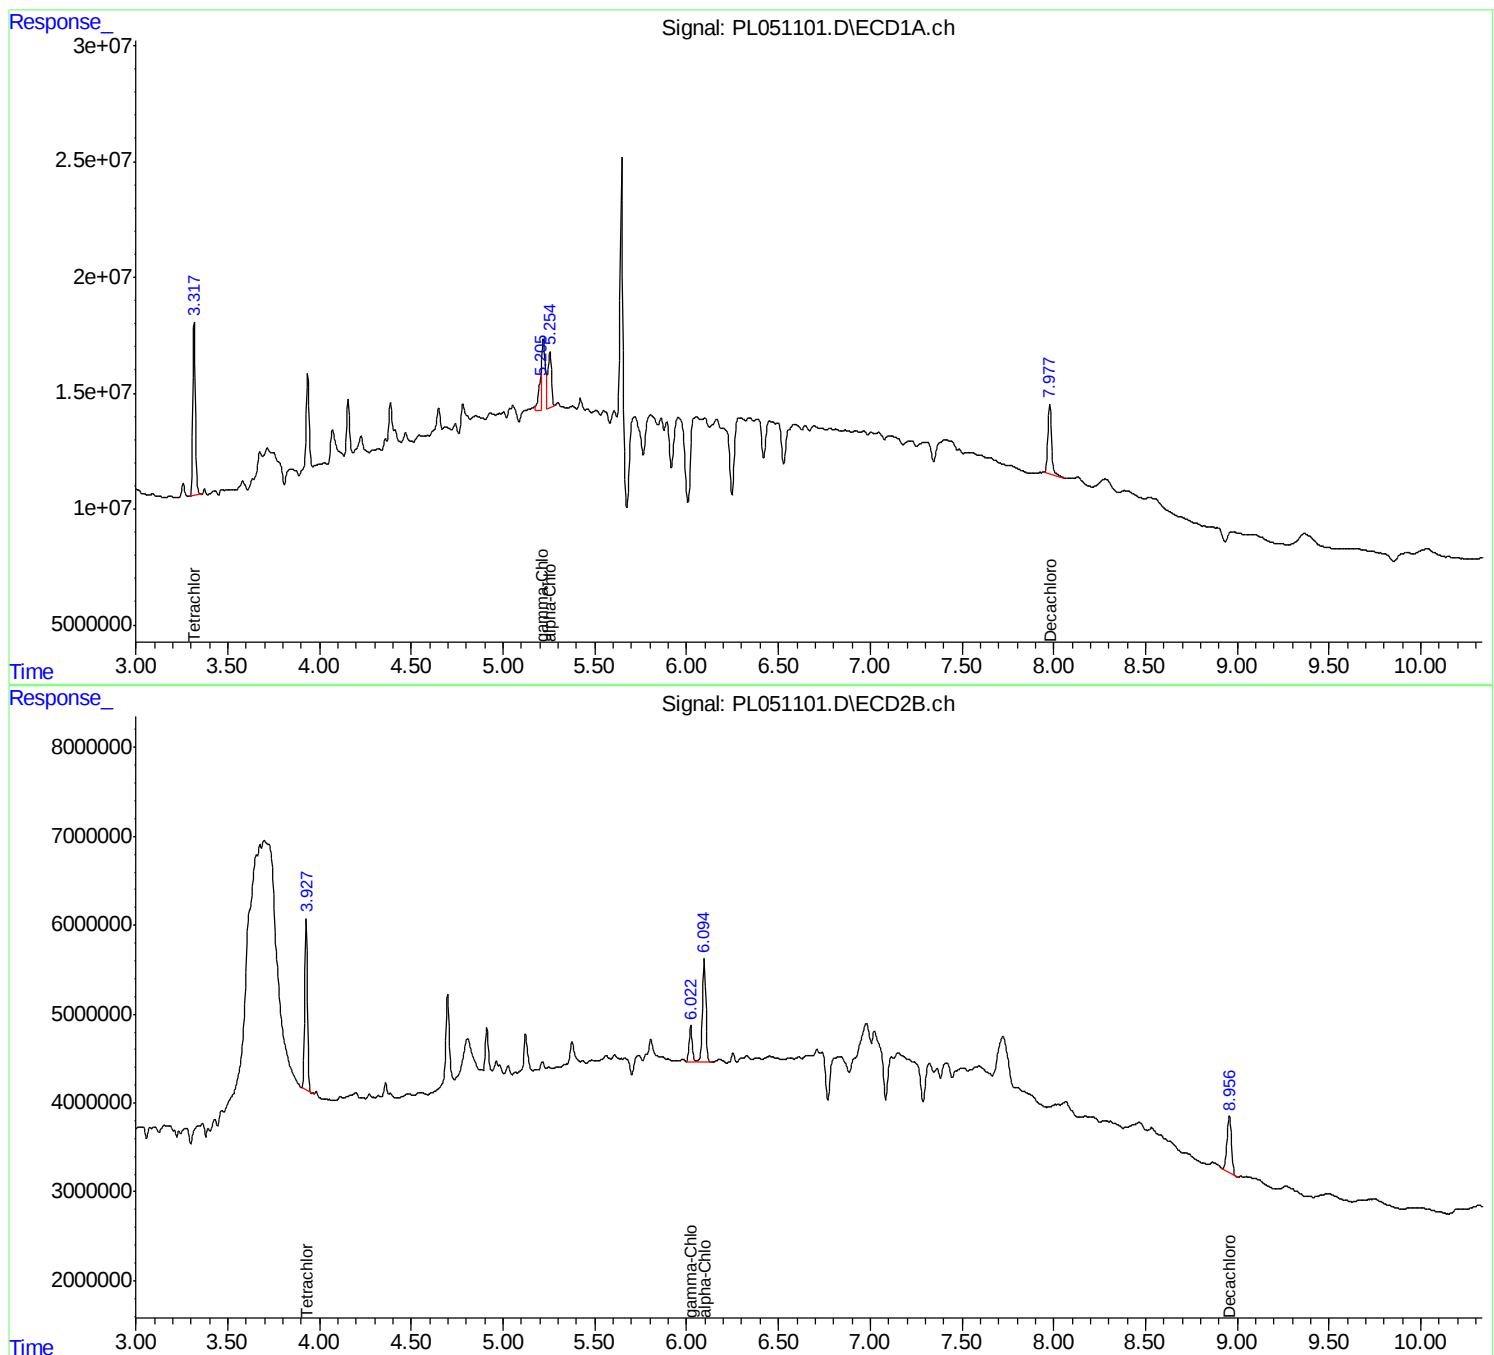

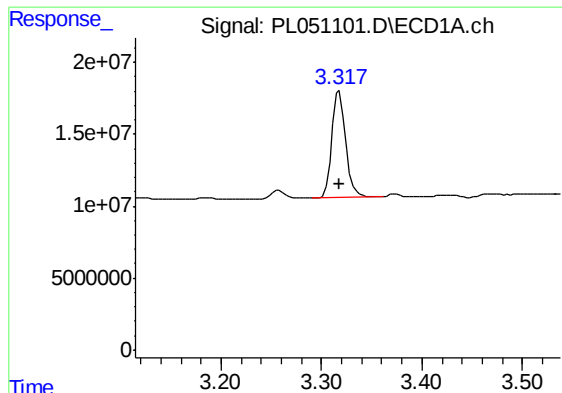


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 71173591
Conc: 7.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PS-1


Manual Integrations
APPROVED

Ankita
8/7/2019 5:44:22 PM

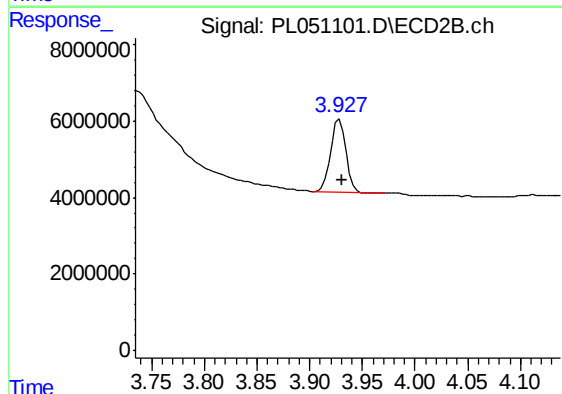


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 19037564
Conc: 6.67 ng/ml

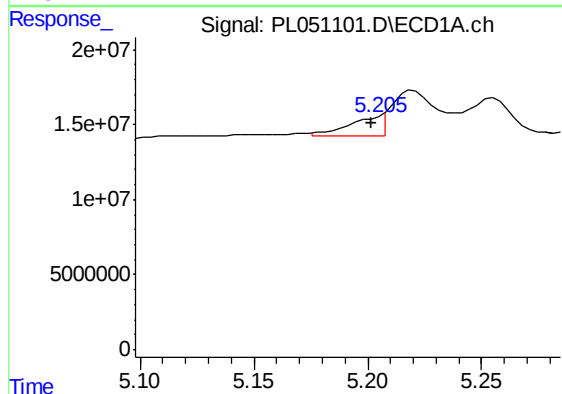


#10 gamma-Chlordane

R.T.: 5.205 min
Delta R.T.: 0.003 min
Response: 11949462
Conc: 0.76 ng/ml m

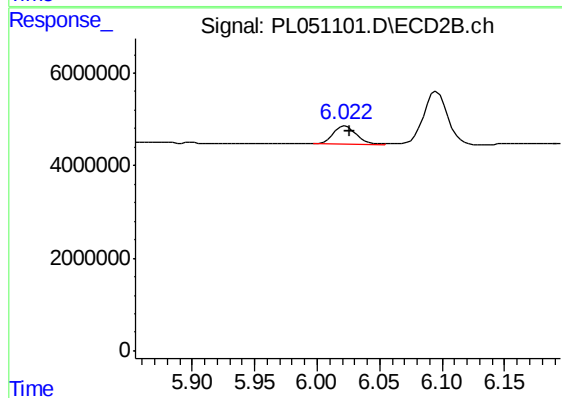

#10 gamma-Chlordane

R.T.: 6.023 min
Delta R.T.: -0.003 min
Response: 5075737
Conc: 1.37 ng/ml

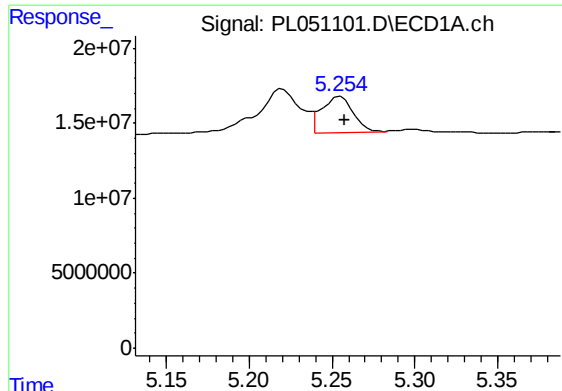


#11 alpha-Chlordane

R.T.: 5.255 min
Delta R.T.: -0.002 min
Response: 32778221
Conc: 2.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PS-1


Manual Integrations
APPROVED

Ankita
8/7/2019 5:44:22 PM

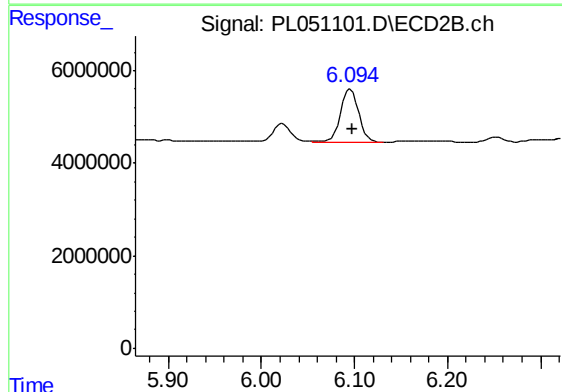


#11 alpha-Chlordane

R.T.: 6.096 min
Delta R.T.: -0.002 min
Response: 15384330
Conc: 4.20 ng/ml

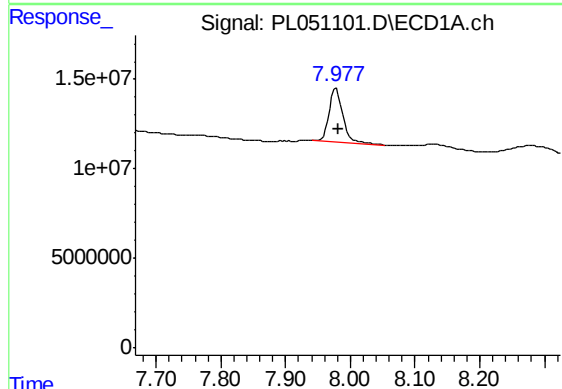

#28 Decachlorobiphenyl

R.T.: 7.978 min
Delta R.T.: -0.002 min
Response: 44008935
Conc: 4.35 ng/ml

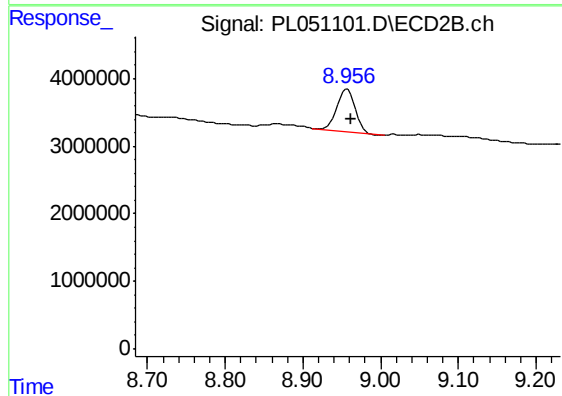

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.004 min
Response: 10311204
Conc: 3.65 ng/ml