

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080619\
 Data File : PL051106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 16:10
 Operator : SM\AJ
 Sample : K4154-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PS-4

Manual Integrations
 APPROVED

Ankita
 8/7/2019 5:44:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 00:41:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.928	108.0E6	29088862	10.745	10.195
28)	SA Decachlor...	7.976	8.956	86127005	25303274	8.506	8.948
Target Compounds							
10)	B gamma-Chl...	5.204	6.021	15808044	5017003	1.002m	1.358m#
11)	B alpha-Chl...	5.252	6.095	26974440	13550869	1.768	3.697 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080619\
Data File : PL051106.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 16:10
Operator : SM\AJ
Sample : K4154-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PS-4


Manual Integrations
APPROVED

Ankita
8/7/2019 5:44:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 00:41:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

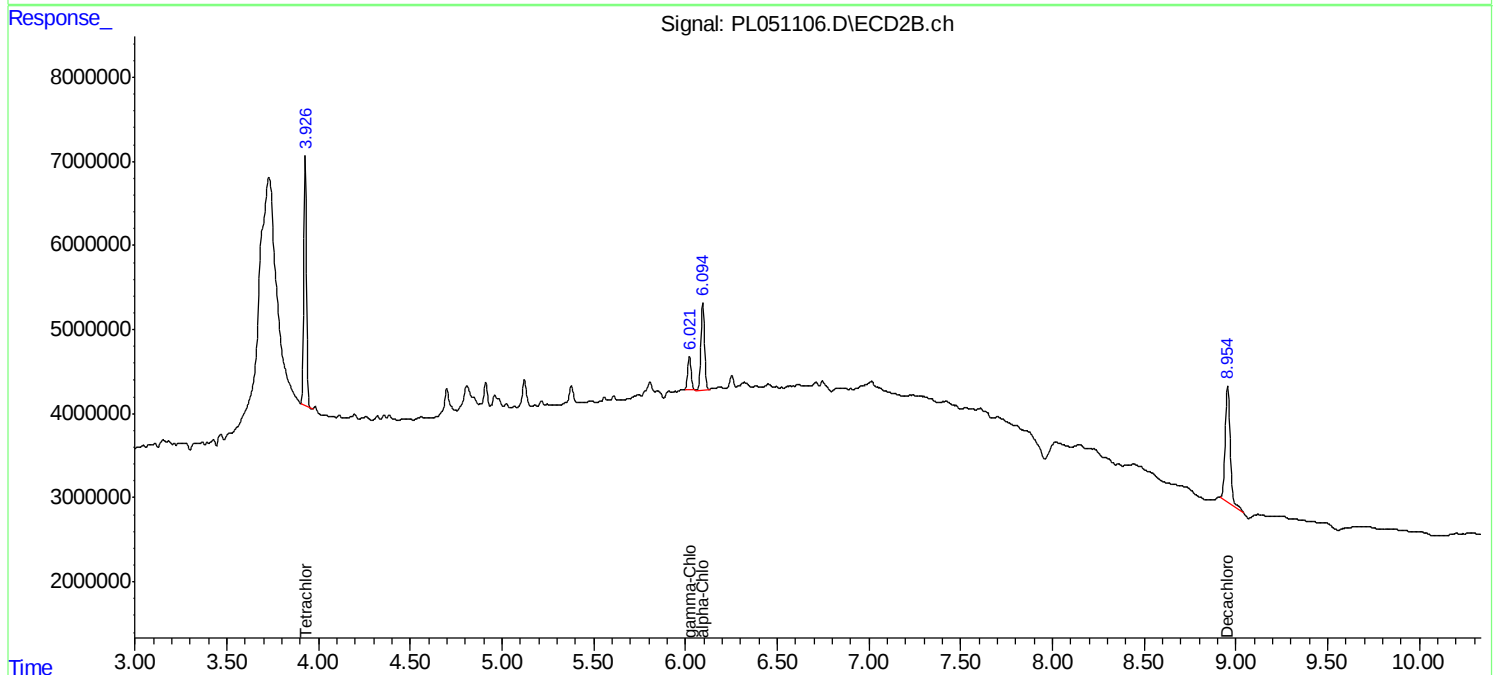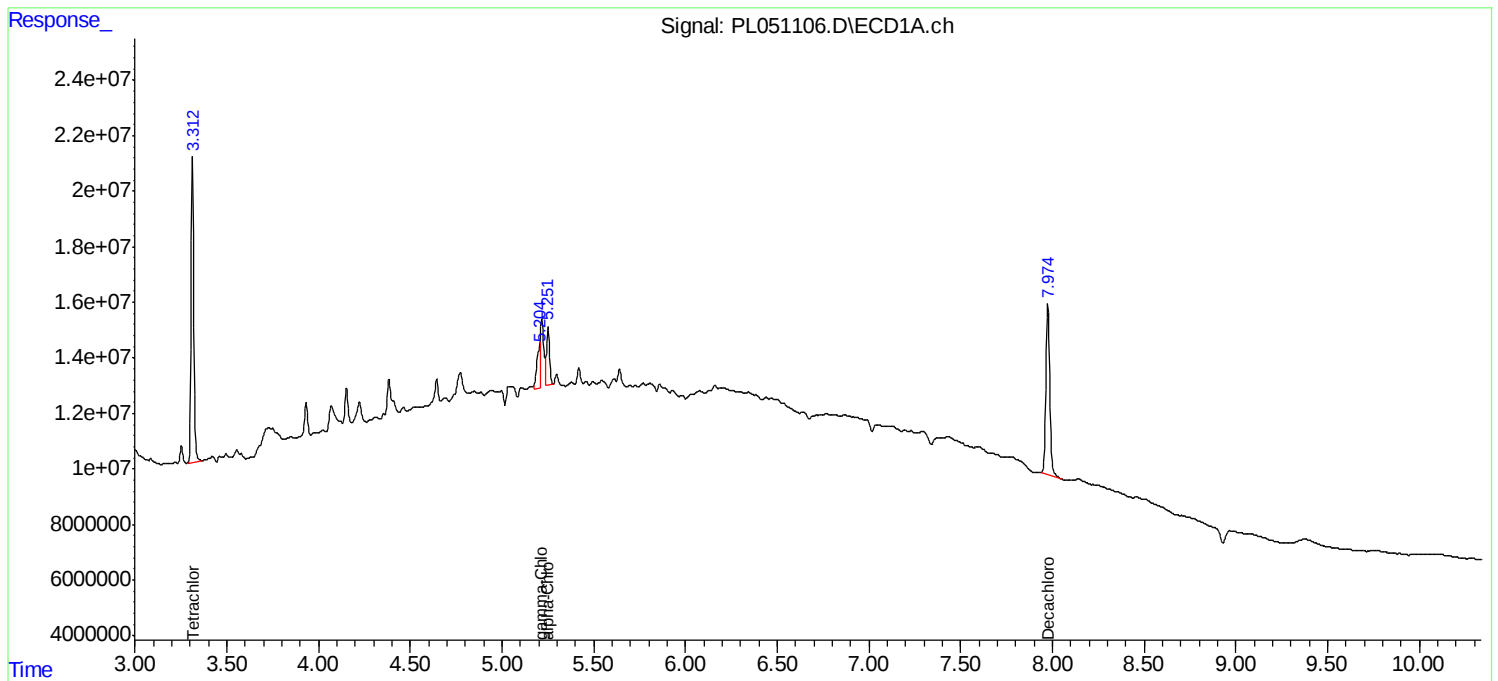

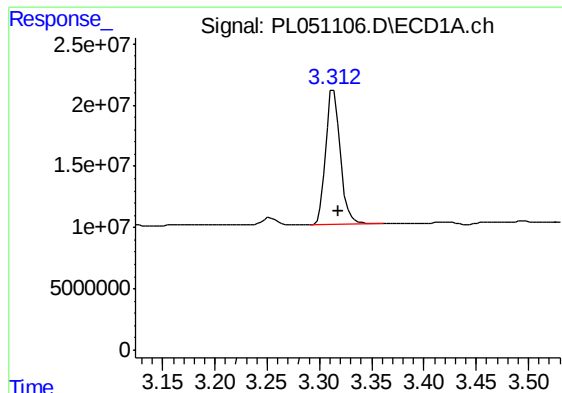


#1 Tetrachloro-m-xylene

R.T.: 3.314 min
Delta R.T.: -0.004 min
Response: 107961326
Conc: 10.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PS-4


Manual Integrations
APPROVED

Ankita
8/7/2019 5:44:40 PM

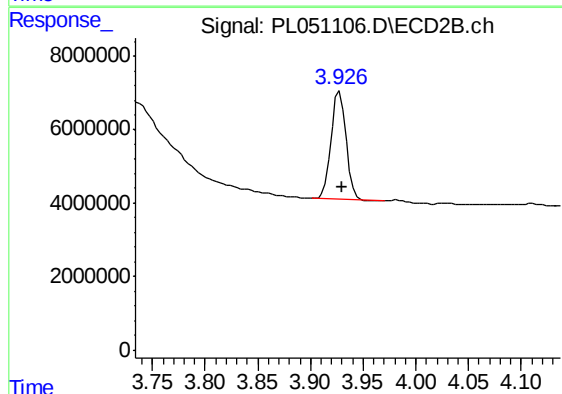


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.003 min
Response: 29088862
Conc: 10.20 ng/ml

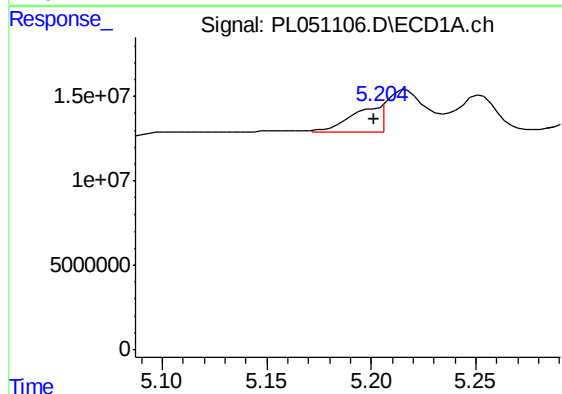


#10 gamma-Chlordane

R.T.: 5.204 min
Delta R.T.: 0.002 min
Response: 15808044
Conc: 1.00 ng/ml m

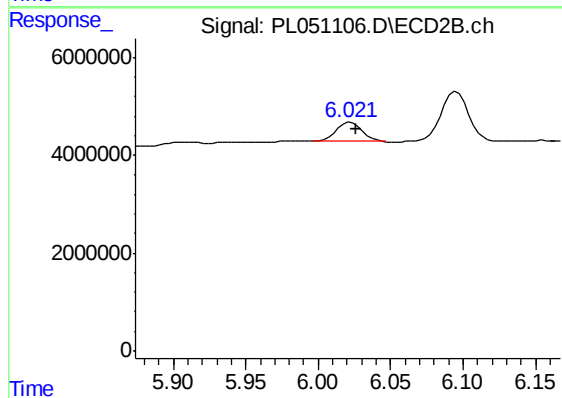

#10 gamma-Chlordane

R.T.: 6.021 min
Delta R.T.: -0.005 min
Response: 5017003
Conc: 1.36 ng/ml m

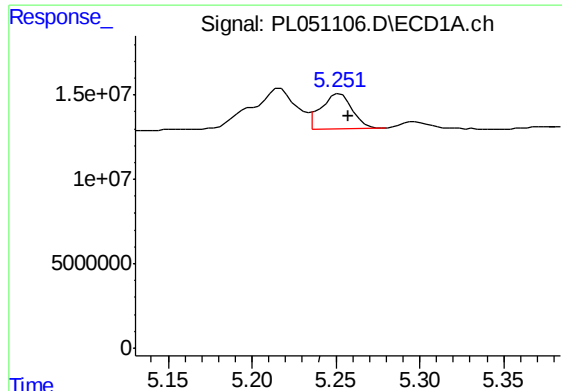


#11 alpha-Chlordane

R.T.: 5.252 min
Delta R.T.: -0.005 min
Response: 26974440
Conc: 1.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PS-4


Manual Integrations
APPROVED

Ankita
8/7/2019 5:44:40 PM

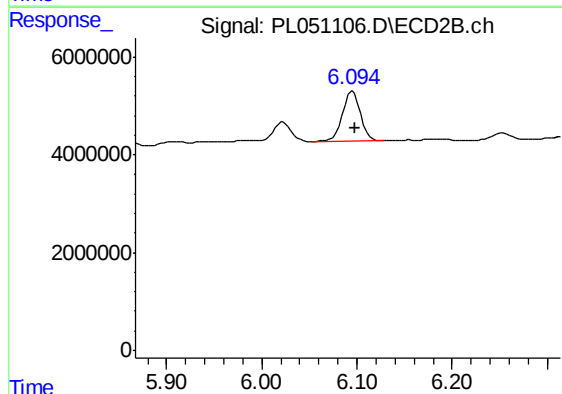


#11 alpha-Chlordane

R.T.: 6.095 min
Delta R.T.: -0.003 min
Response: 13550869
Conc: 3.70 ng/ml

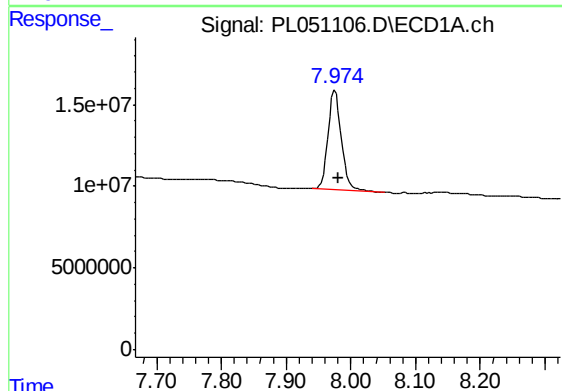

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.005 min
Response: 86127005
Conc: 8.51 ng/ml

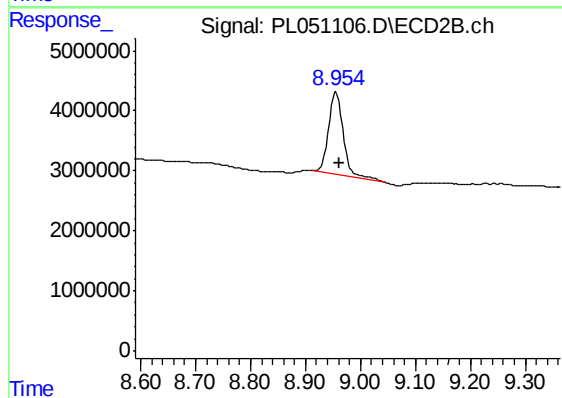

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: -0.006 min
Response: 25303274
Conc: 8.95 ng/ml