

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080619\
 Data File : PL051109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 16:52
 Operator : SM\AJ
 Sample : K4154-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PS-7

Manual Integrations
 APPROVED

Ankita
 8/8/2019 2:37:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 00:42:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.928	155.2E6	43552545	15.443	15.264
28)	SA Decachlor...	7.976	8.955	66178831	18506498	6.536	6.544
Target Compounds							
10)	B gamma-Chl...	5.195	6.019	33497993	9297579	2.122m	2.516m
11)	B alpha-Chl...	5.250	6.093	40081571	11148135	2.627m	3.042m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080619\
Data File : PL051109.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 16:52
Operator : SM\AJ
Sample : K4154-07
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampled :
PS-7


Manual Integrations
APPROVED

Ankita
8/8/2019 2:37:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 00:42:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

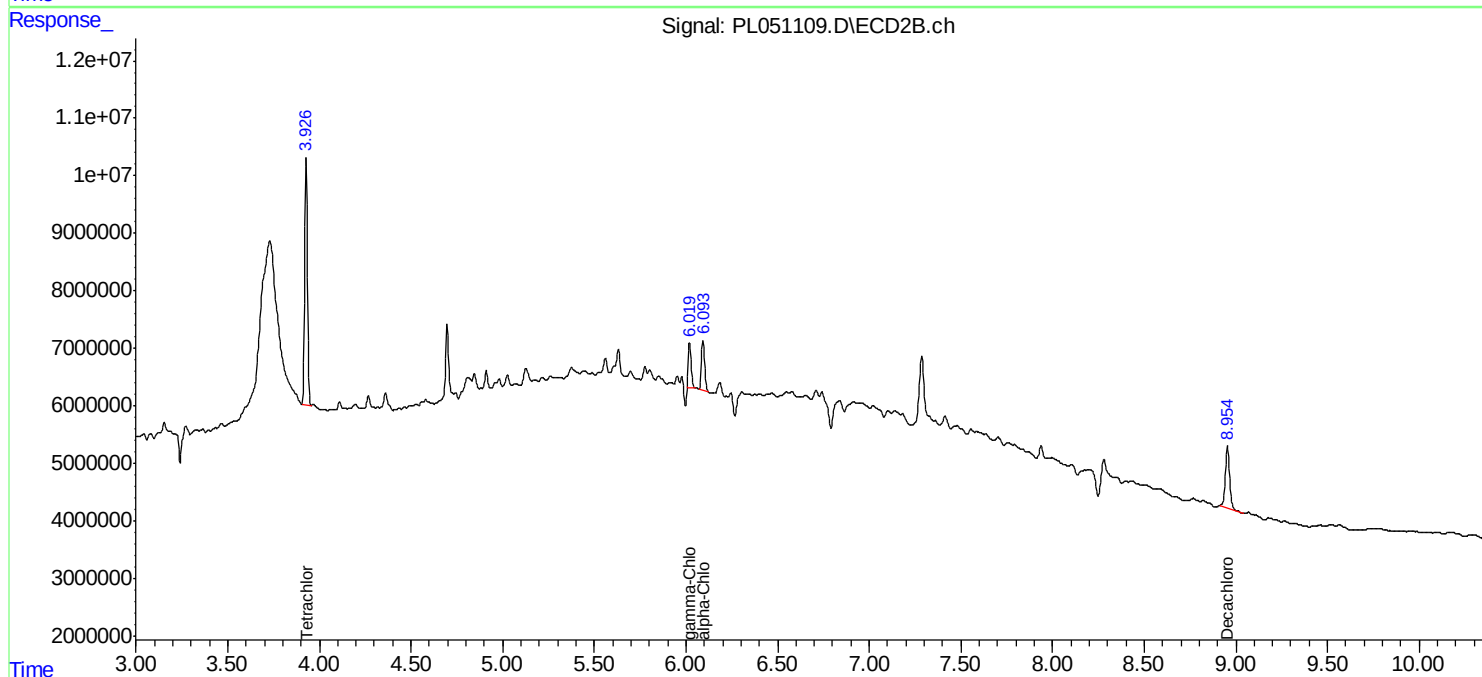

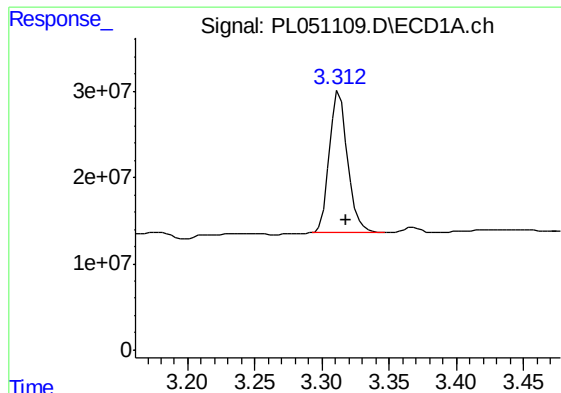


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.005 min
Response: 155164440
Conc: 15.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PS-7


Manual Integrations
APPROVED

Ankita
8/8/2019 2:37:47 PM

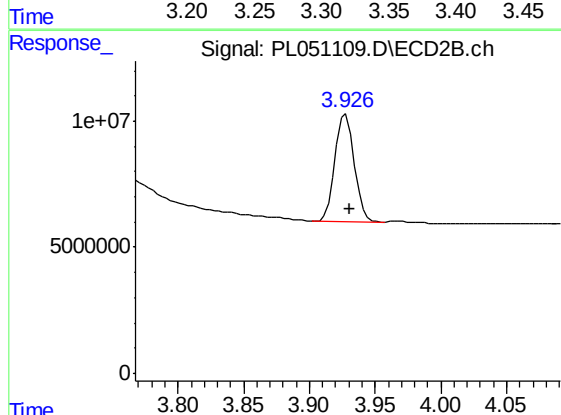


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.003 min
Response: 43552545
Conc: 15.26 ng/ml

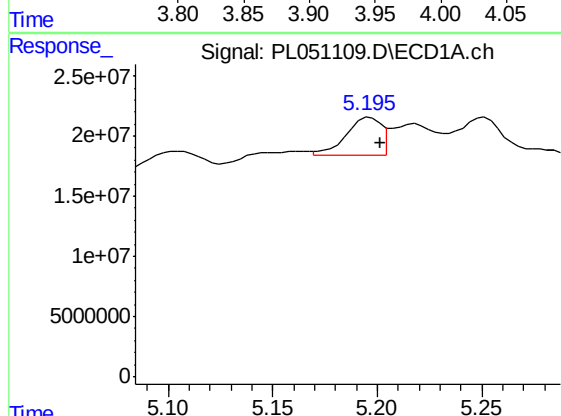


#10 gamma-Chlordane

R.T.: 5.195 min
Delta R.T.: -0.007 min
Response: 33497993
Conc: 2.12 ng/ml m

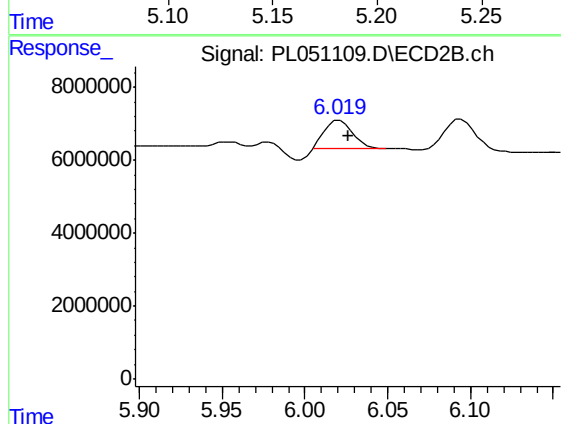

#10 gamma-Chlordane

R.T.: 6.019 min
Delta R.T.: -0.007 min
Response: 9297579
Conc: 2.52 ng/ml m

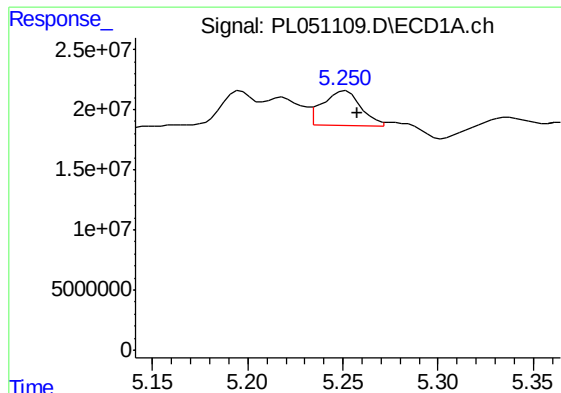


#11 alpha-Chlordane

R.T.: 5.250 min
Delta R.T.: -0.008 min
Response: 40081571
Conc: 2.63 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PS-7


Manual Integrations
APPROVED

Ankita
8/8/2019 2:37:47 PM

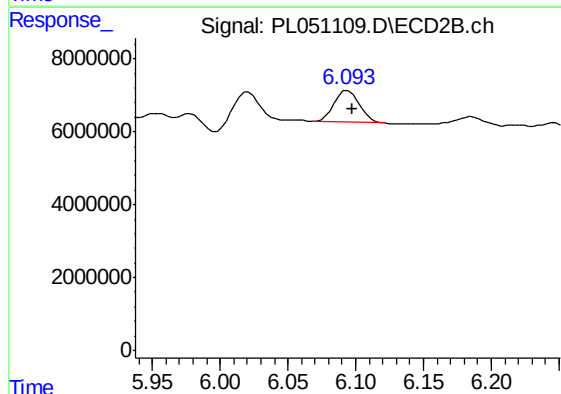


#11 alpha-Chlordane

R.T.: 6.093 min
Delta R.T.: -0.005 min
Response: 11148135
Conc: 3.04 ng/ml m

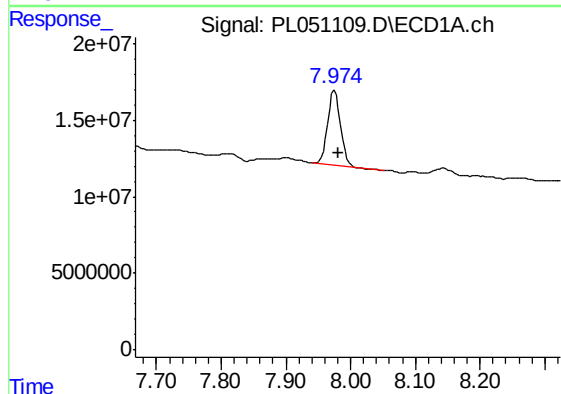

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.005 min
Response: 66178831
Conc: 6.54 ng/ml

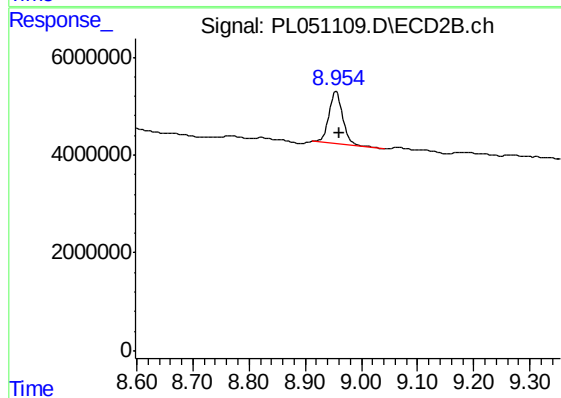

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.006 min
Response: 18506498
Conc: 6.54 ng/ml