

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080619\
 Data File : PL051110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 17:05
 Operator : SM\AJ
 Sample : K4154-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PS-8

Manual Integrations
 APPROVED

Ankita
 8/8/2019 2:37:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 00:42:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.928	119.0E6	32856989	11.843	11.516
28)	SA Decachlor...	7.975	8.956	90778806	25648457	8.965	9.070
Target Compounds							
10)	B gamma-Chl...	5.203	6.022	85264742	27393506	5.402m	7.413m#
11)	B alpha-Chl...	5.250	6.094	139.7E6	72110186	9.158m	19.675m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080619\
Data File : PL051110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 17:05
Operator : SM\AJ
Sample : K4154-08
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
PS-8


Manual Integrations
APPROVED

Ankita
8/8/2019 2:37:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 00:42:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

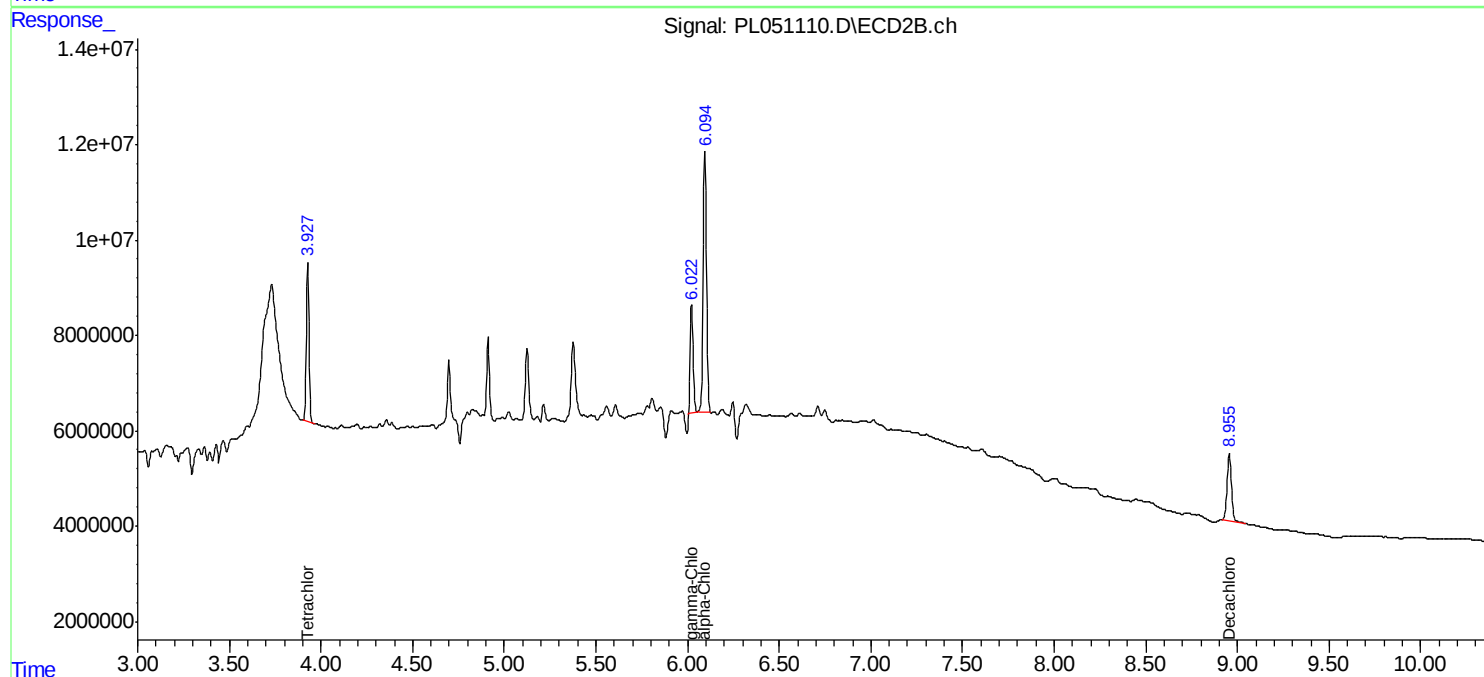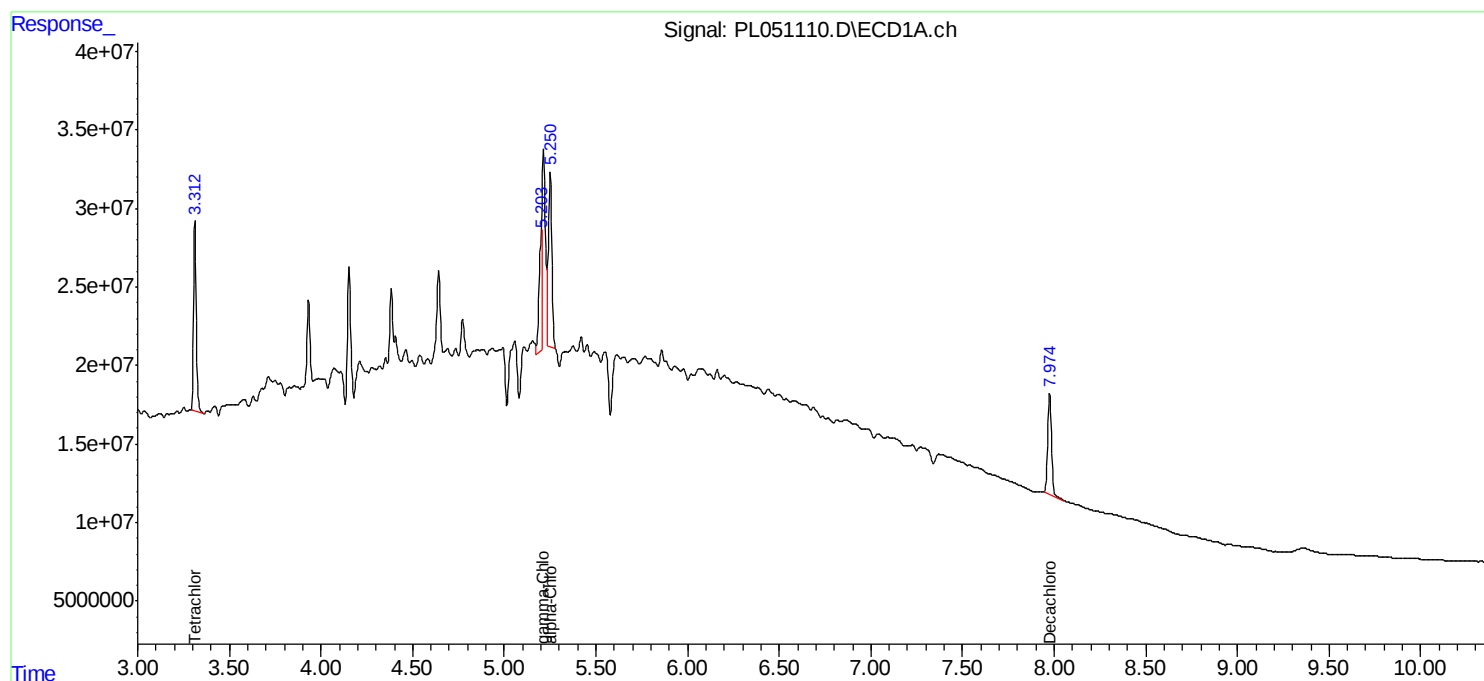

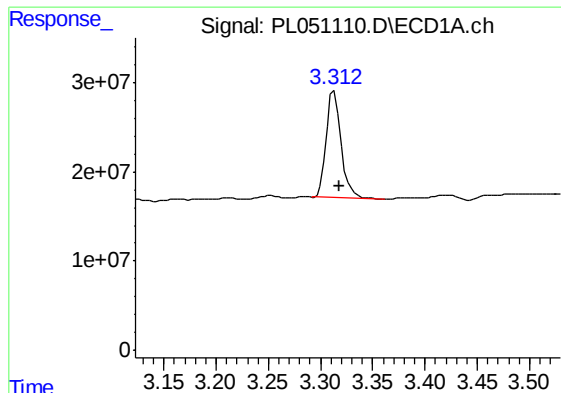


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.005 min
Response: 118995374
Conc: 11.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PS-8


Manual Integrations
APPROVED

Ankita
8/8/2019 2:37:49 PM

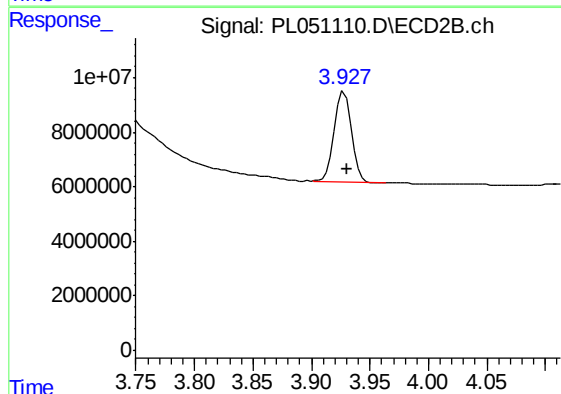


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.003 min
Response: 32856989
Conc: 11.52 ng/ml

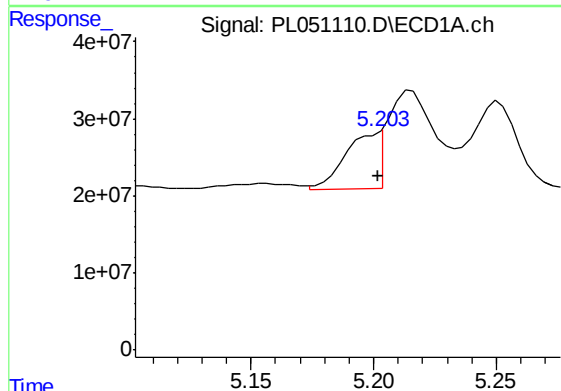


#10 gamma-Chlordane

R.T.: 5.203 min
Delta R.T.: 0.001 min
Response: 85264742
Conc: 5.40 ng/ml m

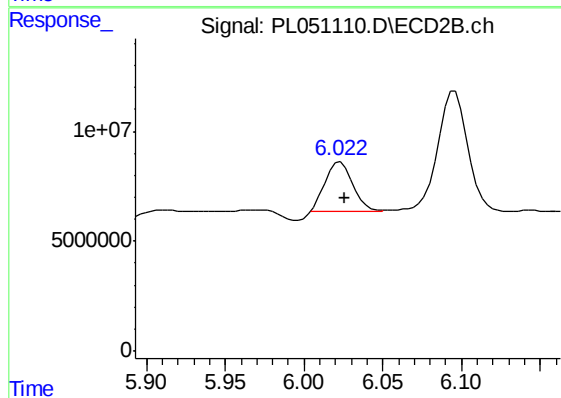

#10 gamma-Chlordane

R.T.: 6.022 min
Delta R.T.: -0.005 min
Response: 27393506
Conc: 7.41 ng/ml m

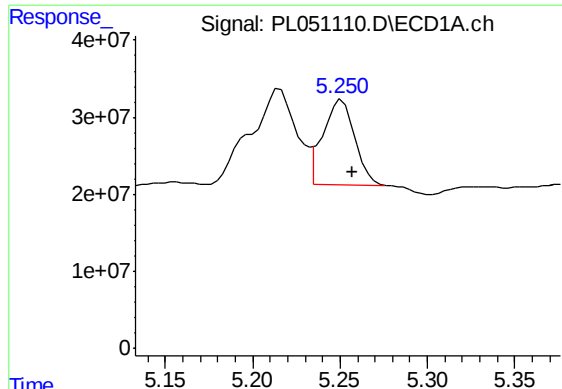


#11 alpha-Chlordane

R.T.: 5.250 min
Delta R.T.: -0.008 min
Response: 139711477
Conc: 9.16 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PS-8


Manual Integrations
APPROVED

Ankita
8/8/2019 2:37:49 PM

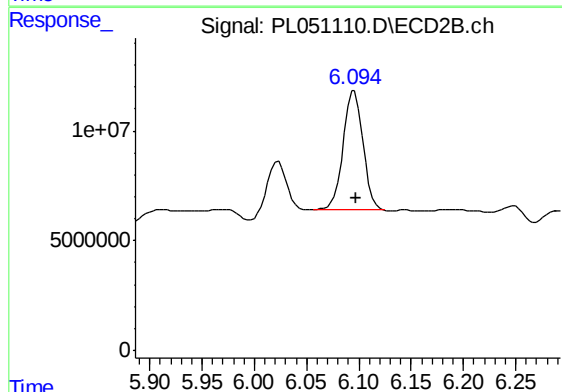


#11 alpha-Chlordane

R.T.: 6.094 min
Delta R.T.: -0.004 min
Response: 72110186
Conc: 19.67 ng/ml m

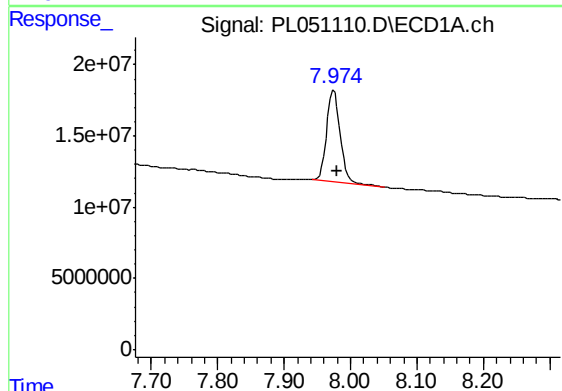

#28 Decachlorobiphenyl

R.T.: 7.975 min
Delta R.T.: -0.005 min
Response: 90778806
Conc: 8.97 ng/ml

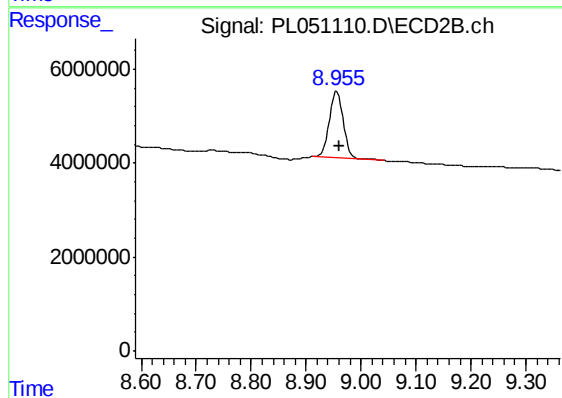

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: -0.006 min
Response: 25648457
Conc: 9.07 ng/ml