

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080619\
 Data File : PL051126.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 21:06
 Operator : SM\AJ
 Sample : K4144-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-007-SW125-073119

Manual Integrations
 APPROVED

Ankita
 8/7/2019 5:45:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 00:48:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.928	224.5E6	59595466	22.344	20.887
28)	SA Decachlor...	7.979	8.957	208.4E6	55388015	20.587	19.586
Target Compounds							
17)	MA 4,4'-DDT	6.167	7.041	7403011	846194	0.598m	0.313m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080619\
Data File : PL051126.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 21:06
Operator : SM\AJ
Sample : K4144-03
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EXT-007-SW125-073119


Manual Integrations
APPROVED

Ankita
8/7/2019 5:45:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 00:48:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

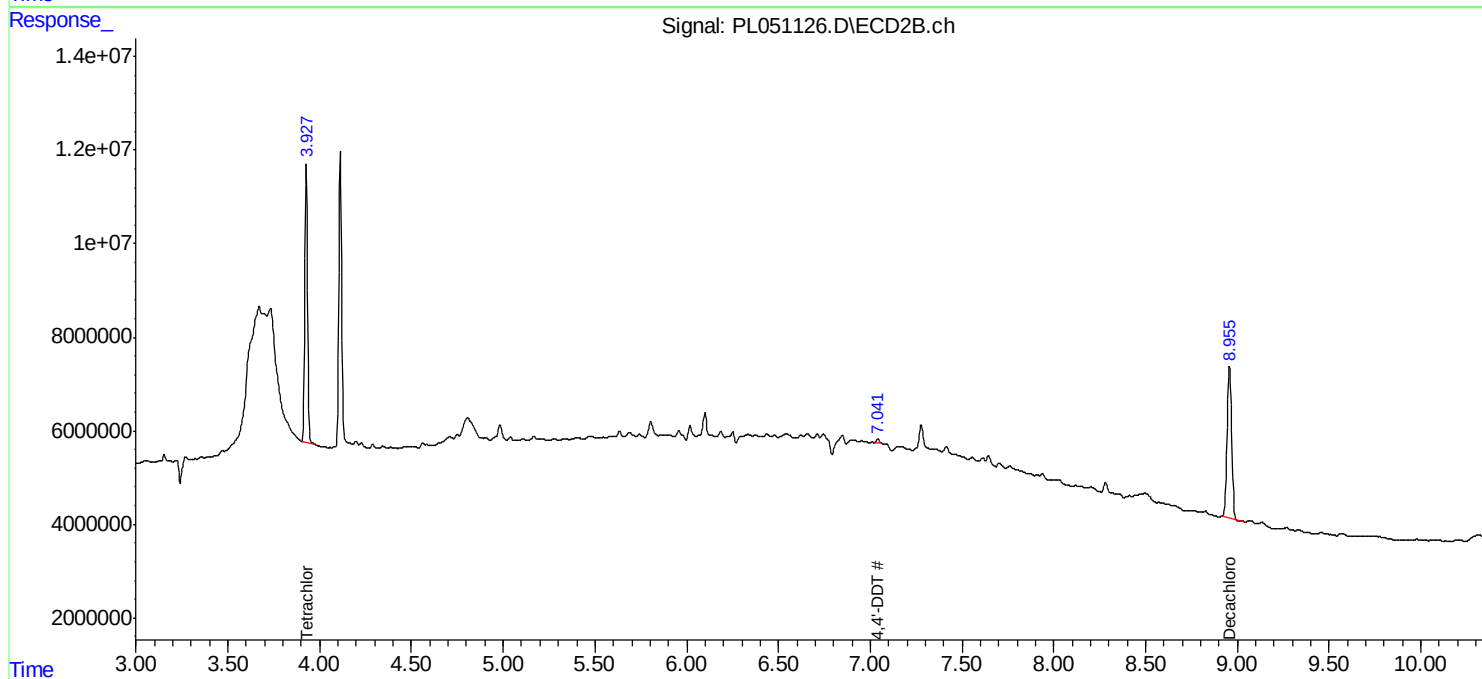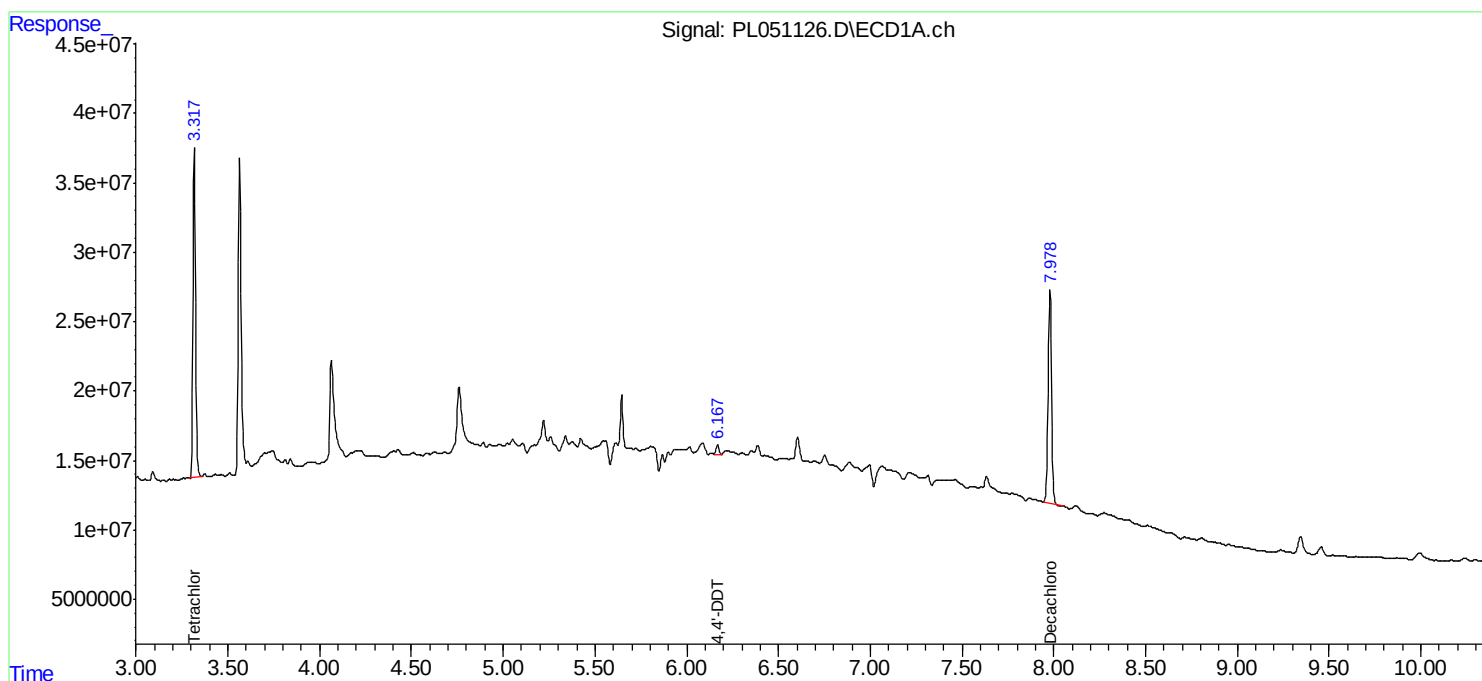

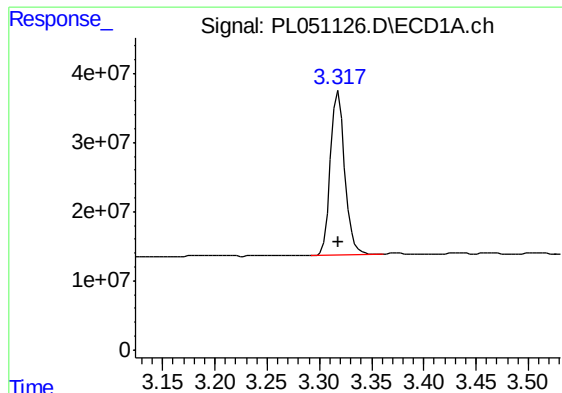


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 224508809
Conc: 22.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-007-SW125-073119


Manual Integrations
APPROVED

Ankita
8/7/2019 5:45:30 PM

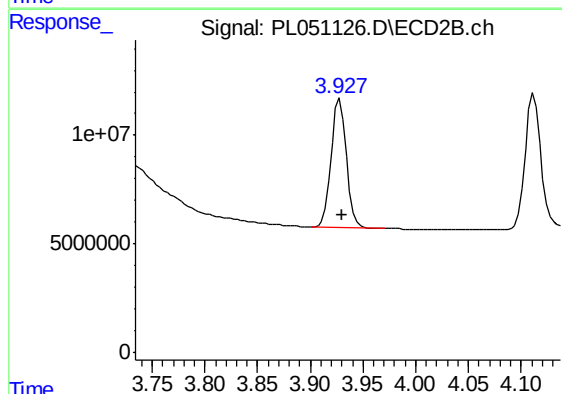


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 59595466
Conc: 20.89 ng/ml

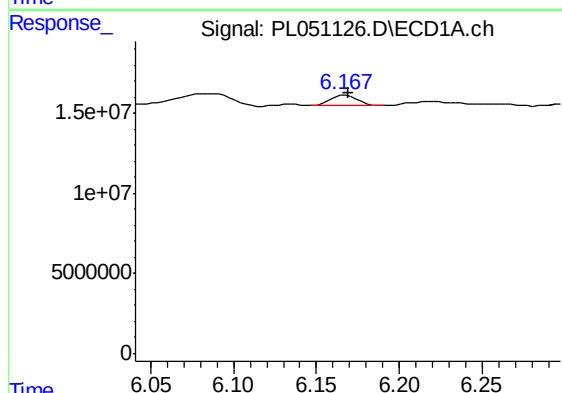


#17 4,4'-DDT

R.T.: 6.167 min
Delta R.T.: -0.003 min
Response: 7403011
Conc: 0.60 ng/ml m

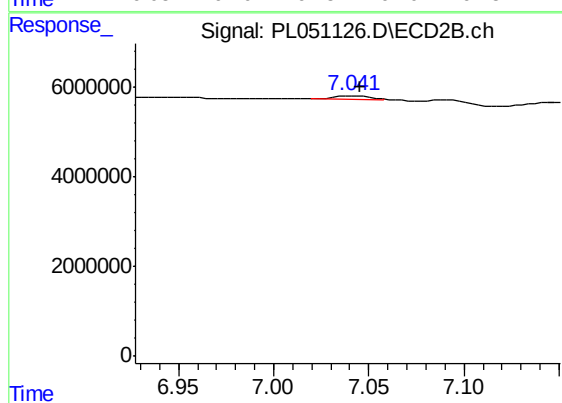

#17 4,4'-DDT

R.T.: 7.041 min
Delta R.T.: -0.005 min
Response: 846194
Conc: 0.31 ng/ml m

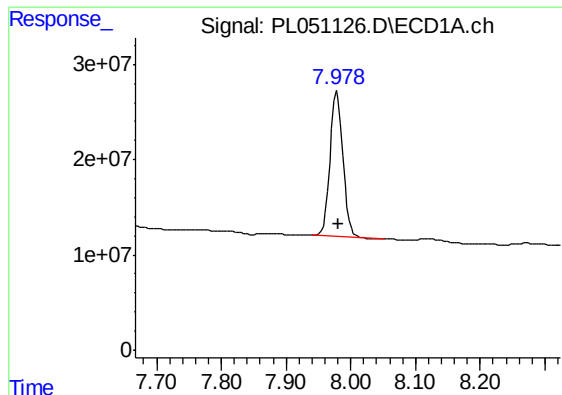


#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.002 min
Response: 208446529
Conc: 20.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-007-SW125-073119

Manual Integrations
APPROVED

Ankita
8/7/2019 5:45:30 PM

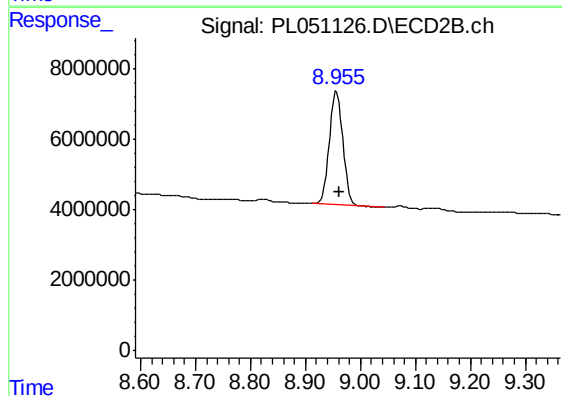

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.005 min
Response: 55388015
Conc: 19.59 ng/ml