

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080620\
 Data File : PL060506.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2020 07:09
 Operator : DD\AJ
 Sample : L3548-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT-019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 08:07:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 30 04:13:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.010	25678396	43919335	12.884	16.791 #
28)	SA Decachlor...	8.219	9.098	24366436	29223194	15.967	16.247
Target Compounds							
8)	B Heptachlo...	0.000	5.882	0	7954900	N.D.	3.283 #
11)	B alpha-Chl...	0.000	6.200	0	3425727	N.D.	1.173 #
12)	B 4,4'-DDE	0.000	6.353	0	8219373	N.D.	3.107 #
14)	MA Endrin	0.000	6.727	0	4417162	N.D.	1.886 #
17)	MA 4,4'-DDT	6.383	7.146	7573456	12674287	5.544	6.267
26)	Chlordane-4	0.000	6.200	0	3425727	N.D.	7.504 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080620\
Data File : PL060506.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2020 07:09
Operator : DD\AJ
Sample : L3548-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CRT-019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 08:07:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
Quant Title : GC Extractables
QLast Update : Thu Jul 30 04:13:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

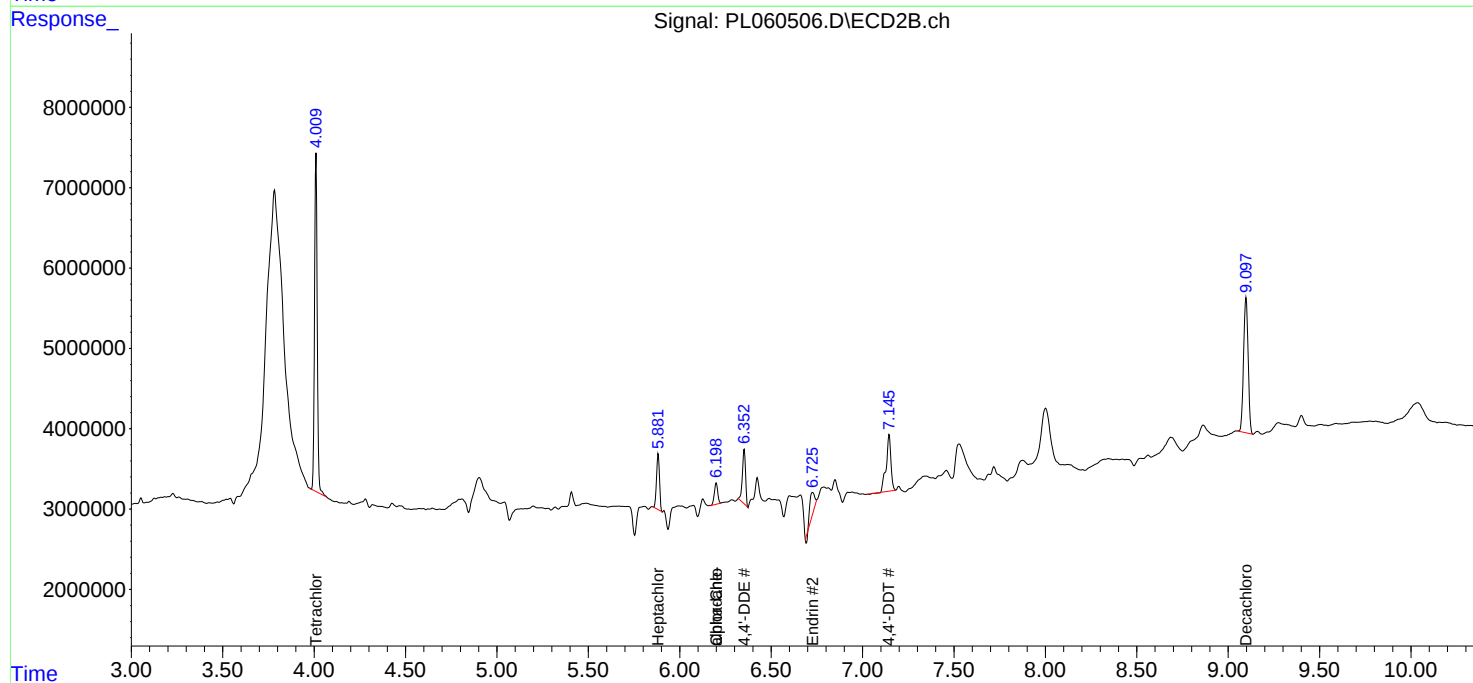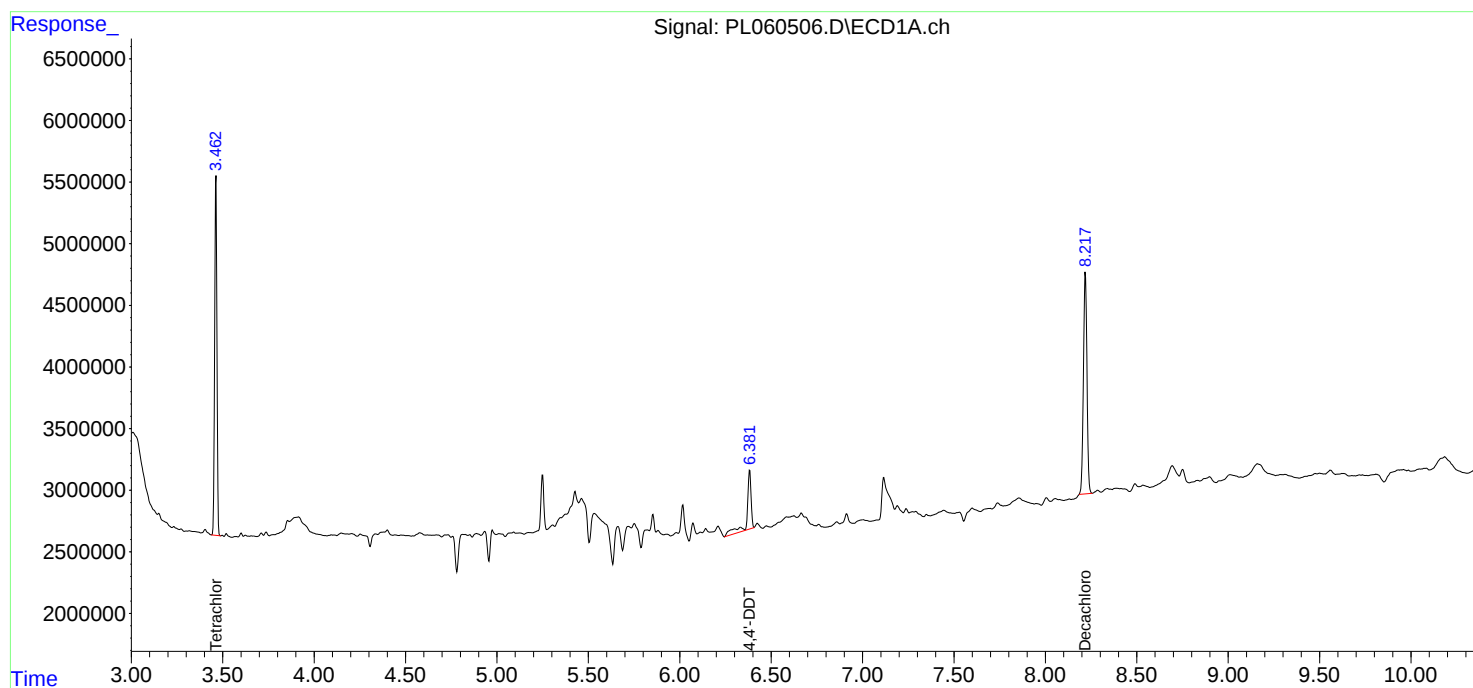


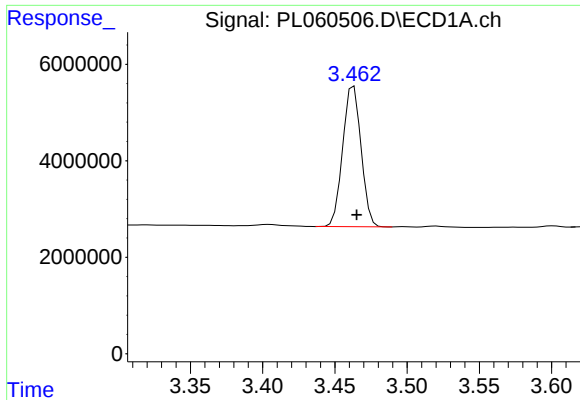

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: -0.002 min
Response: 25678396
Conc: 12.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT-019

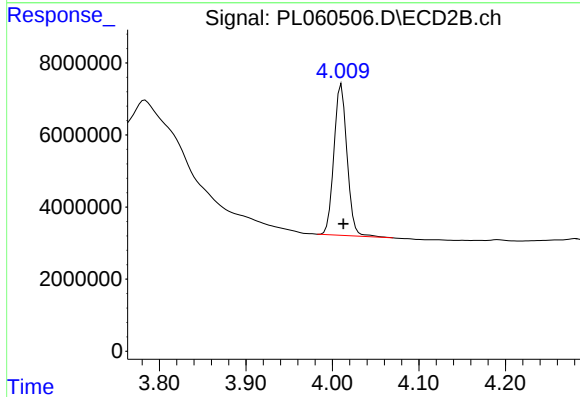


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: -0.002 min
Response: 43919335
Conc: 16.79 ng/ml

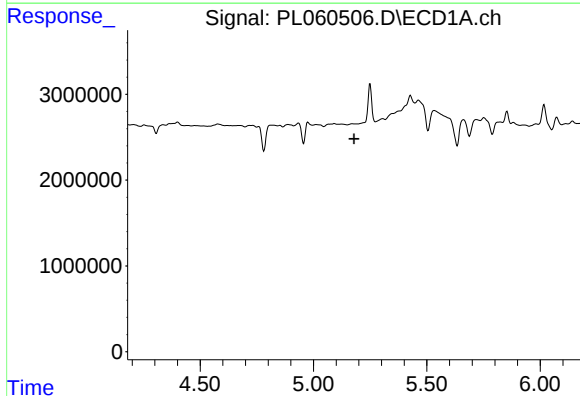


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.180 min
Response: 0
Conc: N.D.

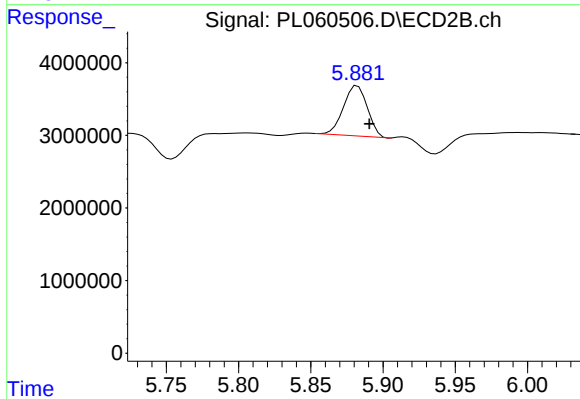

#8 Heptachlor epoxide


R.T.: 5.882 min
Delta R.T.: -0.008 min
Response: 7954900
Conc: 3.28 ng/ml

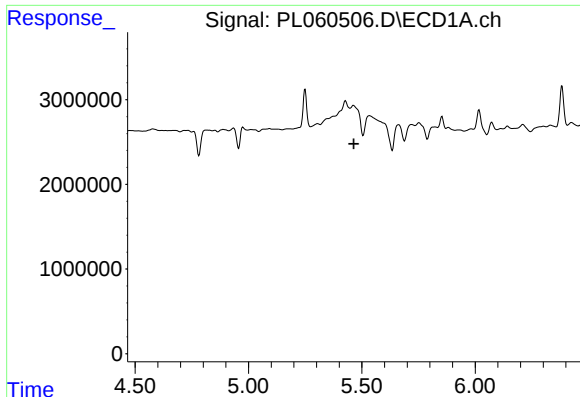

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CRT-019

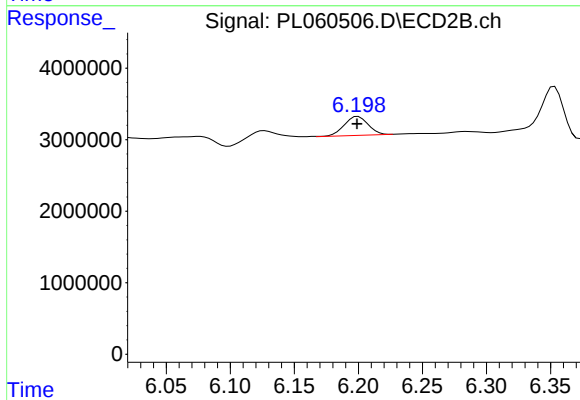


#11 alpha-Chlordane

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 3425727
Conc: 1.17 ng/ml

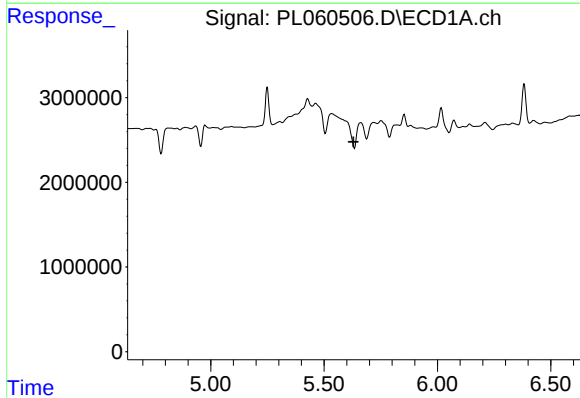


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.630 min
Response: 0
Conc: N.D.

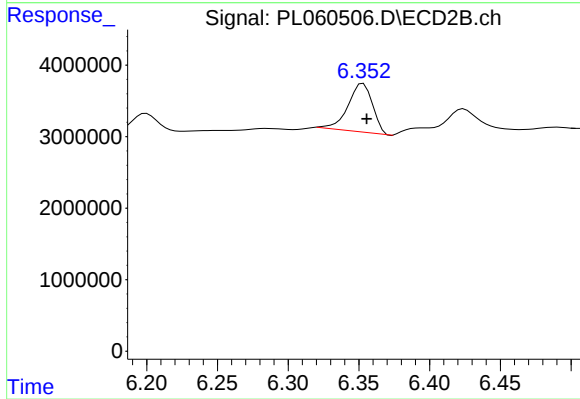

#12 4,4'-DDE


R.T.: 6.353 min
Delta R.T.: -0.003 min
Response: 8219373
Conc: 3.11 ng/ml

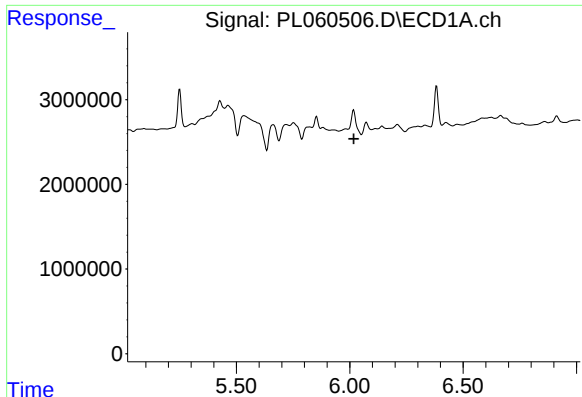

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.018 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CRT-019

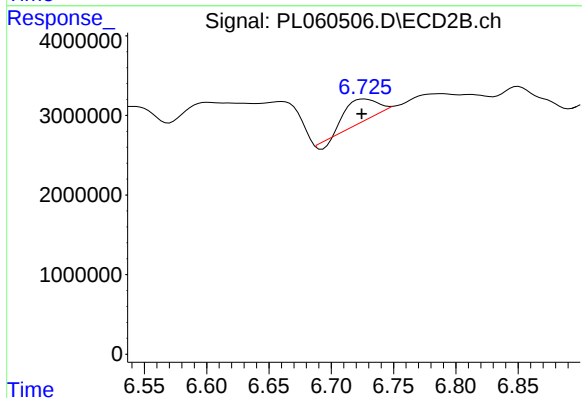


#14 Endrin

R.T.: 6.727 min
Delta R.T.: 0.002 min
Response: 4417162
Conc: 1.89 ng/ml

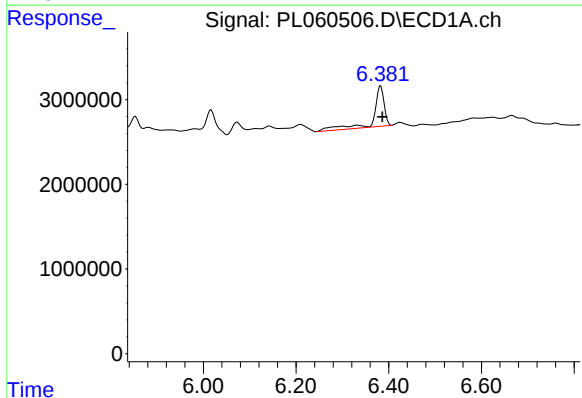


#17 4,4'-DDT

R.T.: 6.383 min
Delta R.T.: -0.004 min
Response: 7573456
Conc: 5.54 ng/ml

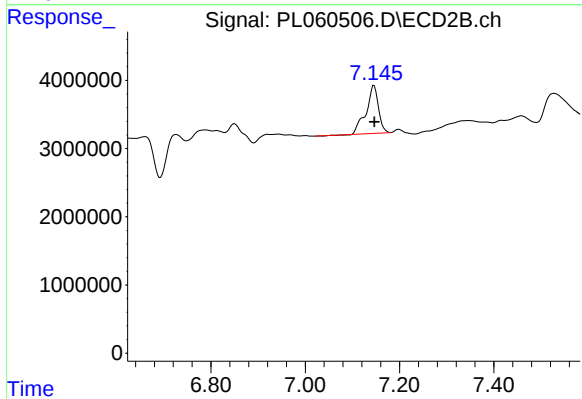

#17 4,4'-DDT


R.T.: 7.146 min
Delta R.T.: -0.001 min
Response: 12674287
Conc: 6.27 ng/ml

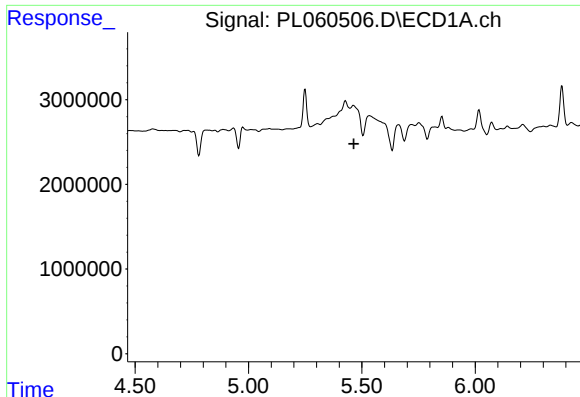

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CRT-019

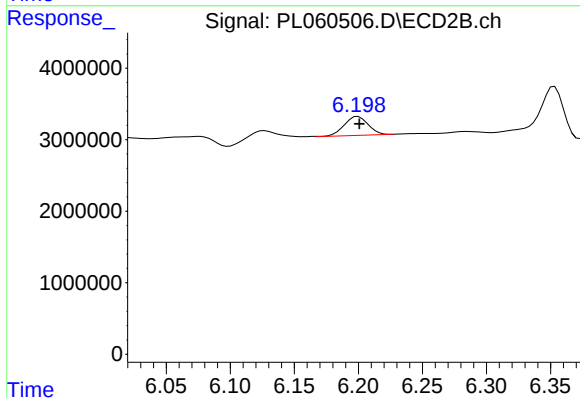


#26 Chlordane-4

R.T.: 6.200 min
Delta R.T.: -0.001 min
Response: 3425727
Conc: 7.50 ng/ml

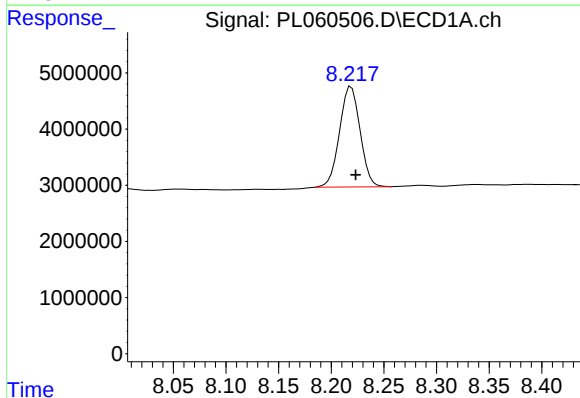

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: -0.004 min
Response: 24366436
Conc: 15.97 ng/ml

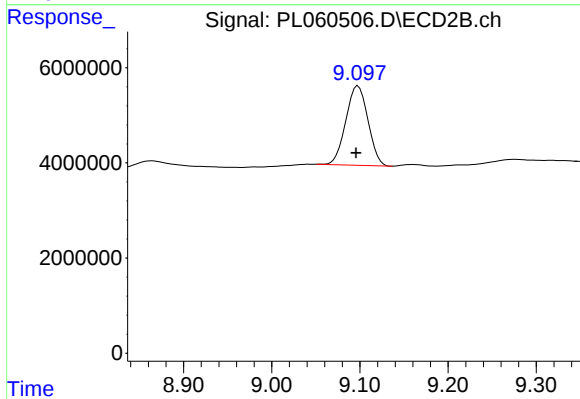

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.002 min
Response: 29223194
Conc: 16.25 ng/ml