

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080620\
 Data File : PL060534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2020 15:47
 Operator : DD\AJ
 Sample : L3568-05
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 8/5-F-J

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 16:25:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 30 04:13:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.010	24830116	35003416	12.458	13.383
28)	SA Decachlor...	8.219	9.098	23505438	32279313	15.402	17.947
Target Compounds							
3)	MA gamma-BHC...	0.000	4.691	0	2478384	N.D.	0.688 #
4)	MA Heptachlor	0.000	5.184	0	3762258	N.D.	1.105 #
8)	B Heptachlo...	5.174	0.000	4984484	0	2.629	N.D. #
9)	A Endosulfan I	5.534f	0.000	11841127	0	7.082	N.D. #
23)	Chlordane-1	0.000	4.981f	0	1249412	N.D.	13.149 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080620\
Data File : PL060534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2020 15:47
Operator : DD\AJ
Sample : L3568-05
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
8/5-F-J

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 16:25:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
Quant Title : GC Extractables
QLast Update : Thu Jul 30 04:13:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

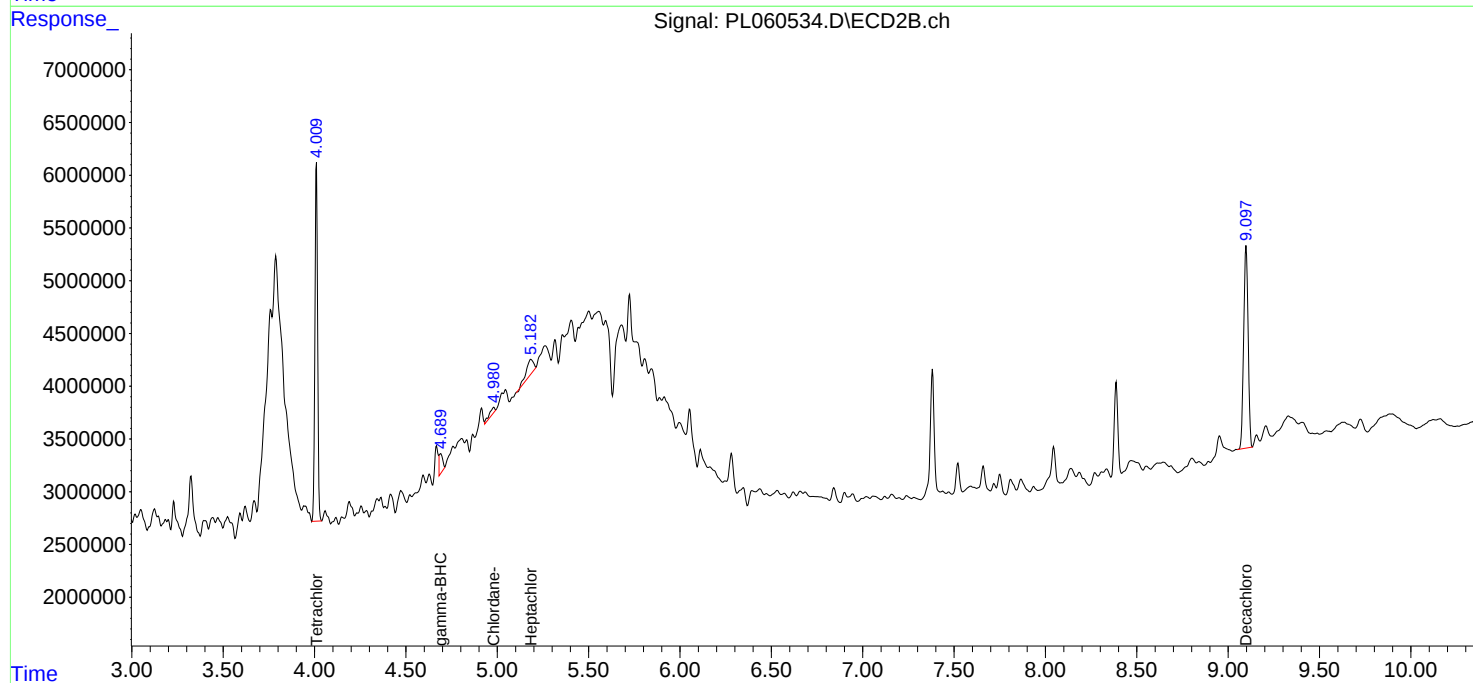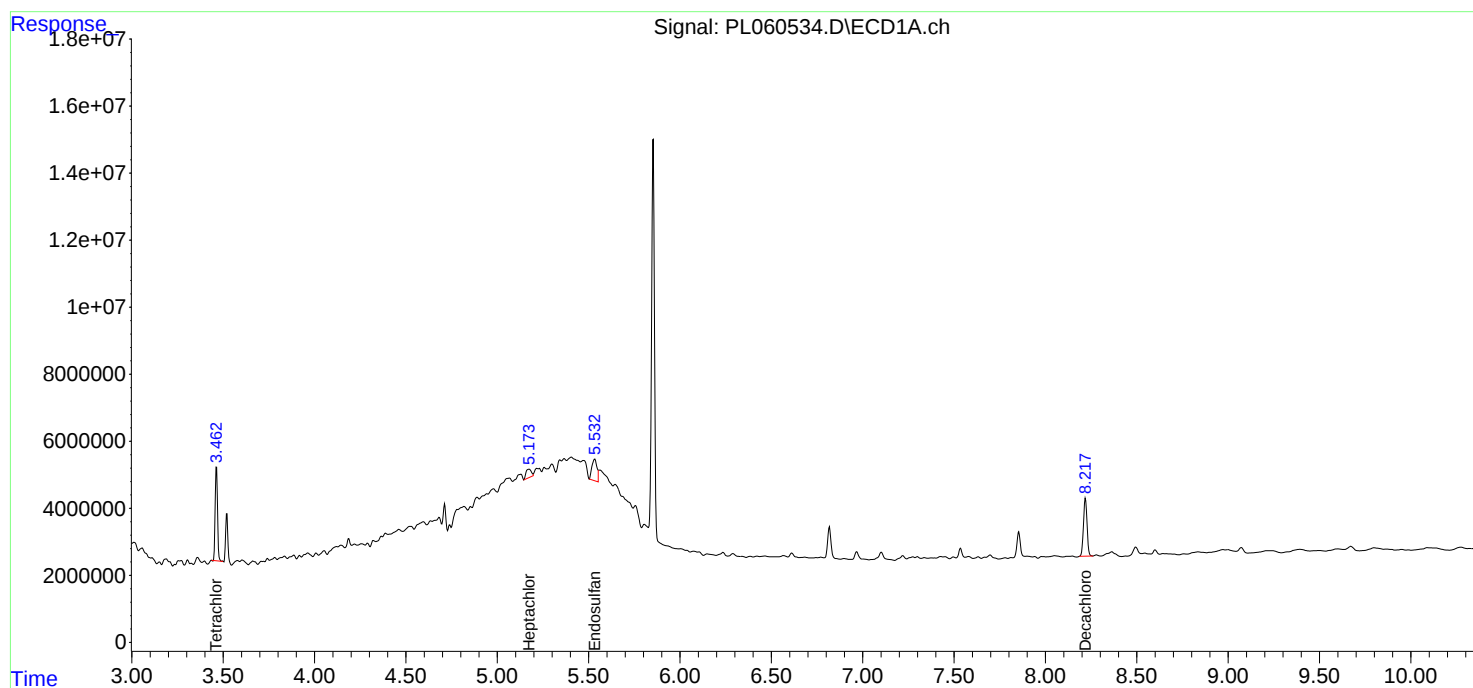


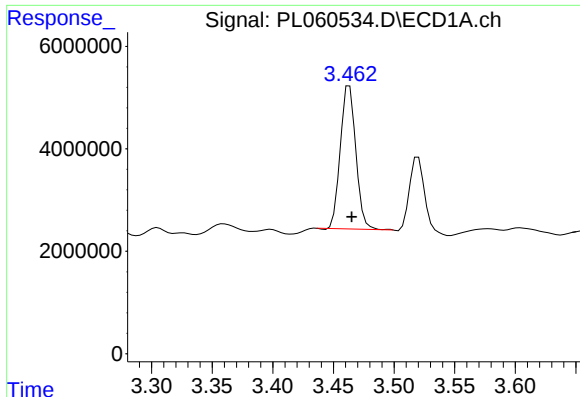

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: -0.002 min
Response: 24830116
Conc: 12.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
8/5-F-J

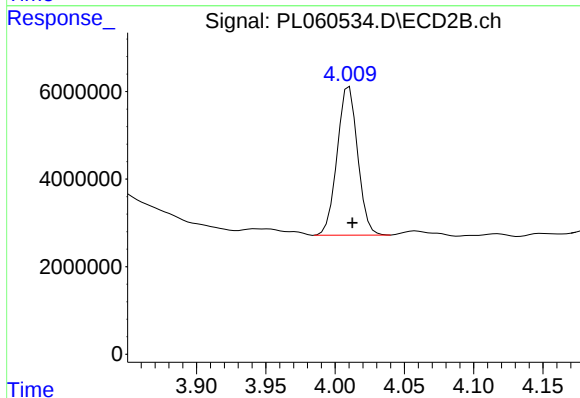


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: -0.002 min
Response: 35003416
Conc: 13.38 ng/ml

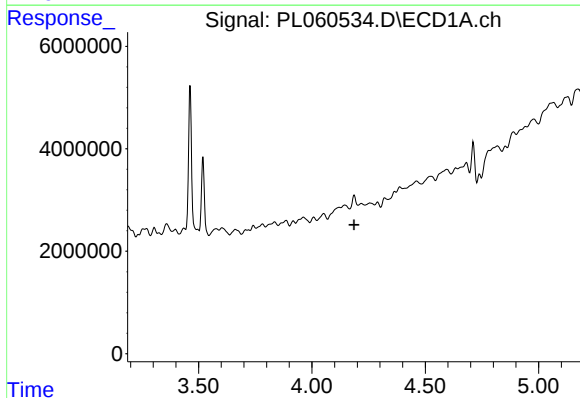


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.186 min
Response: 0
Conc: N.D.

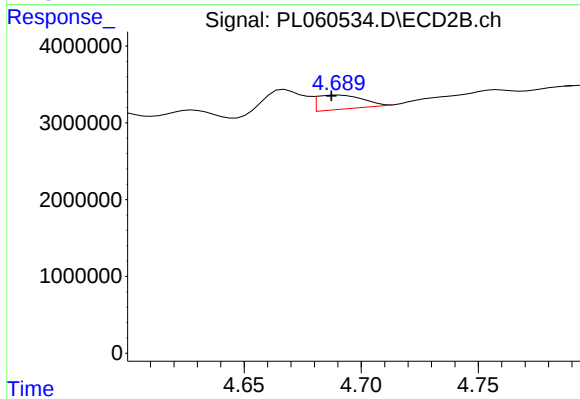

#3 gamma-BHC (Lindane)


R.T.: 4.691 min
Delta R.T.: 0.003 min
Response: 2478384
Conc: 0.69 ng/ml

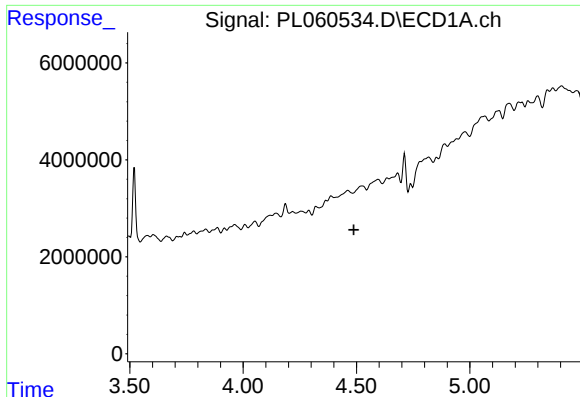

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.488 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
8/5-F-J

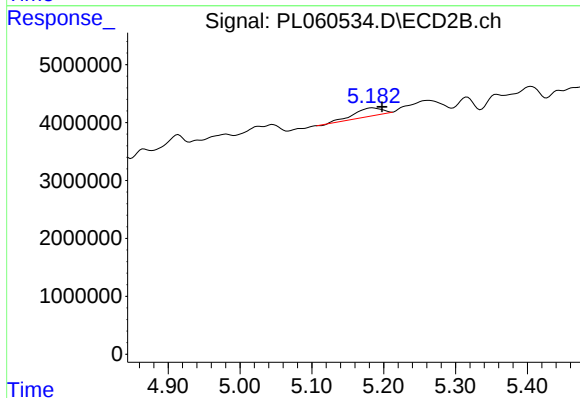


#4 Heptachlor

R.T.: 5.184 min
Delta R.T.: -0.014 min
Response: 3762258
Conc: 1.11 ng/ml

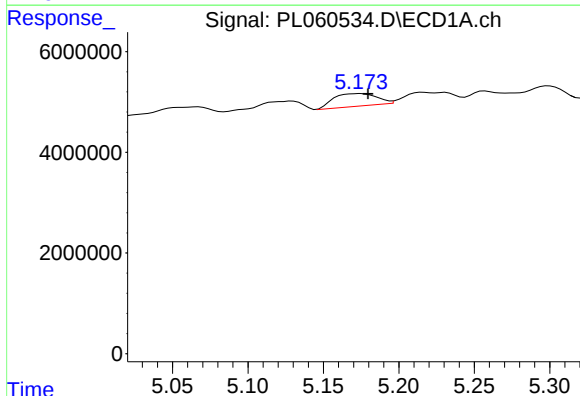


#8 Heptachlor epoxide

R.T.: 5.174 min
Delta R.T.: -0.005 min
Response: 4984484
Conc: 2.63 ng/ml

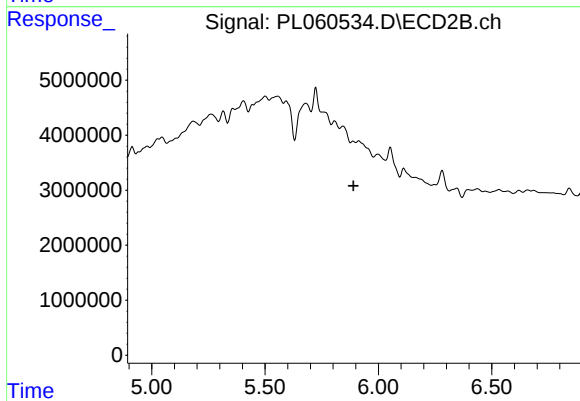

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.891 min
Response: 0
Conc: N.D.

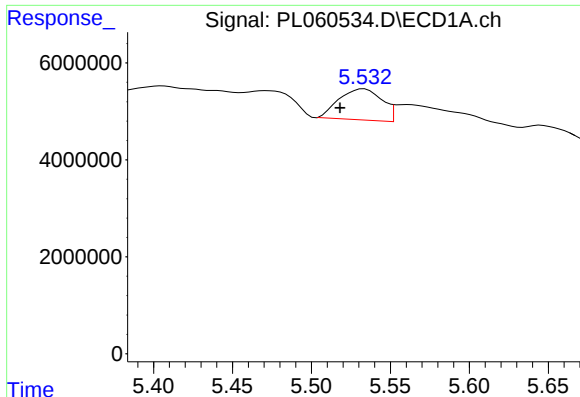

#9 Endosulfan I


R.T.: 5.534 min
Delta R.T.: 0.015 min
Response: 11841127
Conc: 7.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
8/5-F-J

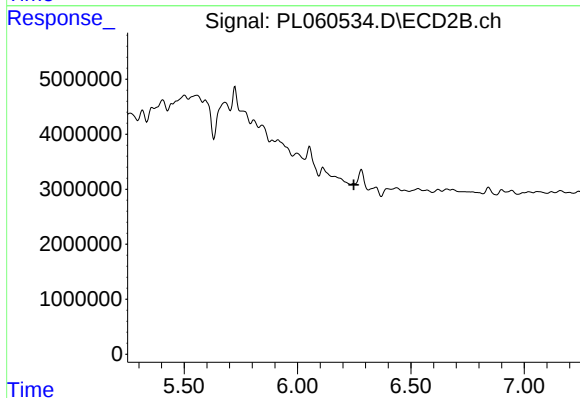


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.249 min
Response: 0
Conc: N.D.

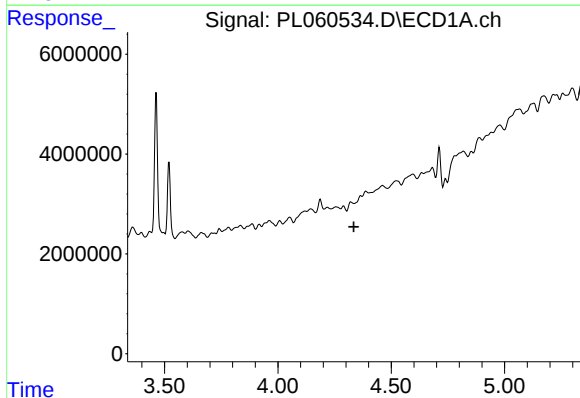


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.336 min
Response: 0
Conc: N.D.

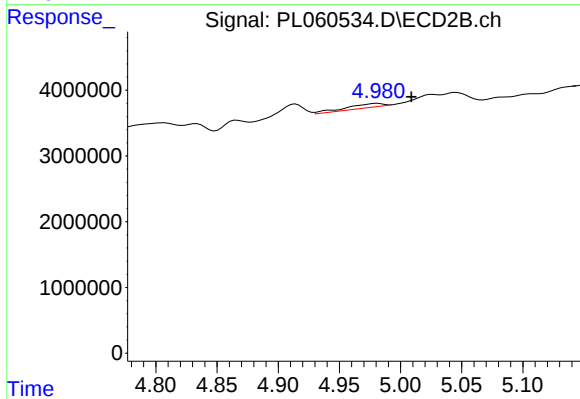

#23 Chlordane-1


R.T.: 4.981 min
Delta R.T.: -0.028 min
Response: 1249412
Conc: 13.15 ng/ml

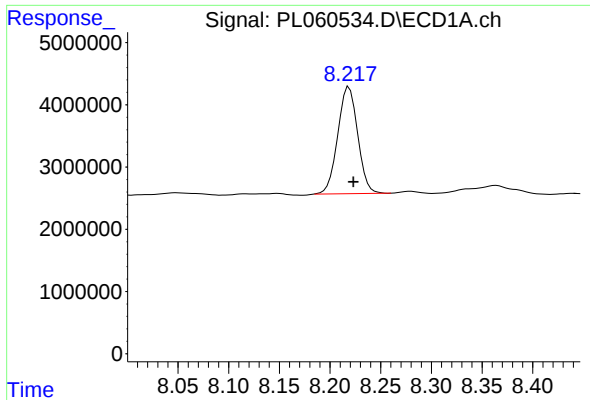

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: -0.004 min
Response: 23505438
Conc: 15.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
8/5-F-J

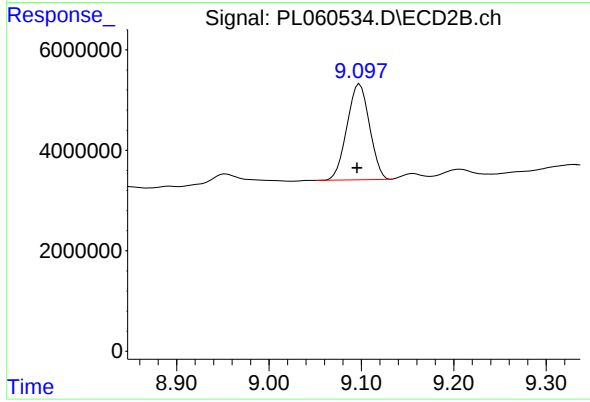

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.003 min
Response: 32279313
Conc: 17.95 ng/ml