

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080620\
 Data File : PL060534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2020 15:47
 Operator : DD\AJ
 Sample : L3568-05
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 8/5-F-J

Manual Integrations
 APPROVED

Ankita
 8/7/2020 1:09:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 16:25:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 30 04:13:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.010	25118261	35003416	12.603m	13.383
28)	SA Decachlor...	8.219	9.098	23505438	32279313	15.402	17.947

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080620\
Data File : PL060534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2020 15:47
Operator : DD\AJ
Sample : L3568-05
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
8/5-F-J


Manual Integrations
APPROVED

Ankita
8/7/2020 1:09:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 16:25:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
Quant Title : GC Extractables
QLast Update : Thu Jul 30 04:13:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

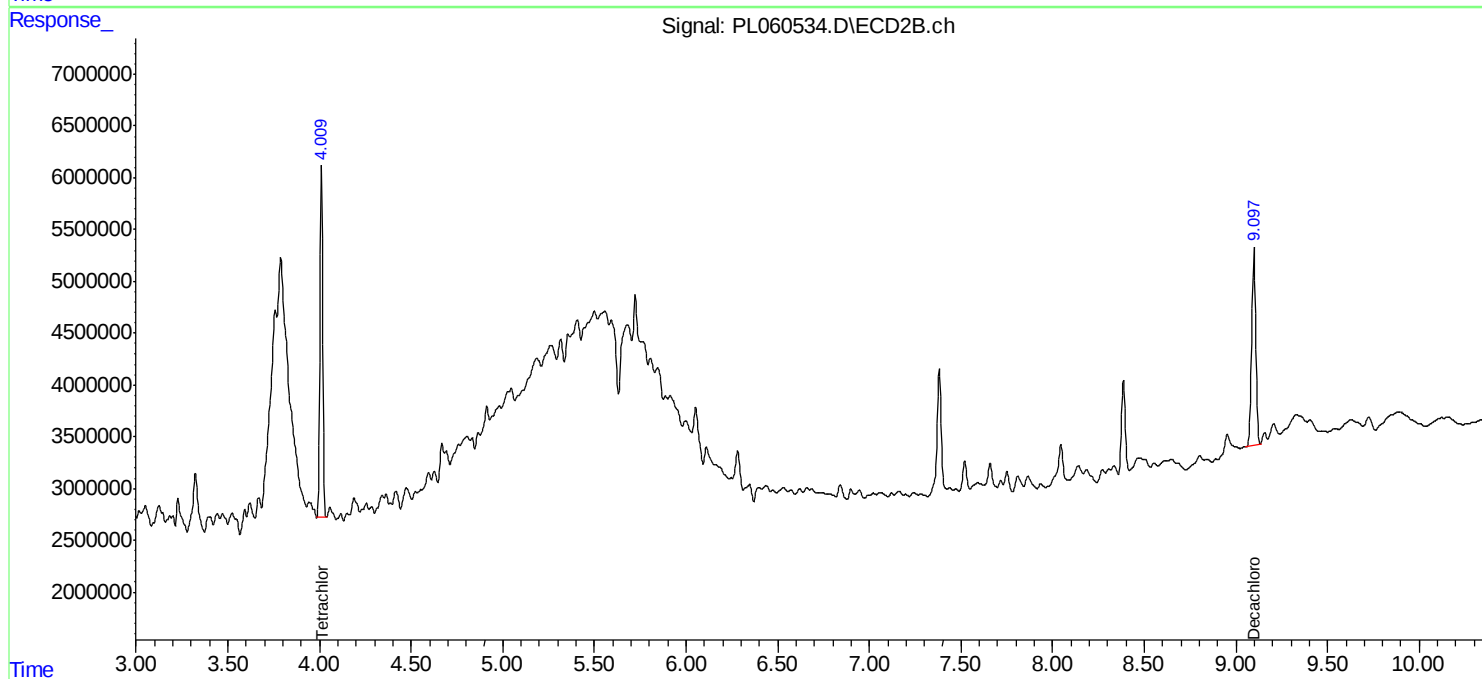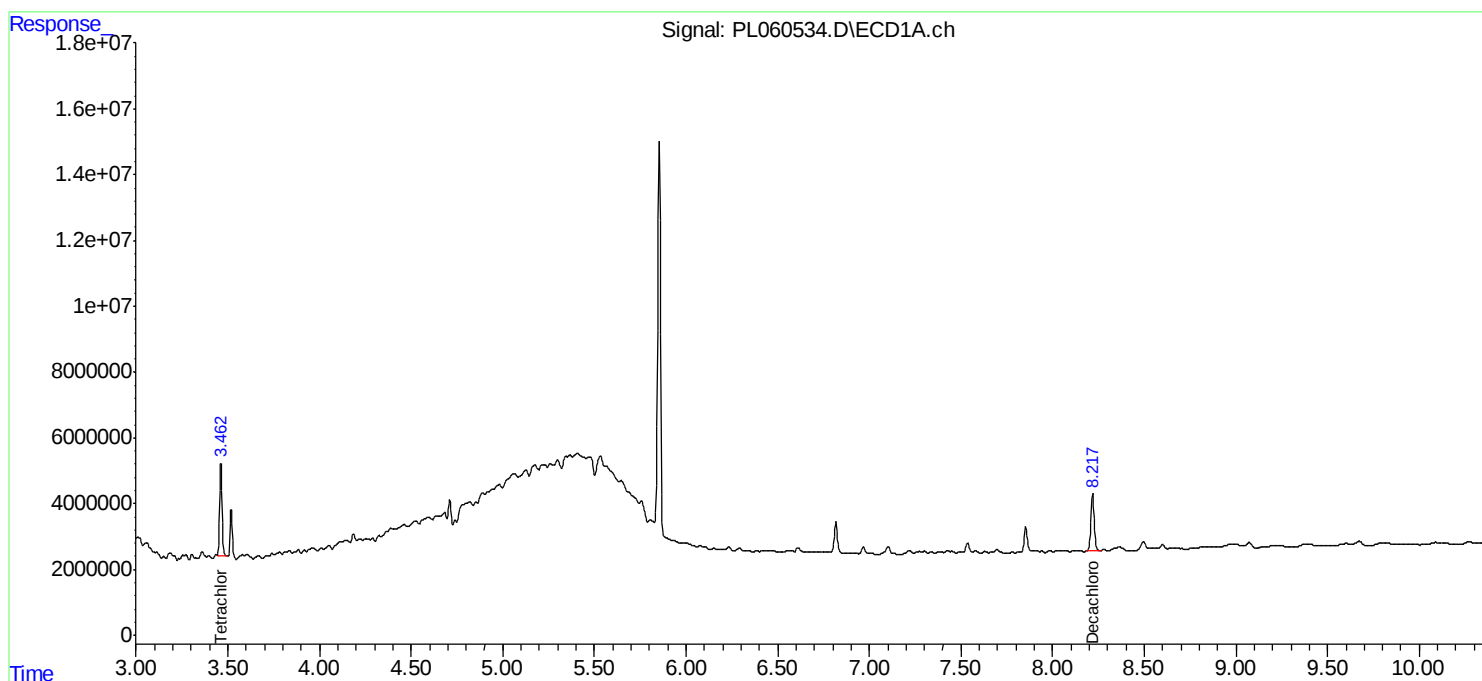

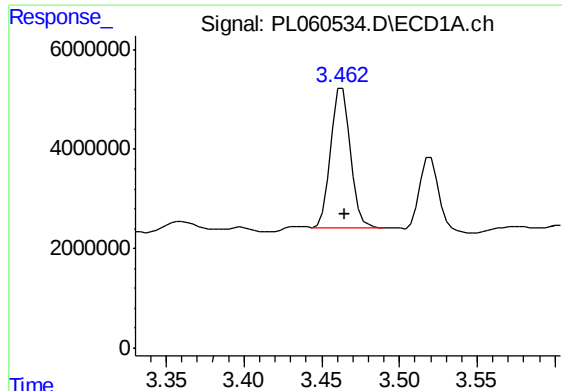


#1 Tetrachloro-m-xylene

R.T.: 3.462 min
Delta R.T.: -0.003 min
Response: 25118261
Conc: 12.60 ng/ml m

Instrument :
ECD_L
ClientSampleId :
8/5-F-J


Manual Integrations
APPROVED

Ankita
8/7/2020 1:09:02 PM

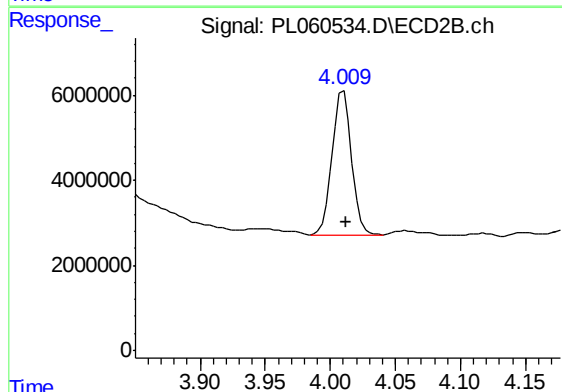


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: -0.002 min
Response: 35003416
Conc: 13.38 ng/ml

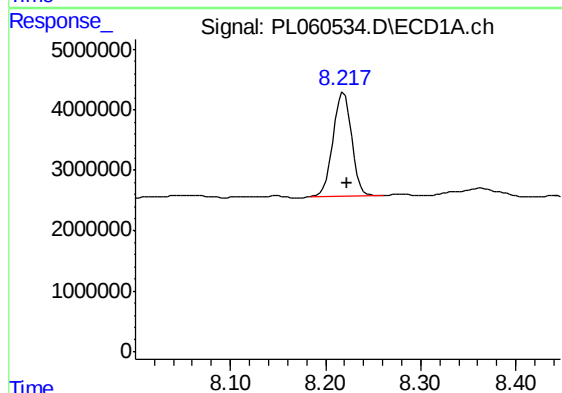

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: -0.004 min
Response: 23505438
Conc: 15.40 ng/ml

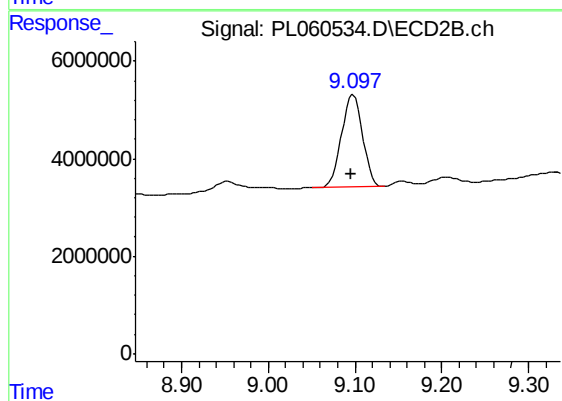

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.003 min
Response: 32279313
Conc: 17.95 ng/ml